
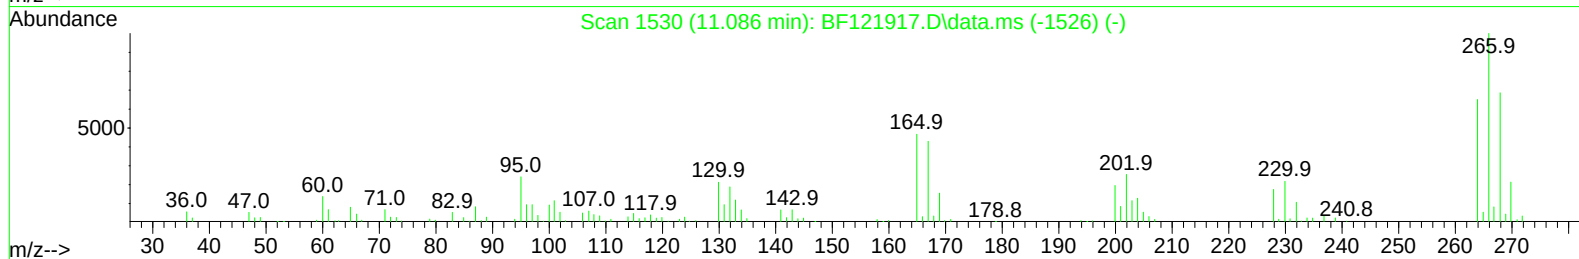
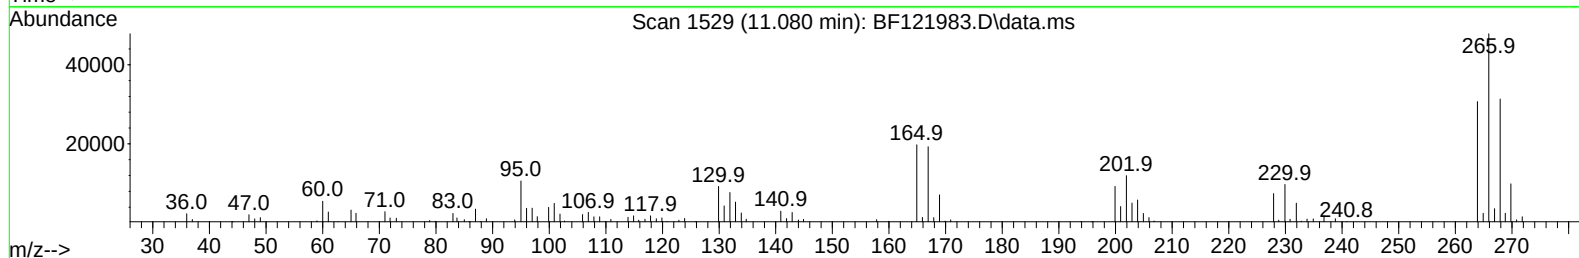


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121983.D
Acq On : 15 Oct 2020 10:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 02:51:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

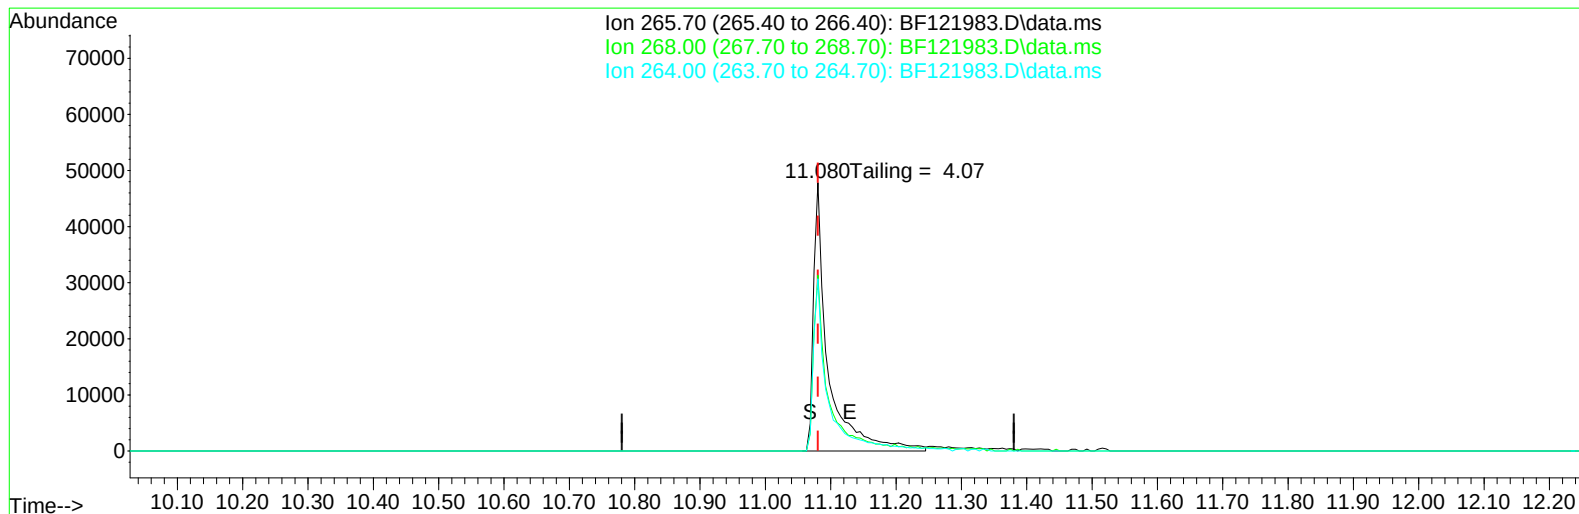

TIC: BF121983.D\data.ms

(70) Pentachlorophenol (C)




11.080min (+ 0.000) 63085.14 ng

response 74895

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	65.47
264.00	62.40	64.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121983.D
Acq On : 15 Oct 2020 10:19
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 02:51:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

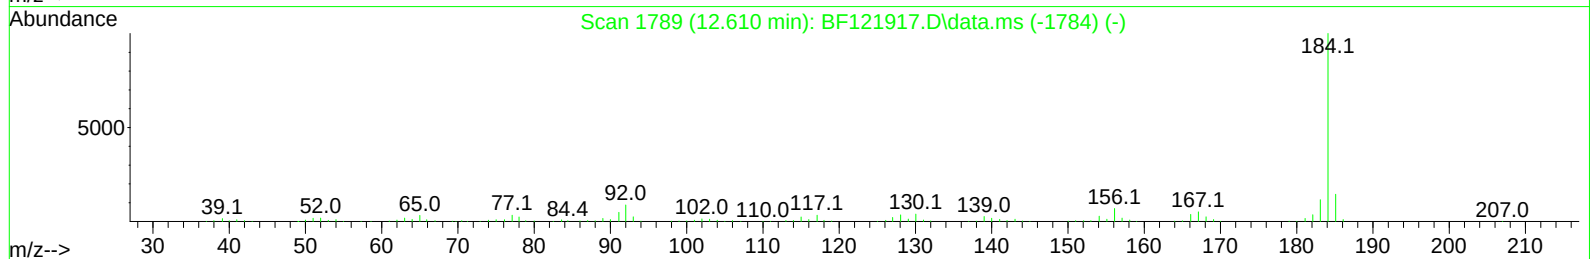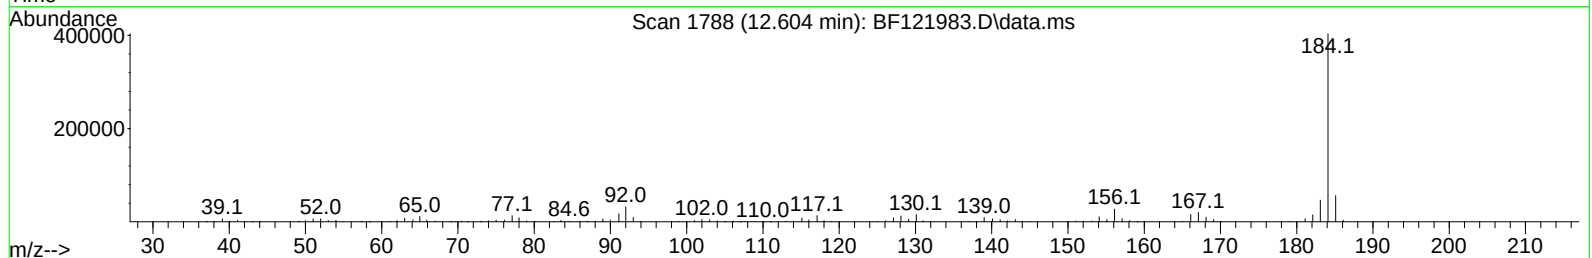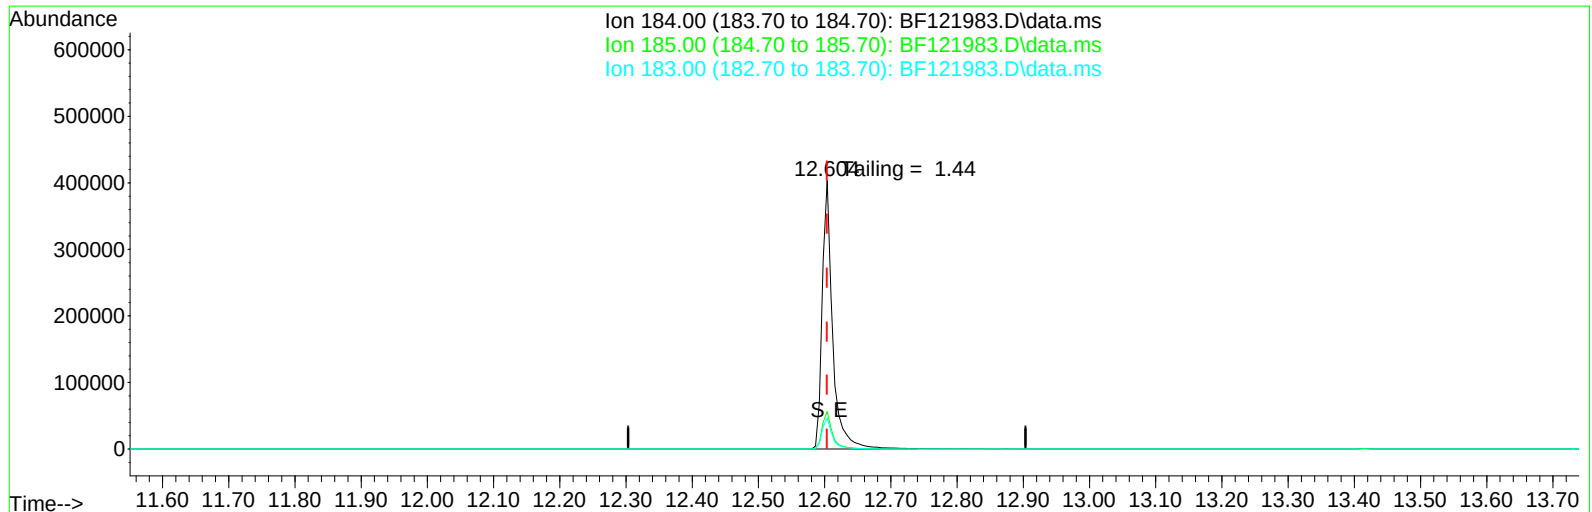

TIC: BF121983.D\data.ms

(77) Benzidine

12.604min (+ 0.000) 0.00 ng

response 442360

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.94
183.00	11.70	11.56
0.00	0.00	0.00