

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
 Data File : BF121993.D
 Acq On : 15 Oct 2020 16:15
 Operator : JU/CG
 Sample : L4407-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-02-062-A

Manual Integrations
 APPROVED

mohammad
 10/16/2020 12:47:52 PM

Quant Time: Oct 15 17:52:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 12:55:05 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.739	152	101465	20.00	ng	0.00
21) Naphthalene-d8	8.028	136	397505	20.00	ng	0.00
39) Acenaphthene-d10	9.775	164	204750	20.00	ng	0.00
64) Phenanthrene-d10	11.263	188	368911	20.00	ng	0.00
76) Chrysene-d12	13.904	240	221275	20.00	ng	0.00
86) Perylene-d12	15.339	264	217695	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	559927	81.45	ng	0.00
7) Phenol-d6	6.387	99	717702	81.10	ng	0.00
23) Nitrobenzene-d5	7.310	82	480790	62.03	ng	0.00
42) 2,4,6-Tribromophenol	10.569	330	149708	59.11	ng	0.00
45) 2-Fluorobiphenyl	9.098	172	837604	60.19	ng	0.00
79) Terphenyl-d14	12.845	244	705326	60.75	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.498	163	139891	9.34	ng	100
71) Phenanthrene	11.286	178	48228	2.38	ng	99
75) Fluoranthene	12.474	202	275006	12.68	ng	98
78) Pyrene	12.704	202	231898	13.75	ng	98
81) Benzo(a)anthracene	13.892	228	158900	10.96	ng	97
83) Chrysene	13.927	228	127174	8.93	ng	98
87) Indeno(1,2,3-cd)pyrene	16.751	276	81332	5.75	ng	94
88) Benzo(b)fluoranthene	14.927	252	168954m	11.48	ng	
89) Benzo(k)fluoranthene	14.951	252	53590m	3.83	ng	
90) Benzo(a)pyrene	15.280	252	121453	9.56	ng	100
91) Dibenzo(a,h)anthracene	16.751	278	24134m	2.07	ng	
92) Benzo(g,h,i)perylene	17.180	276	66189	5.68	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121993.D
Acq On : 15 Oct 2020 16:15
Operator : JU/CG
Sample : L4407-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED


mohammad
10/16/2020 12:47:52 PM

Quant Time: Oct 15 17:52:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration


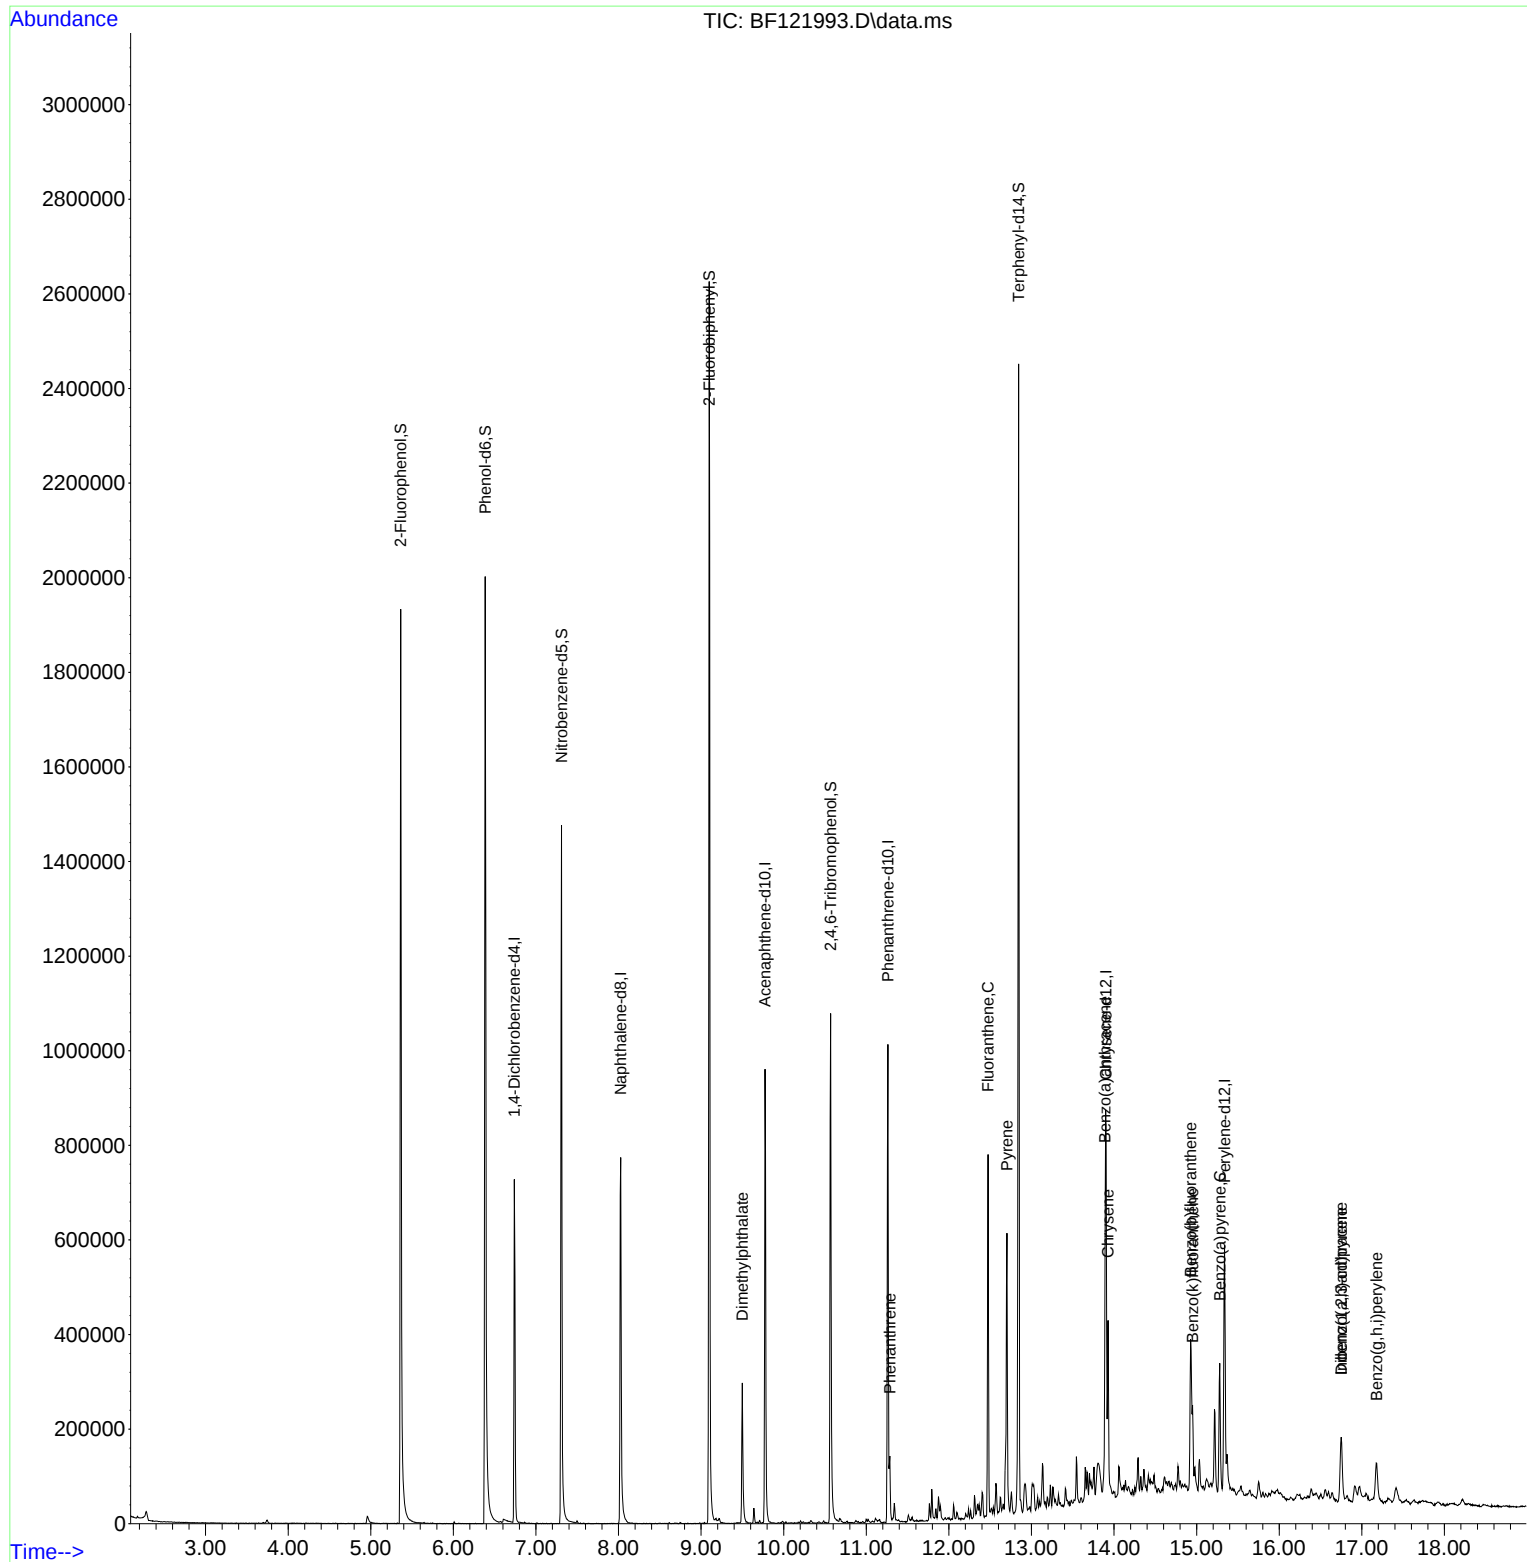




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.739 min Scan# 791
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

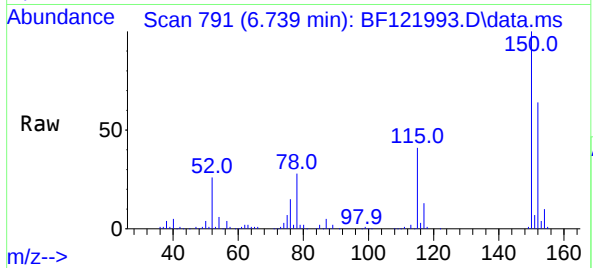


Tgt Ion:152 Resp: 101465
Ion Ratio Lower Upper
152 100
150 156.1 125.3 187.9
115 63.9 51.9 77.9

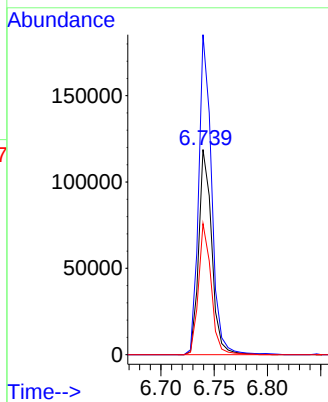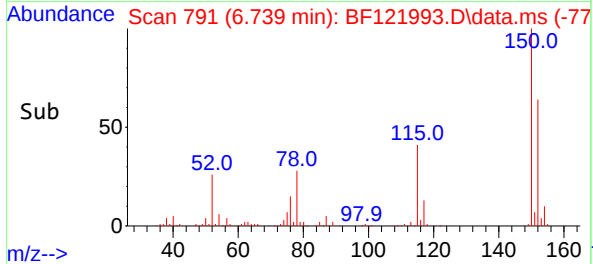


Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED



mohammad
10/16/2020 12:47:52 PM

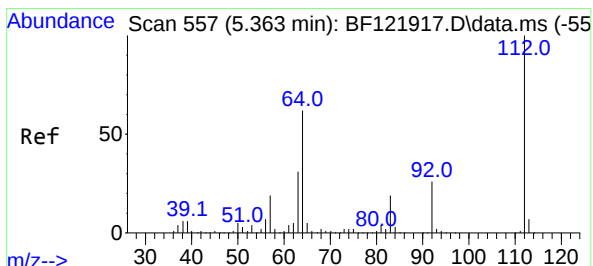

#5
2-Fluorophenol
Concen: 81.45 ng
RT: 5.363 min Scan# 557
Delta R.T. 0.000 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

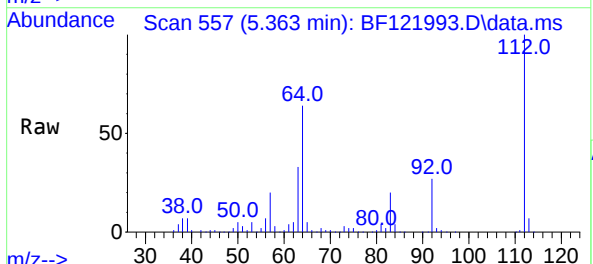

Tgt Ion:112 Resp: 559927
Ion Ratio Lower Upper
112 100
64 63.9 50.4 75.6
63 32.8 25.8 38.6

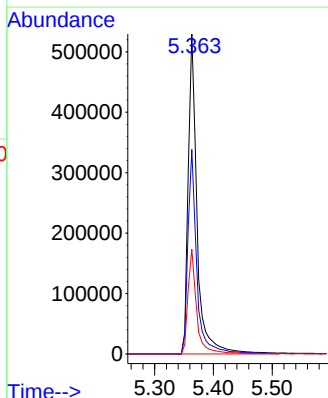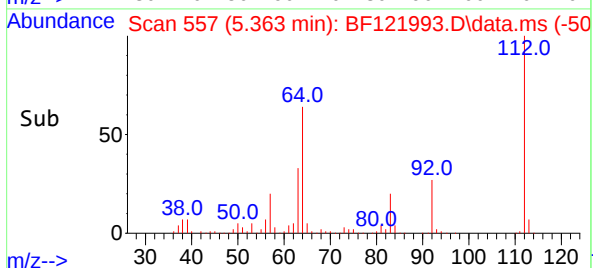



#7
Phenol-d6
Concen: 81.10 ng
RT: 6.387 min Scan# 731
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15





Tgt Ion: 99 Resp: 717702

Ion	Ratio	Lower	Upper
99	100		
42	20.6	15.9	23.9
71	34.3	27.1	40.7

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED




mohammad
10/16/2020 12:47:52 PM

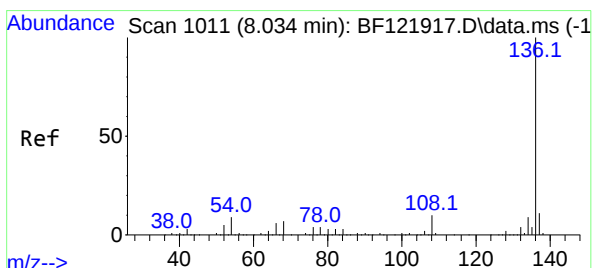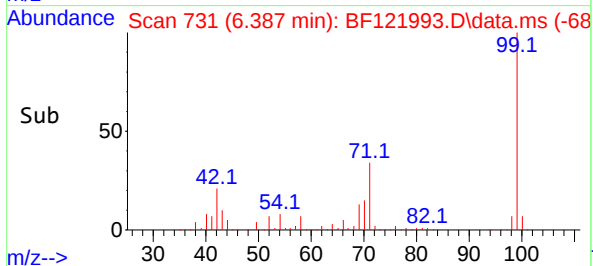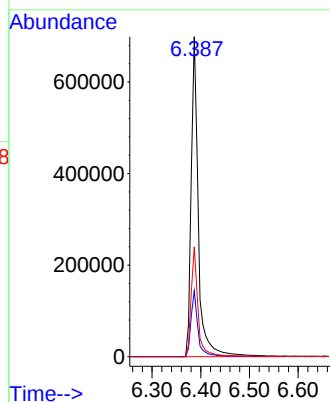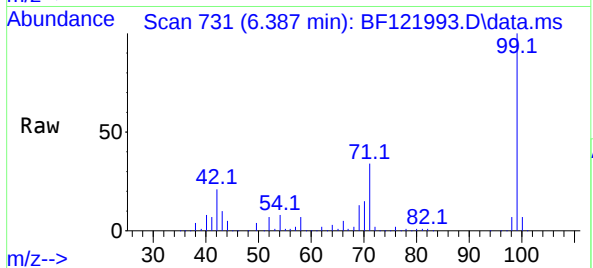


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion: 136 Resp: 397505

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	13.0
54	8.6	7.1	10.7
68	5.9	5.0	7.4

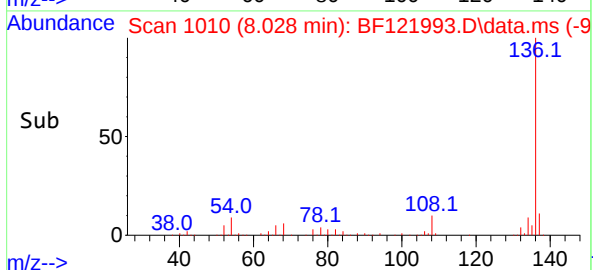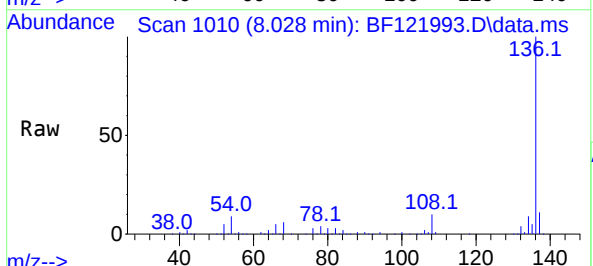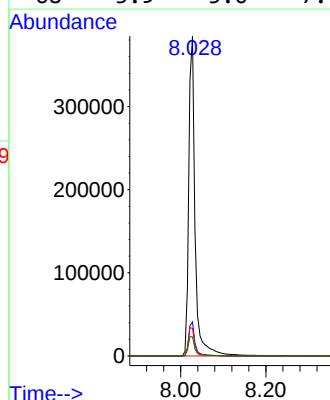

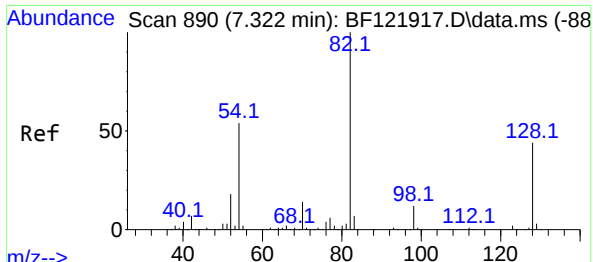





#23
Nitrobenzene-d5
Concen: 62.03 ng
RT: 7.310 min Scan# 888
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion: 82 Resp: 480790
Ion Ratio Lower Upper
82 100
128 42.8 35.0 52.4
54 54.0 43.9 65.9

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A




Manual Integrations
APPROVED

mohammad
10/16/2020 12:47:52 PM

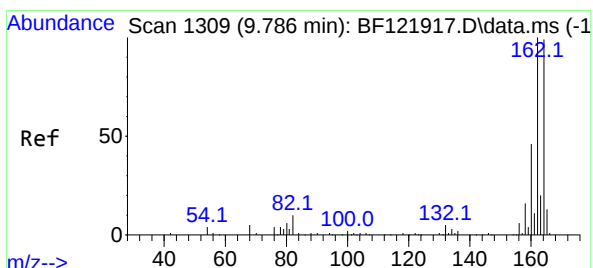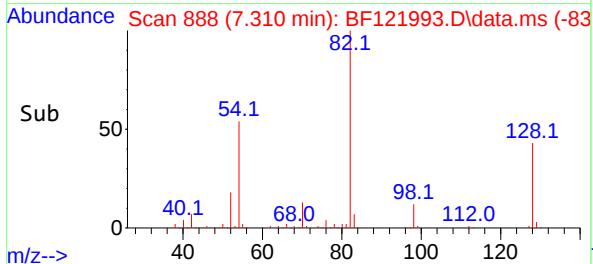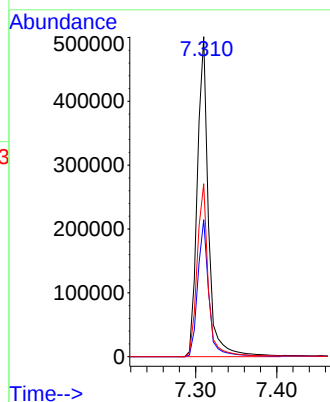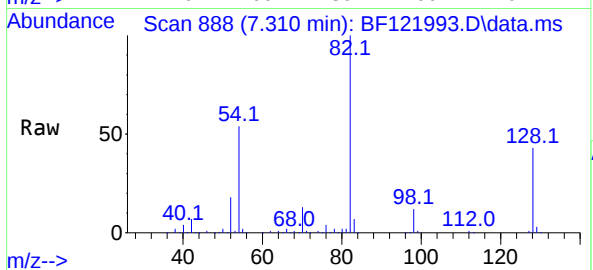


#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.775 min Scan# 1307
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:164 Resp: 204750
Ion Ratio Lower Upper
164 100
162 103.0 83.2 124.8
160 46.6 37.5 56.3

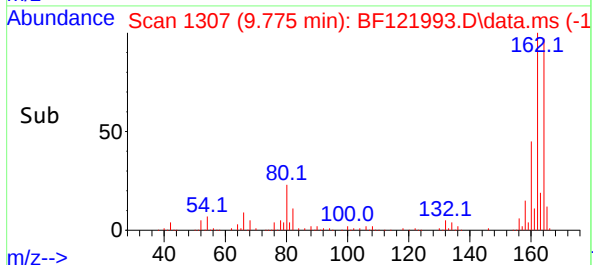
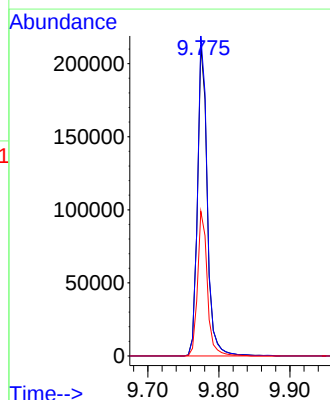
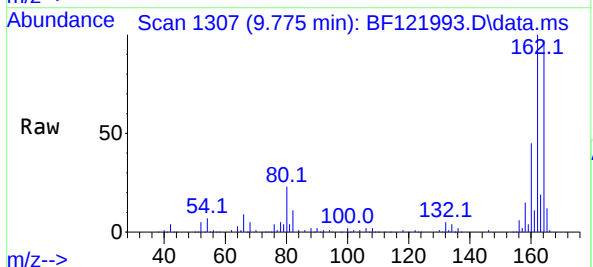





#42
2,4,6-Tribromophenol
Concen: 59.11 ng
RT: 10.569 min Scan# 1442
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

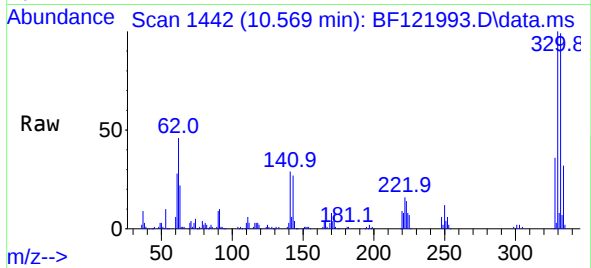



Tgt Ion: 330 Resp: 149708
Ion Ratio Lower Upper
330 100
332 96.7 77.3 115.9
141 30.4 22.3 33.5

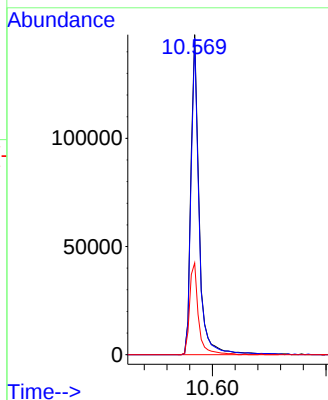

#45
2-Fluorobiphenyl
Concen: 60.19 ng
RT: 9.098 min Scan# 1192
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15



Tgt Ion: 172 Resp: 837604
Ion Ratio Lower Upper
172 100
171 35.8 29.1 43.7
170 23.9 19.8 29.6

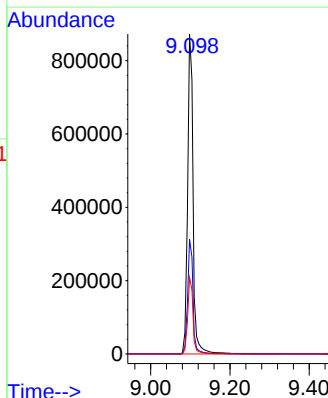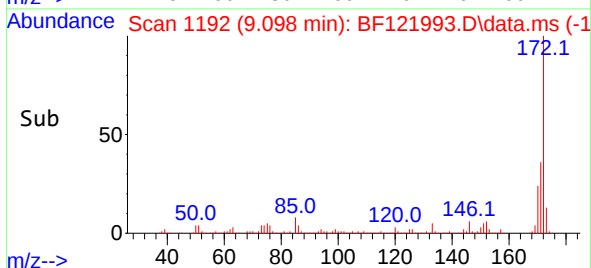

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED

mohammad
10/16/2020 12:47:52 PM







#50
Dimethylphthalate
Concen: 9.34 ng
RT: 9.498 min Scan# 1260
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:163 Resp: 139891
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.4 8.2 12.4

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A




Manual Integrations
APPROVED


mohammad
10/16/2020 12:47:52 PM

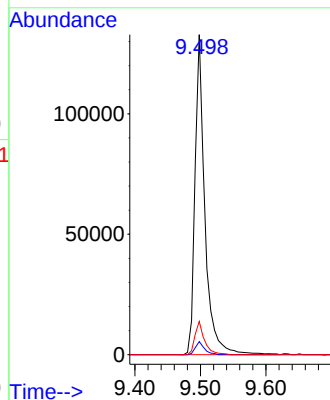


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.263 min Scan# 1560
Delta R.T. 0.000 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:188 Resp: 368911
Ion Ratio Lower Upper
188 100
94 9.9 8.3 12.5
80 10.3 9.1 13.7

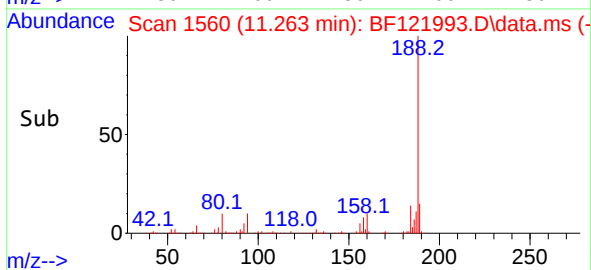
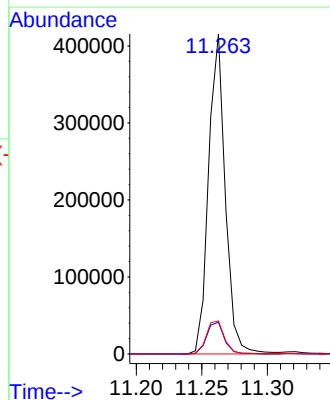






#71
Phenanthrene
Concen: 2.38 ng
RT: 11.286 min Scan# 1564
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

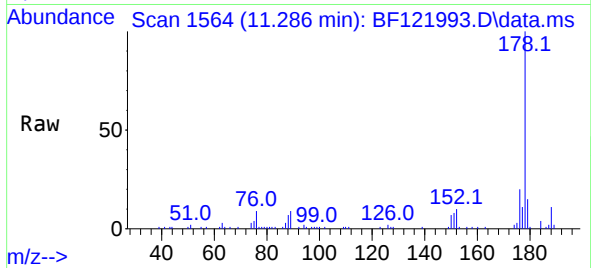



Tgt Ion:178 Resp: 48228
Ion Ratio Lower Upper
178 100
176 19.5 15.9 23.9
179 15.4 12.2 18.4

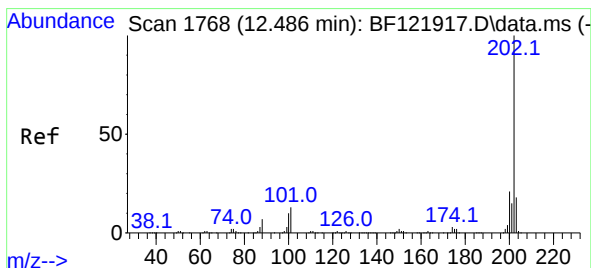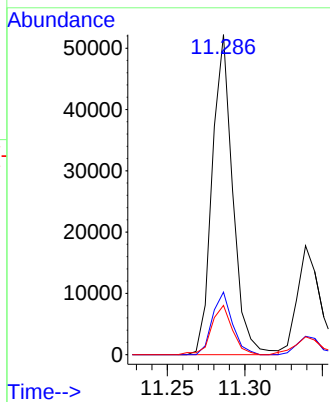

#75
Fluoranthene
Concen: 12.68 ng
RT: 12.474 min Scan# 1766
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

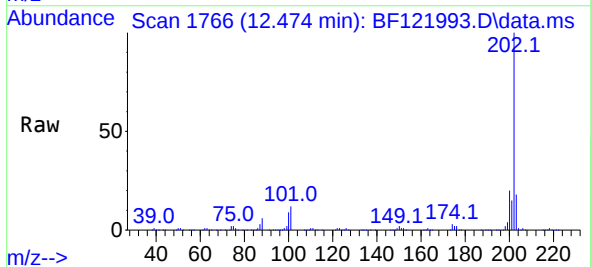


Tgt Ion:202 Resp: 275006
Ion Ratio Lower Upper
202 100
101 12.3 0.0 33.4
203 17.5 0.0 37.9

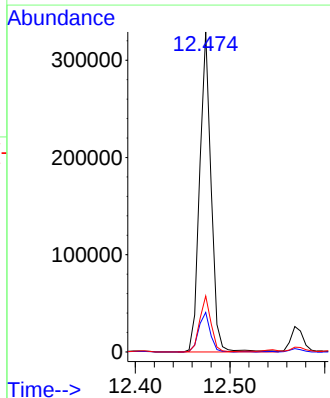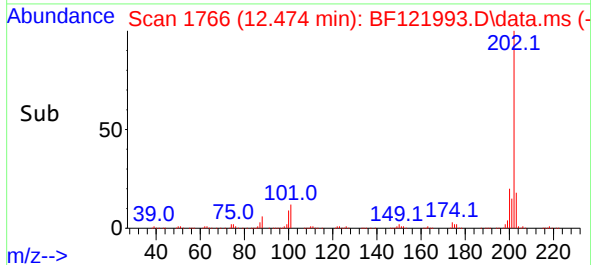


Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED



mohammad
10/16/2020 12:47:52 PM



#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.904 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

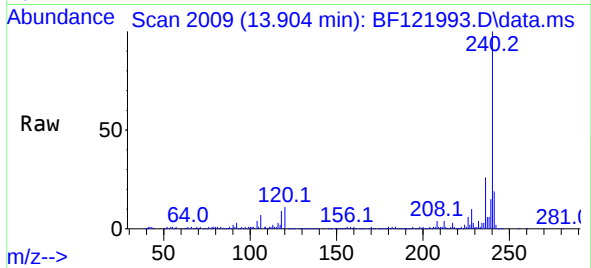


Tgt Ion:240 Resp: 221275
Ion Ratio Lower Upper
240 100
120 10.8 9.2 13.8
236 25.8 20.9 31.3

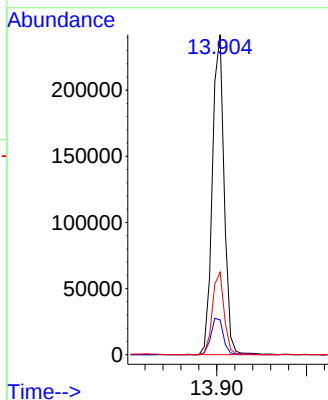


Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED



mohammad
10/16/2020 12:47:52 PM




#78
Pyrene
Concen: 13.75 ng
RT: 12.704 min Scan# 1805
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

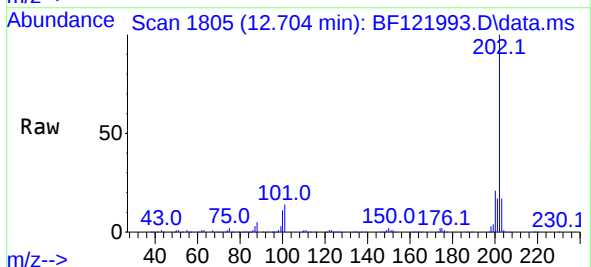


Tgt Ion:202 Resp: 231898
Ion Ratio Lower Upper
202 100
200 20.6 17.4 26.2
203 17.2 14.6 21.8

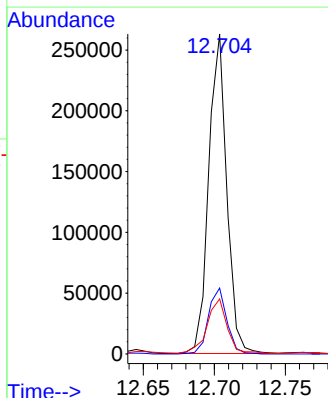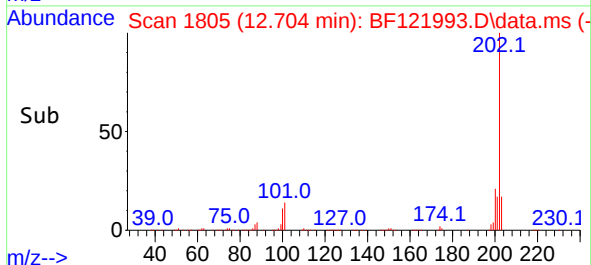



#79
Terphenyl-d14
Concen: 60.75 ng
RT: 12.845 min Scan# 1829
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15




Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

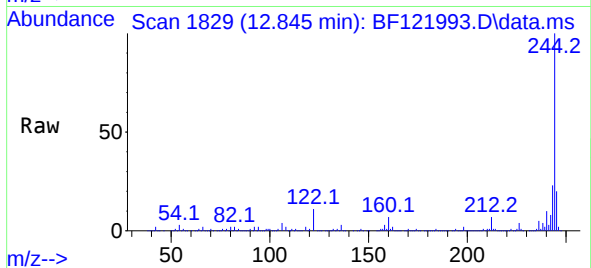


Tgt Ion:244 Resp: 705326
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 11.4 8.1 12.1

Manual Integrations
APPROVED



mohammad
10/16/2020 12:47:52 PM

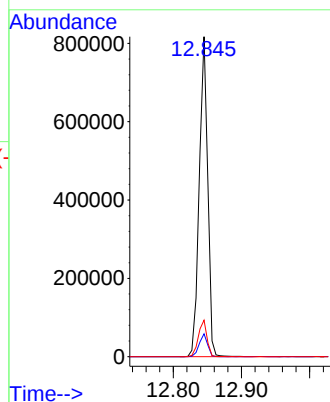


#81
Benzo(a)anthracene
Concen: 10.96 ng
RT: 13.892 min Scan# 2007
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15



Tgt Ion:228 Resp: 158900
Ion Ratio Lower Upper
228 100
226 30.2 22.3 33.5
229 20.0 16.2 24.4

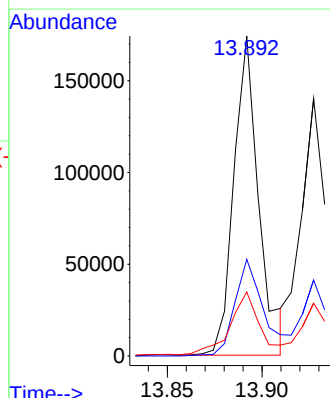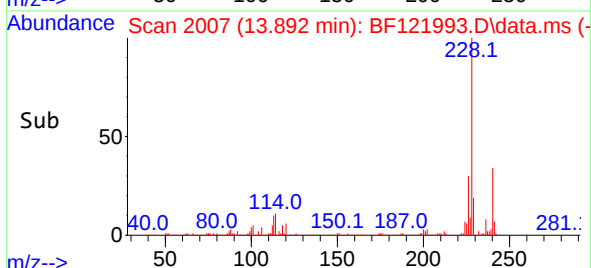







#83
Chrysene
Concen: 8.93 ng
RT: 13.927 min Scan# 2013
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt	Ion:228	Resp:	127174
Ion	Ratio	Lower	Upper
228	100		
226	29.5	24.6	37.0
229	20.5	15.9	23.9

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A




Manual Integrations
APPROVED


mohammad
10/16/2020 12:47:52 PM

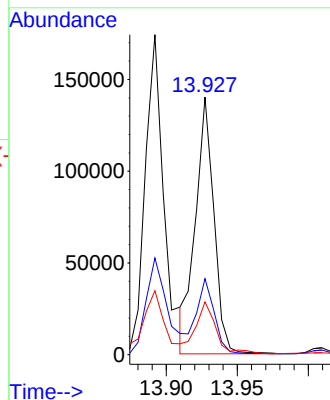

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.339 min Scan# 2253
Delta R.T. 0.000 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:264	Resp: 217695		
Ion Ratio	Lower	Upper	
264	100		
260	23.4	18.7	28.1
265	21.6	17.3	25.9

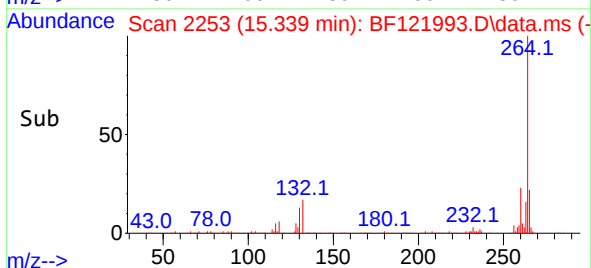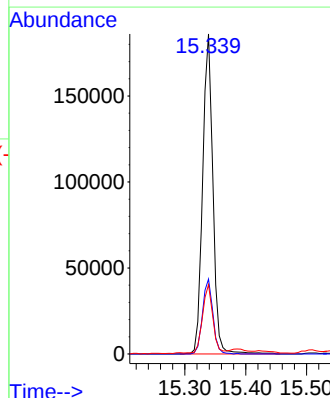







#87
Indeno(1,2,3-cd)pyrene
Concen: 5.75 ng
RT: 16.751 min Scan# 2493
Delta R.T. -0.012 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:	276	Resp:	81332
Ion Ratio	Lower	Upper	
276	100		
138	21.2	19.9	29.9
277	23.2	20.4	30.6

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A




Manual Integrations
APPROVED


mohammad
10/16/2020 12:47:52 PM

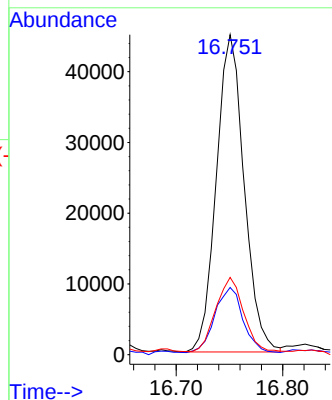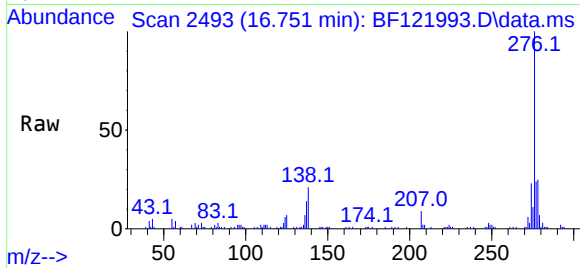

#88
Benzo(b)fluoranthene
Concen: 11.48 ng m
RT: 14.927 min Scan# 2183
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:	252	Resp:	168954
Ion Ratio	Lower	Upper	
252	100		
253	22.6	18.2	27.2
125	12.3	8.0	12.0#

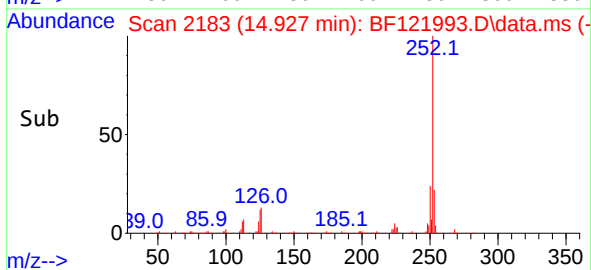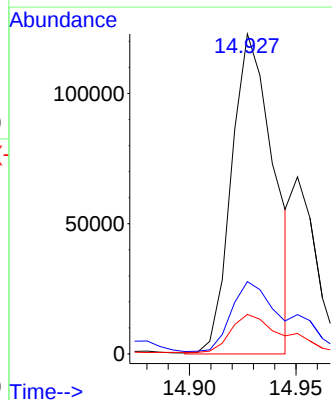







#89
Benzo(k)fluoranthene
Concen: 3.83 ng m
RT: 14.951 min Scan# 2187
Delta R.T. -0.012 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:252 Resp: 53590
Ion Ratio Lower Upper
252 100
253 22.2 17.8 26.6
125 11.6 7.7 11.5#

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A




Manual Integrations
APPROVED


mohammad
10/16/2020 12:47:52 PM

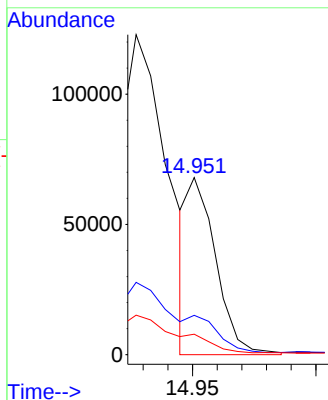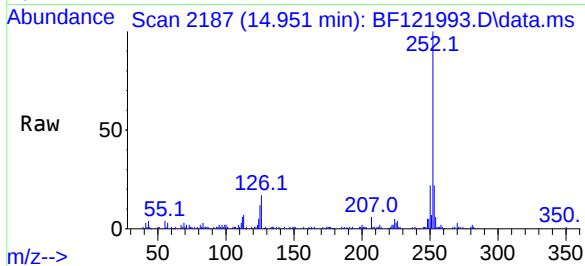

#90
Benzo(a)pyrene
Concen: 9.56 ng
RT: 15.280 min Scan# 2243
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion:252 Resp: 121453
Ion Ratio Lower Upper
252 100
253 21.3 17.3 25.9
125 10.8 8.6 13.0

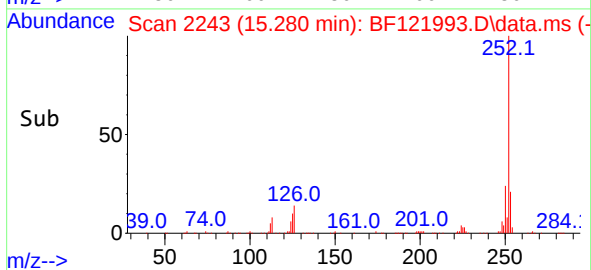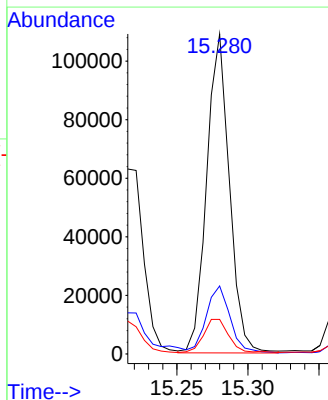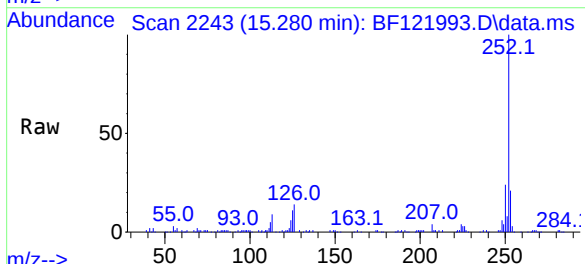







#91
Dibenzo(a,h)anthracene
Concen: 2.07 ng m
RT: 16.751 min Scan# 2493
Delta R.T. -0.018 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion: 278 Resp: 24134
Ion Ratio Lower Upper
278 100
139 0.0 13.0 19.4#
279 28.0 19.0 28.4

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-A

Manual Integrations
APPROVED

mohammad
10/16/2020 12:47:52 PM

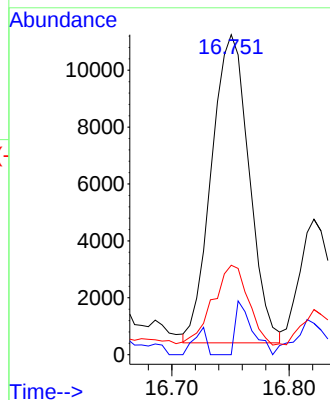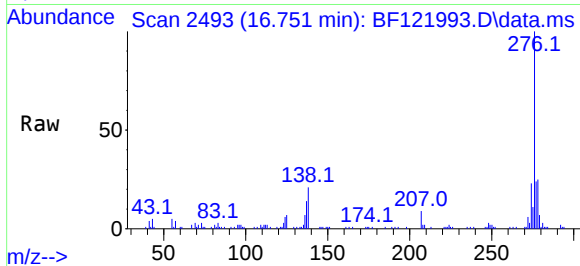

#92
Benzo(g,h,i)perylene
Concen: 5.68 ng
RT: 17.180 min Scan# 2566
Delta R.T. -0.006 min
Lab File: BF121993.D
Acq: 15 Oct 2020 16:15

Tgt Ion: 276 Resp: 66189
Ion Ratio Lower Upper
276 100
277 23.0 19.4 29.2
138 19.3 17.8 26.6

