

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
 Data File : BF121999.D
 Acq On : 15 Oct 2020 19:19
 Operator : JU/CG
 Sample : L4406-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-101420-B

Quant Time: Oct 16 01:08:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 12:55:05 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.740	152	103044	20.00	ng	0.00
21) Naphthalene-d8	8.028	136	394277	20.00	ng	0.00
39) Acenaphthene-d10	9.775	164	191553	20.00	ng	0.00
64) Phenanthrene-d10	11.263	188	320452	20.00	ng	0.00
76) Chrysene-d12	13.904	240	201185	20.00	ng	0.00
86) Perylene-d12	15.339	264	231196	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.363	112	575427	82.42	ng	0.00
7) Phenol-d6	6.387	99	727957	81.00	ng	0.00
23) Nitrobenzene-d5	7.310	82	491326	63.91	ng	0.00
42) 2,4,6-Tribromophenol	10.569	330	113148	47.75	ng	0.00
45) 2-Fluorobiphenyl	9.098	172	759464	58.34	ng	0.00
79) Terphenyl-d14	12.845	244	517872	49.06	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.498	163	87395	6.24	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121999.D
Acq On : 15 Oct 2020 19:19
Operator : JU/CG
Sample : L4406-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B


Quant Time: Oct 16 01:08:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

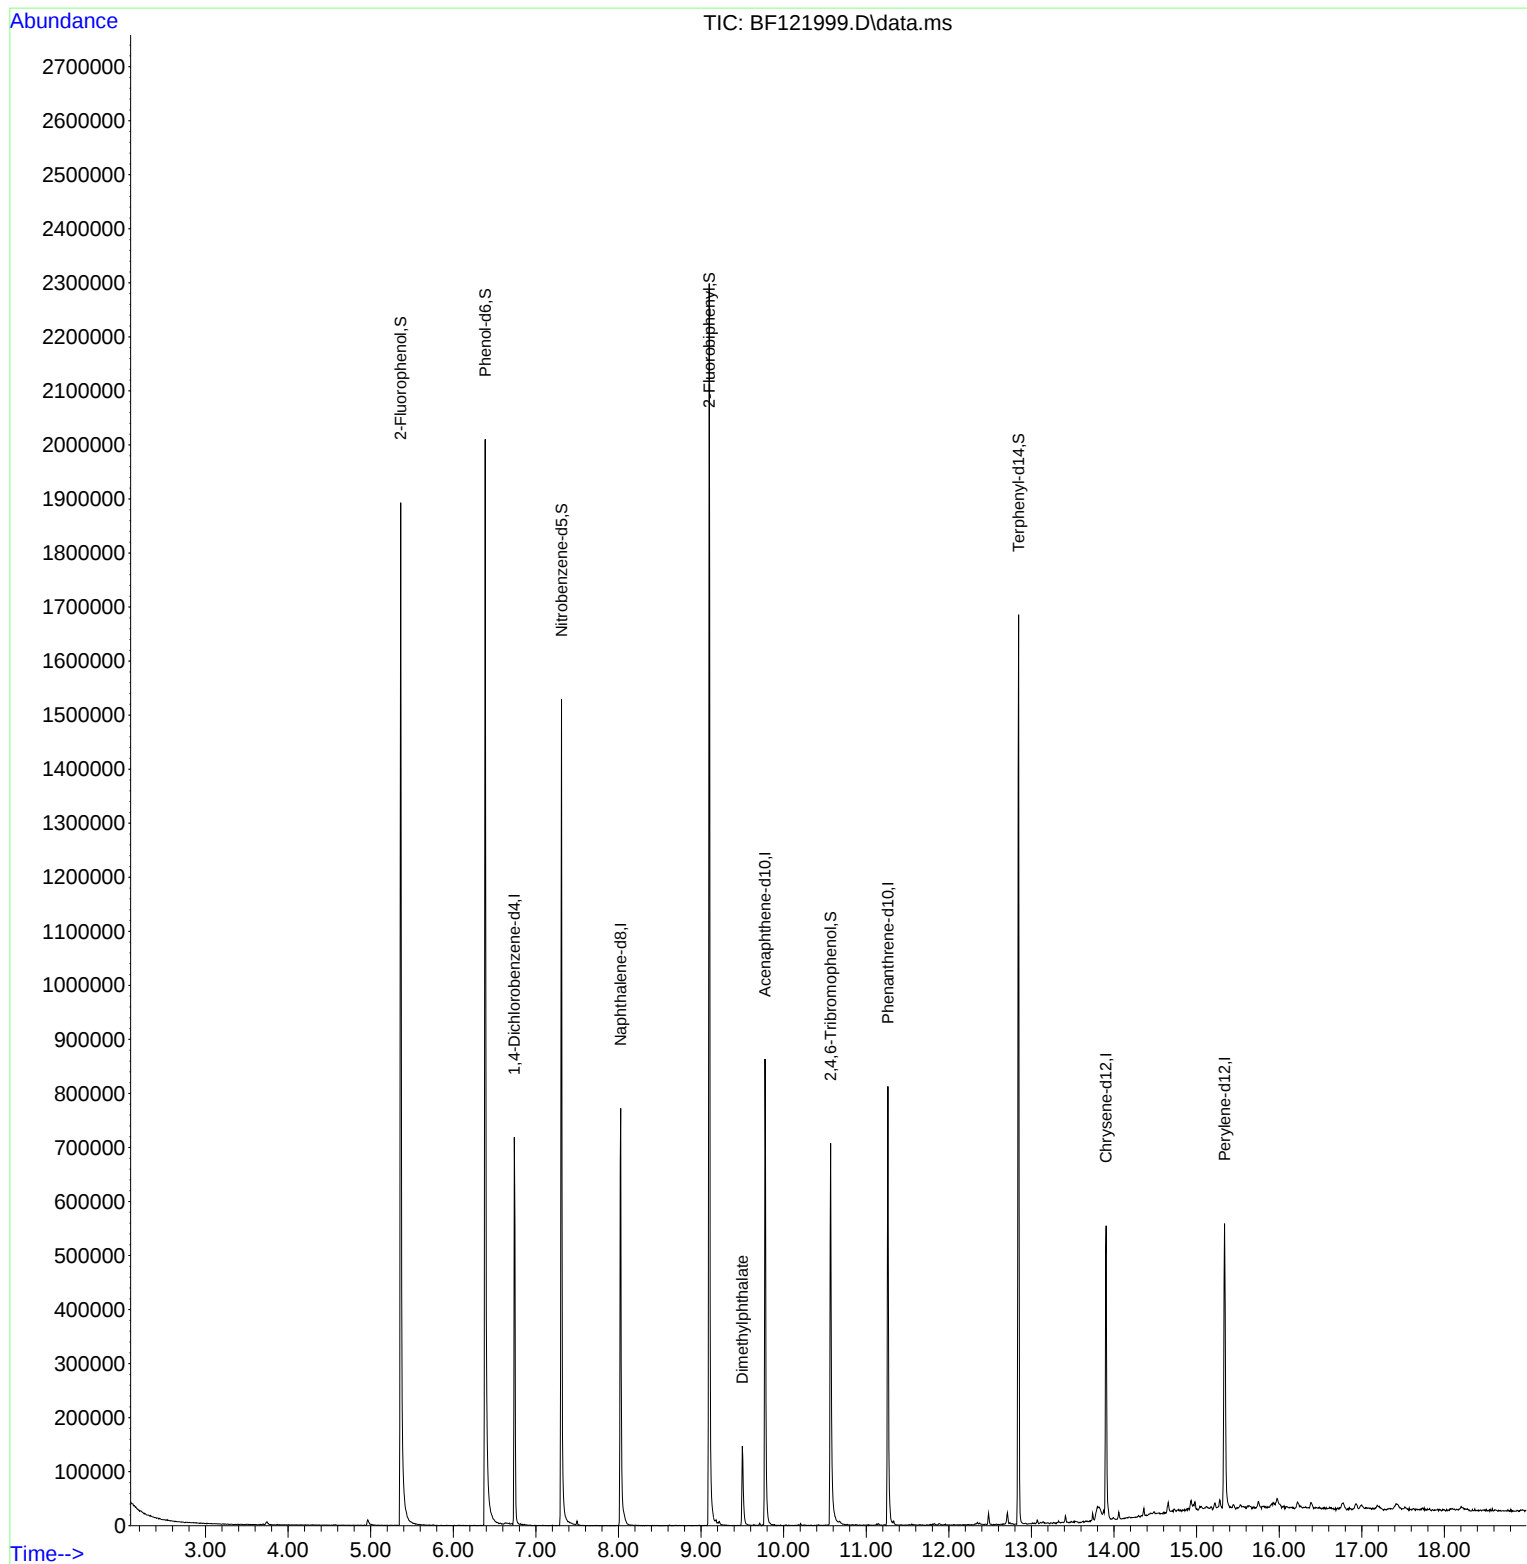


Abundance Scan 792 (6.745 min): BF121917.D\data.ms (-78

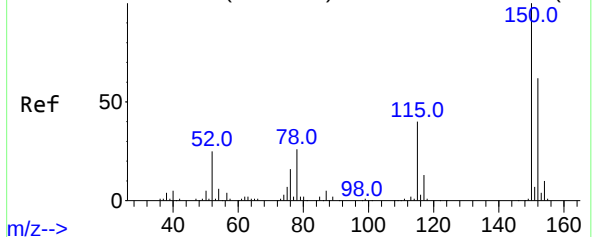

m/z--> Scan 791 (6.740 min): BF121999.D\data.ms

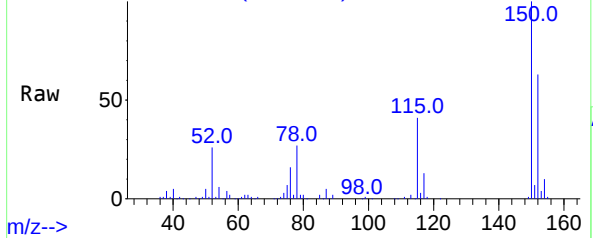

Abundance Scan 791 (6.740 min): BF121999.D\data.ms (-77

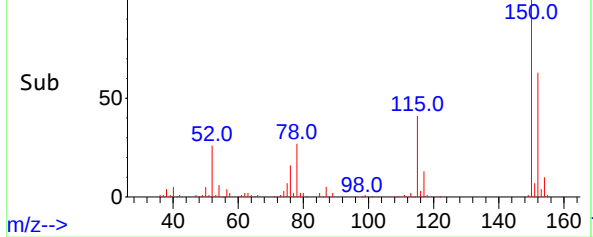


m/z-->


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.740 min Scan# 791
Delta R.T. -0.005 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19


Tgt Ion:	152	Resp:	103044
Ion	Ratio	Lower	Upper
152	100		
150	157.6	125.3	187.9
115	65.2	51.9	77.9

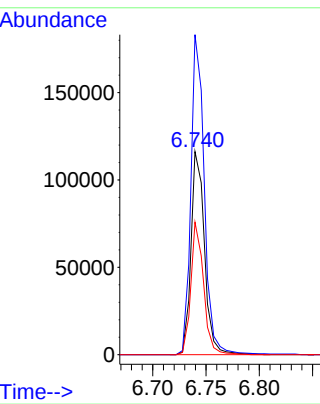


Abundance Scan 557 (5.363 min): BF121917.D\data.ms (-55

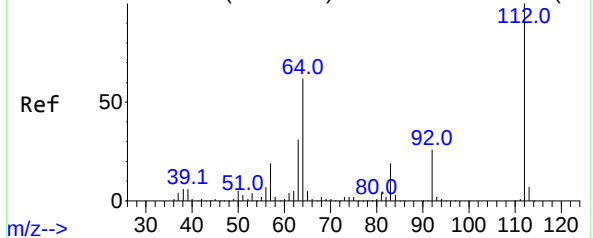

m/z--> Scan 557 (5.363 min): BF121999.D\data.ms

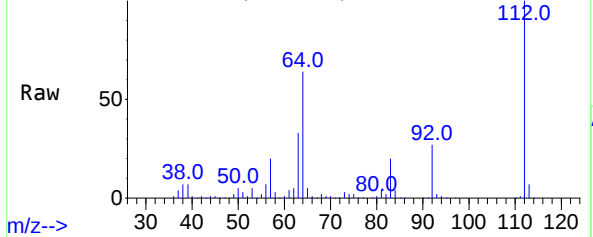

Abundance Scan 557 (5.363 min): BF121999.D\data.ms (-50

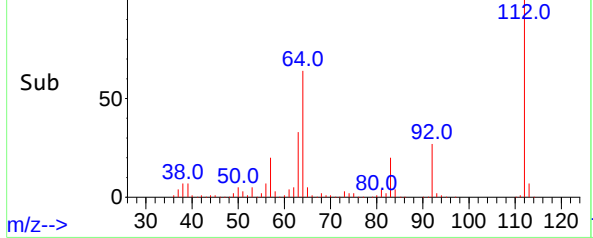


m/z-->

#5

2-Fluorophenol
Concen: 82.42 ng
RT: 5.363 min Scan# 557
Delta R.T. 0.000 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion:	112	Resp:	575427
Ion	Ratio	Lower	Upper
112	100		
64	64.3	50.4	75.6
63	33.0	25.8	38.6



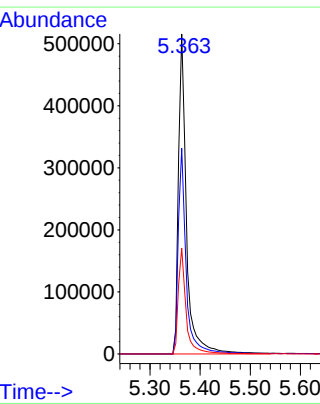




#7
Phenol-d6
Concen: 81.00 ng
RT: 6.387 min Scan# 731
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19




Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B


Tgt Ion: 99 Resp: 727957
Ion Ratio Lower Upper
99 100
42 20.2 15.9 23.9
71 34.4 27.1 40.7

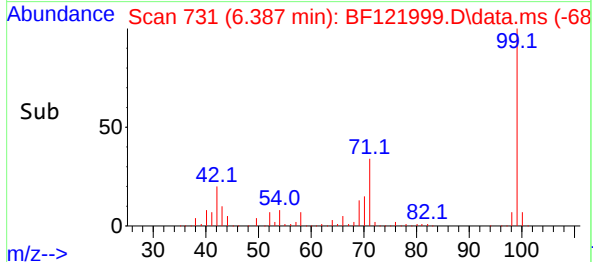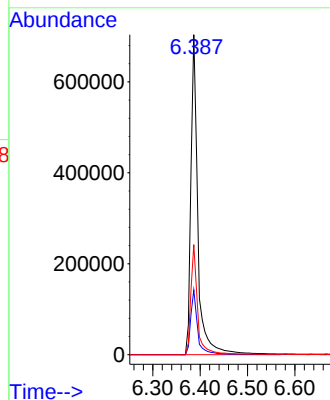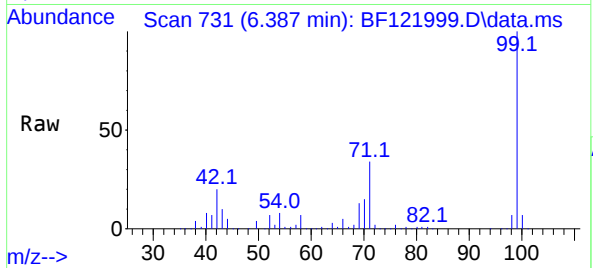

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion:136 Resp: 394277
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 8.5 7.1 10.7
68 6.3 5.0 7.4


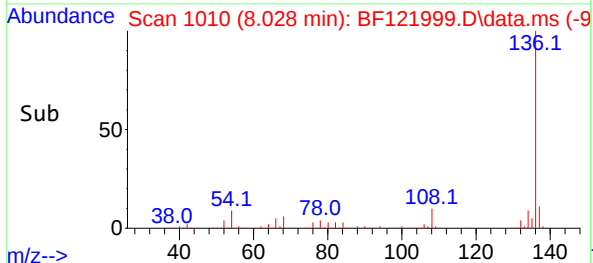
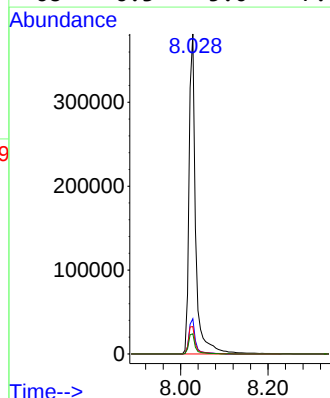
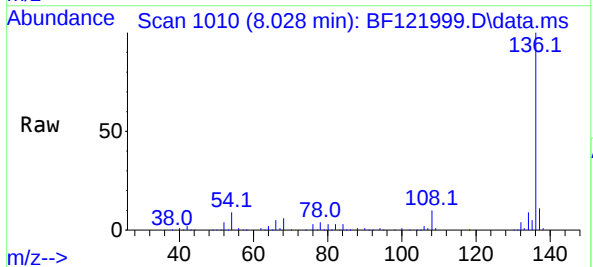


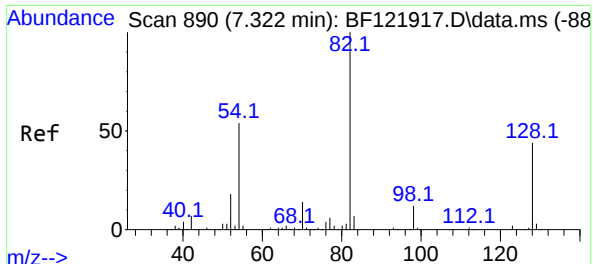

#23
Nitrobenzene-d5
Concen: 63.91 ng
RT: 7.310 min Scan# 888
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19




Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B

Tgt Ion: 82 Resp: 491326
Ion Ratio Lower Upper
82 100
128 42.3 35.0 52.4
54 53.1 43.9 65.9

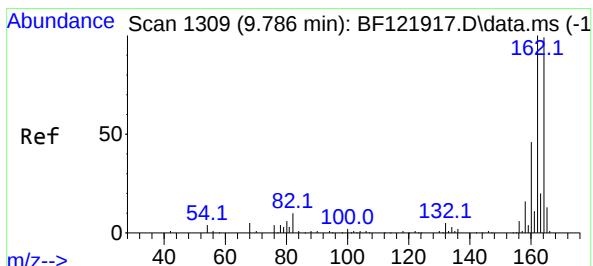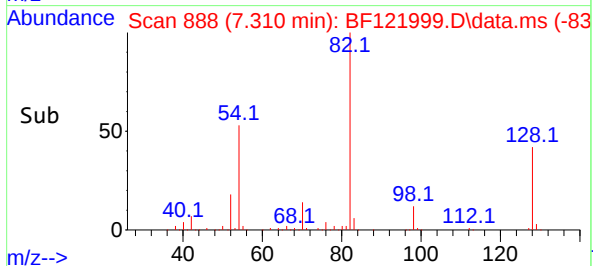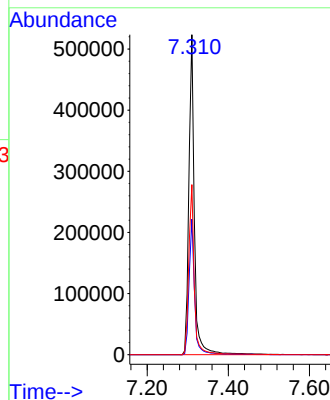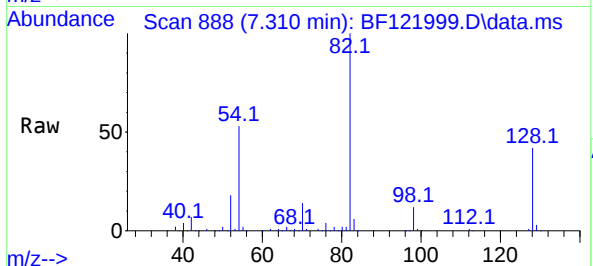

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.775 min Scan# 1307
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion: 164 Resp: 191553
Ion Ratio Lower Upper
164 100
162 103.1 83.2 124.8
160 46.5 37.5 56.3

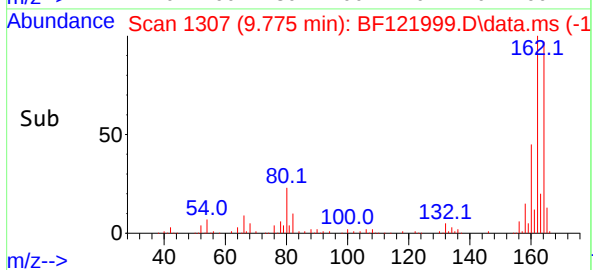
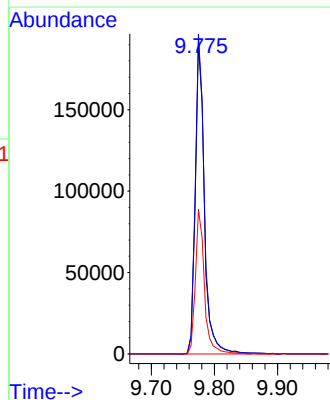
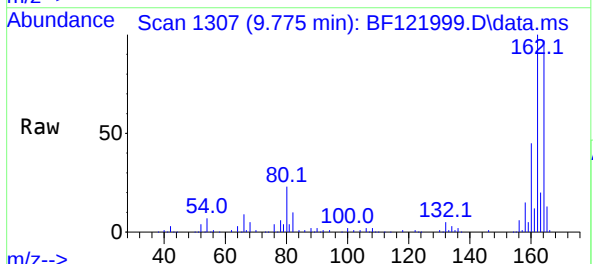




#42
2,4,6-Tribromophenol
Concen: 47.75 ng
RT: 10.569 min Scan# 1442
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19




Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B

Tgt Ion:330 Resp: 113148
Ion Ratio Lower Upper
330 100
332 96.8 77.3 115.9
141 31.7 22.3 33.5

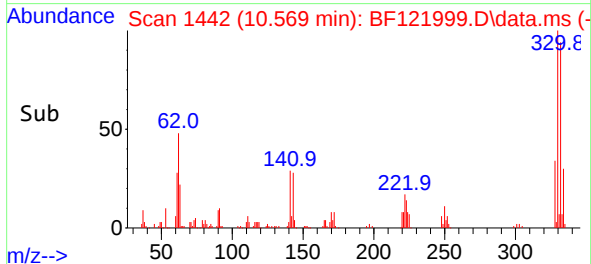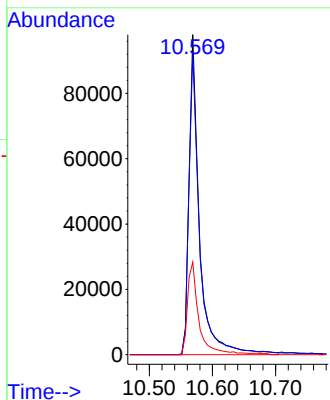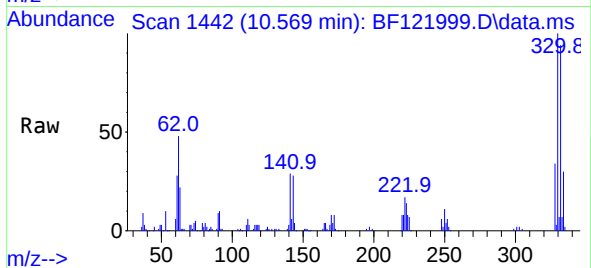

#45
2-Fluorobiphenyl
Concen: 58.34 ng
RT: 9.098 min Scan# 1192
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion:172 Resp: 759464
Ion Ratio Lower Upper
172 100
171 35.6 29.1 43.7
170 23.6 19.8 29.6

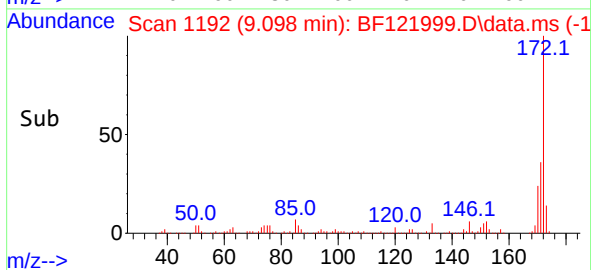
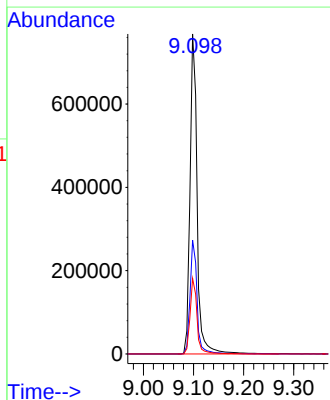
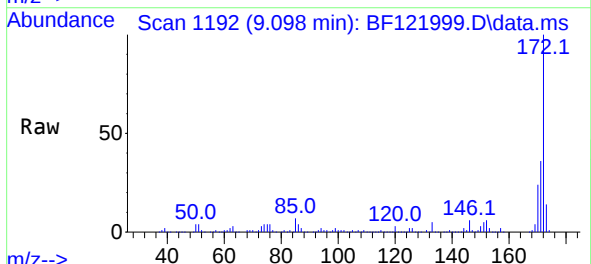




#50
Dimethylphthalate
Concen: 6.24 ng
RT: 9.498 min Scan# 1260
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19




Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B


Tgt Ion:163 Resp: 87395
Ion Ratio Lower Upper
163 100
194 4.4 3.3 4.9
164 11.1 8.2 12.4

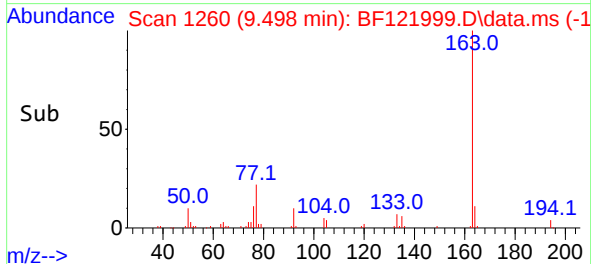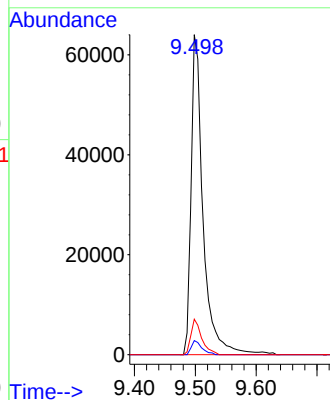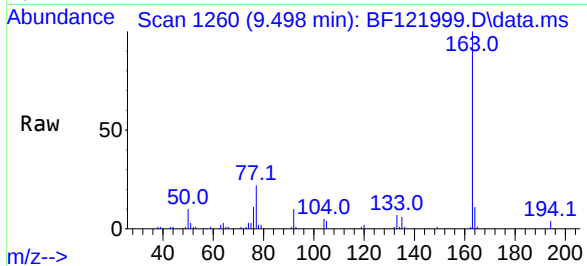

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.263 min Scan# 1560
Delta R.T. 0.000 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion:188 Resp: 320452
Ion Ratio Lower Upper
188 100
94 10.1 8.3 12.5
80 10.9 9.1 13.7


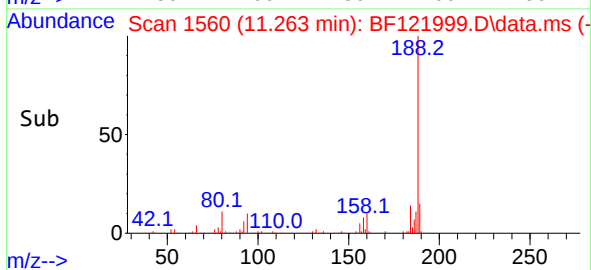
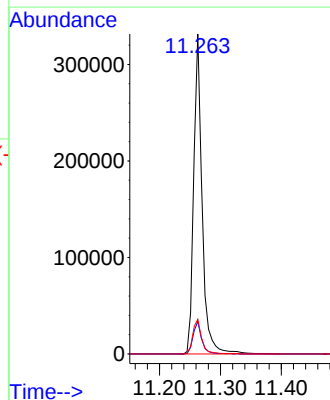
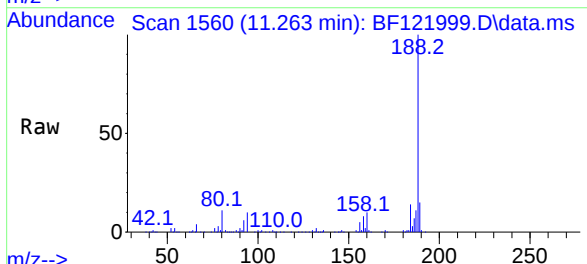


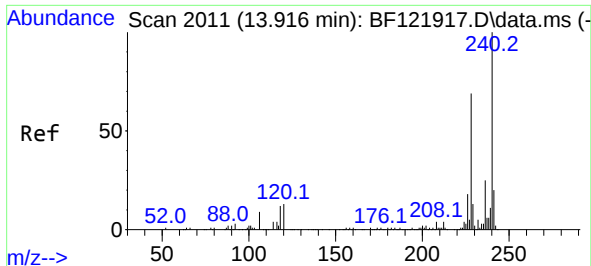

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.904 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19




Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B


Tgt Ion:240 Resp: 201185
Ion Ratio Lower Upper
240 100
120 10.9 9.2 13.8
236 26.1 20.9 31.3

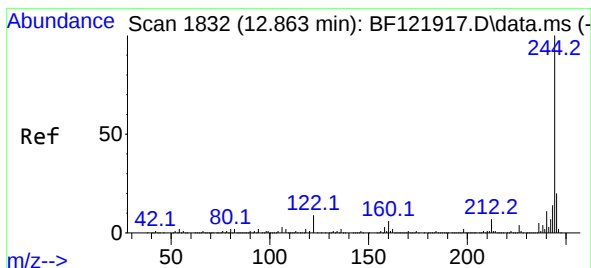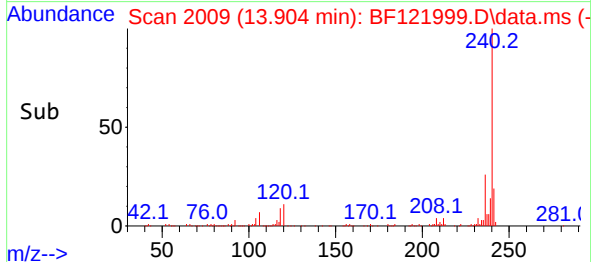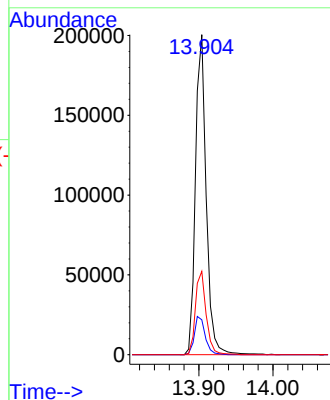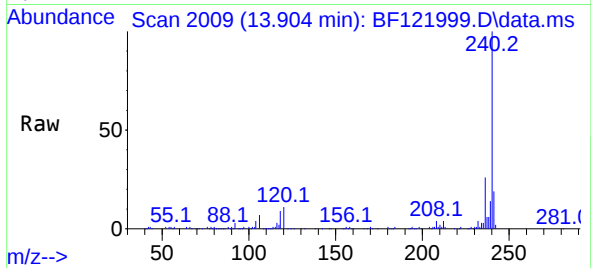

#79
Terphenyl-d14
Concen: 49.06 ng
RT: 12.845 min Scan# 1829
Delta R.T. -0.006 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Tgt Ion:244 Resp: 517872
Ion Ratio Lower Upper
244 100
212 7.0 5.4 8.2
122 10.5 8.1 12.1

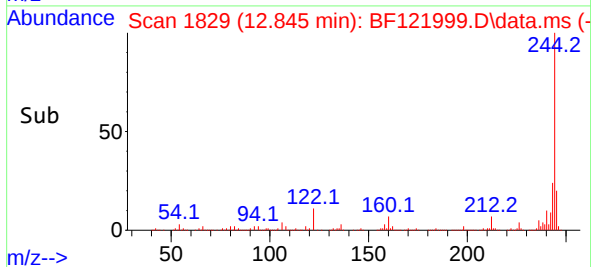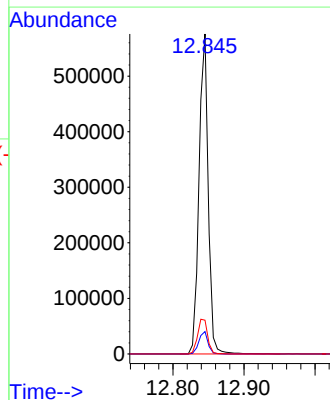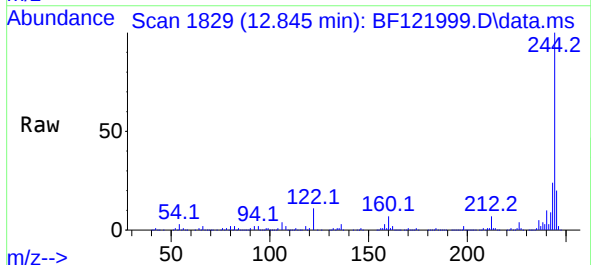

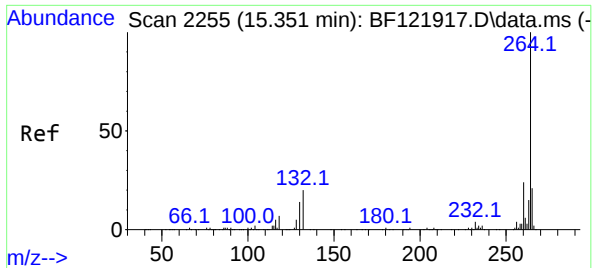

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.339 min Scan# 2253
Delta R.T. 0.000 min
Lab File: BF121999.D
Acq: 15 Oct 2020 19:19

Instrument :
BNA_F
ClientSampleId :
JC-02-101420-B

Tgt Ion:264 Resp: 231196

Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.7	28.1
265	21.3	17.3	25.9

