

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
 Data File : BF121994.D
 Acq On : 15 Oct 2020 16:45
 Operator : JU/CG
 Sample : L4407-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-GF-02-062-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF121994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	485	489	500	rBV	18706	33448	1.33%	0.196%
2	5.363	554	557	581	rBV	1975276	2185790	87.08%	12.825%
3	6.386	727	731	756	rBV	2175408	2267183	90.33%	13.303%
4	6.739	788	791	798	rVB	696639	587821	23.42%	3.449%
5	7.310	884	888	902	rBV	1619562	1529599	60.94%	8.975%
6	8.028	1006	1010	1027	rBV	744569	765182	30.49%	4.490%
7	9.098	1188	1192	1204	rBV	2690693	2510009	100.00%	14.728%
8	9.498	1256	1260	1272	rVB	288897	307442	12.25%	1.804%
9	9.774	1303	1307	1323	rVB	944578	874826	34.85%	5.133%
10	10.569	1438	1442	1454	rBV	1149237	1174786	46.80%	6.893%
11	11.263	1556	1560	1567	rBV	929824	866305	34.51%	5.083%
12	12.474	1764	1766	1770	rVB	69780	59892	2.39%	0.351%
13	12.704	1803	1805	1810	rVB	59245	54937	2.19%	0.322%
14	12.845	1825	1829	1832	rBV	2288599	2021961	80.56%	11.864%
15	13.033	1854	1861	1864	rBV5	12818	26535	1.06%	0.156%
16	13.809	1986	1993	2002	rBV5	63098	209585	8.35%	1.230%
17	13.904	2005	2009	2018	rVB	647556	669907	26.69%	3.931%
18	14.362	2084	2087	2090	rVB2	25536	25738	1.03%	0.151%
19	14.927	2180	2183	2186	rBV	28296	39800	1.59%	0.234%
20	14.980	2189	2192	2197	rVB	55185	66327	2.64%	0.389%
21	15.280	2240	2243	2248	rVB	31243	41444	1.65%	0.243%
22	15.339	2248	2253	2262	rBV	521224	670195	26.70%	3.932%
23	15.751	2319	2323	2329	rVB	35858	53840	2.15%	0.316%




Sum of corrected areas: 17042552

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121994.D
Acq On : 15 Oct 2020 16:45
Operator : JU/CG
Sample : L4407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

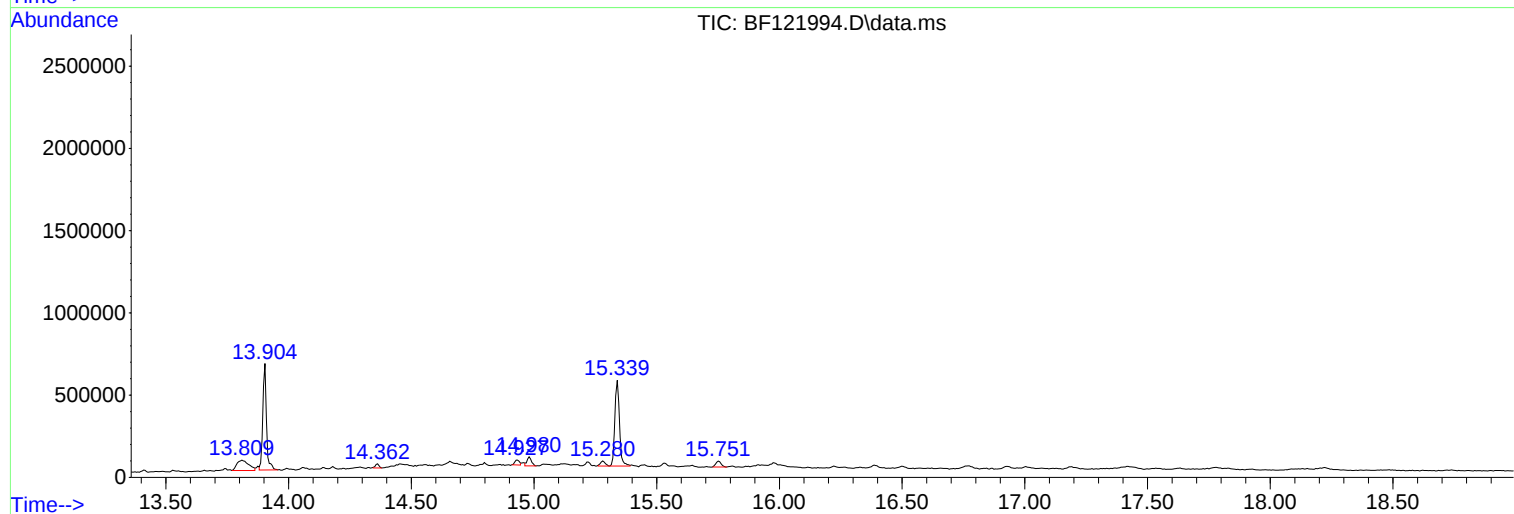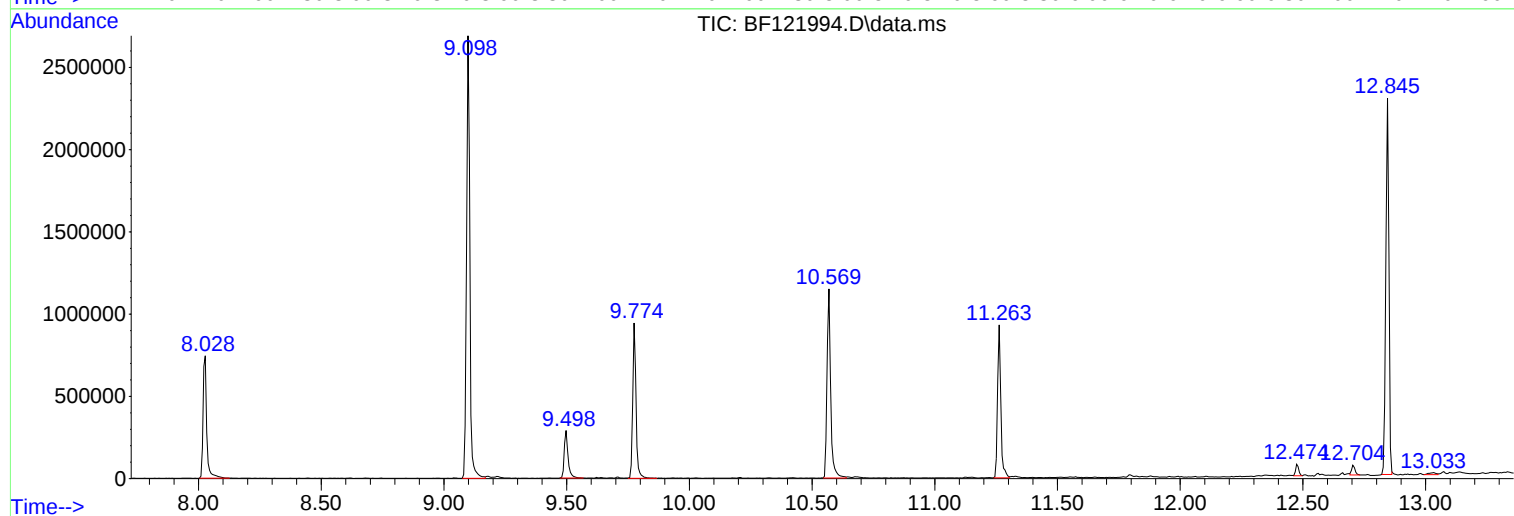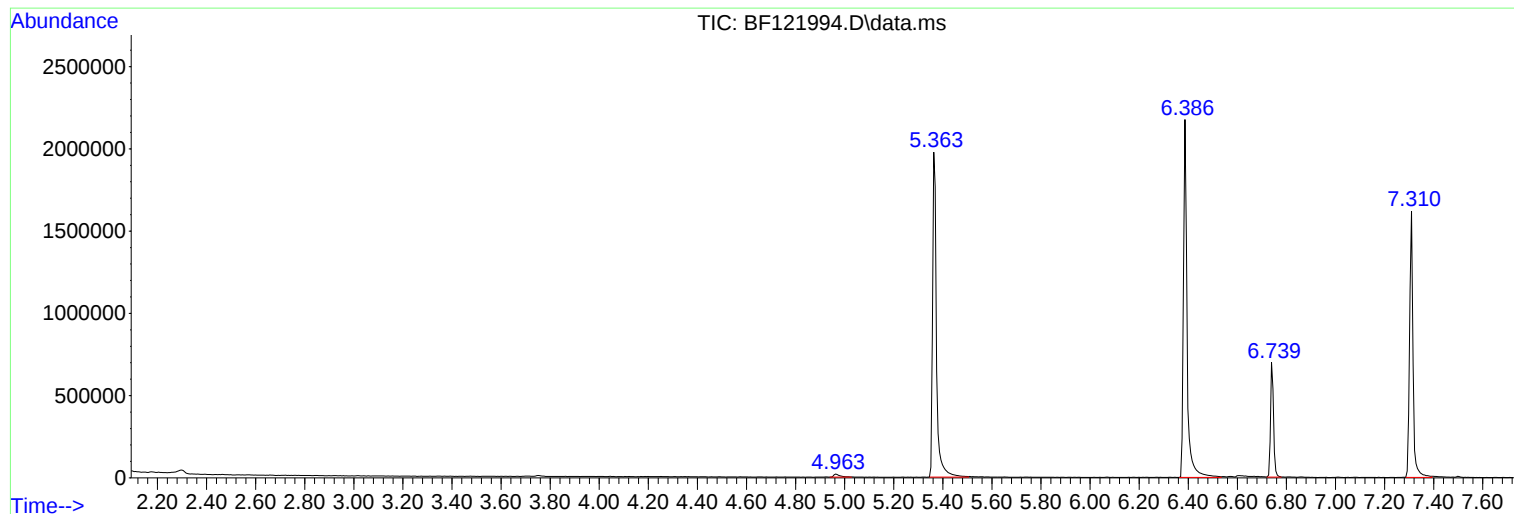

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121994.D
Acq On : 15 Oct 2020 16:45
Operator : JU/CG
Sample : L4407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.810	6.26 ng	209585	Chrysene-d12	13.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	94
2			Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	94
3			Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	93
4			n-Nonadecanol-1	284	C19H40O	001454-84-8	91
5			11-Tricosene	322	C23H46	052078-56-5	91

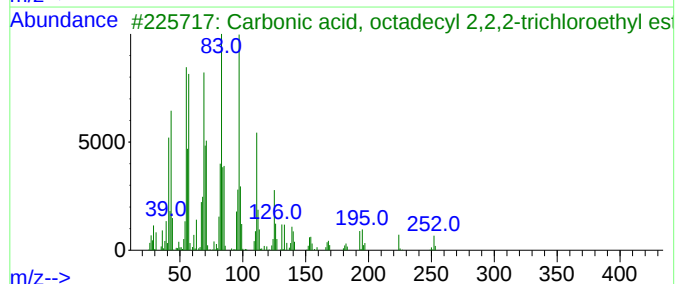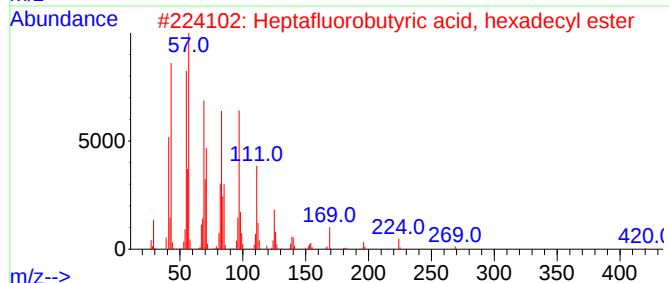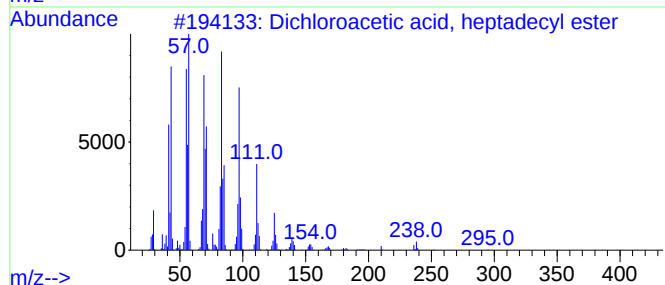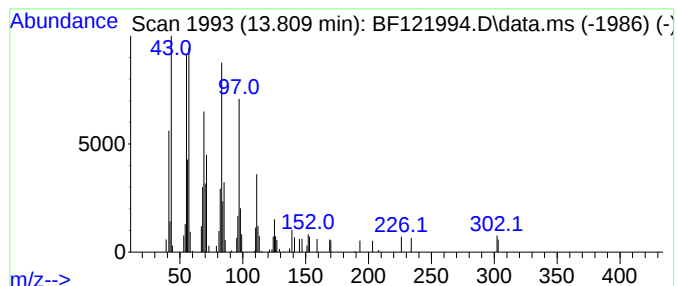

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101520\
Data File : BF121994.D
Acq On : 15 Oct 2020 16:45
Operator : JU/CG
Sample : L4407-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-GF-02-062-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	13.810	6.3	ng	209585	5	13.904	669907	20.0