


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101521\
Data File : BF125857.D
Acq On : 15 Oct 2021 10:55
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 14:56:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 14:50:00 2021
Response via : Initial Calibration

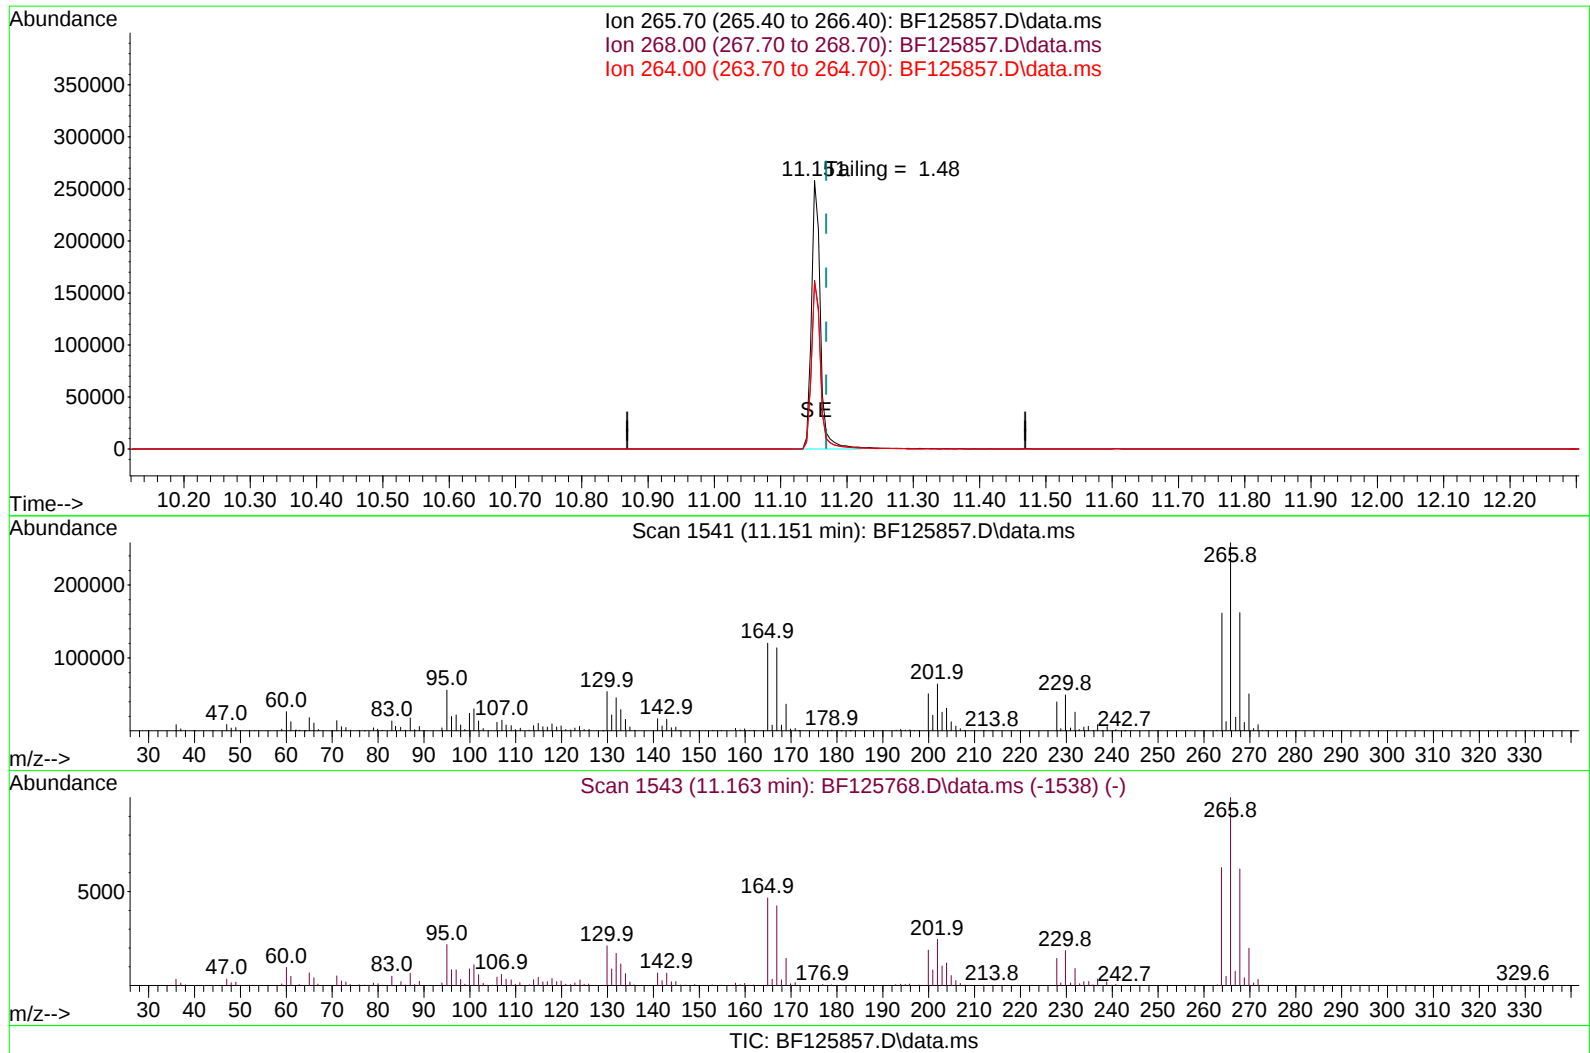

(70) Pentachlorophenol (C)




11.151min (-0.018) 36384.00 ng

response 244346

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.86
264.00	69.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101521\
 Data File : BF125857.D
 Acq On : 15 Oct 2021 10:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 14:56:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 14:50:00 2021
 Response via : Initial Calibration

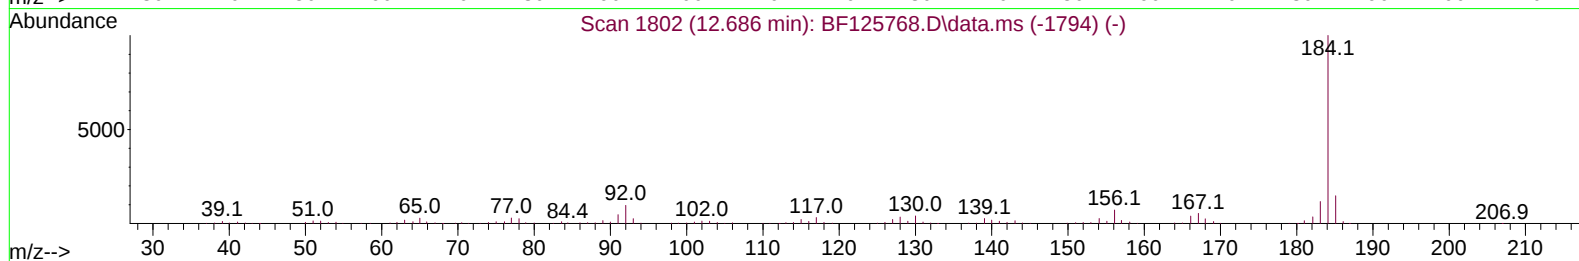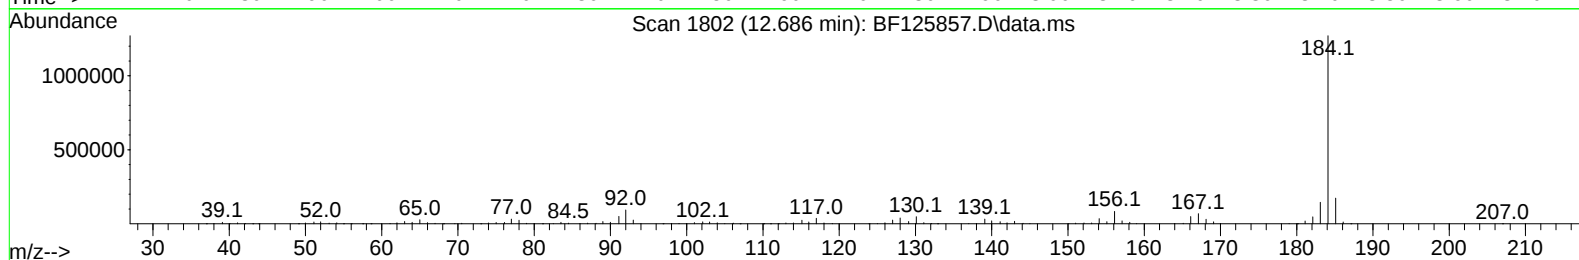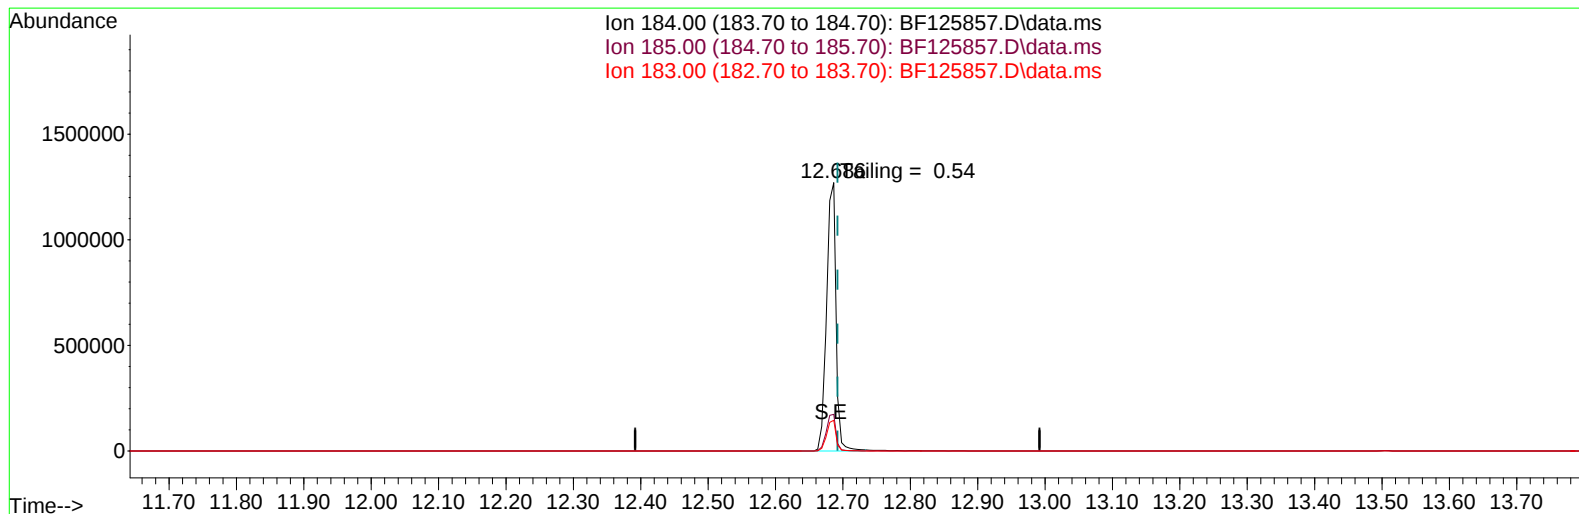

TIC: BF125857.D\data.ms

(77) Benzidine

12.686min (-0.006) 0.00 ng

response 1244010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.65
183.00	10.10	11.44
0.00	0.00	0.00