


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101521\
 Data File : BF125857.D
 Acq On : 15 Oct 2021 10:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 18 12:43:03 2021

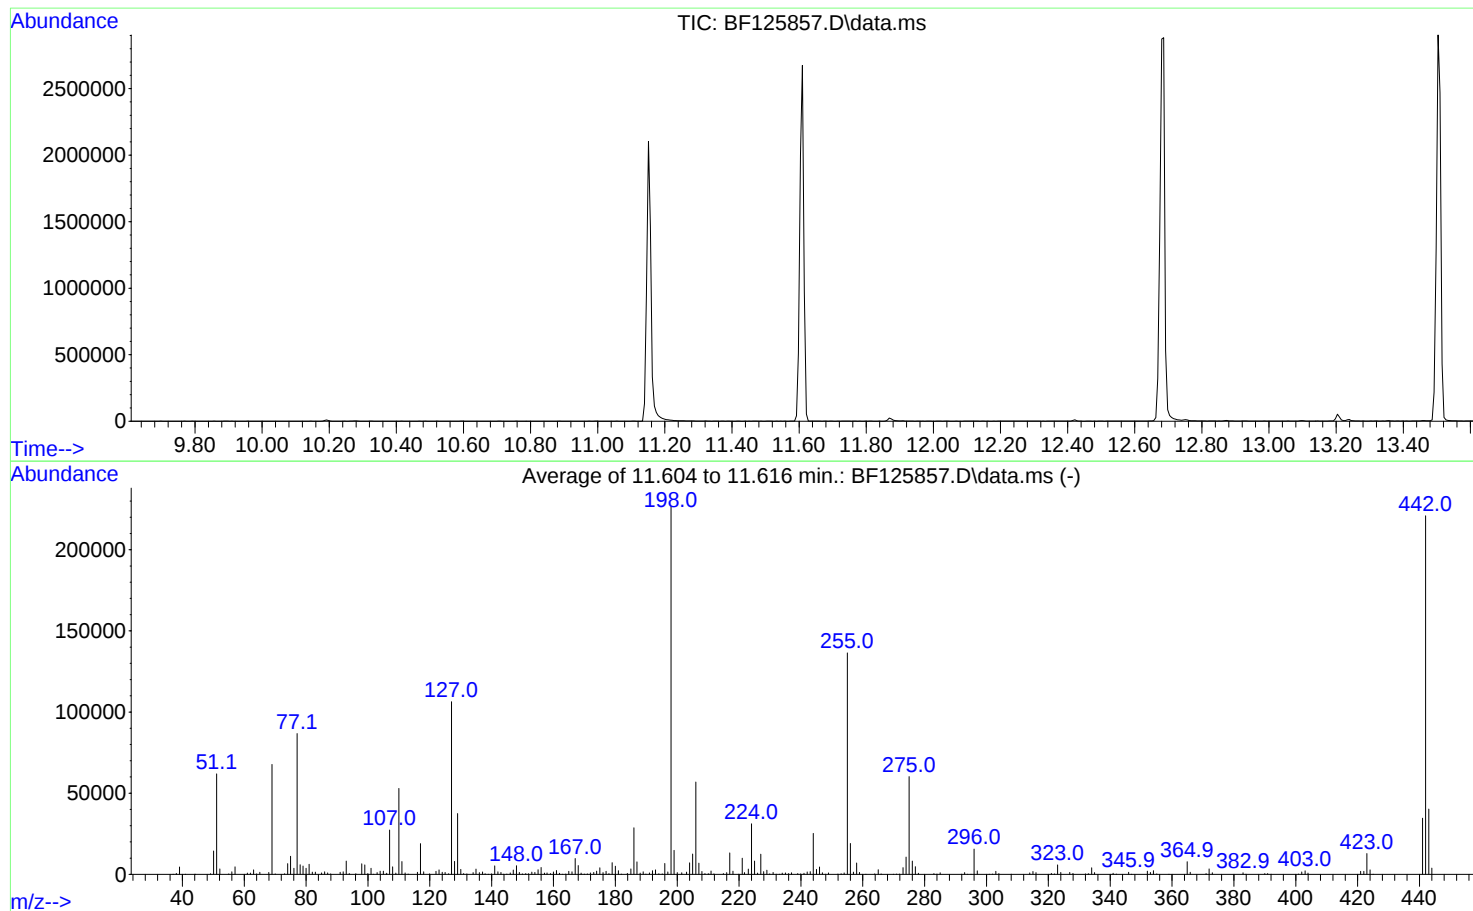


AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.3	61901	PASS
68	69	0.00	2	1.7	1144	PASS
69	198	0.00	100	29.9	67707	PASS
70	69	0.00	2	0.4	286	PASS
127	198	10	80	46.9	106355	PASS
197	198	0.00	2	0.7	1504	PASS
198	198	100	100	100.0	226632	PASS
199	198	5	9	6.5	14820	PASS
275	198	10	60	26.6	60240	PASS
365	198	1	100	3.4	7807	PASS
441	198	0.01	100	15.3	34592	PASS
442	442	50	100	100.0	220907	PASS
443	442	15	24	18.2	40221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101521\
 Data File : BF125857.D
 Acq On : 15 Oct 2021 10:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 15 14:56:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 14:50:00 2021
 Response via : Initial Calibration

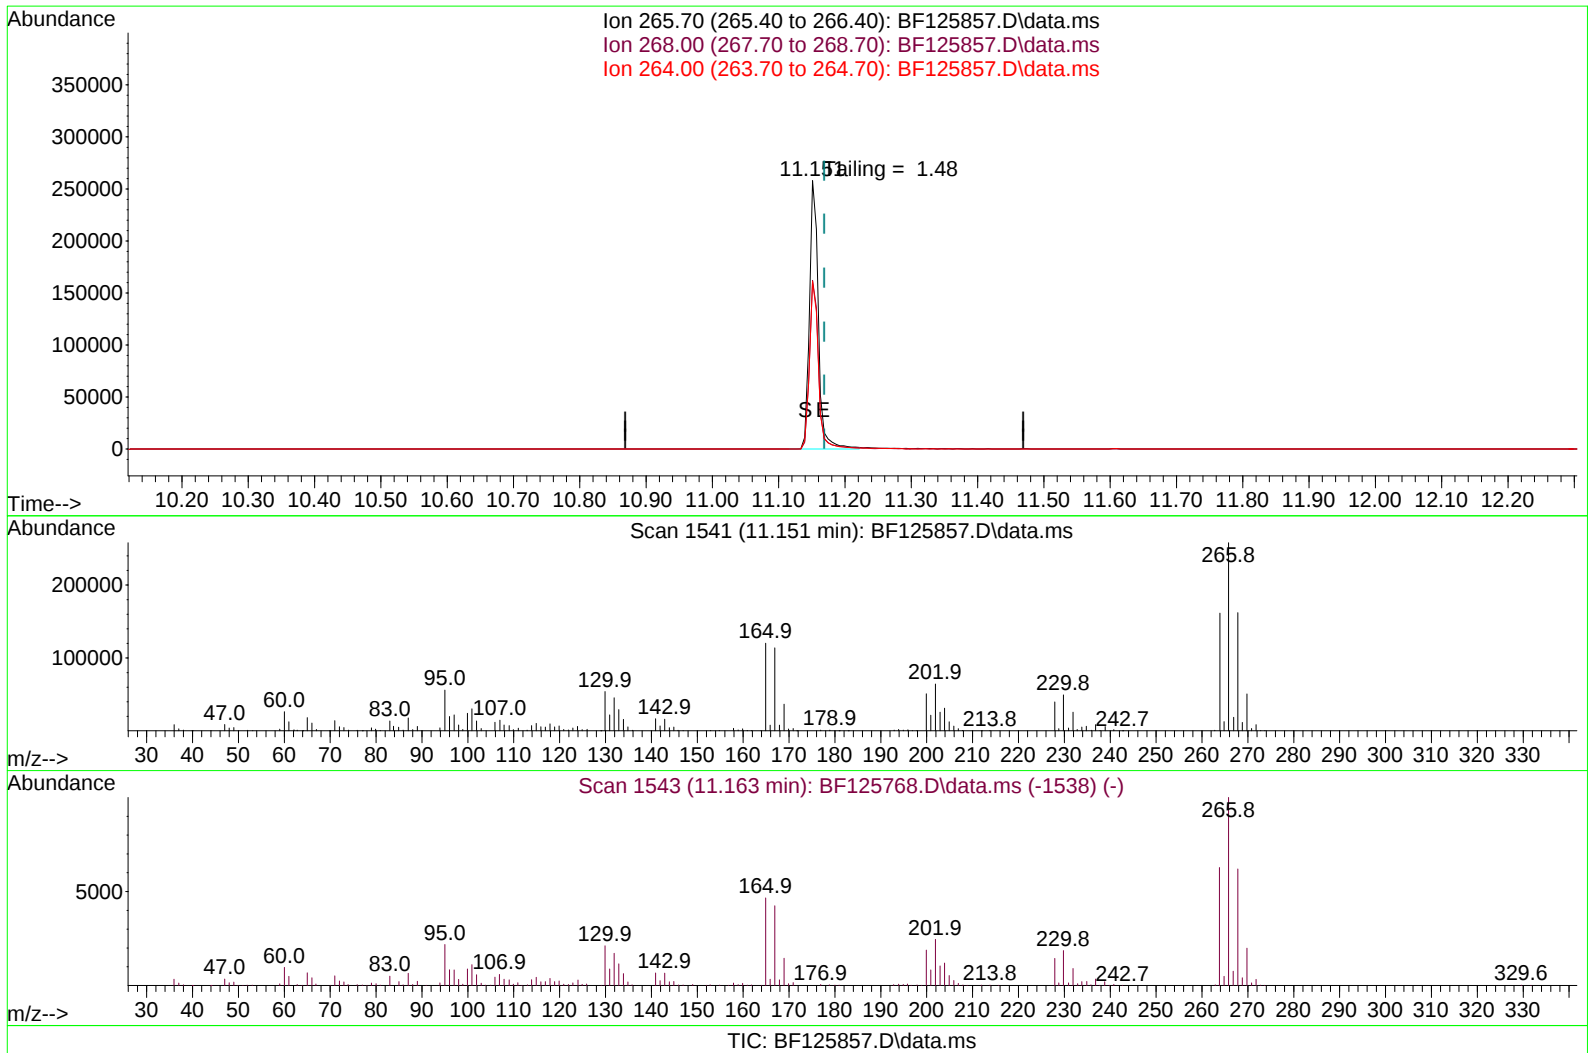

(70) Pentachlorophenol (C)

11.151min (-0.018) 36384.00 ng




response 244346

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.86
264.00	69.90	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101521\
 Data File : BF125857.D
 Acq On : 15 Oct 2021 10:55
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 15 14:56:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 15 14:50:00 2021
 Response via : Initial Calibration

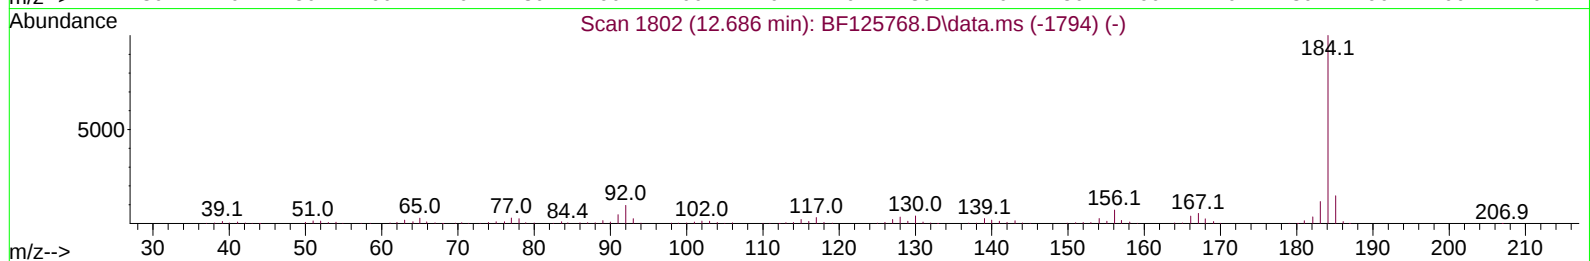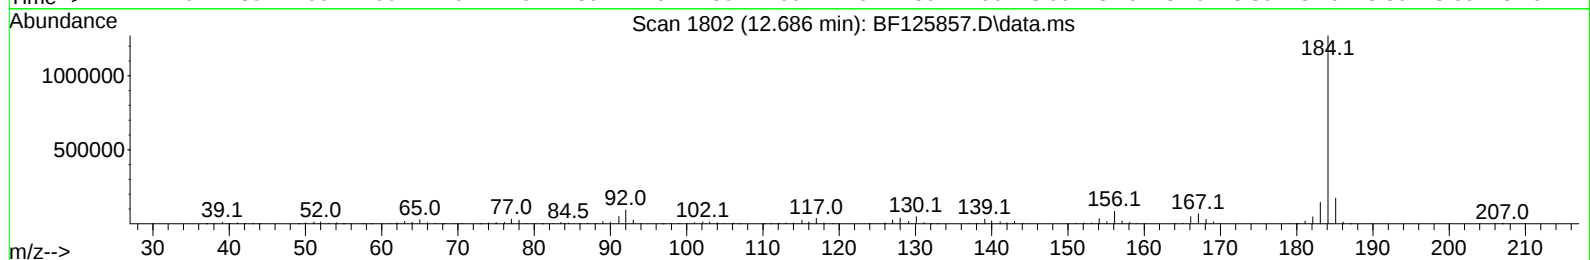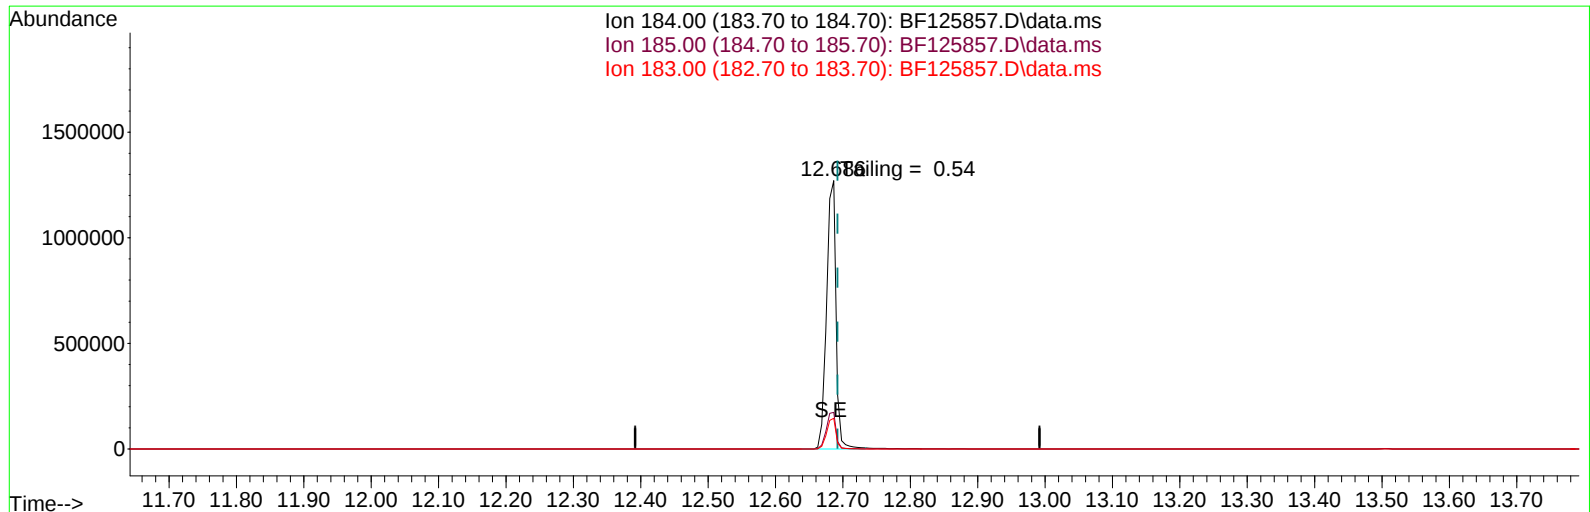

TIC: BF125857.D\data.ms

(77) Benzidine

12.686min (-0.006) 0.00 ng

response 1244010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.65
183.00	10.10	11.44
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/15/2021	BNA_F	<u>BF125857.D</u>
Compound Name	Response	Retention Time
DDT	533012	13.5
DDD	10273	13.2
DDE	982	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11255	544267	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP