


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101524\
Data File : BF139804.D
Acq On : 15 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 15 16:41:54 2024

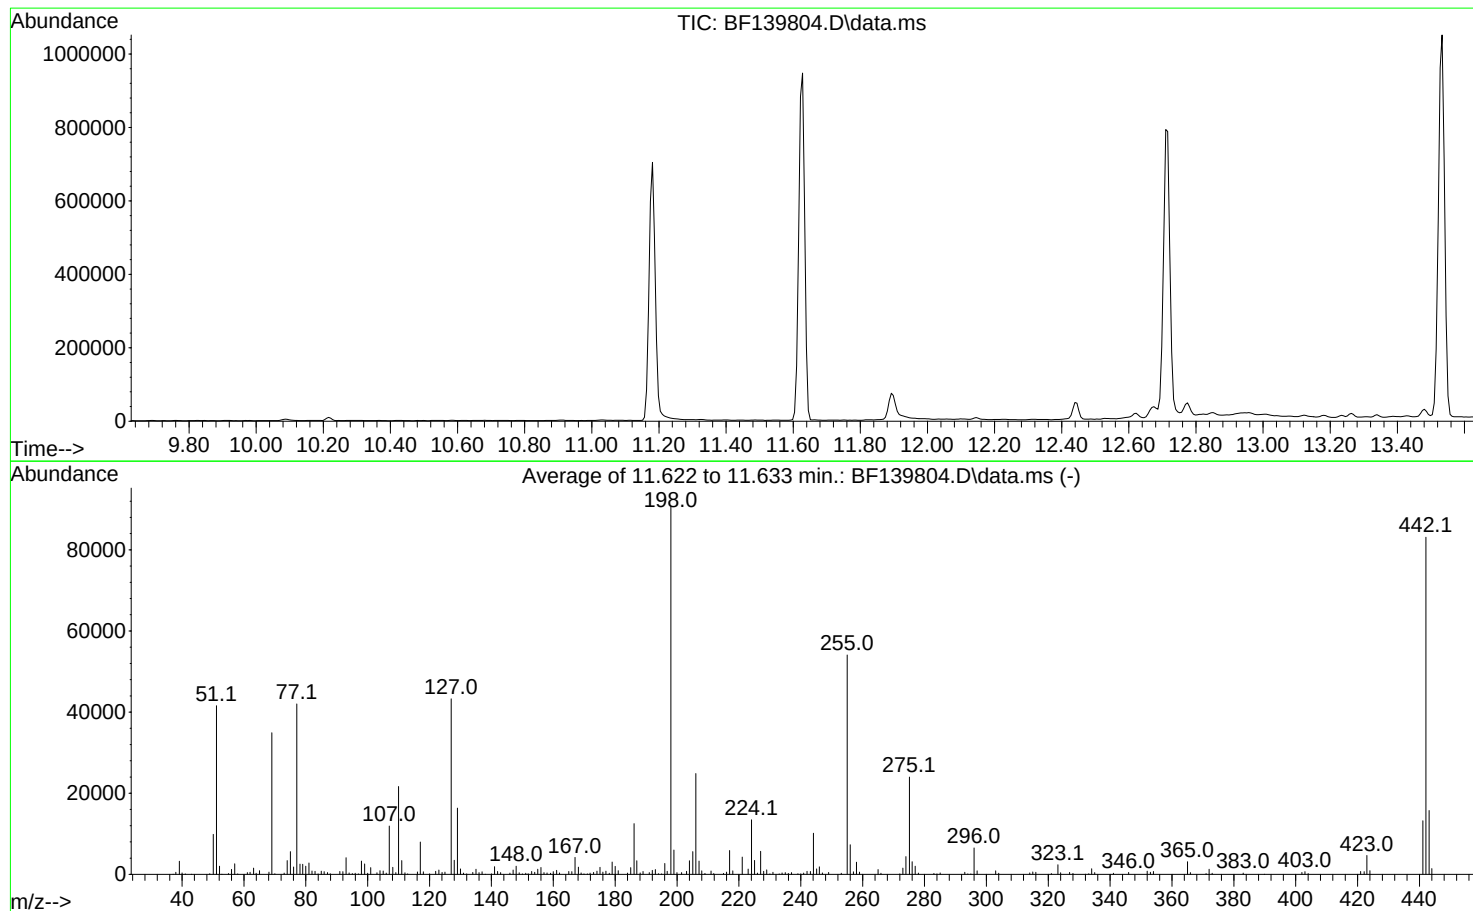




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	41568	PASS
68	69	0.00	2	1.6	545	PASS
69	198	0.00	100	38.5	34915	PASS
70	69	0.00	2	0.5	166	PASS
127	198	10	80	47.7	43288	PASS
197	198	0.00	2	0.8	738	PASS
198	198	100	100	100.0	90683	PASS
199	198	5	9	6.6	5986	PASS
275	198	10	60	26.4	23973	PASS
365	198	1	100	3.4	3115	PASS
441	198	0.01	100	14.6	13235	PASS
442	442	50	100	100.0	83120	PASS
443	442	15	24	18.9	15746	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101524\
Data File : BF139804.D
Acq On : 15 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 15 11:29:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

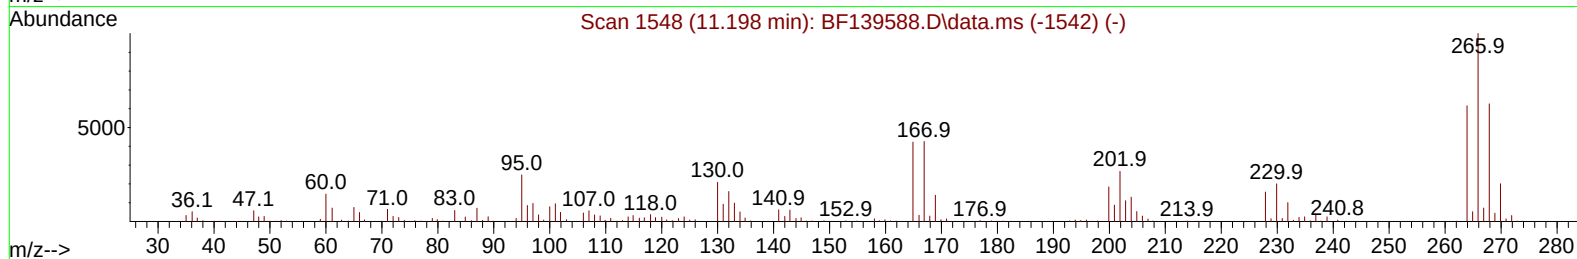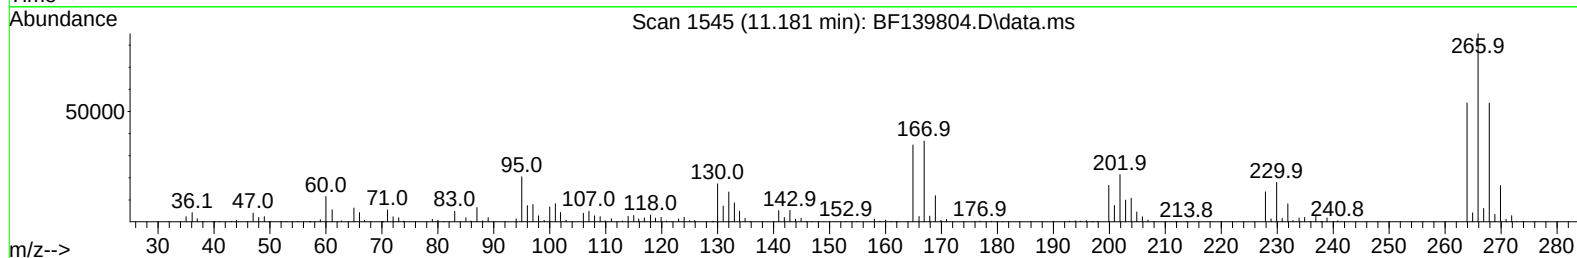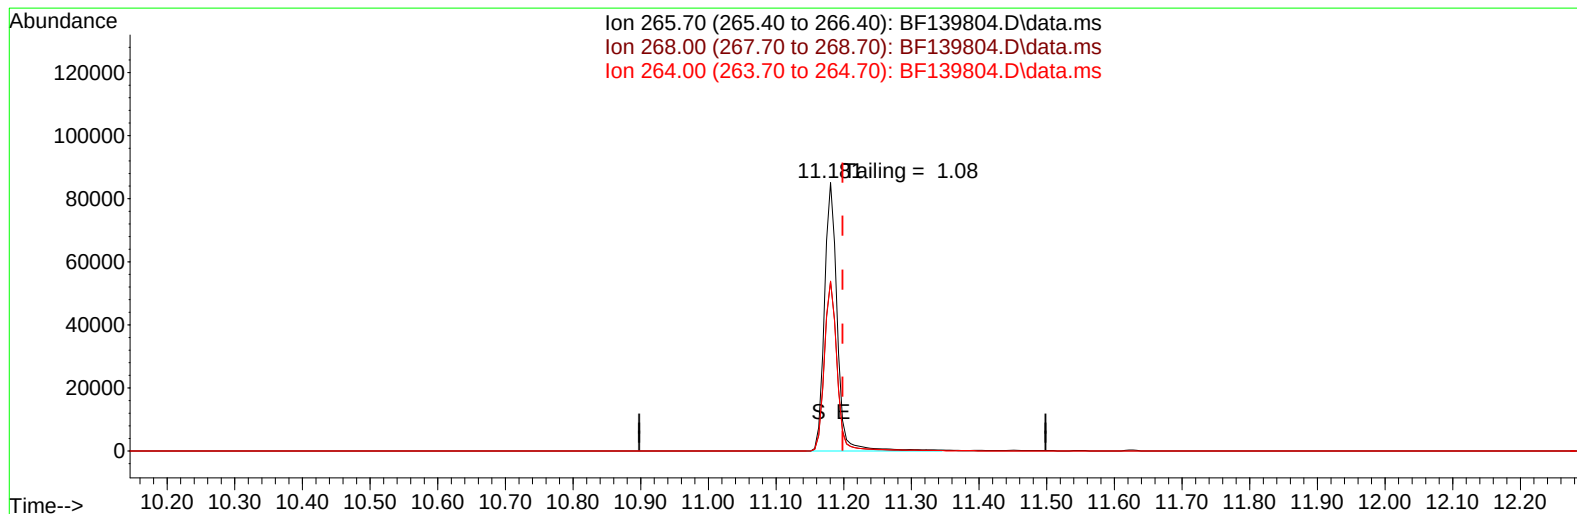

TIC: BF139804.D\data.ms

(70) Pentachlorophenol (C)

11.181min (-0.018) 40759.65 ng




response 111004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.50	63.20
264.00	61.60	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101524\
Data File : BF139804.D
Acq On : 15 Oct 2024 10:51
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 15 11:29:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 02 04:58:47 2024
Response via : Initial Calibration

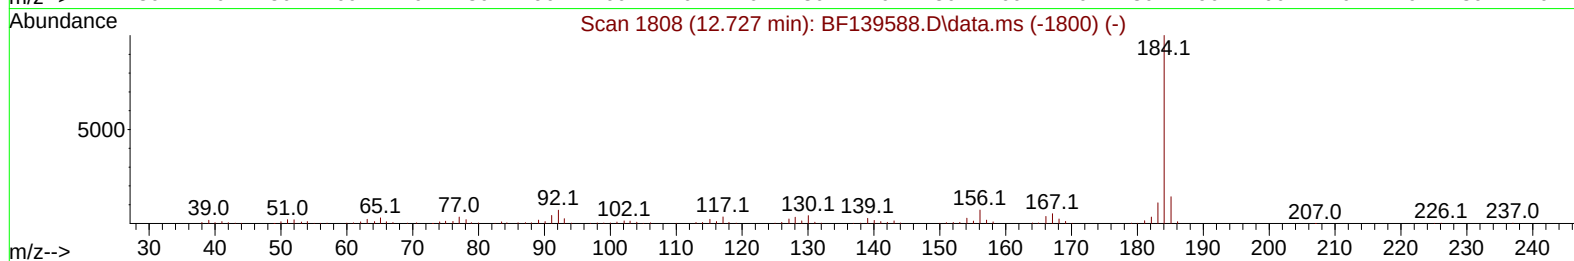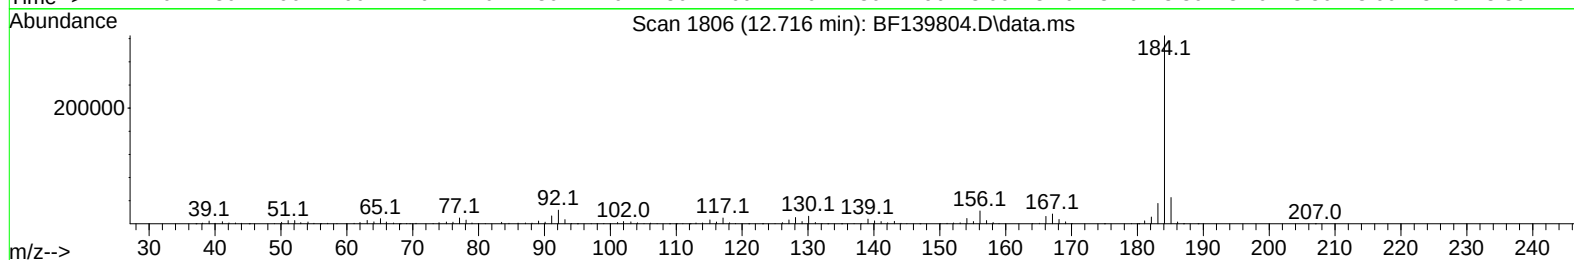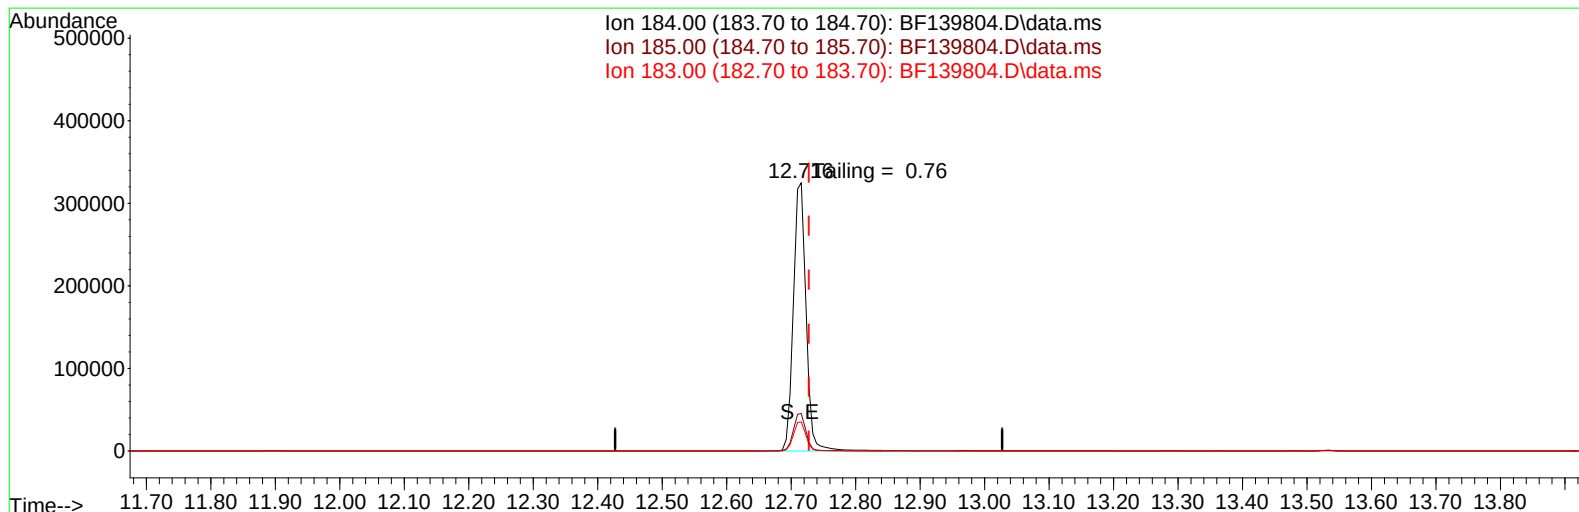

TIC: BF139804.D\data.ms

(77) Benzidine

12.716min (-0.012) 68500.72 ng

response 449477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.99
183.00	11.00	10.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/15/2024	BNA_F	<u>BF139804.D</u>
Compound Name	Response	Retention Time
DDT	260060	13.533
DDD	4784	13.263
DDE	56	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4840	264900	1.83

Instrument :
BNA_F
ClientSampleId :
DFTPP