
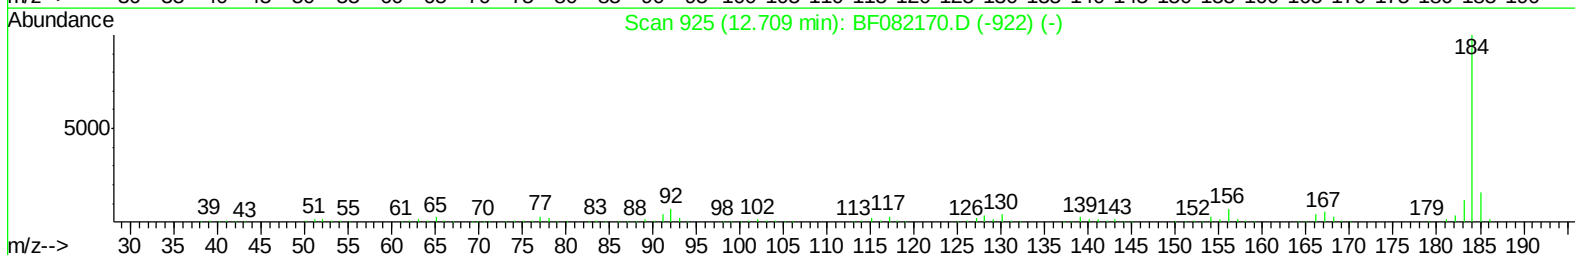
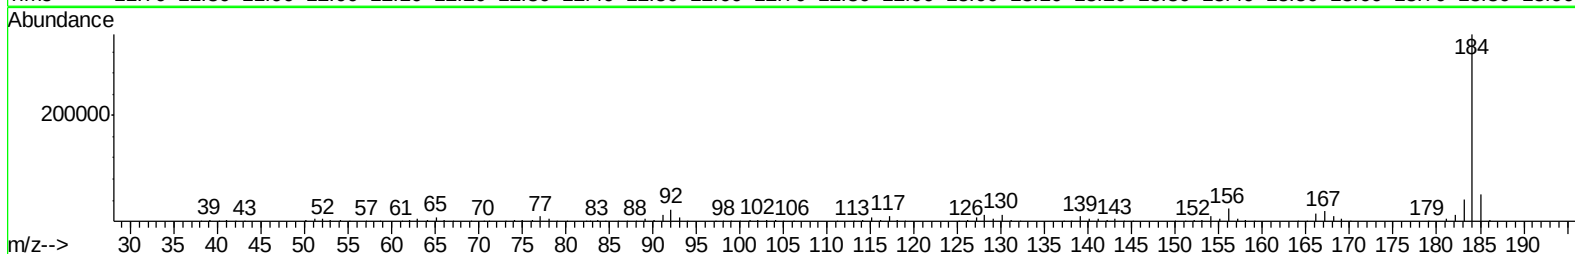


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
Data File : BF082294.D
Acq On : 15 Oct 2015 7:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 08:16:05 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

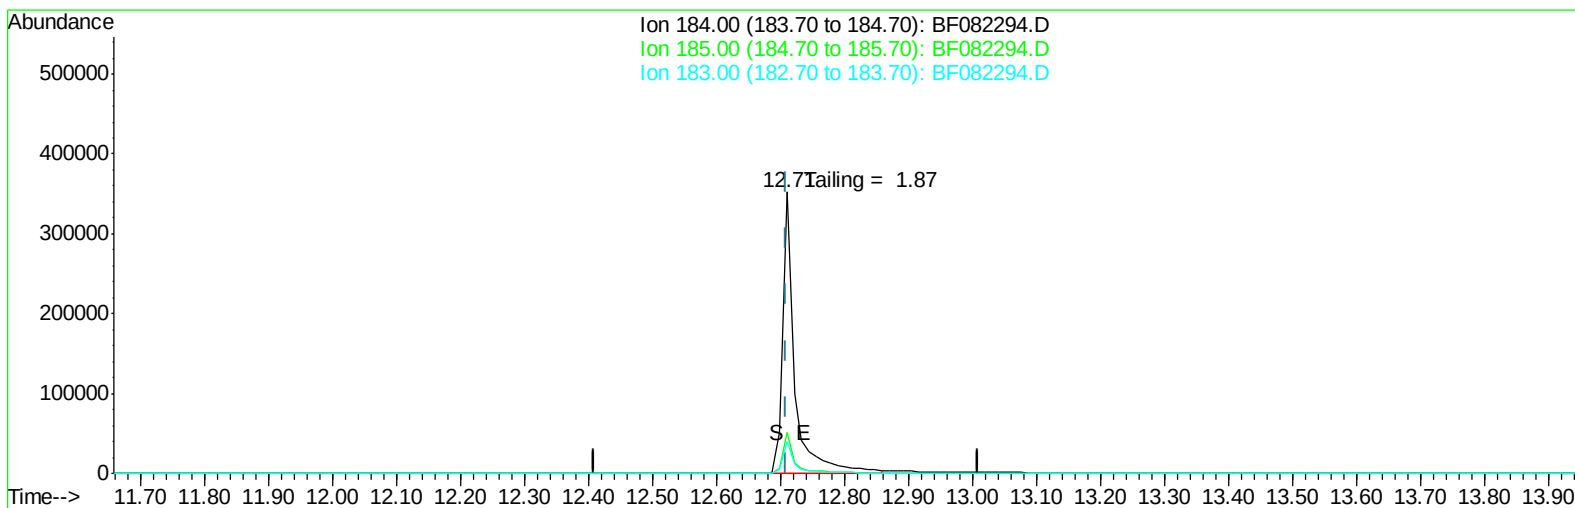

TIC: BF082294.D

(76) Benzidine




12.709min (-0.000) 0.00ng

response 473070

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.36
183.00	11.40	11.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101515\
Data File : BF082294.D
Acq On : 15 Oct 2015 7:40
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 08:16:05 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

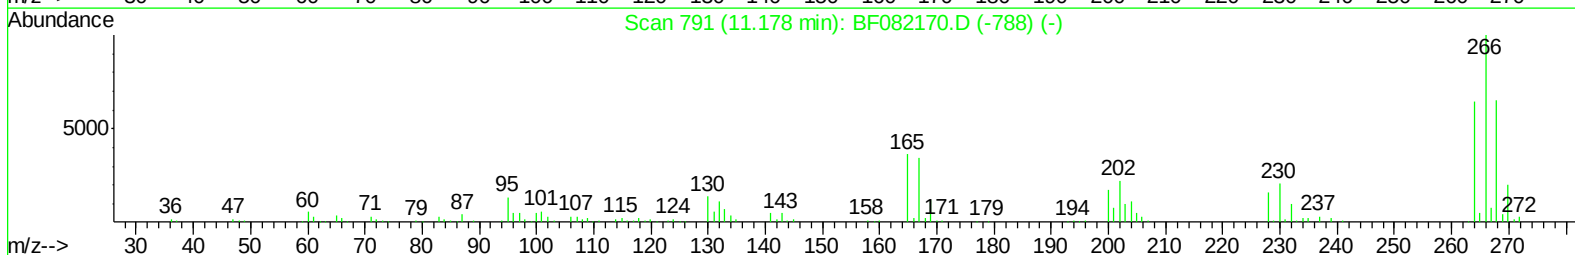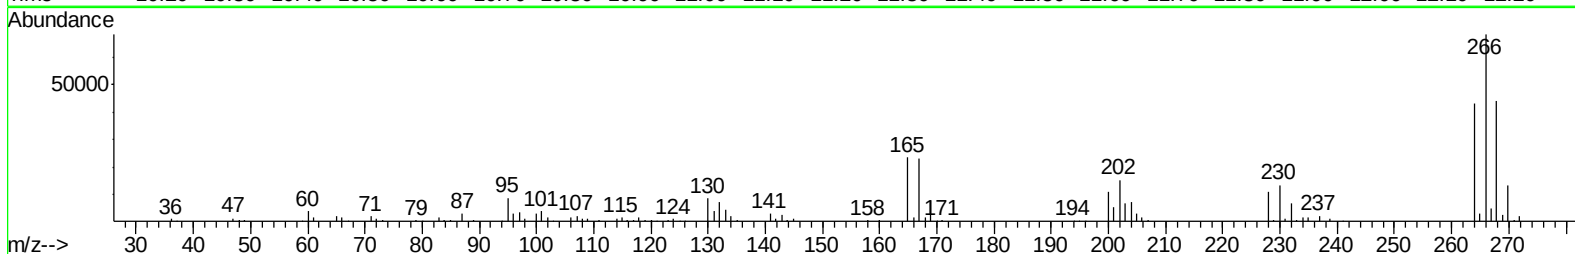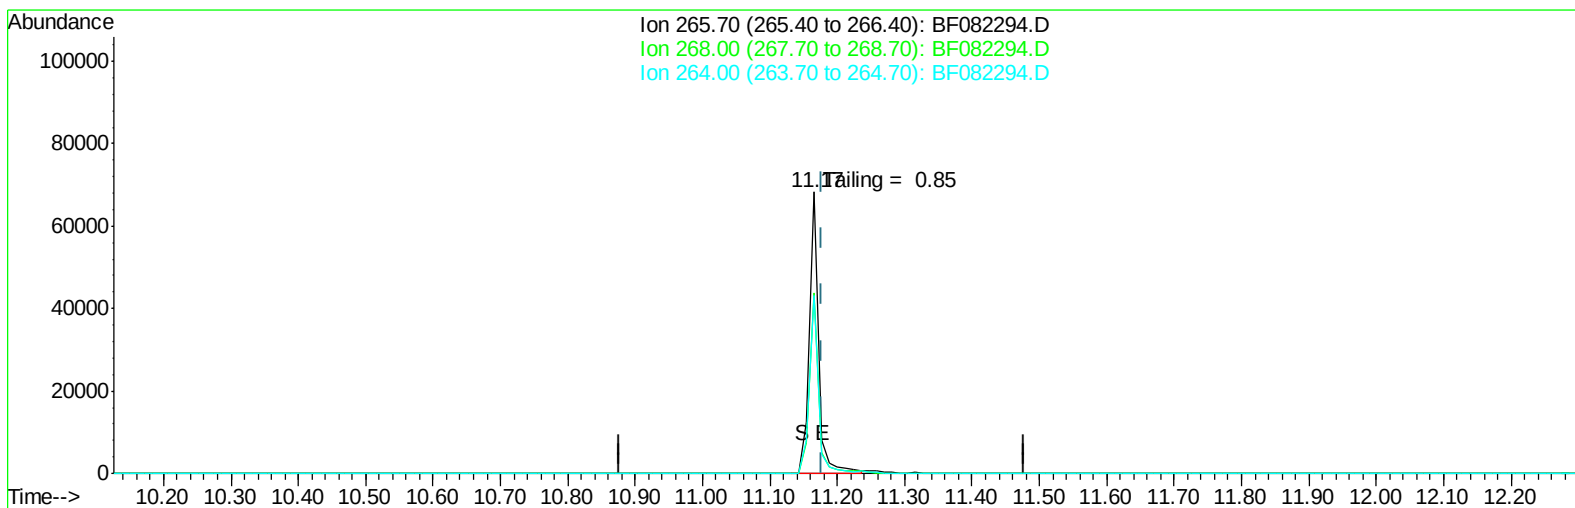

TIC: BF082294.D

(69) Pentachlorophenol (C)

11.166min (-0.012) 40460.75ng

response 67153

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.23
264.00	64.20	63.01
0.00	0.00	0.00