

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101615\
 Data File : BF082304.D
 Acq On : 15 Oct 2015 12:47
 Operator : UM/IZ
 Sample : G4016-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-10

Quant Time: Oct 16 01:46:52 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:04:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	79387	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	312809	20.00	ng	0.00
38) Acenaphthene-d10	9.87	164	156675	20.00	ng	0.00
63) Phenanthrene-d10	11.36	188	300560	20.00	ng	0.00
75) Chrysene-d12	14.09	240	191595	20.00	ng	0.00
86) Perylene-d12	15.67	264	167885	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	364223	92.59	ng	0.00
7) Phenol-d6	6.46	99	431089	84.22	ng	-0.01
23) Nitrobenzene-d5	7.39	82	308499	66.23	ng	-0.01
41) 2,4,6-Tribromophenol	10.66	330	134279	91.39	ng	-0.01
44) 2-Fluorobiphenyl	9.19	172	594158	62.89	ng	-0.01
78) Terphenyl-d14	12.96	244	561917	77.72	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.59	163	117260	10.63	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101615\
Data File : BF082304.D
Acq On : 15 Oct 2015 12:47
Operator : UM/IZ
Sample : G4016-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-10

Quant Time: Oct 16 01:46:52 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:04:42 2015
Response via : Initial Calibration

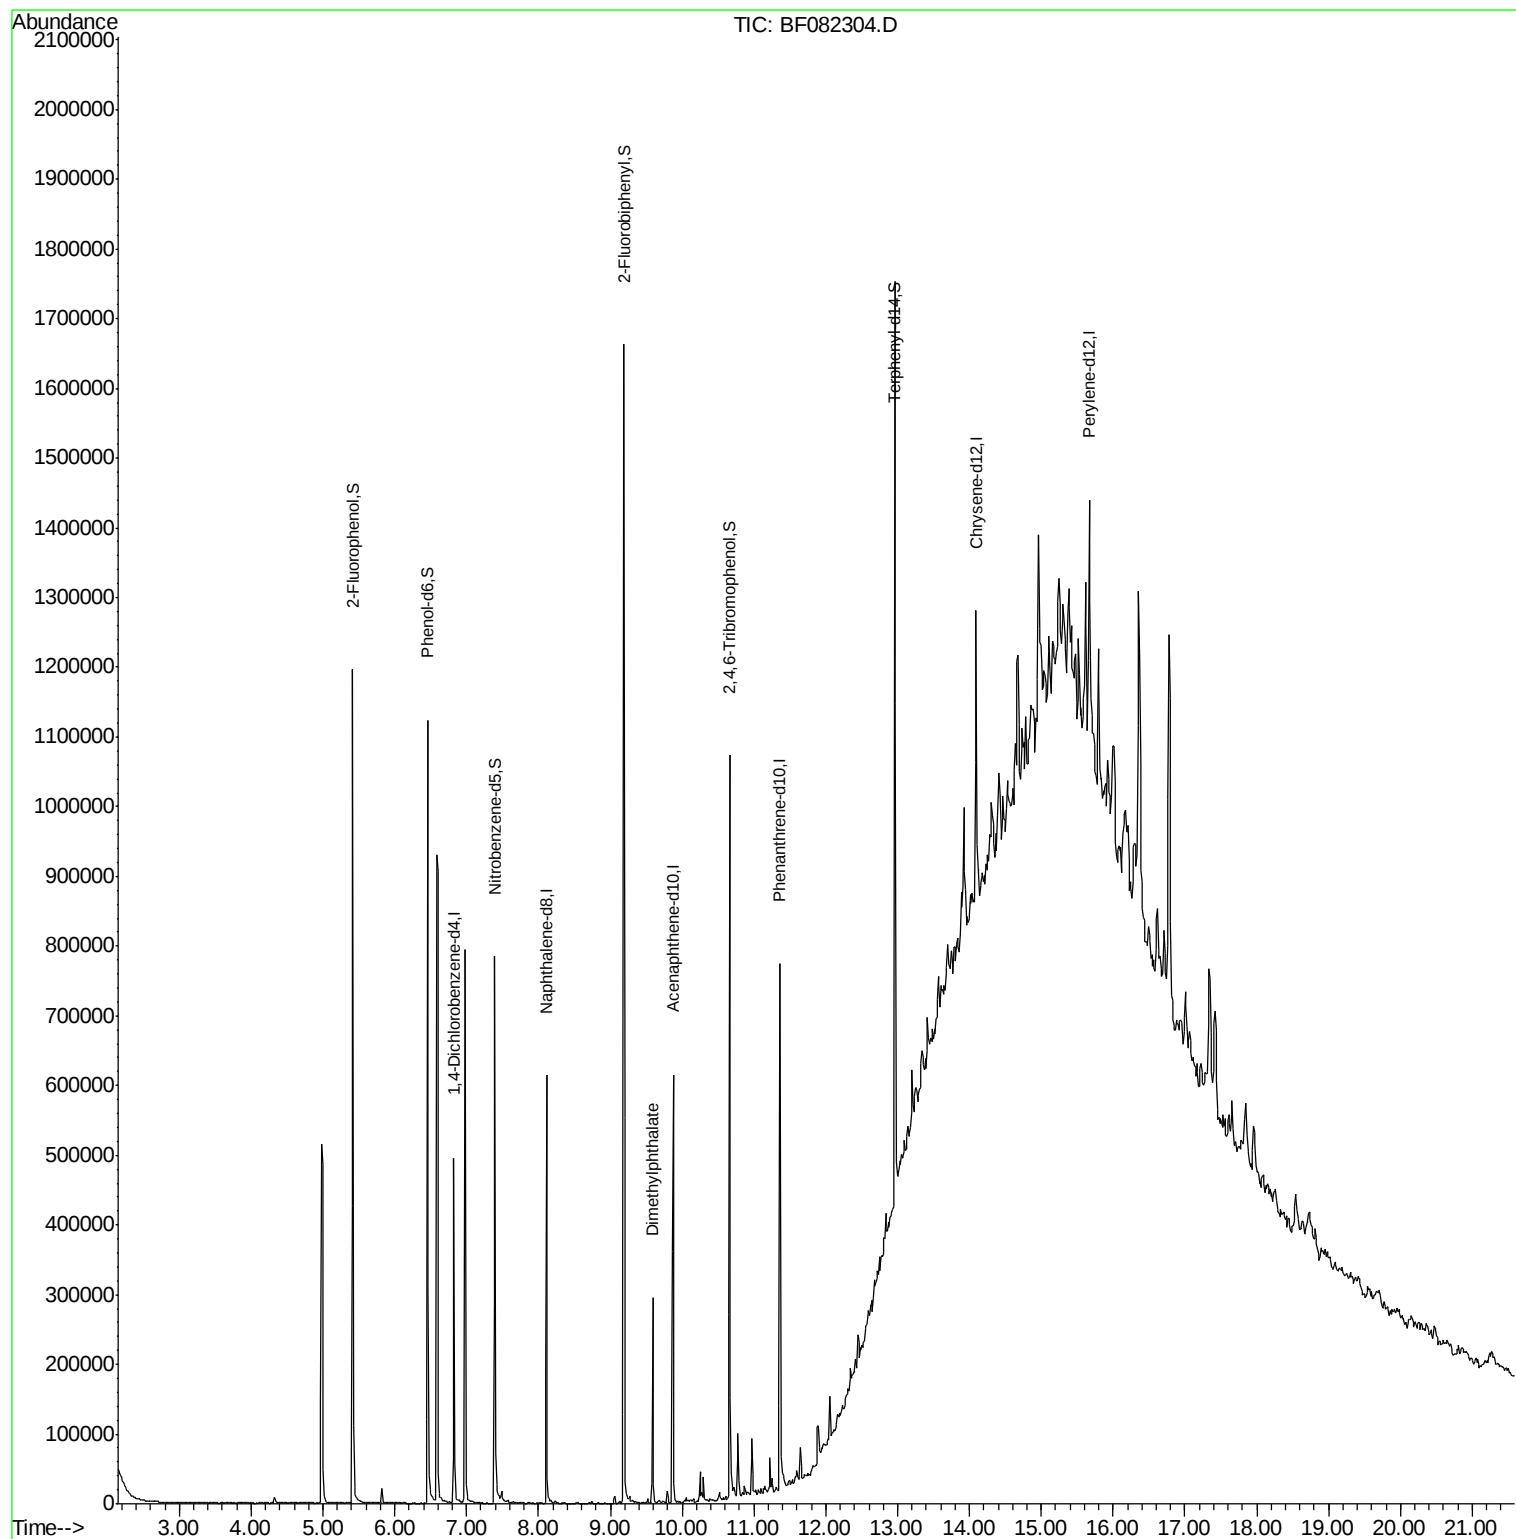




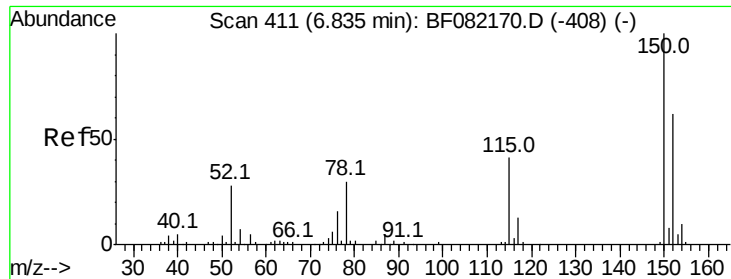


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.82 min Scan# 410
Delta R.T. 0.00 min
Lab File: BF082304.D
Acq: 15 Oct 2015 12:47

Instrument :
BNA_F
ClientSampleId :
CS-10




Tot Ion:152 Resp: 79387
Ion Ratio Lower Upper
152 100
150 159.5 129.0 193.4
115 56.0 52.1 78.1

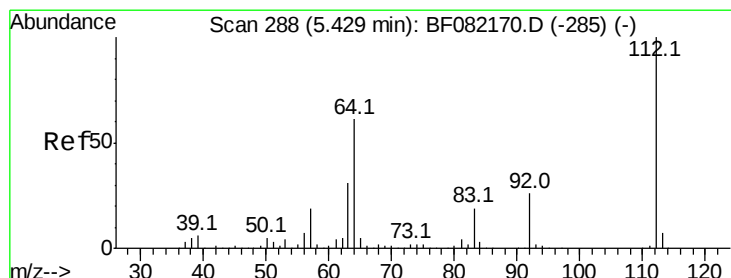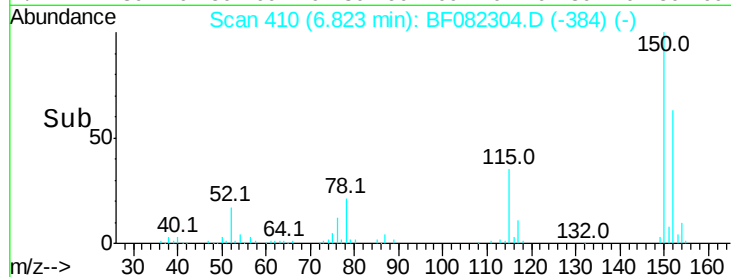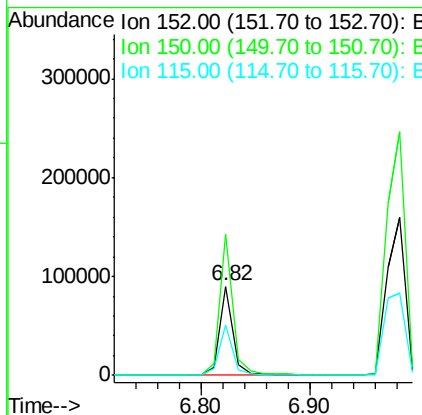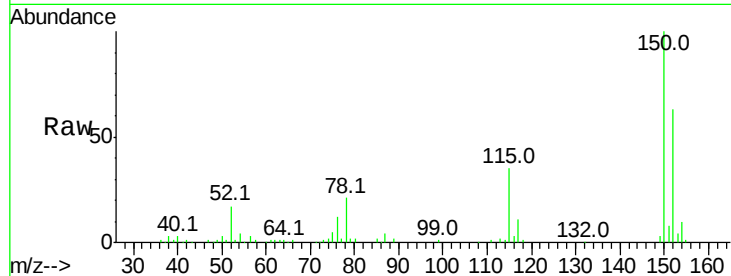


#5

2-Fluorophenol
Concen: 92.59 ng
RT: 5.42 min Scan# 287
Delta R.T. 0.00 min
Lab File: BF082304.D
Acq: 15 Oct 2015 12:47

Tgt Ion:112 Resp: 364223
Ion Ratio Lower Upper
112 100
64 56.6 48.6 73.0
63 29.8 25.1 37.7

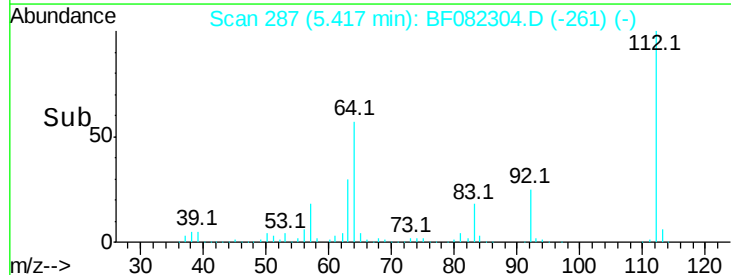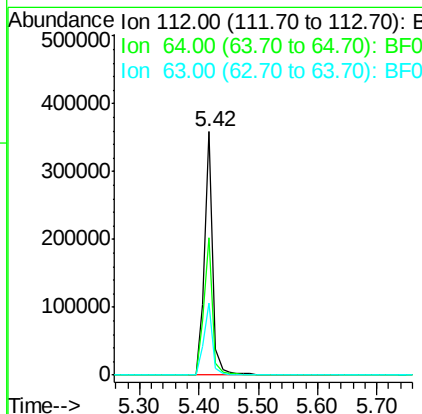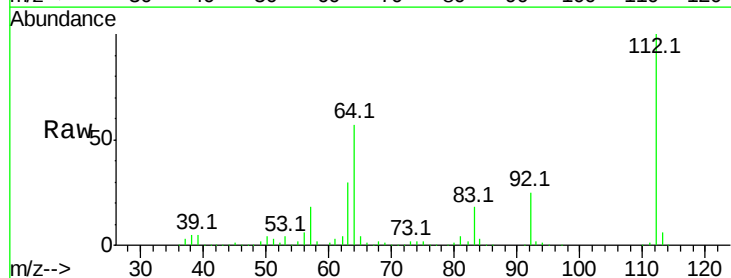

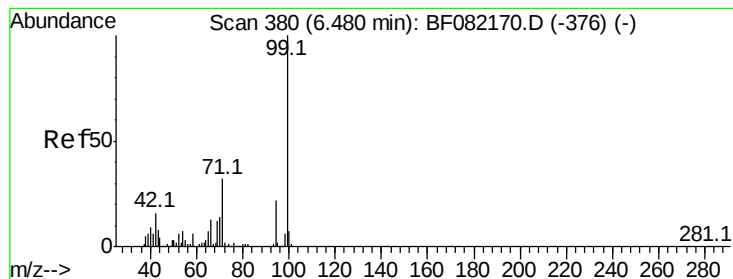

#7

Phenol-d6

Concen: 84.22 ng

RT: 6.46 min Scan# 378

Delta R.T. -0.01 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47

Instrument :

BNA_F

ClientSampled :

CS-10





Tot Ion: 99 Resp: 431089

Ion Ratio Lower Upper

99 100

42 18.9 13.2 19.8

71 35.7 25.6 38.4

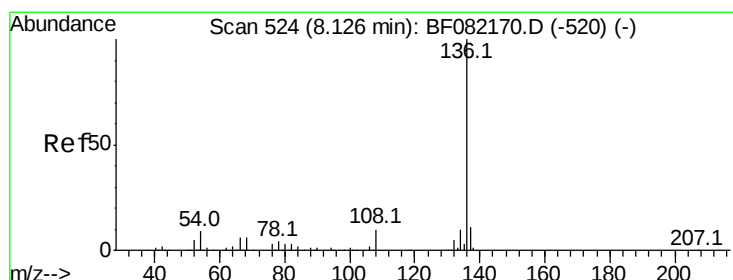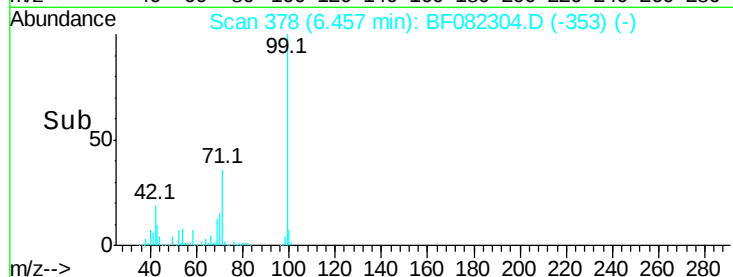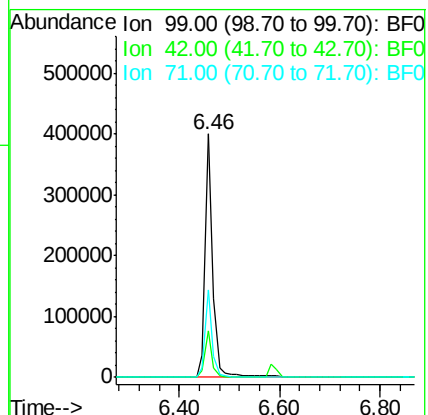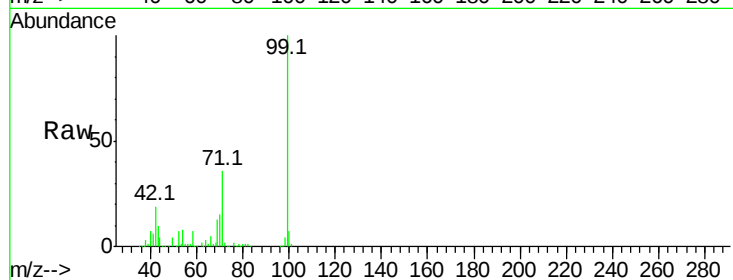

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.11 min Scan# 523

Delta R.T. 0.00 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47

Tgt Ion: 136 Resp: 312809




Ion Ratio Lower Upper


136 100

137 10.6 9.0 13.6

54 6.3 7.5 11.3#

68 4.2 4.6 7.0#


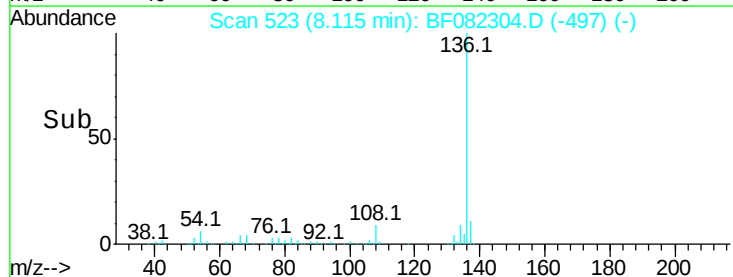
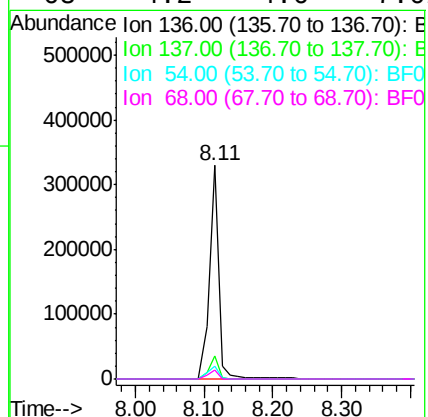
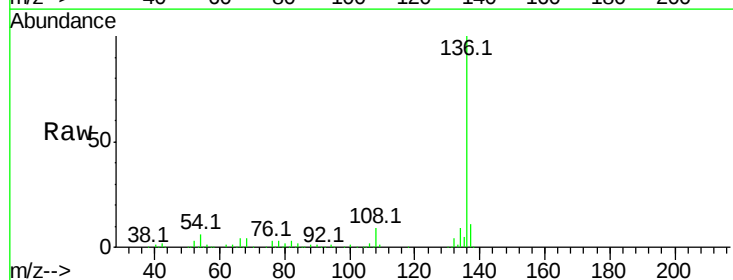


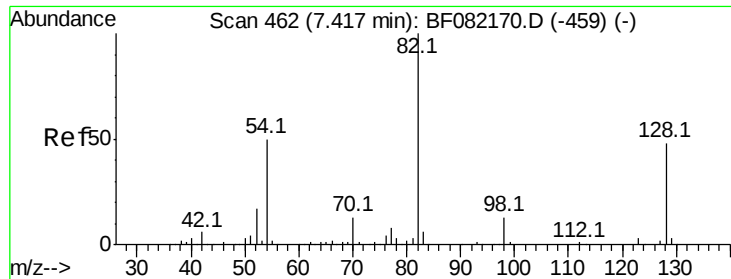

#23
 Nitrobenzene-d5
 Concen: 66.23 ng
 RT: 7.39 min Scan# 460
 Delta R.T. -0.01 min
 Lab File: BF082304.D
 Acq: 15 Oct 2015 12:47




Instrument :
 BNA_F
 ClientSampled :
 CS-10


Tot Ion: 82 Resp: 308499
 Ion Ratio Lower Upper
 82 100
 128 48.3 38.7 58.1
 54 49.1 40.1 60.1

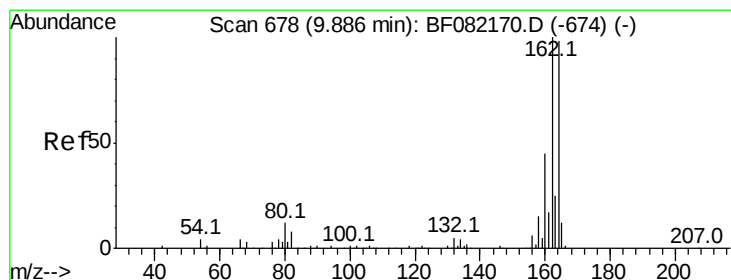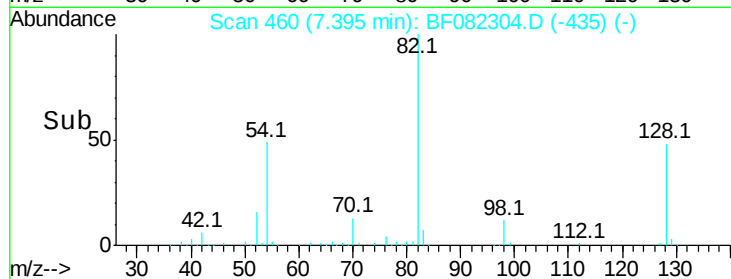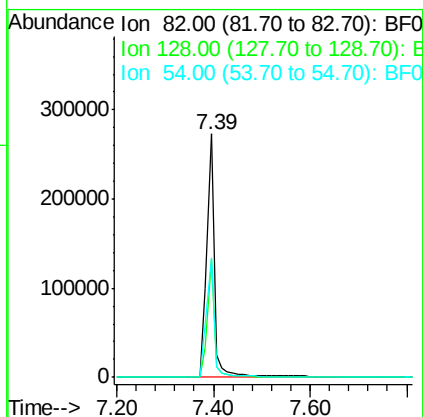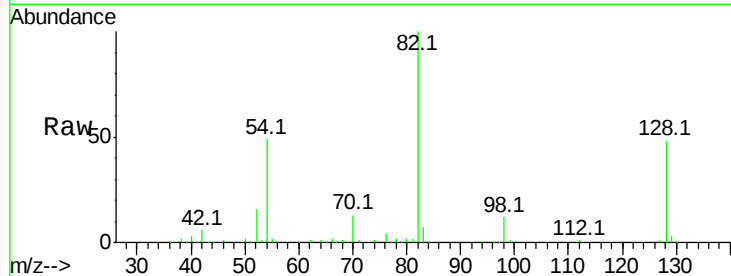

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.87 min Scan# 677
 Delta R.T. 0.00 min
 Lab File: BF082304.D
 Acq: 15 Oct 2015 12:47

Tgt Ion:164 Resp: 156675
 Ion Ratio Lower Upper
 164 100
 162 104.0 81.6 122.4
 160 45.8 36.4 54.6

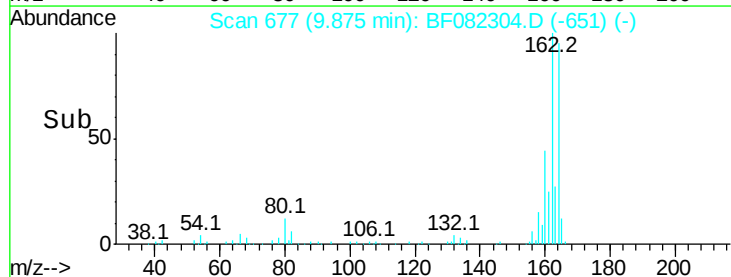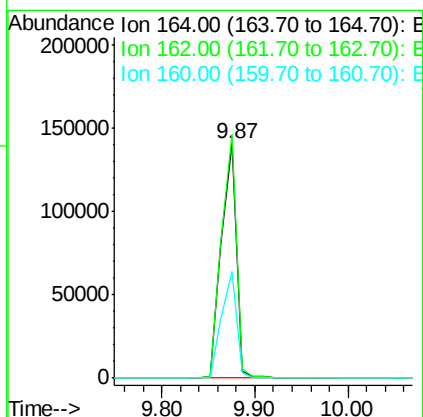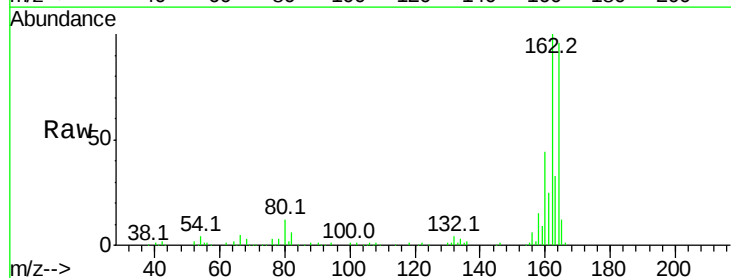


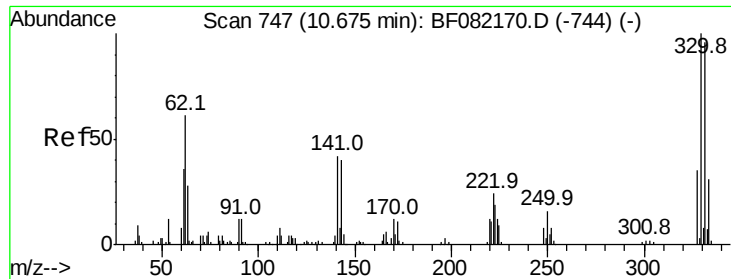




#41
 2,4,6-Tribromophenol
 Concen: 91.39 ng
 RT: 10.66 min Scan# 746
 Delta R.T. -0.01 min
 Lab File: BF082304.D
 Acq: 15 Oct 2015 12:47

Instrument :
 BNA_F
 ClientSampleId :
 CS-10

Tot Ion:330 Resp: 134279
 Ion Ratio Lower Upper
 330 100
 332 94.0 77.1 115.7
 141 36.5 29.8 44.8

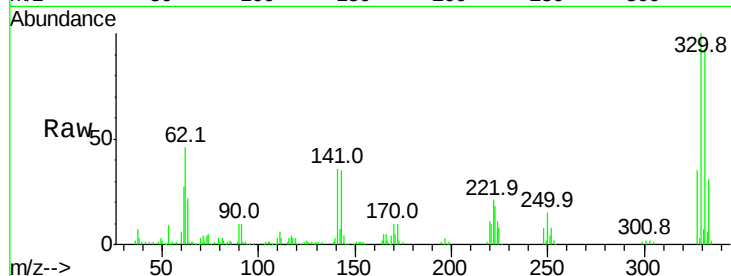


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

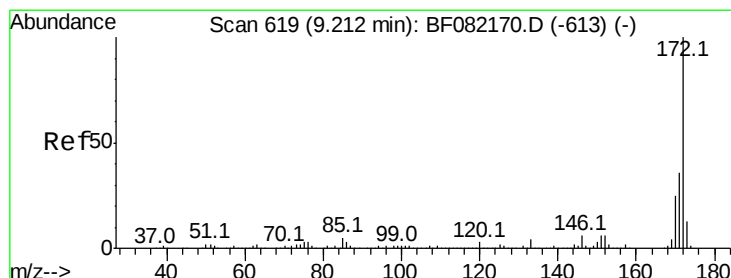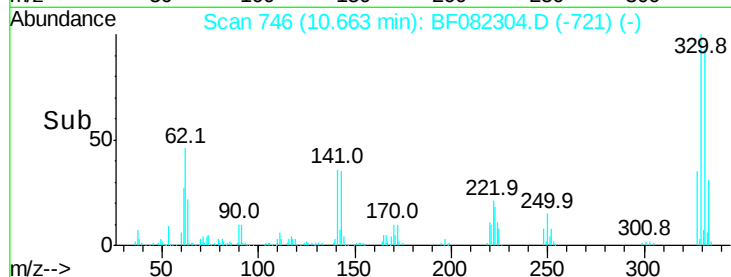
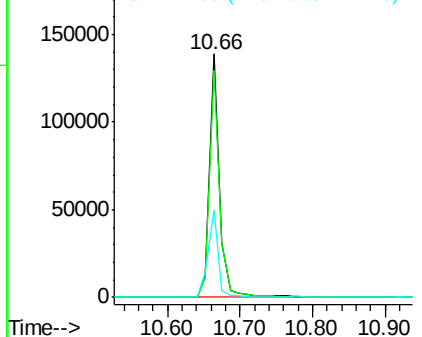



#44
 2-Fluorobiphenyl
 Concen: 62.89 ng
 RT: 9.19 min Scan# 617
 Delta R.T. -0.01 min
 Lab File: BF082304.D
 Acq: 15 Oct 2015 12:47

Tgt Ion:172 Resp: 594158
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.6 42.8
 170 24.1 19.7 29.5

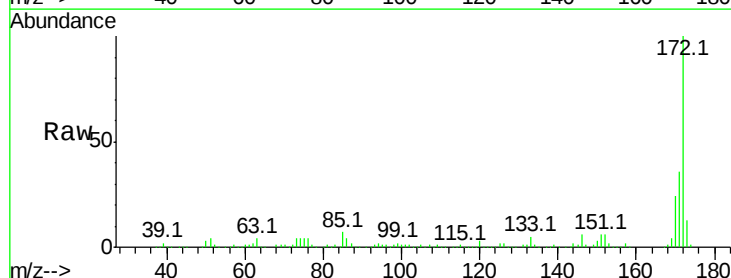

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

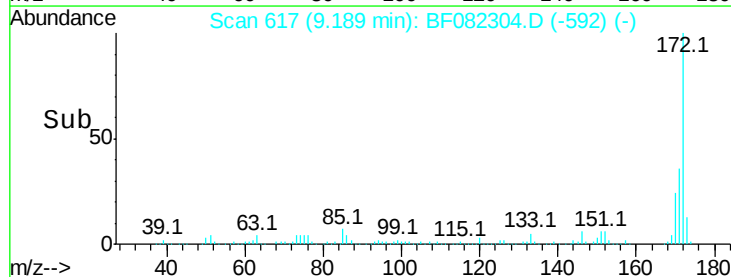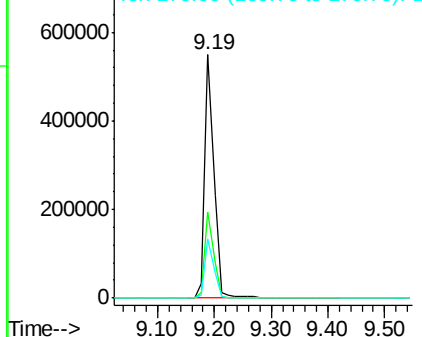

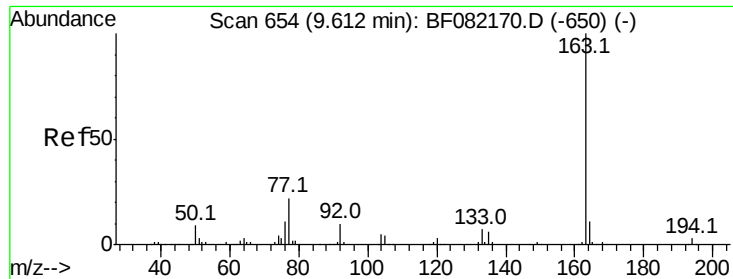

#49

Dimethylphthalate

Concen: 10.63 ng

RT: 9.59 min Scan# 652

Delta R.T. -0.02 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47

Instrument :

BNA_F

ClientSampleId :

CS-10


Tot Ion:163 Resp: 117260

Ion Ratio Lower Upper

163 100

194 3.2 2.6 4.0




164 10.5 8.5 12.7

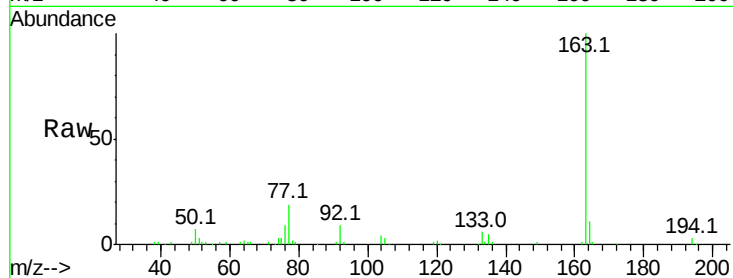

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

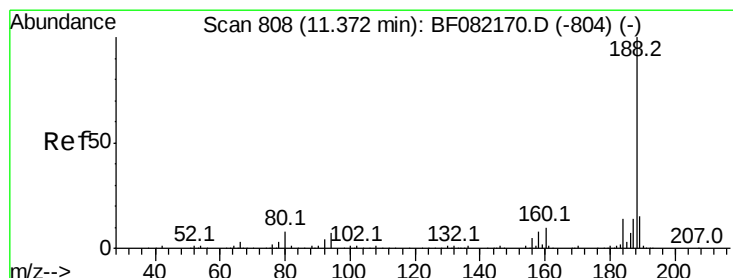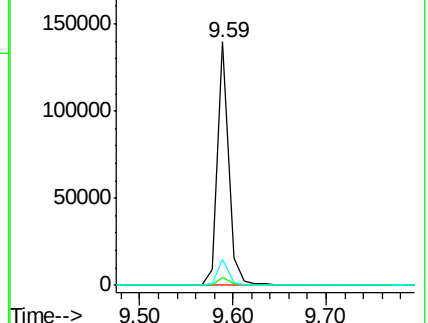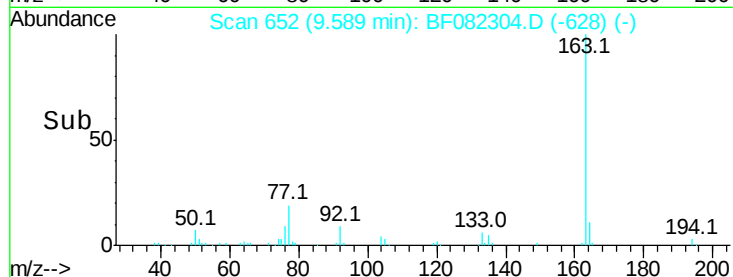

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.36 min Scan# 807

Delta R.T. 0.00 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47


Tgt Ion:188 Resp: 300560

Ion Ratio Lower Upper

188 100

94 7.5 5.8 8.6



80 7.7 6.4 9.6

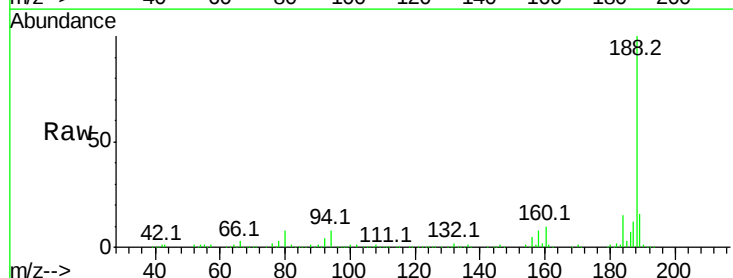


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

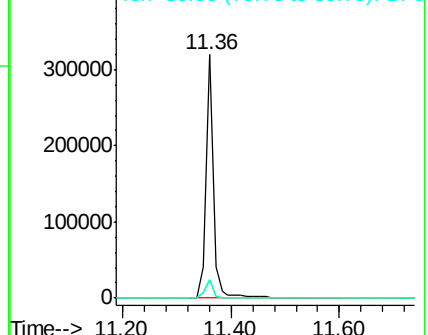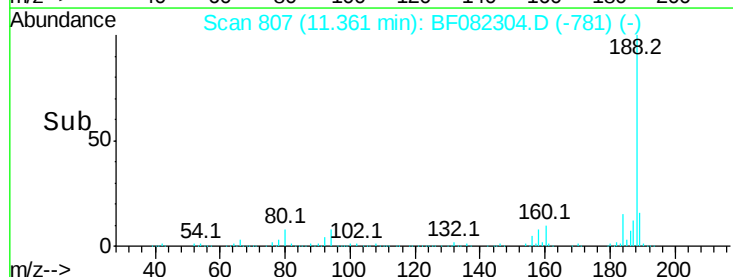

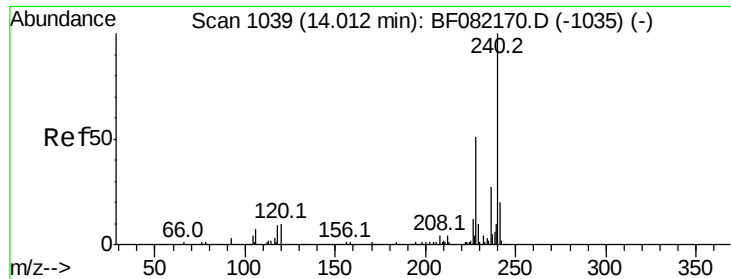

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.09 min Scan# 1046

Delta R.T. 0.00 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47

Instrument :

BNA_F

ClientSampleId :

CS-10


Tot Ion:240 Resp: 191595

Ion Ratio Lower Upper

240 100

120 9.4 8.1 12.1




236 25.7 21.3 31.9

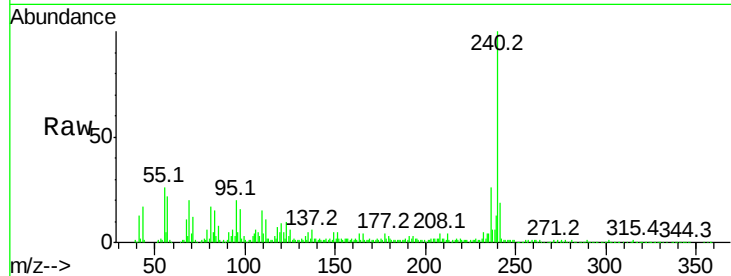

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

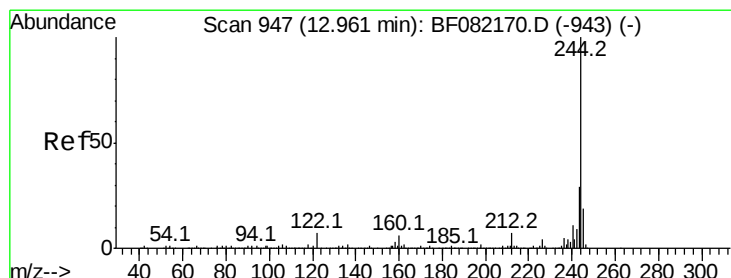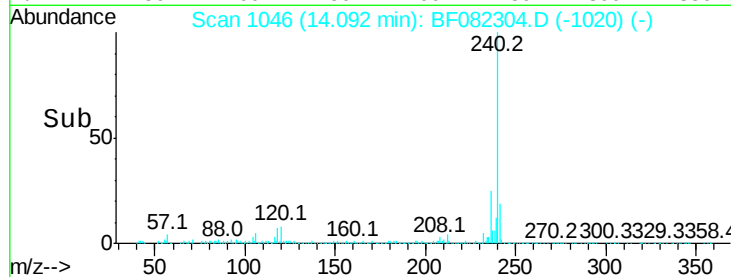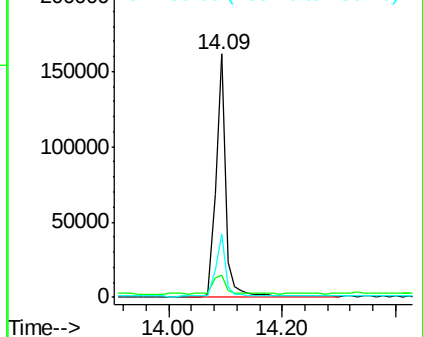

#78

Terphenyl-d14

Concen: 77.72 ng

RT: 12.96 min Scan# 947

Delta R.T. -0.01 min

Lab File: BF082304.D

Acq: 15 Oct 2015 12:47


Tgt Ion:244 Resp: 561917

Ion Ratio Lower Upper

244 100

212 7.6 5.8 8.6



122 12.7 5.9 8.9#

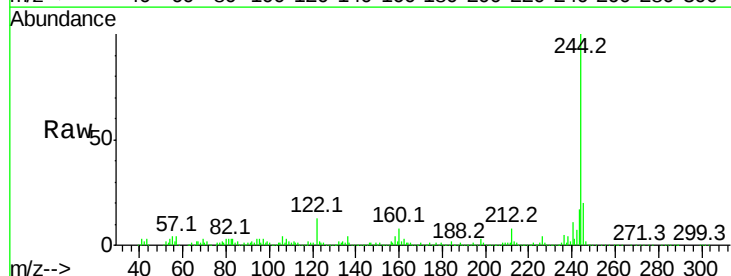


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

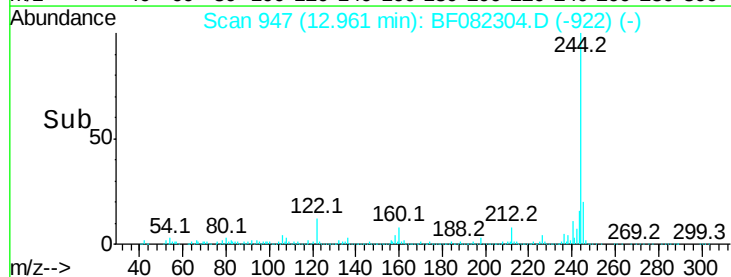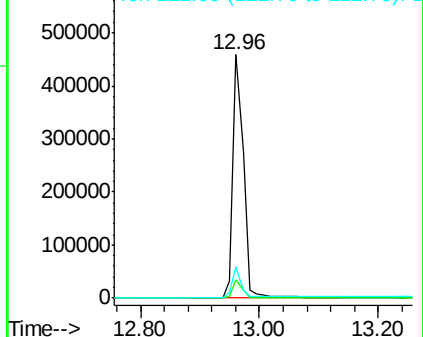

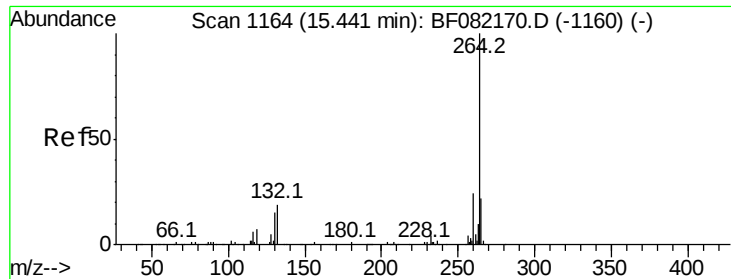

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.67 min Scan# 1184
Delta R.T. 0.01 min
Lab File: BF082304.D
Acq: 15 Oct 2015 12:47

Instrument :
BNA_F
ClientSampleId :
CS-10

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.0	28.6
265	22.4	17.3	25.9

