
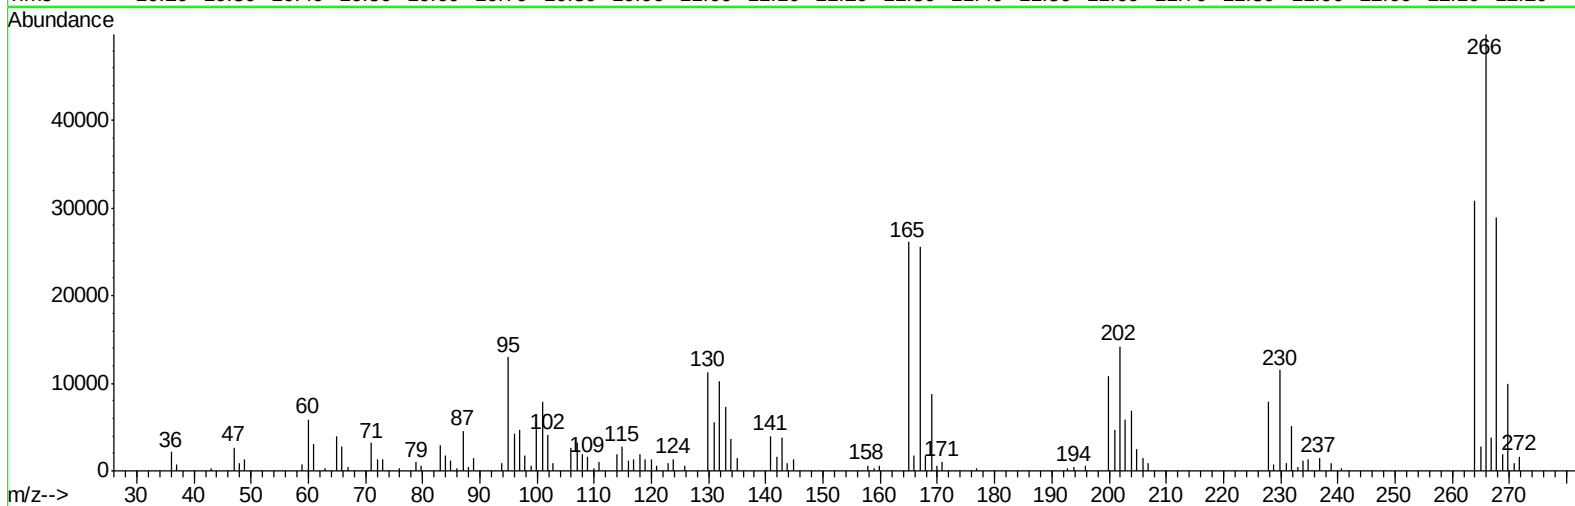


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101617\
Data File : BF099548.D
Acq On : 16 Oct 2017 17:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 06:48:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

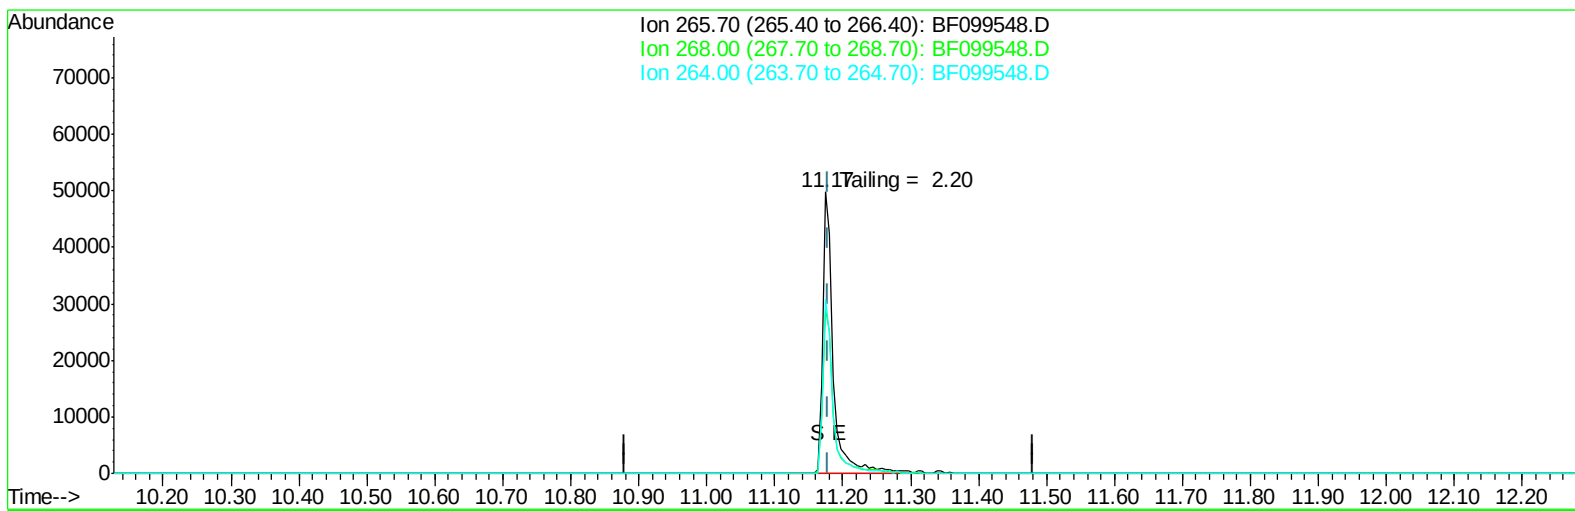

TIC: BF099548.D

(69) Pentachlorophenol (C)



11.175min (-0.006) 56358.36ng

response 54270

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.10
264.00	61.90	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101617\
Data File : BF099548.D
Acq On : 16 Oct 2017 17:07
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 06:48:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 11 16:25:21 2017
Response via : Initial Calibration

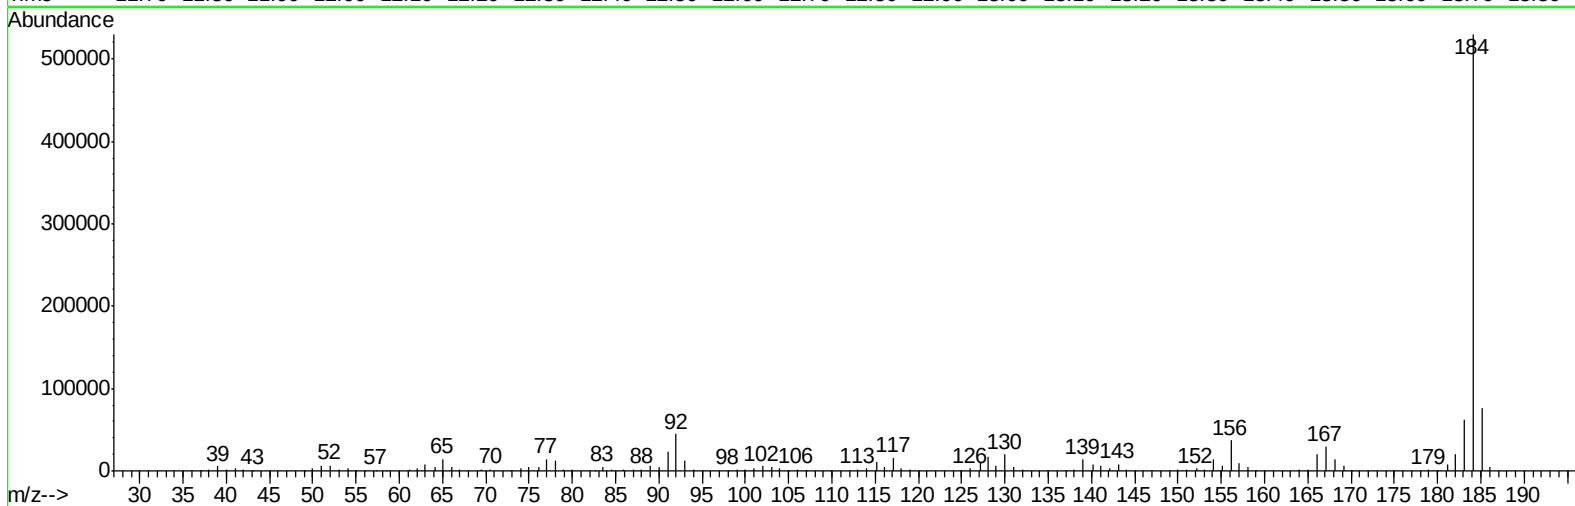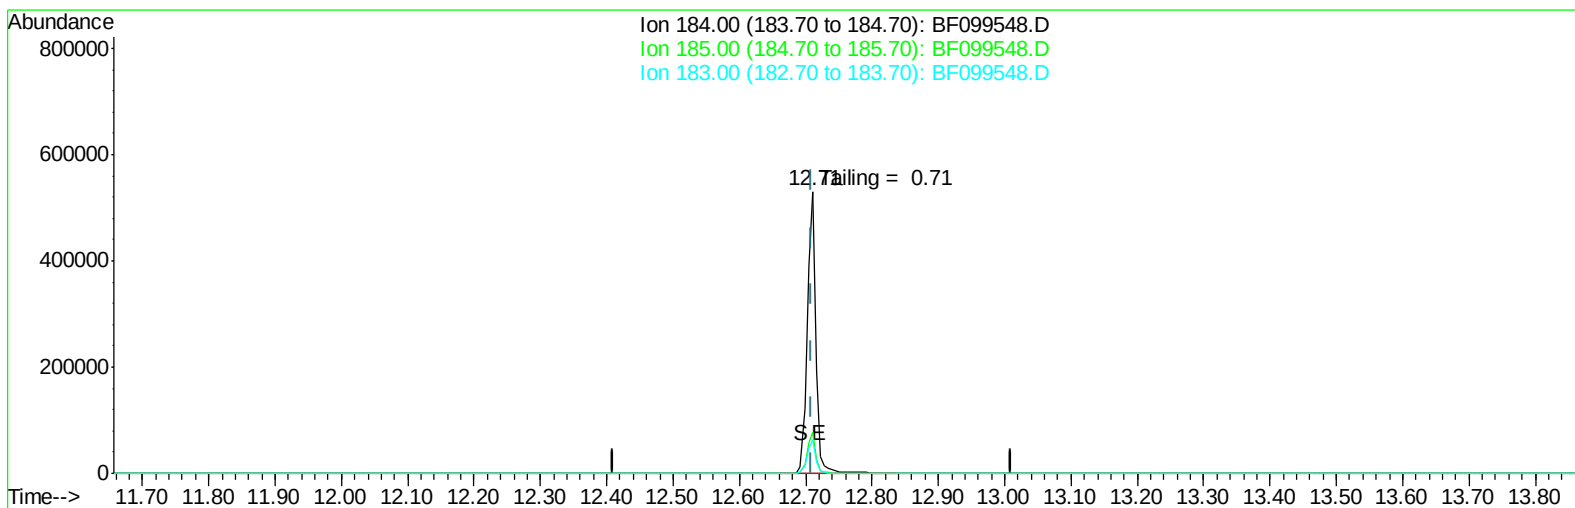

TIC: BF099548.D

(76) Benzidine

12.710min (+0.000) 0.00ng

response 472802

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.34
183.00	11.60	11.75
0.00	0.00	0.00