


Data Path : Z:\HPCHEM1\BNA_F\Data\BF101617\
 Data File : BF099534.D
 Acq On : 16 Oct 2017 9:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

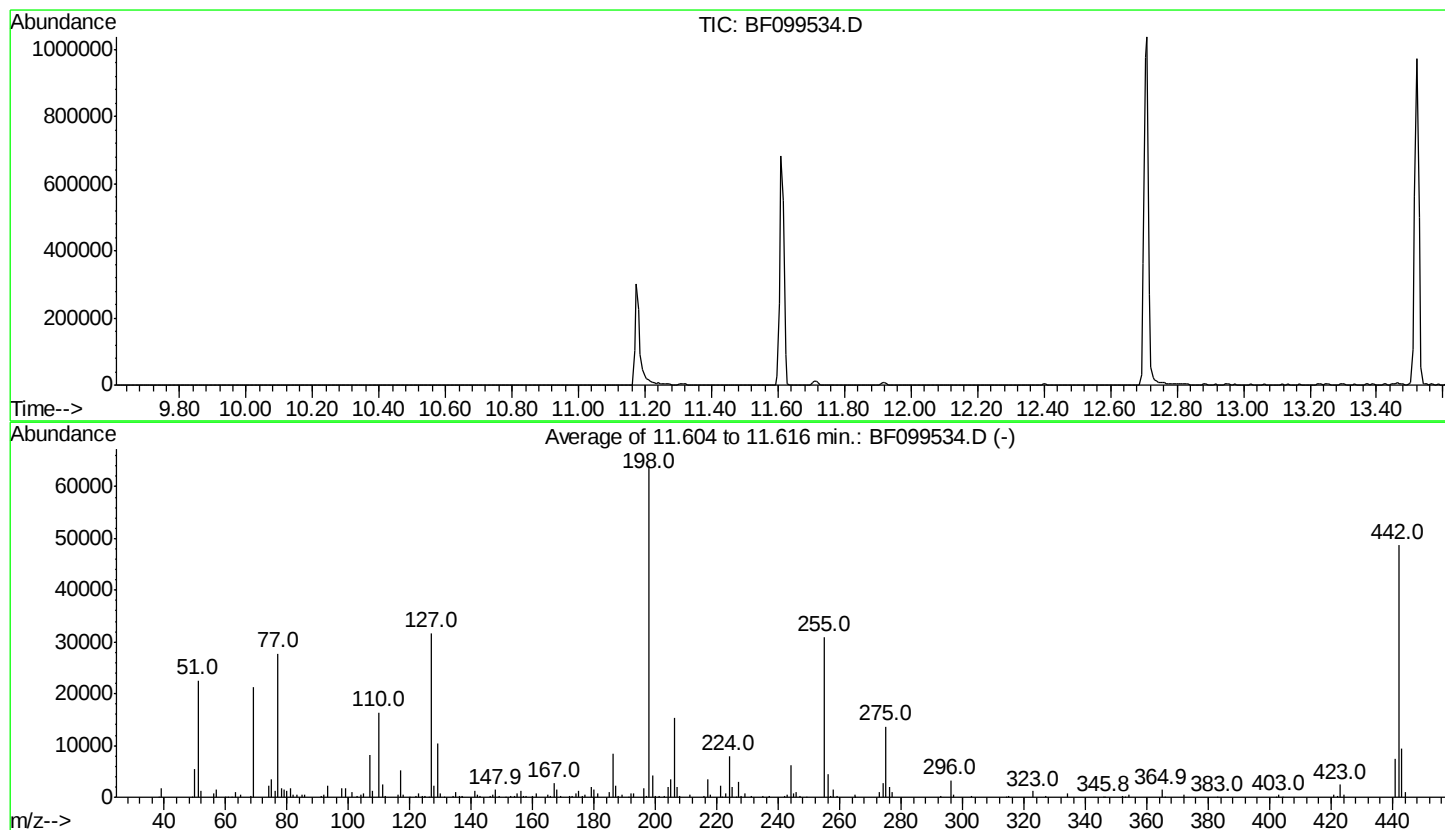

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	22573	PASS
68	69	0.00	2	0.8	161	PASS
69	198	0.00	100	33.3	21307	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	31690	PASS
197	198	0.00	2	0.6	370	PASS
198	198	100	100	100.0	64066	PASS
199	198	5	9	6.6	4217	PASS
275	198	10	60	21.4	13730	PASS
365	198	1	100	2.3	1454	PASS
441	442	0.01	24	15.0	7330	PASS
442	198	50	100	76.2	48829	PASS
443	442	15	24	19.0	9301	PASS