


Data Path : Z:\HPCHEM1\BNA F\Data\BF101617\
 Data File : BF099548.D
 Acq On : 16 Oct 2017 17:07
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 11 16:25:21 2017

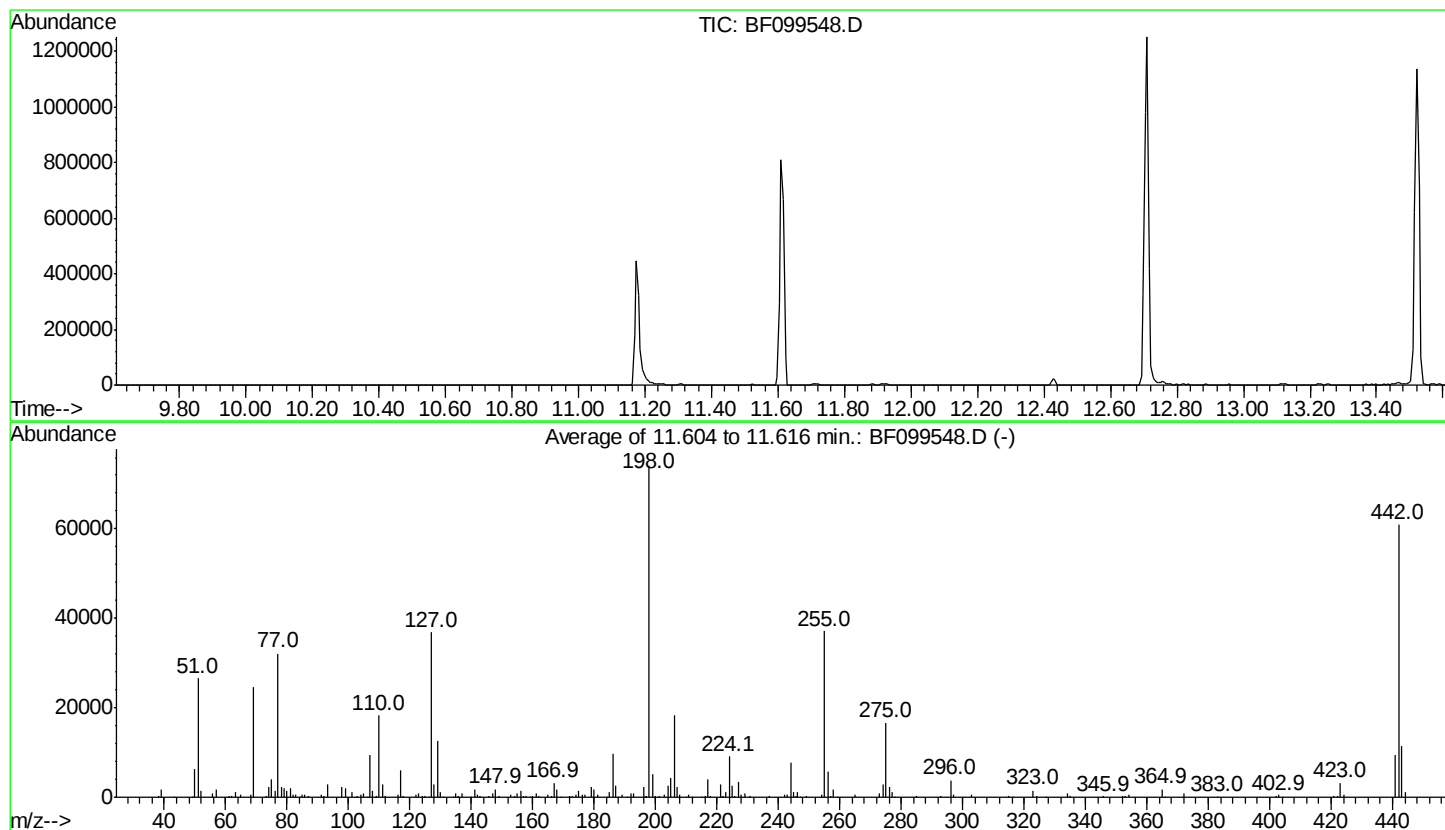

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	26525	PASS
68	69	0.00	2	1.9	460	PASS
69	198	0.00	100	33.1	24546	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	36906	PASS
197	198	0.00	2	0.5	351	PASS
198	198	100	100	100.0	74149	PASS
199	198	5	9	6.9	5121	PASS
275	198	10	60	22.5	16692	PASS
365	198	1	100	2.5	1860	PASS
441	442	0.01	24	15.6	9511	PASS
442	198	50	100	82.1	60850	PASS
443	442	15	24	18.8	11467	PASS