
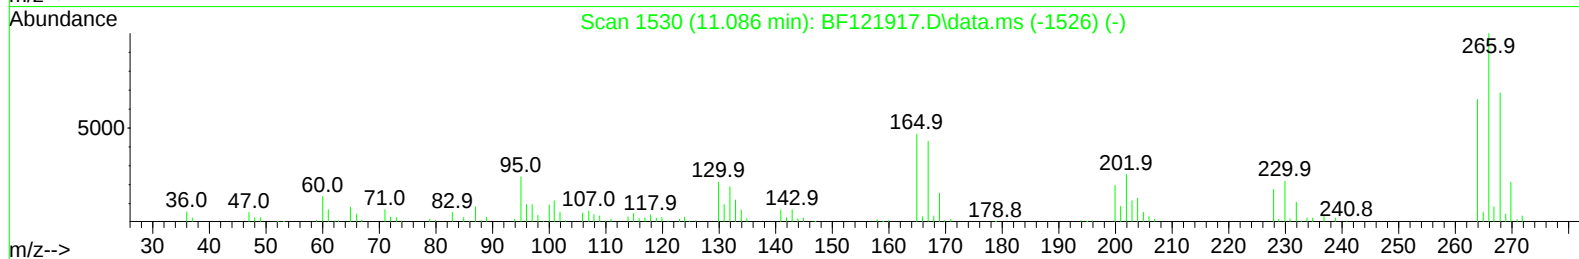
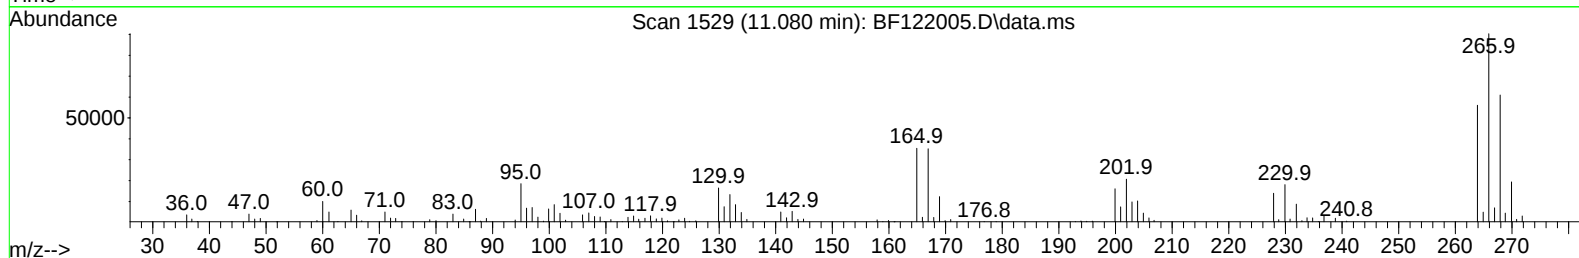


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122005.D
Acq On : 16 Oct 2020 10:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:12:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

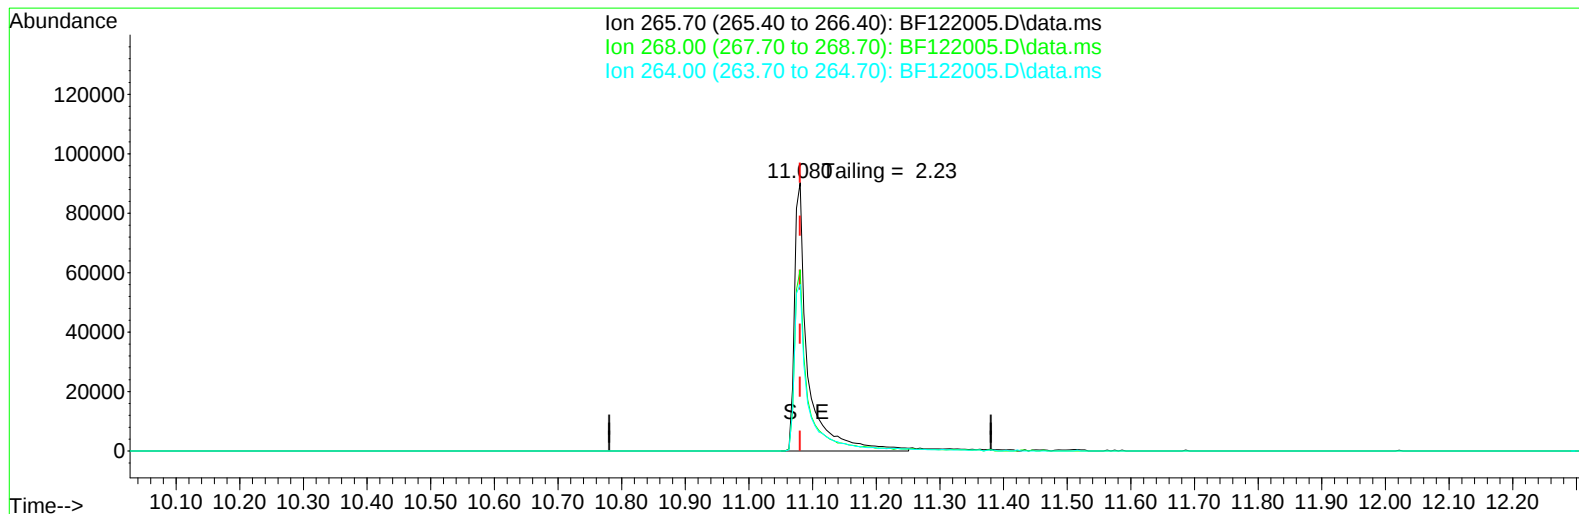




TIC: BF122005.D\data.ms

(70) Pentachlorophenol (C)**11.080min (+ 0.000) 152138.86 ng****response 135475**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	67.48
264.00	62.40	62.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122005.D
Acq On : 16 Oct 2020 10:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 02:12:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration

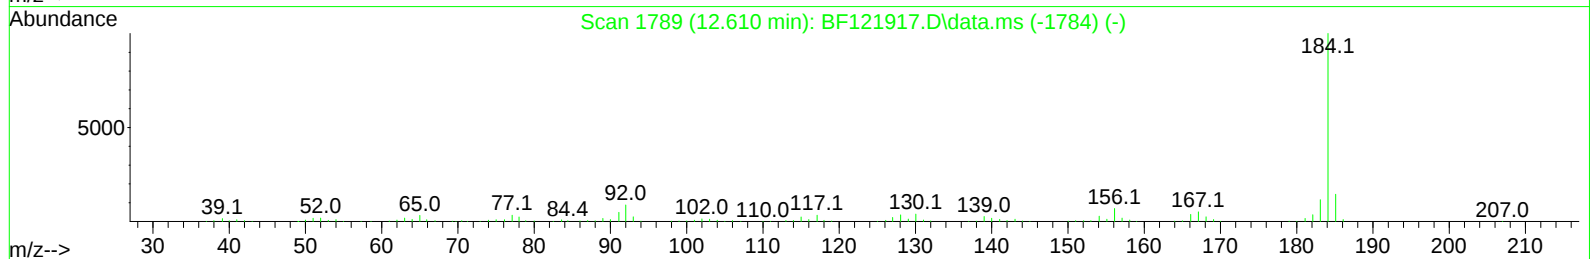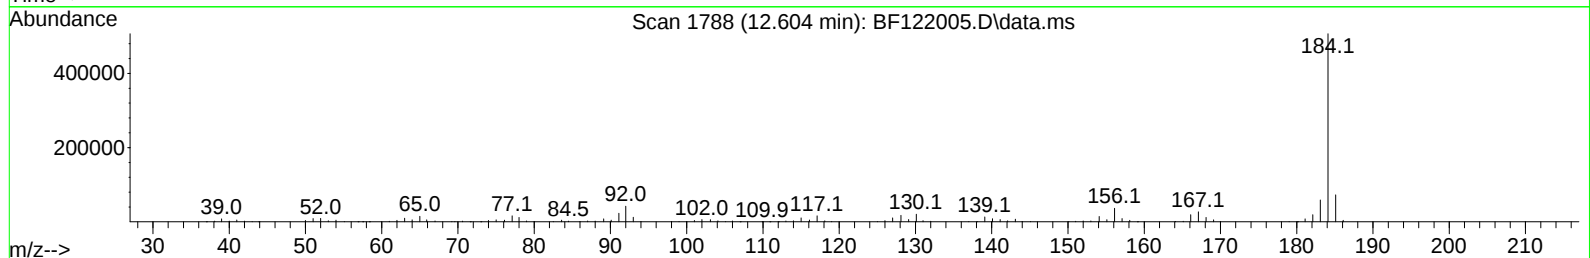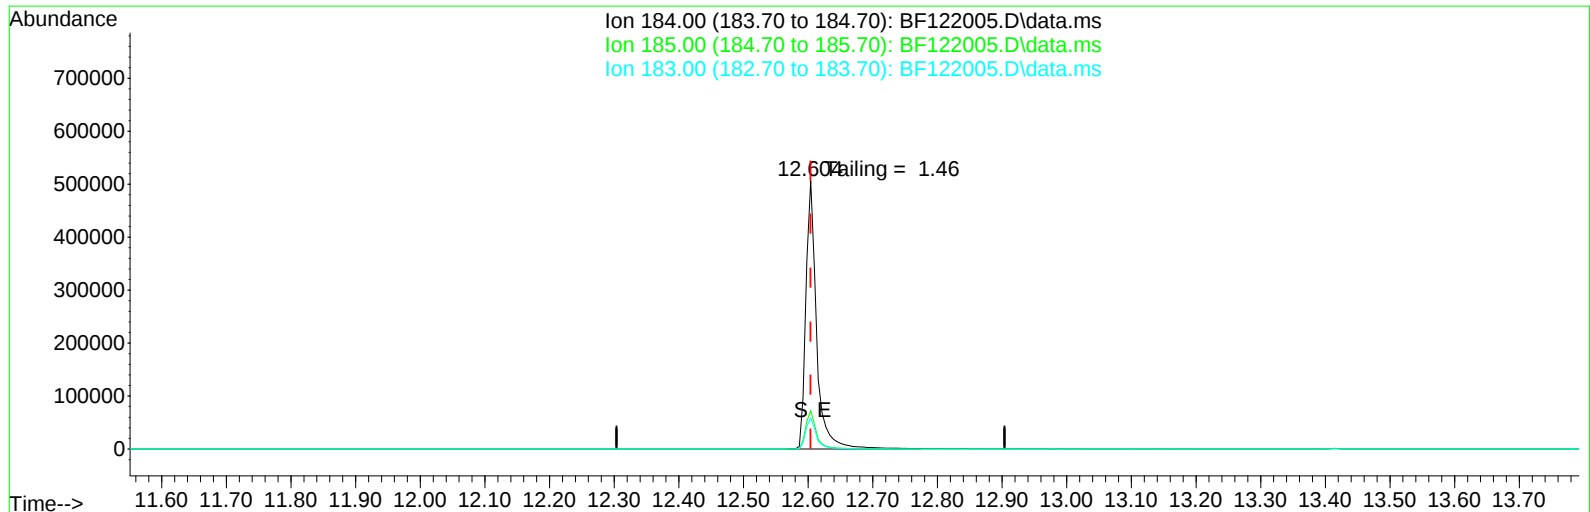

TIC: BF122005.D\data.ms

(77) Benzidine

12.604min (+ 0.000) 0.00 ng m

response 587748

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.39
183.00	11.70	11.65
0.00	0.00	0.00