

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
 Data File : BF122017.D
 Acq On : 16 Oct 2020 18:19
 Operator : JU/CG
 Sample : L4223-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-01-101420

Quant Time: Oct 16 19:23:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 12:55:05 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.745	152	111447	20.00	ng	0.00
21) Naphthalene-d8	8.028	136	433953	20.00	ng	0.00
39) Acenaphthene-d10	9.775	164	207985	20.00	ng	0.00
64) Phenanthrene-d10	11.263	188	338197	20.00	ng	0.00
76) Chrysene-d12	13.904	240	243387	20.00	ng	0.00
86) Perylene-d12	15.345	264	246833	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.381	112	830902	110.04	ng	0.02
7) Phenol-d6	6.393	99	971620	99.96	ng	0.00
23) Nitrobenzene-d5	7.316	82	777984	91.94	ng	0.00
42) 2,4,6-Tribromophenol	10.569	330	306597	119.17	ng	0.00
45) 2-Fluorobiphenyl	9.104	172	1255570	88.82	ng	0.00
79) Terphenyl-d14	12.845	244	1044001	81.75	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.498	163	72758	4.78	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122017.D
Acq On : 16 Oct 2020 18:19
Operator : JU/CG
Sample : L4223-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Quant Time: Oct 16 19:23:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 12:55:05 2020
Response via : Initial Calibration




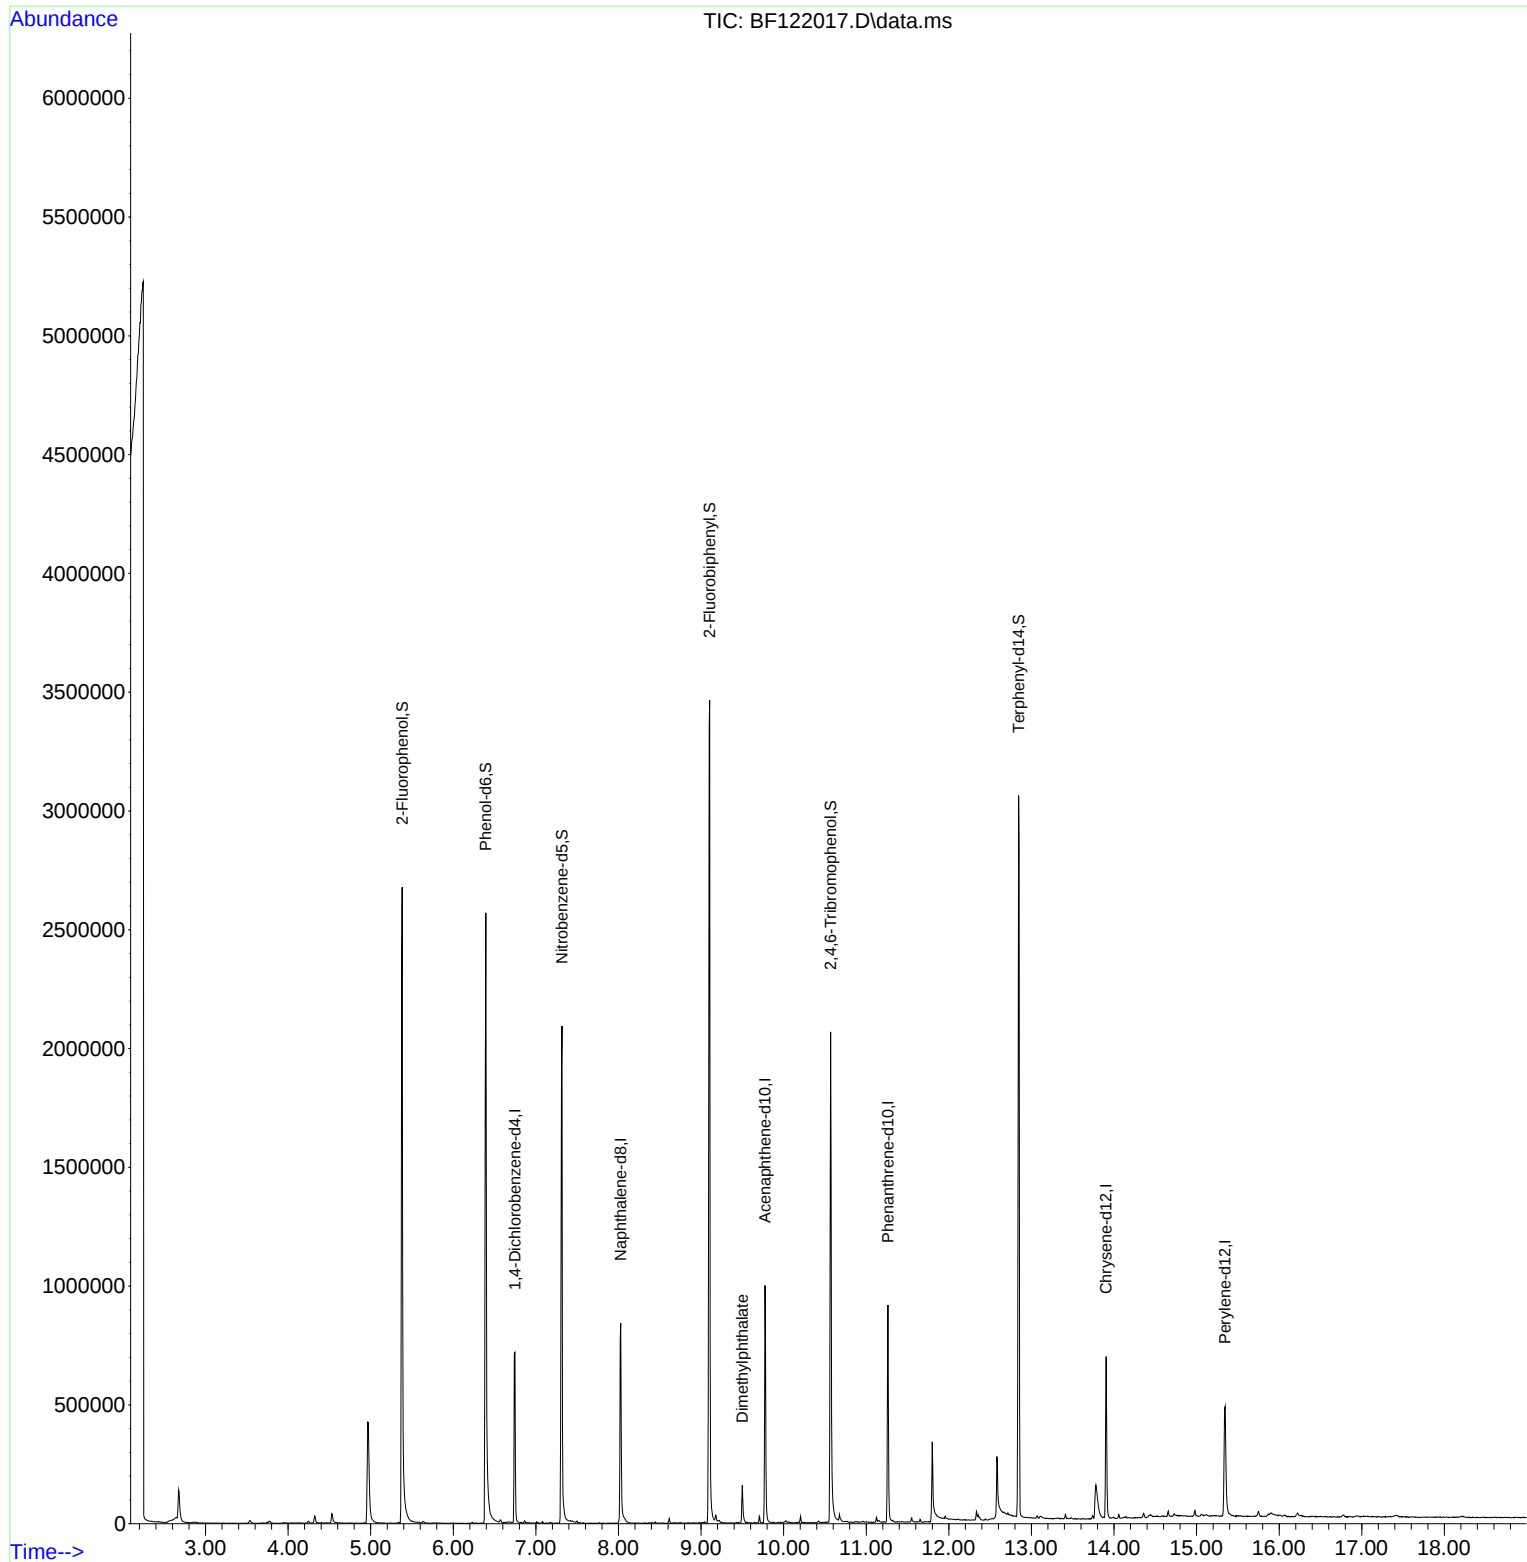




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.745 min Scan# 792
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19




Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Tgt Ion:152 Resp: 111447
Ion Ratio Lower Upper
152 100
150 156.7 125.3 187.9
115 61.6 51.9 77.9

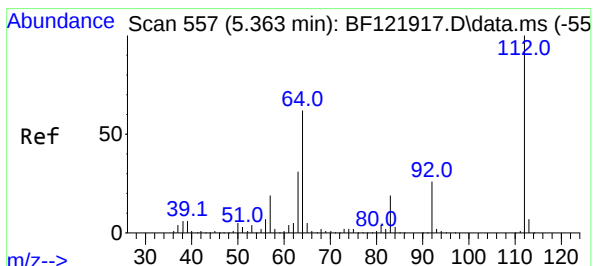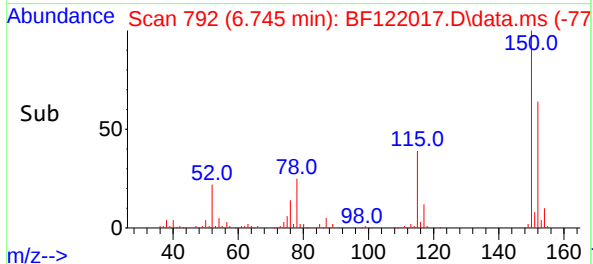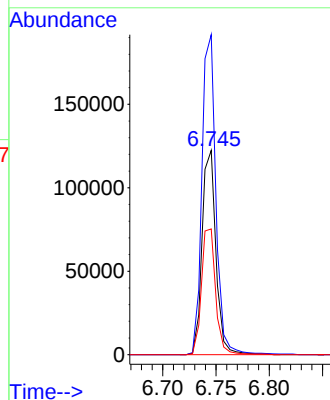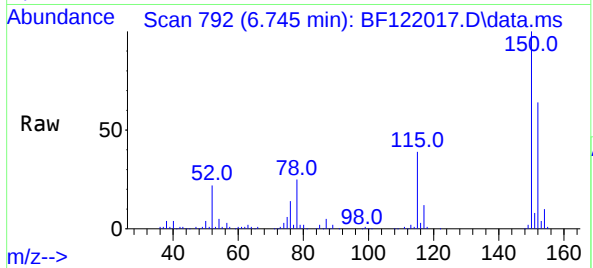

#5
2-Fluorophenol
Concen: 110.04 ng
RT: 5.381 min Scan# 560
Delta R.T. 0.018 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion:112 Resp: 830902
Ion Ratio Lower Upper
112 100
64 62.9 50.4 75.6
63 32.1 25.8 38.6


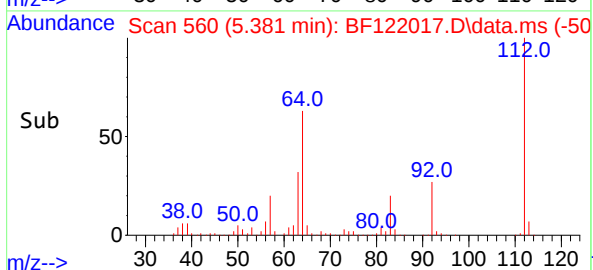
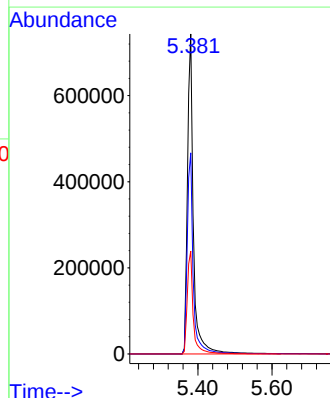
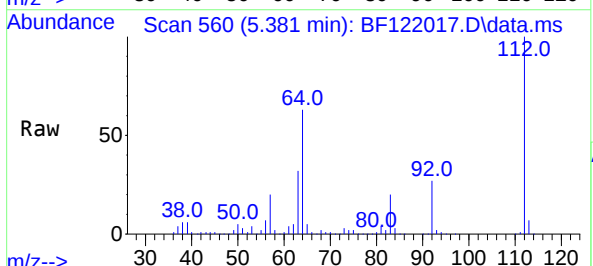




#7
Phenol-d6
Concen: 99.96 ng
RT: 6.393 min Scan# 732
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19




Tgt Ion: 99 Resp: 971620
Ion Ratio Lower Upper
99 100
42 20.8 15.9 23.9
71 35.8 27.1 40.7


Instrument :
BNA_F
ClientSampleId :
PL-01-101420

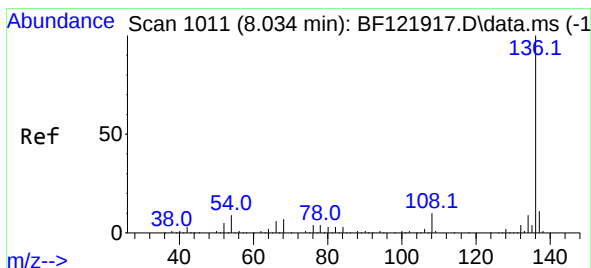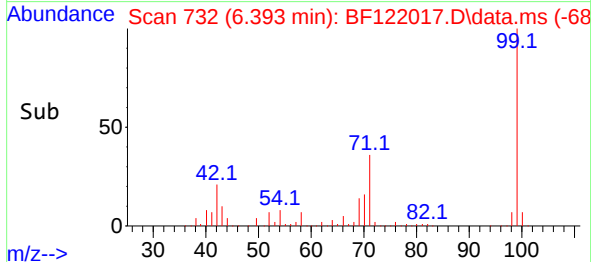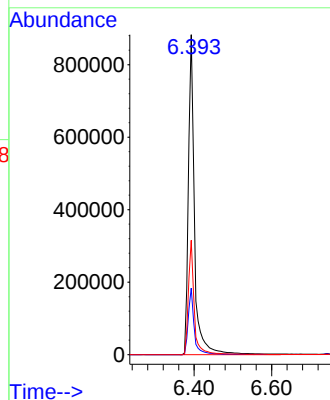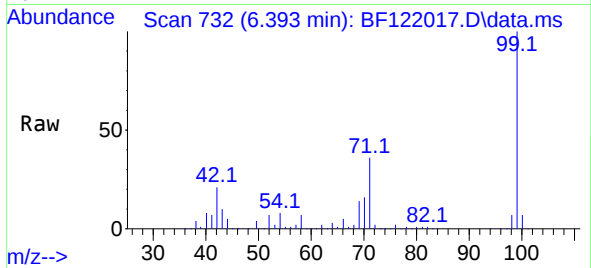

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.028 min Scan# 1010
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion: 136 Resp: 433953
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 8.3 7.1 10.7
68 6.0 5.0 7.4


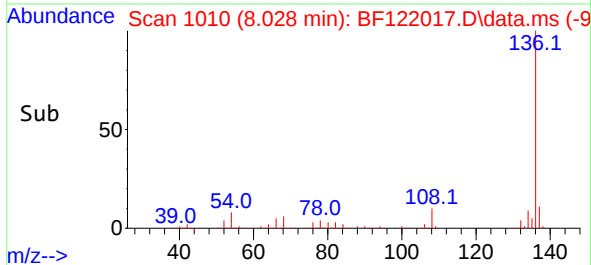
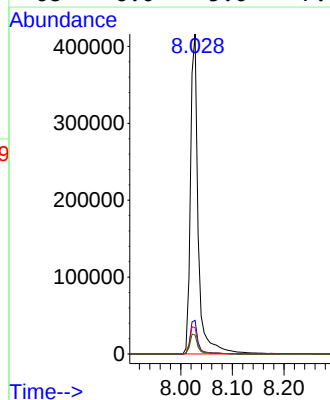
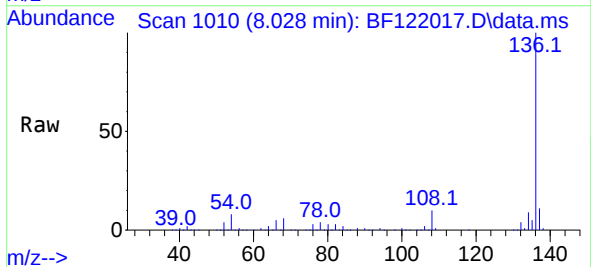


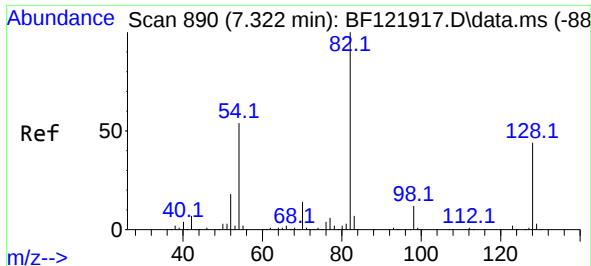

#23
Nitrobenzene-d5
Concen: 91.94 ng
RT: 7.316 min Scan# 889
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19




Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Tgt Ion: 82 Resp: 777984
Ion Ratio Lower Upper
82 100
128 44.7 35.0 52.4
54 52.8 43.9 65.9

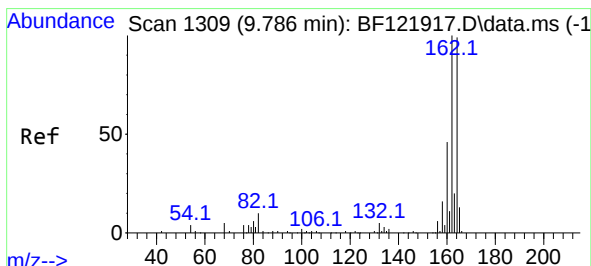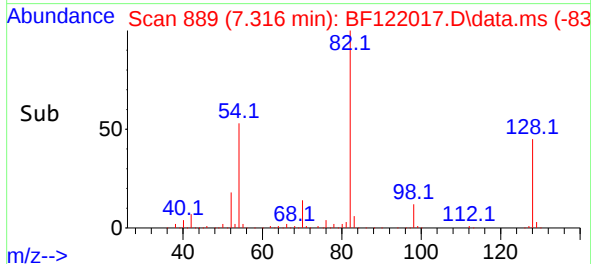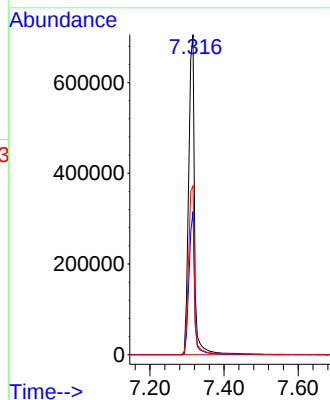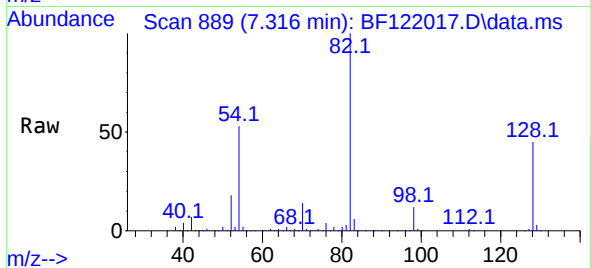

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.775 min Scan# 1307
Delta R.T. -0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion: 164 Resp: 207985
Ion Ratio Lower Upper
164 100
162 104.1 83.2 124.8
160 47.1 37.5 56.3


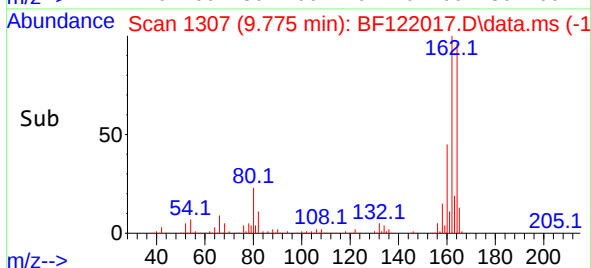
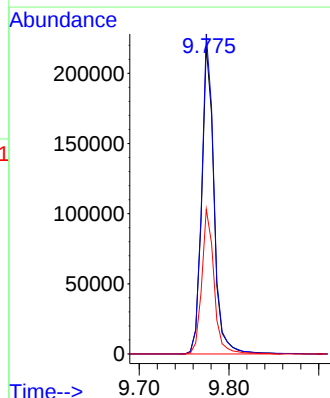
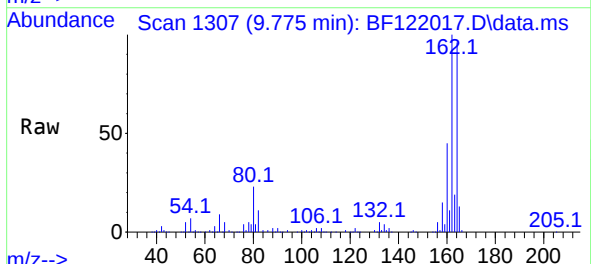




#42
2,4,6-Tribromophenol
Concen: 119.17 ng
RT: 10.569 min Scan# 1442
Delta R.T. -0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19




Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Tgt Ion:330 Resp: 306597
Ion Ratio Lower Upper
330 100
332 96.1 77.3 115.9
141 28.7 22.3 33.5

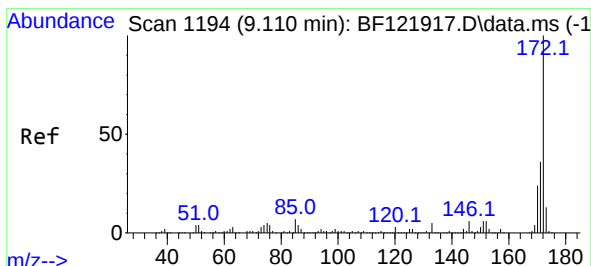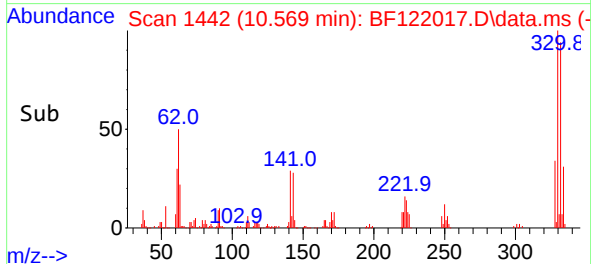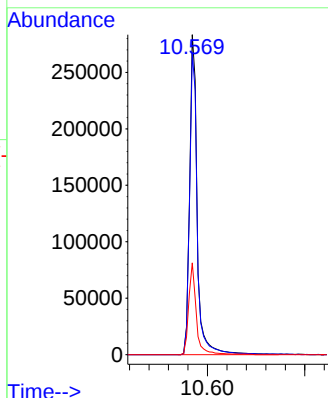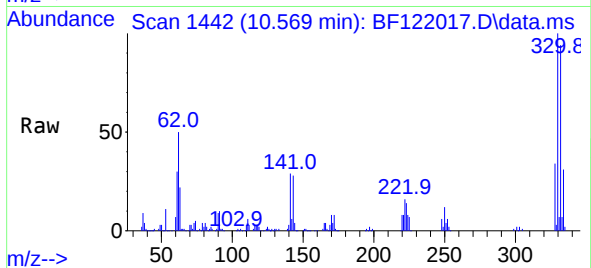

#45
2-Fluorobiphenyl
Concen: 88.82 ng
RT: 9.104 min Scan# 1193
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion:172 Resp: 1255570
Ion Ratio Lower Upper
172 100
171 36.2 29.1 43.7
170 24.1 19.8 29.6

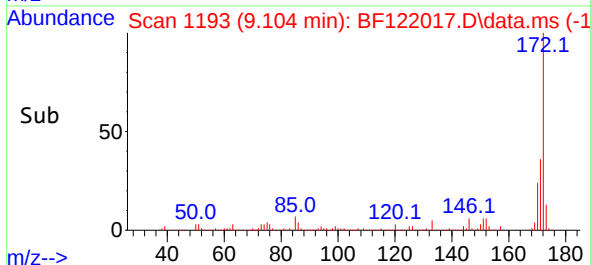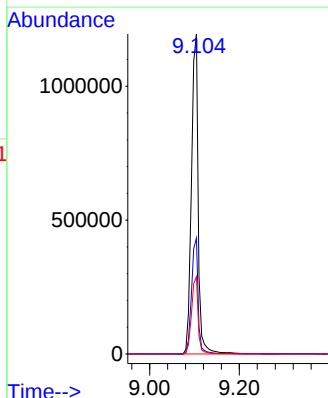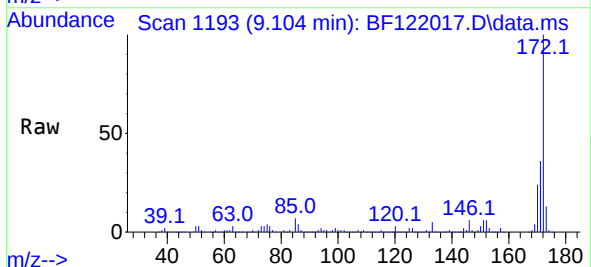







#50
Dimethylphthalate
Concen: 4.78 ng
RT: 9.498 min Scan# 1260
Delta R.T. -0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Tgt Ion:163 Resp: 72758




Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.3	4.9
164	10.1	8.2	12.4

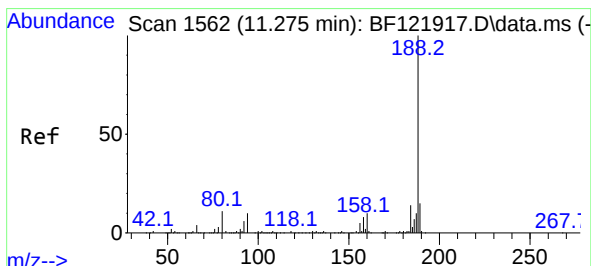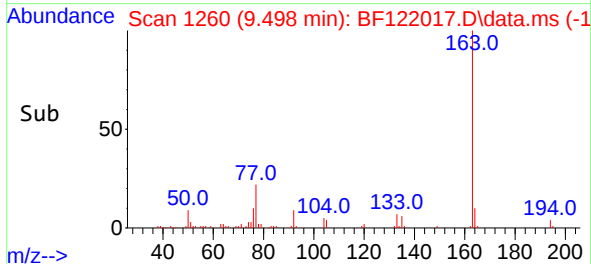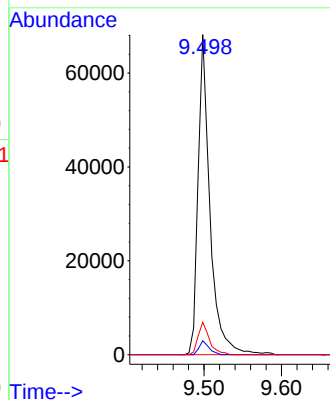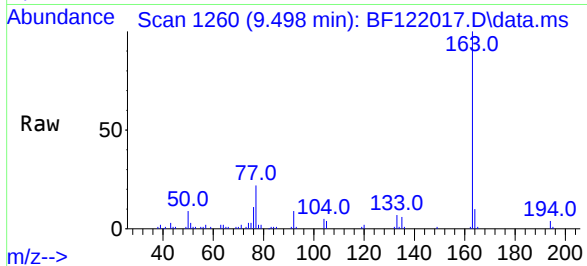


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.263 min Scan# 1560
Delta R.T. 0.000 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion:188 Resp: 338197

Ion	Ratio	Lower	Upper
188	100		
94	10.2	8.3	12.5
80	11.1	9.1	13.7


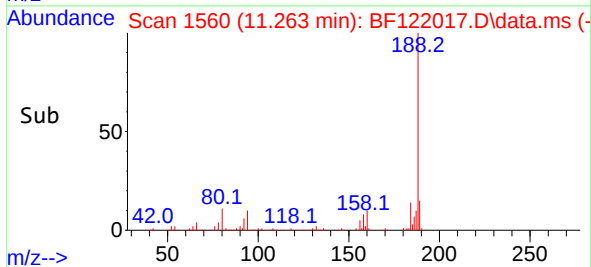
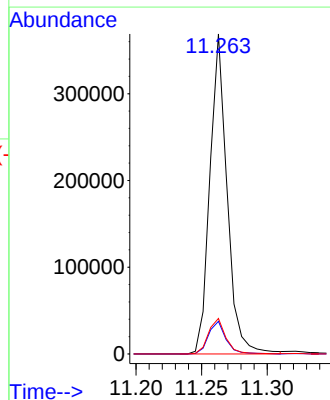
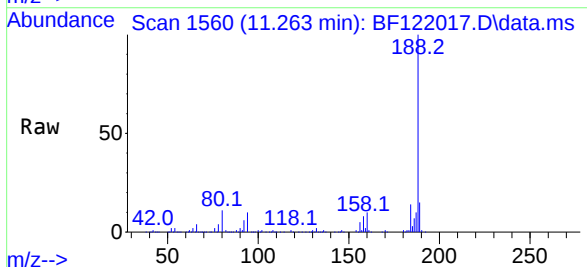


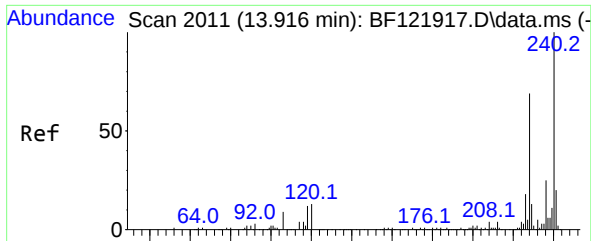

#76
Chrysene-d12
Concen: 20.00 ng
RT: 13.904 min Scan# 2009
Delta R.T. -0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19




Instrument :
BNA_F
ClientSampleId :
PL-01-101420


Tgt Ion:240 Resp: 243387
Ion Ratio Lower Upper
240 100
120 11.6 9.2 13.8
236 25.3 20.9 31.3

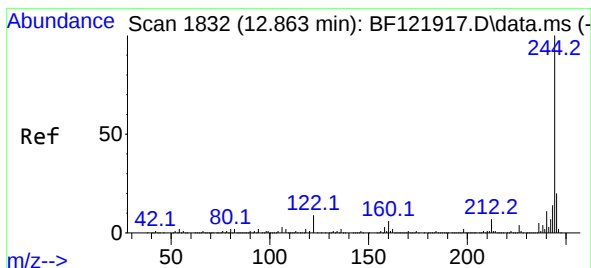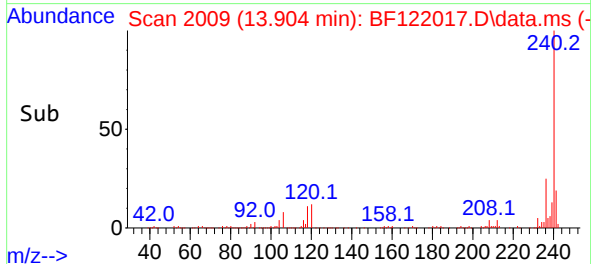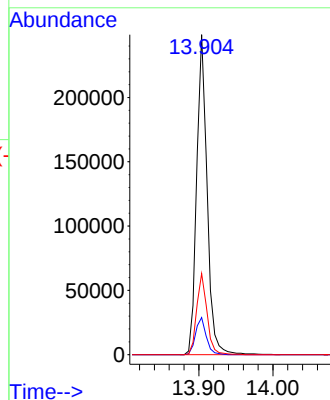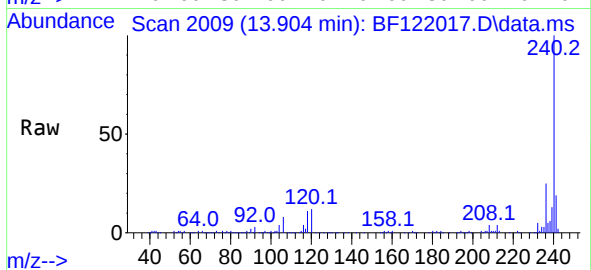

#79
Terphenyl-d14
Concen: 81.75 ng
RT: 12.845 min Scan# 1829
Delta R.T. -0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Tgt Ion:244 Resp: 1044001
Ion Ratio Lower Upper
244 100
212 7.2 5.4 8.2
122 11.6 8.1 12.1

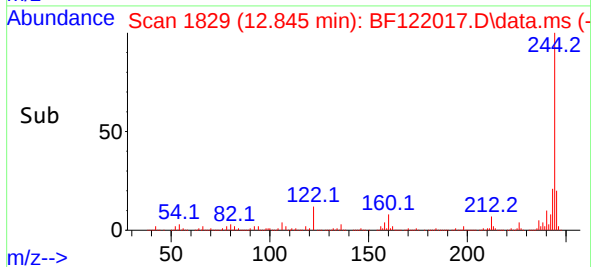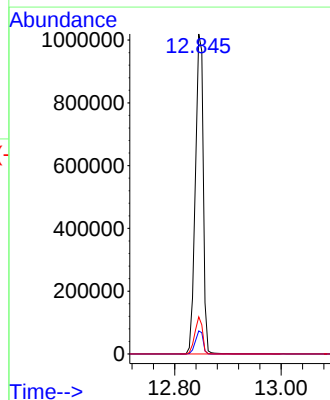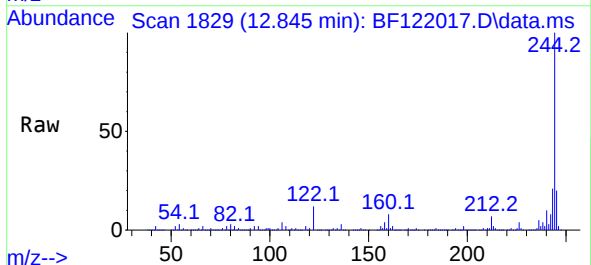

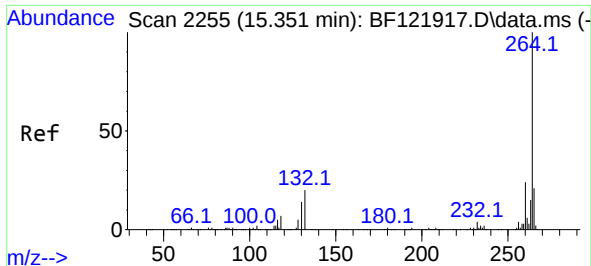

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.345 min Scan# 2254
Delta R.T. 0.006 min
Lab File: BF122017.D
Acq: 16 Oct 2020 18:19

Instrument :
BNA_F
ClientSampleId :
PL-01-101420

Tgt Ion:264 Resp: 246833
Ion Ratio Lower Upper
264 100
260 23.6 18.7 28.1
265 21.5 17.3 25.9

