

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
 Data File : BF122014.D
 Acq On : 16 Oct 2020 16:45
 Operator : JU/CG
 Sample : L4224-06 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-03-101520

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	554	557	577	rBV	225934	384049	40.78%	4.182%
2	6.393	729	732	755	rBV	228443	413539	43.91%	4.504%
3	6.740	788	791	808	rBV	711282	685965	72.83%	7.470%
4	7.310	885	888	905	rBV	215947	283674	30.12%	3.089%
5	8.028	1006	1010	1035	rBV	822984	897534	95.29%	9.774%
6	8.751	1130	1133	1139	rBV	8030	10407	1.10%	0.113%
7	8.845	1145	1149	1155	rVB	8010	10432	1.11%	0.114%
8	9.098	1189	1192	1204	rBV	492554	525566	55.80%	5.724%
9	9.439	1247	1250	1253	rBV	9546	10784	1.14%	0.117%
10	9.504	1258	1261	1268	rVB	45441	58122	6.17%	0.633%
11	9.639	1281	1284	1289	rVB	10620	9863	1.05%	0.107%
12	9.775	1303	1307	1322	rBV	872132	941870	100.00%	10.257%
13	9.992	1336	1344	1347	rBV2	10337	14841	1.58%	0.162%
14	10.328	1398	1401	1407	rBV	31237	33929	3.60%	0.369%
15	10.575	1439	1443	1453	rBV	138542	165294	17.55%	1.800%
16	10.686	1457	1462	1465	rBV3	7598	12389	1.32%	0.135%
17	10.875	1487	1494	1497	rBV2	8587	11385	1.21%	0.124%
18	11.163	1538	1543	1547	rVB3	14066	16172	1.72%	0.176%
19	11.263	1556	1560	1562	rBV	893940	765084	81.23%	8.332%
20	11.286	1562	1564	1571	rVV	219243	211649	22.47%	2.305%
21	11.339	1571	1573	1577	rVB	43652	42022	4.46%	0.458%
22	11.510	1597	1602	1606	rBV2	12941	16395	1.74%	0.179%
23	11.769	1640	1646	1648	rBV	30158	33820	3.59%	0.368%
24	11.792	1648	1650	1656	rVV	44747	51185	5.43%	0.557%
25	11.845	1656	1659	1661	rVV	13198	14442	1.53%	0.157%
26	11.874	1661	1664	1667	rVV	50545	57410	6.10%	0.625%
27	11.898	1667	1668	1674	rVB	21900	19658	2.09%	0.214%
28	12.057	1692	1695	1699	rBV	15338	16785	1.78%	0.183%
29	12.104	1700	1703	1706	rVB4	9272	9896	1.05%	0.108%
30	12.310	1736	1738	1741	rBV	24034	25388	2.70%	0.276%
31	12.351	1741	1745	1747	rVV4	16144	23318	2.48%	0.254%
32	12.410	1751	1755	1758	rVB3	11480	15047	1.60%	0.164%
33	12.474	1763	1766	1772	rBV	234946	207073	21.99%	2.255%
34	12.574	1780	1783	1789	rBV3	25917	32042	3.40%	0.349%
35	12.627	1789	1792	1794	rVV	12185	10415	1.11%	0.113%
36	12.704	1799	1805	1811	rVV	234058	254156	26.98%	2.768%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
 Data File : BF122014.D
 Acq On : 16 Oct 2020 16:45
 Operator : JU/CG
 Sample : L4224-06 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-03-101520

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	12.757	1811	1814	1818	rVV2	12583	13381	1.42%	0.146%
38	12.839	1825	1828	1833	rBV	436914	407481	43.26%	4.438%
39	12.927	1838	1843	1847	rBV5	18445	33139	3.52%	0.361%
40	12.980	1847	1852	1854	rBV6	8564	12156	1.29%	0.132%
41	13.010	1854	1857	1858	rBV3	18465	17718	1.88%	0.193%
42	13.033	1859	1861	1864	rVB	34476	27396	2.91%	0.298%
43	13.098	1870	1872	1875	rBV	26056	21384	2.27%	0.233%
44	13.139	1875	1879	1884	rVV2	29544	37995	4.03%	0.414%
45	13.227	1891	1894	1897	rBV	21189	23352	2.48%	0.254%
46	13.263	1897	1900	1902	rBV	21266	18411	1.95%	0.200%
47	13.410	1922	1925	1928	rBV5	12235	14939	1.59%	0.163%
48	13.551	1947	1949	1952	rVB	15674	13086	1.39%	0.143%
49	13.657	1964	1967	1968	rBV	18310	13632	1.45%	0.148%
50	13.704	1973	1975	1978	rBV	14015	16556	1.76%	0.180%
51	13.904	2004	2009	2012	rBV2	777295	845651	89.78%	9.209%
52	13.927	2012	2013	2017	rVB	110662	81484	8.65%	0.887%
53	14.010	2025	2027	2030	rVB	15431	14007	1.49%	0.153%
54	14.292	2070	2075	2079	rBV	34503	58864	6.25%	0.641%
55	14.933	2180	2184	2186	rBV	99959	123536	13.12%	1.345%
56	15.221	2230	2233	2237	rVB	64280	72434	7.69%	0.789%
57	15.280	2240	2243	2248	rBV	94181	103166	10.95%	1.124%
58	15.339	2249	2253	2258	rBV	596022	740467	78.62%	8.064%
59	15.974	2358	2361	2370	rVB6	41844	71727	7.62%	0.781%
60	16.762	2491	2495	2502	rVB3	50446	108983	11.57%	1.187%




Sum of corrected areas: 9182545

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122014.D
Acq On : 16 Oct 2020 16:45
Operator : JU/CG
Sample : L4224-06 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-03-101520

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

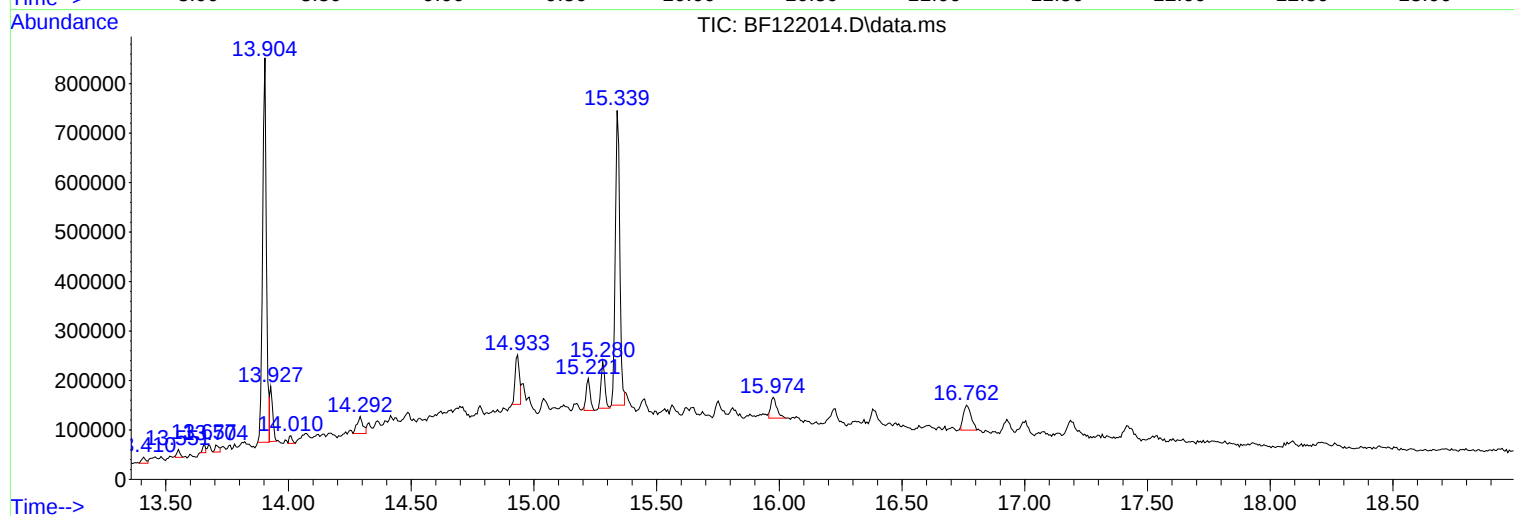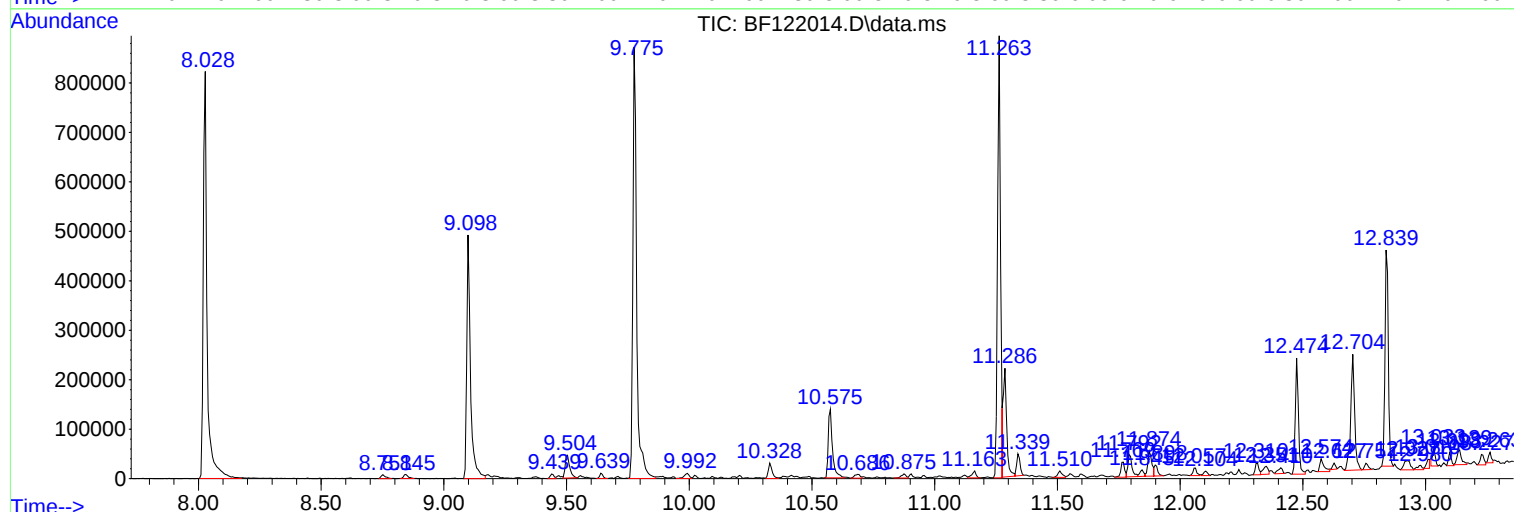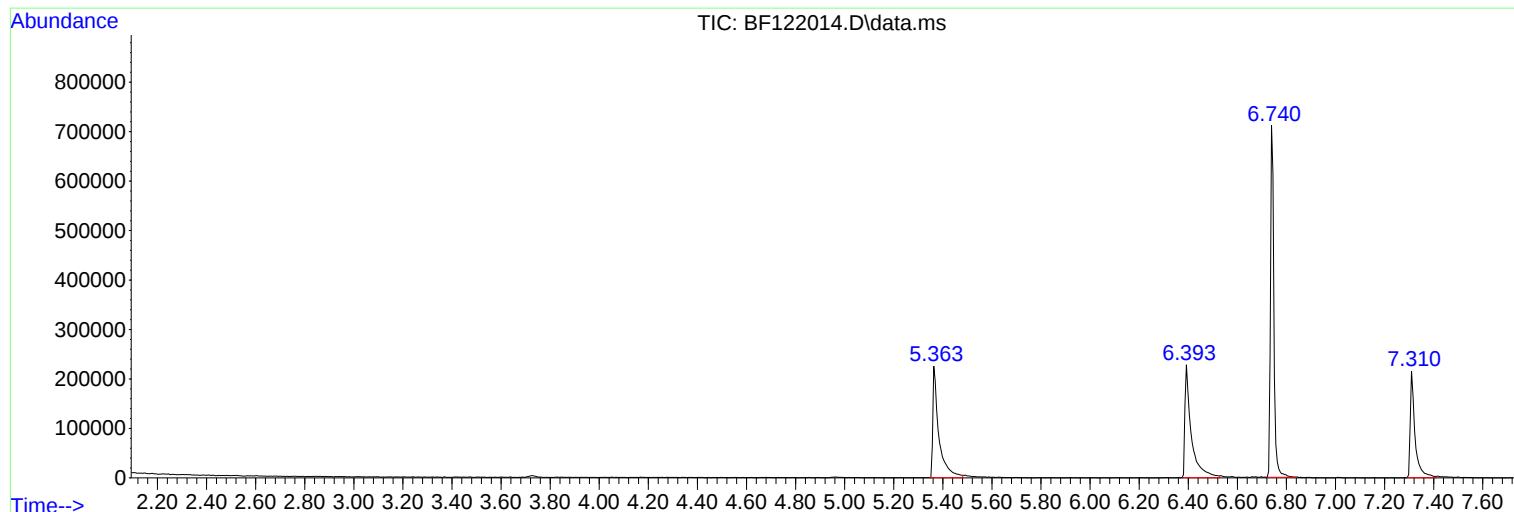

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122014.D
Acq On : 16 Oct 2020 16:45
Operator : JU/CG
Sample : L4224-06 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-03-101520

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
Data File : BF122014.D
Acq On : 16 Oct 2020 16:45
Operator : JU/CG
Sample : L4224-06 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-03-101520

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc