
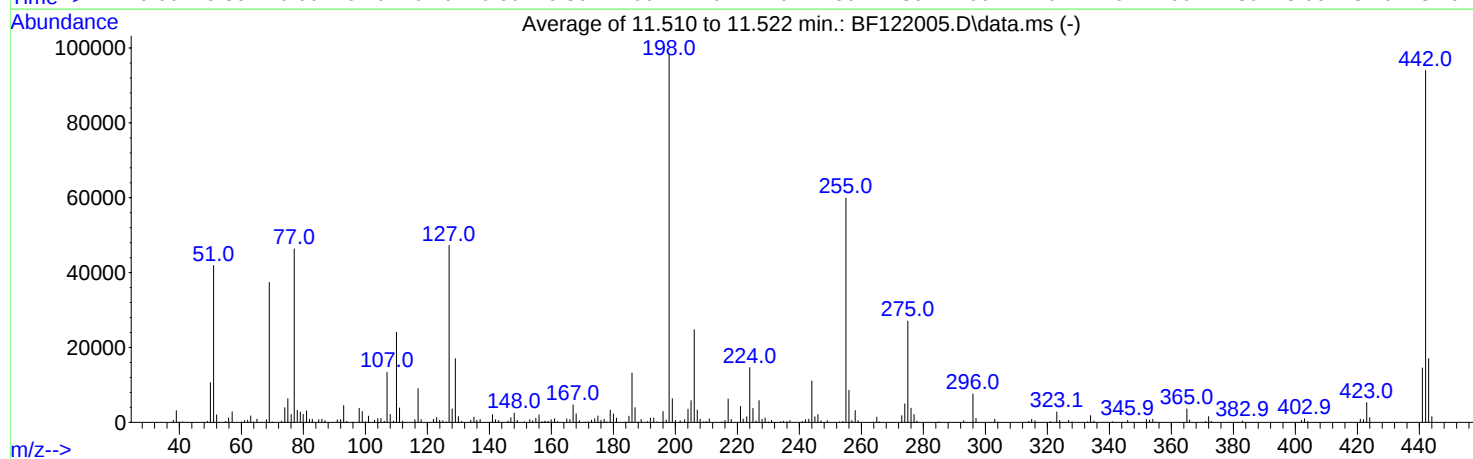


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101620\
 Data File : BF122005.D
 Acq On : 16 Oct 2020 10:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 15 12:55:05 2020

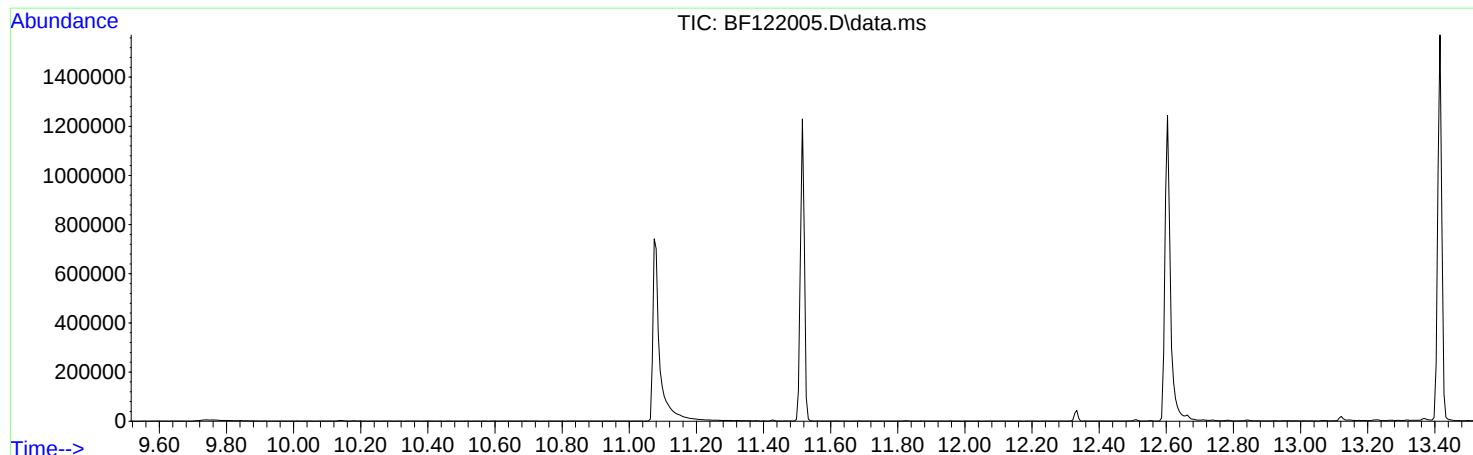

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	41883	PASS
68	69	0.00	2	2.0	732	PASS
69	198	0.00	100	38.0	37355	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	48.1	47256	PASS
197	198	0.00	2	0.6	601	PASS
198	198	100	100	100.0	98267	PASS
199	198	5	9	6.5	6348	PASS
275	198	10	60	27.6	27077	PASS
365	198	1	100	3.7	3609	PASS
441	198	0.01	100	14.8	14547	PASS
442	198	50	100	95.6	93976	PASS
443	442	15	24	18.1	17019	PASS