
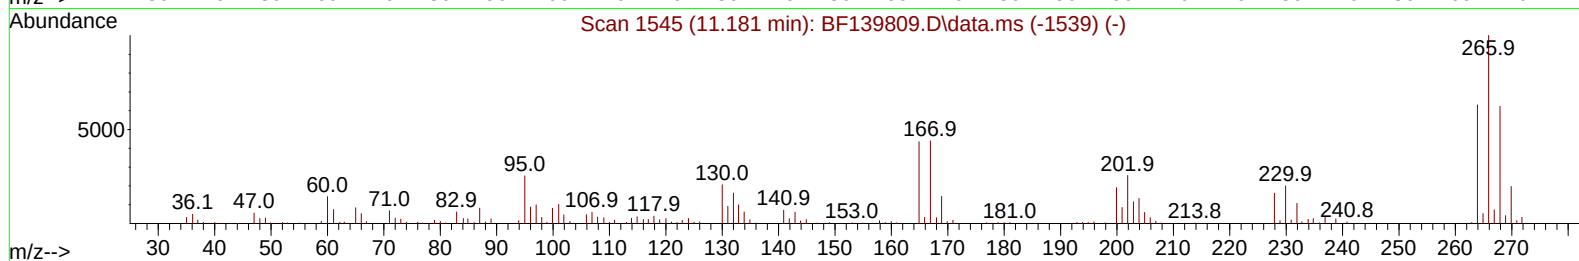
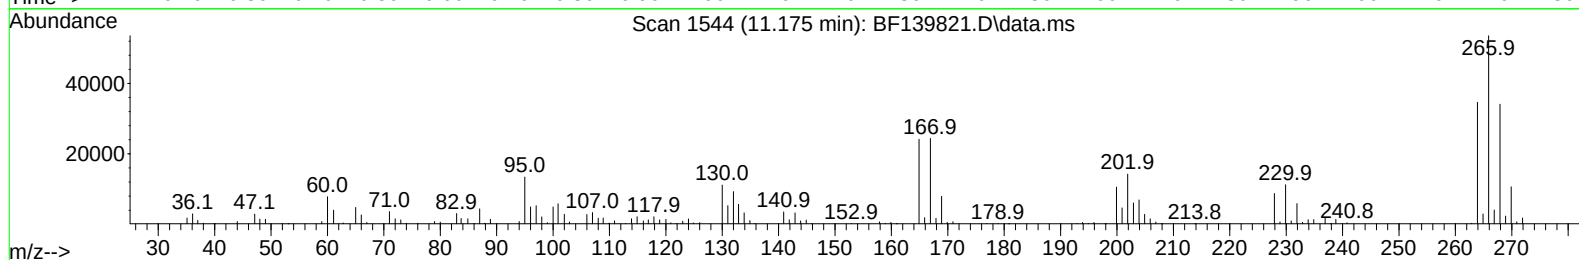


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101624\
Data File : BF139821.D
Acq On : 16 Oct 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 11:28:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 16:41:54 2024
Response via : Initial Calibration

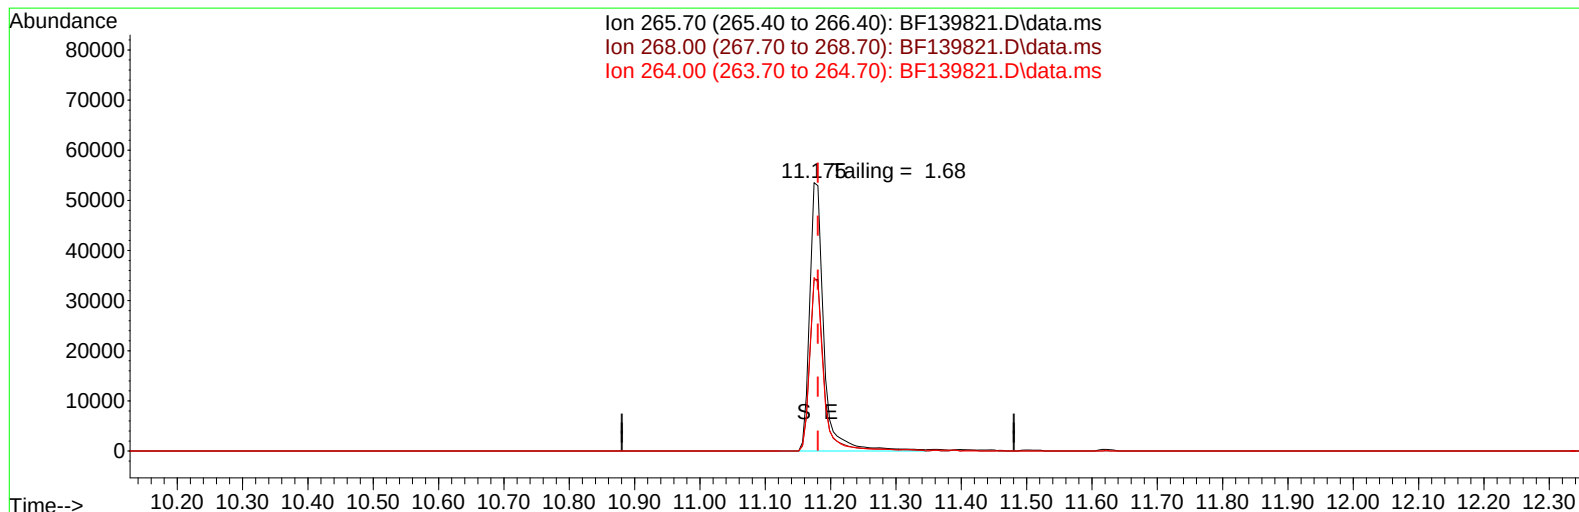

TIC: BF139821.D\data.ms

(70) Pentachlorophenol (C)




11.175min (-0.006) 29604.25 ng

response 81174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.72
264.00	63.10	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101624\
Data File : BF139821.D
Acq On : 16 Oct 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 16 11:28:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 16:41:54 2024
Response via : Initial Calibration

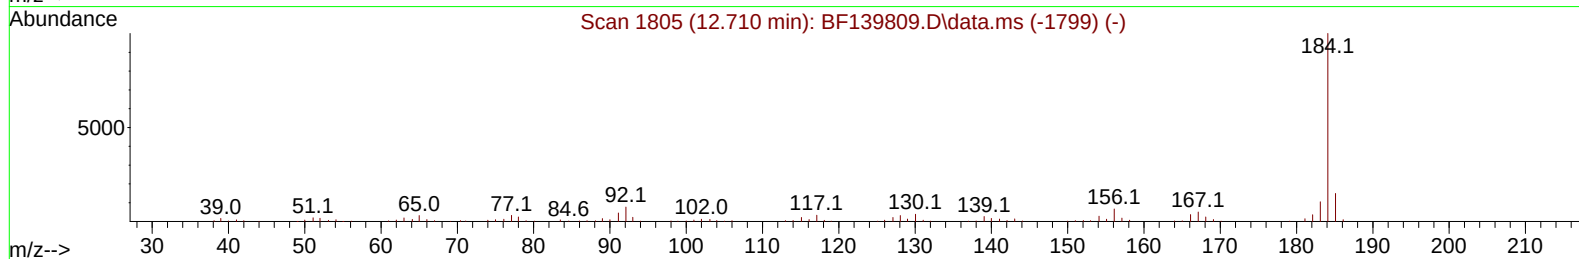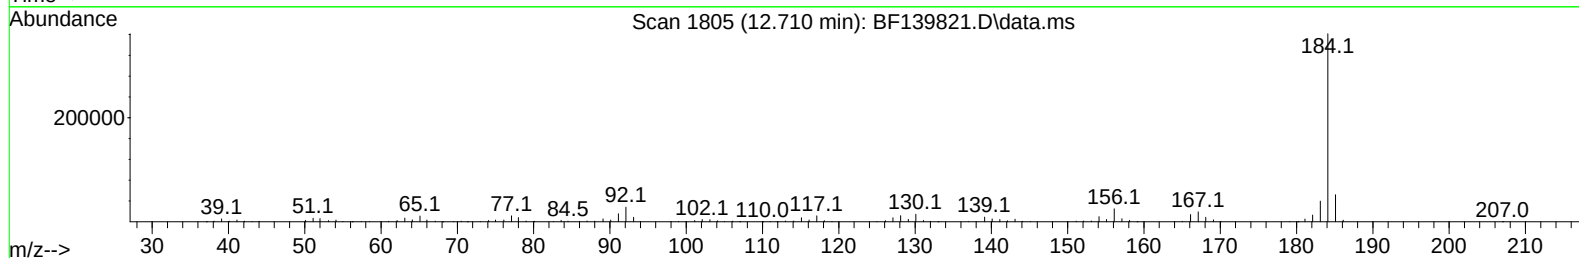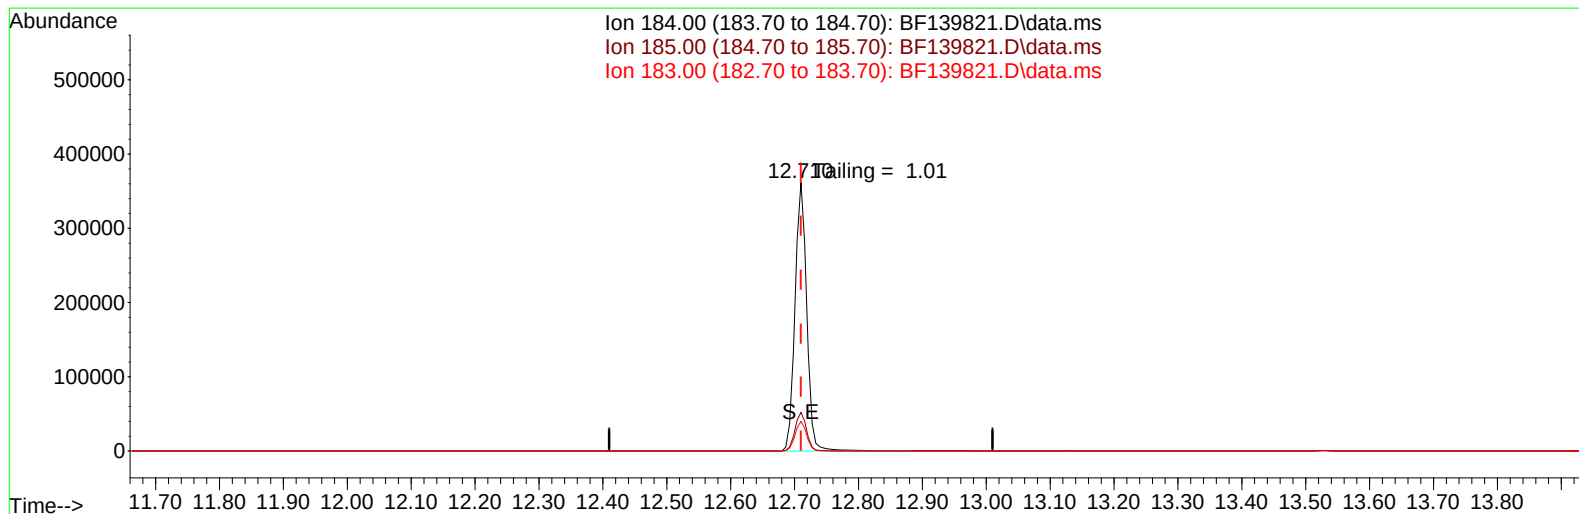

TIC: BF139821.D\data.ms

(77) Benzidine

12.710min (-0.000) 0.00 ng

response 464790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.44
183.00	10.50	11.03
0.00	0.00	0.00