


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101624\
Data File : BF139821.D
Acq On : 16 Oct 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 15 16:41:54 2024

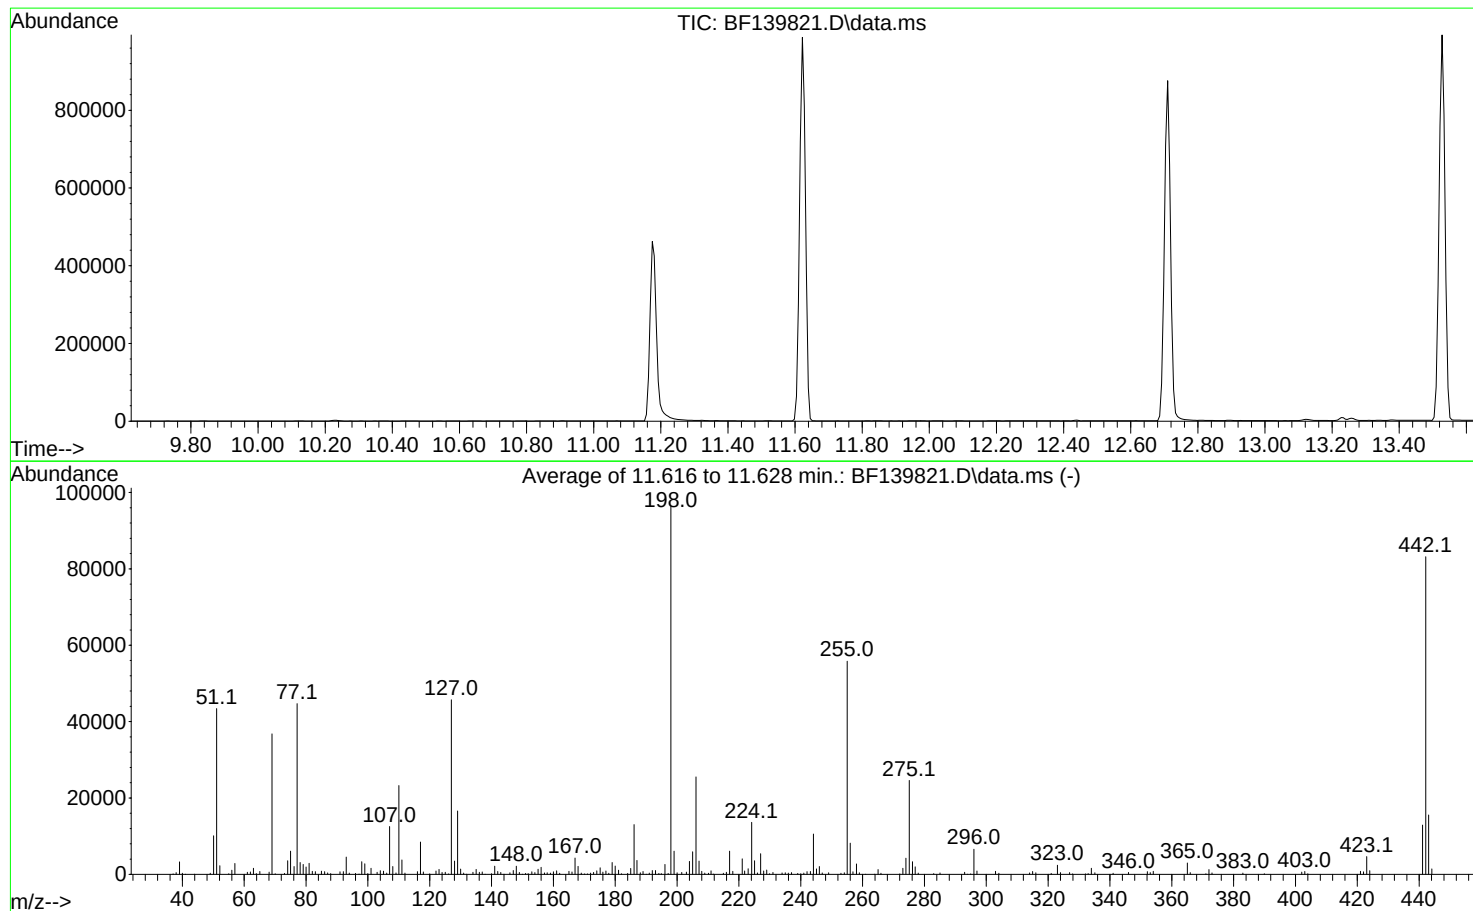




AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	43408	PASS
68	69	0.00	2	1.6	603	PASS
69	198	0.00	100	38.2	36776	PASS
70	69	0.00	2	0.5	177	PASS
127	198	10	80	47.5	45715	PASS
197	198	0.00	2	0.3	249	PASS
198	198	100	100	100.0	96328	PASS
199	198	5	9	6.3	6081	PASS
275	198	10	60	25.5	24592	PASS
365	198	1	100	3.1	2972	PASS
441	198	0.01	100	13.4	12913	PASS
442	442	50	100	100.0	83160	PASS
443	442	15	24	18.7	15566	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101624\
Data File : BF139821.D
Acq On : 16 Oct 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 11:28:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 16:41:54 2024
Response via : Initial Calibration

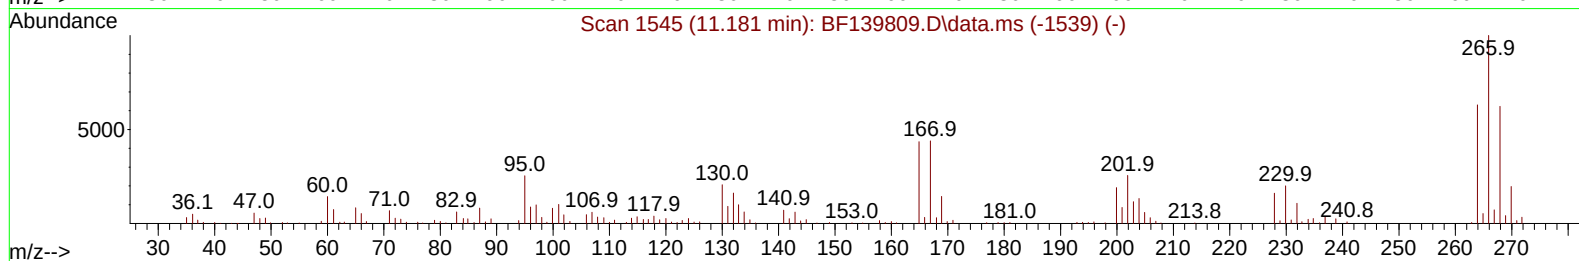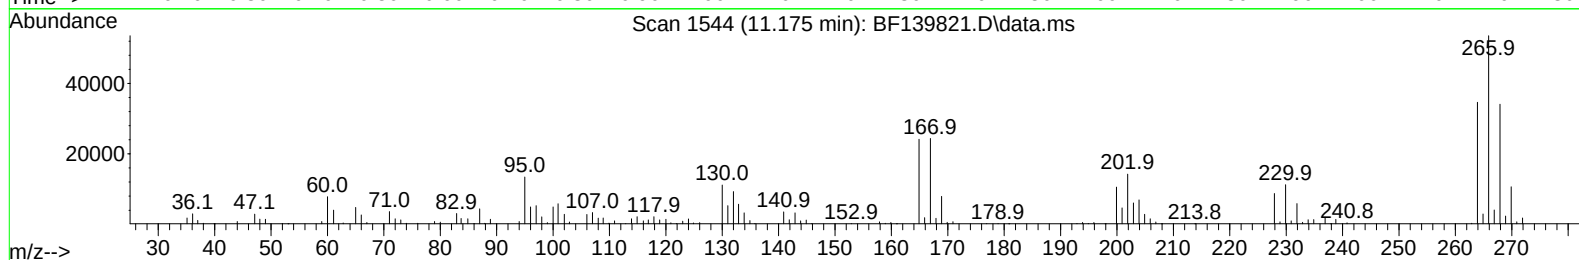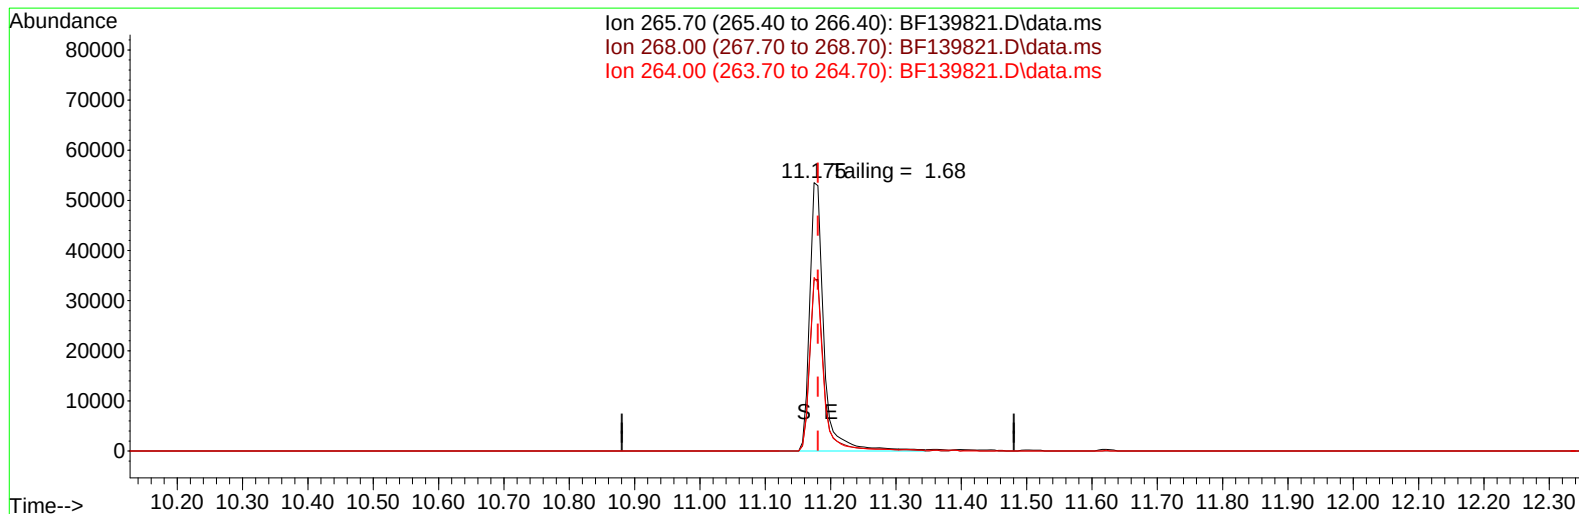

TIC: BF139821.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.006) 29604.25 ng




response 81174

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.72
264.00	63.10	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101624\
Data File : BF139821.D
Acq On : 16 Oct 2024 10:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 11:28:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 15 16:41:54 2024
Response via : Initial Calibration

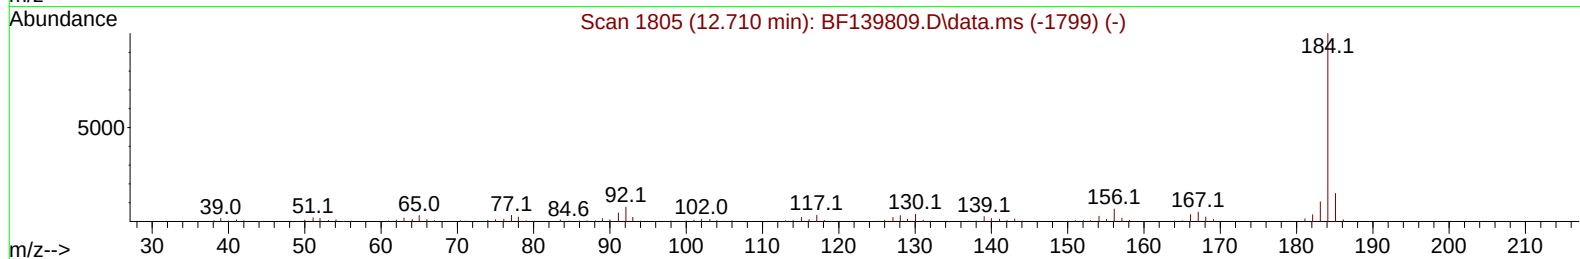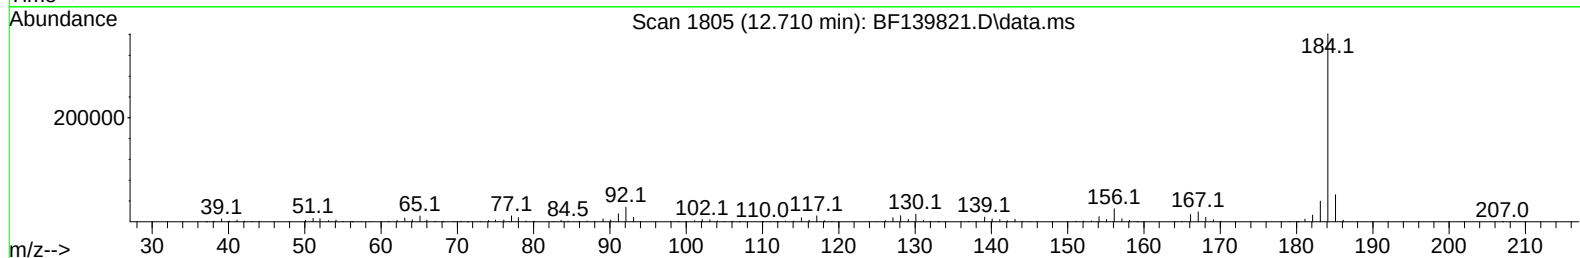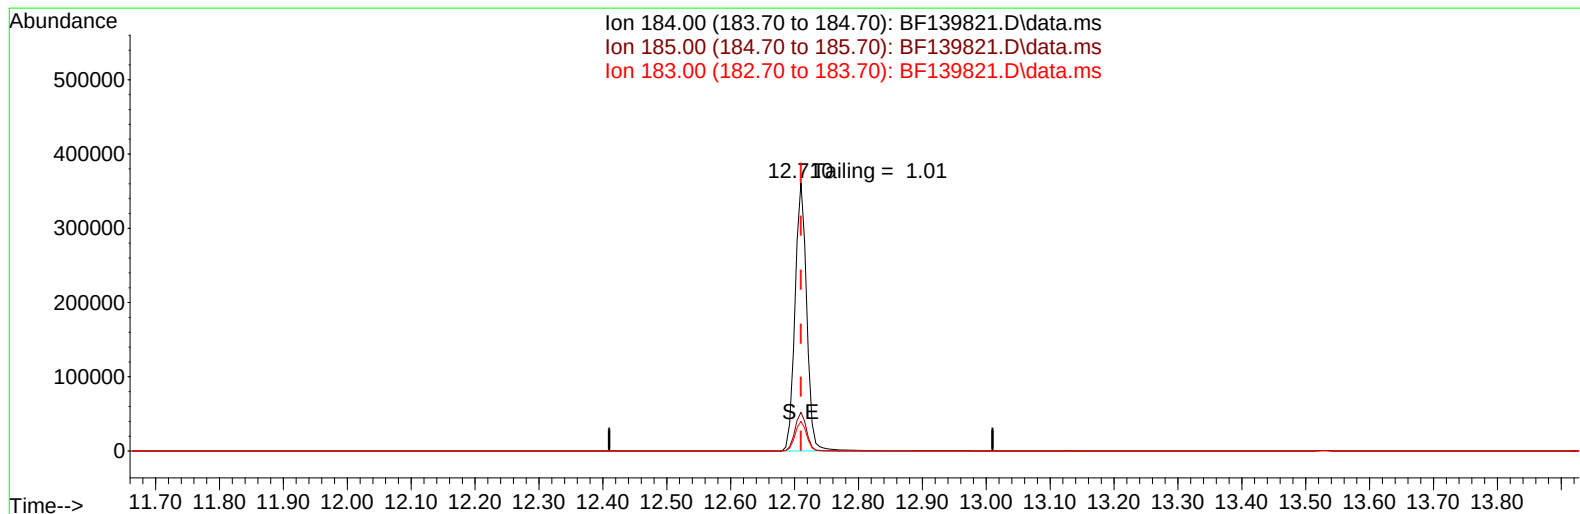

TIC: BF139821.D\data.ms

(77) Benzidine

12.710min (-0.000) 0.00 ng

response 464790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.44
183.00	10.50	11.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2024	BNA_F	<u>BF139821.D</u>
Compound Name	Response	Retention Time
DDT	243003	13.527
DDD	5636	13.227
DDE	431	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6067	249070	2.44

Instrument :
BNA_F
ClientSampleId :
DFTPP