

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143976.D
Acq On : 16 Oct 2025 13:14
Operator : RC/JU
Sample : PB170122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170122BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.128	489	499	508	rBV	36935	61763	1.68%	0.262%
2	5.504	557	563	582	rBV	2331085	3323592	90.19%	14.124%
3	6.504	727	733	739	rBV	2237245	3389068	91.96%	14.403%
4	6.881	792	797	802	rBV	565164	692237	18.78%	2.942%
5	7.440	886	892	911	rBV	1496789	2199817	59.69%	9.349%
6	8.163	1009	1015	1034	rBV	695091	920288	24.97%	3.911%
7	9.239	1192	1198	1209	rBV	2652435	3685280	100.00%	15.661%
8	9.922	1308	1314	1328	rBV	809256	1038023	28.17%	4.411%
9	10.716	1443	1449	1470	rBV	1704358	2320129	62.96%	9.860%
10	11.416	1562	1568	1575	rBV	776190	1032415	28.01%	4.387%
11	13.004	1832	1838	1844	rBV	2669089	3635598	98.65%	15.450%
12	14.063	2013	2018	2030	rBV	477275	657773	17.85%	2.795%
13	15.551	2265	2271	2291	rVB	301687	574892	15.60%	2.443%




Sum of corrected areas: 23530875

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143976.D
Acq On : 16 Oct 2025 13:14
Operator : RC/JU
Sample : PB170122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170122BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

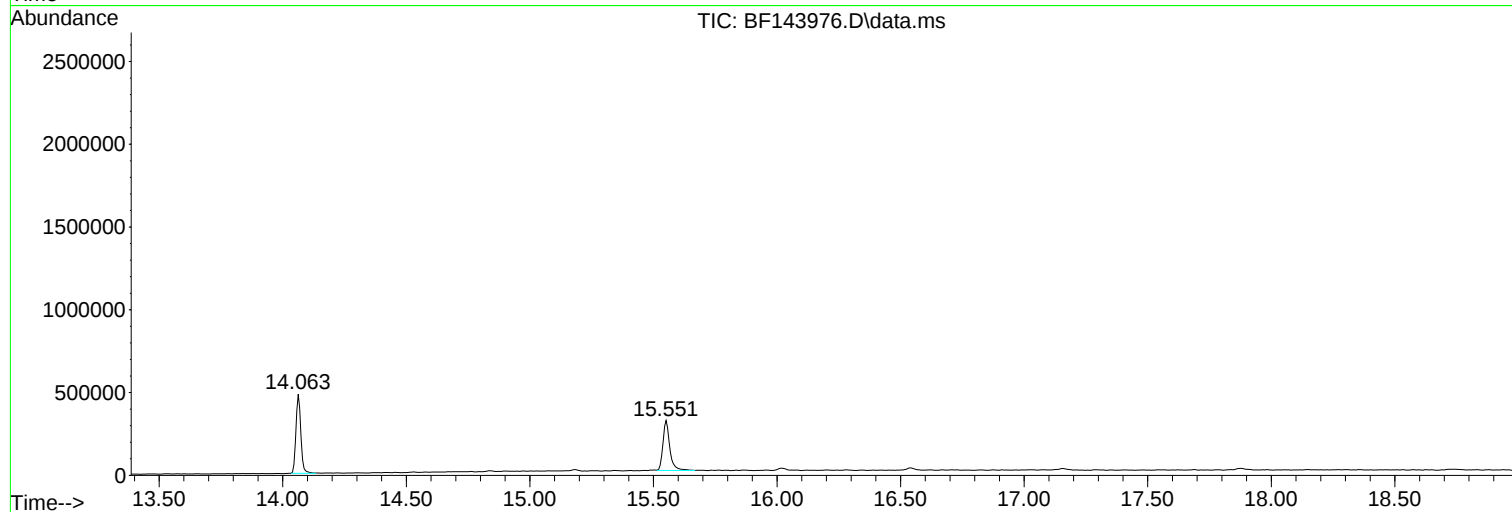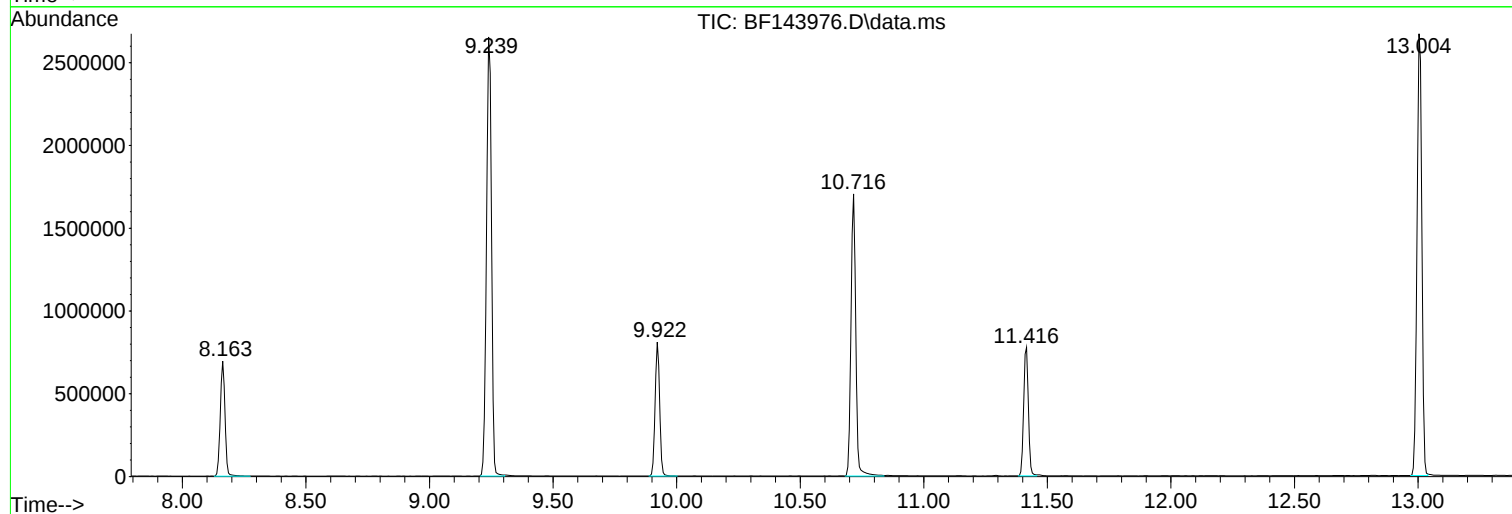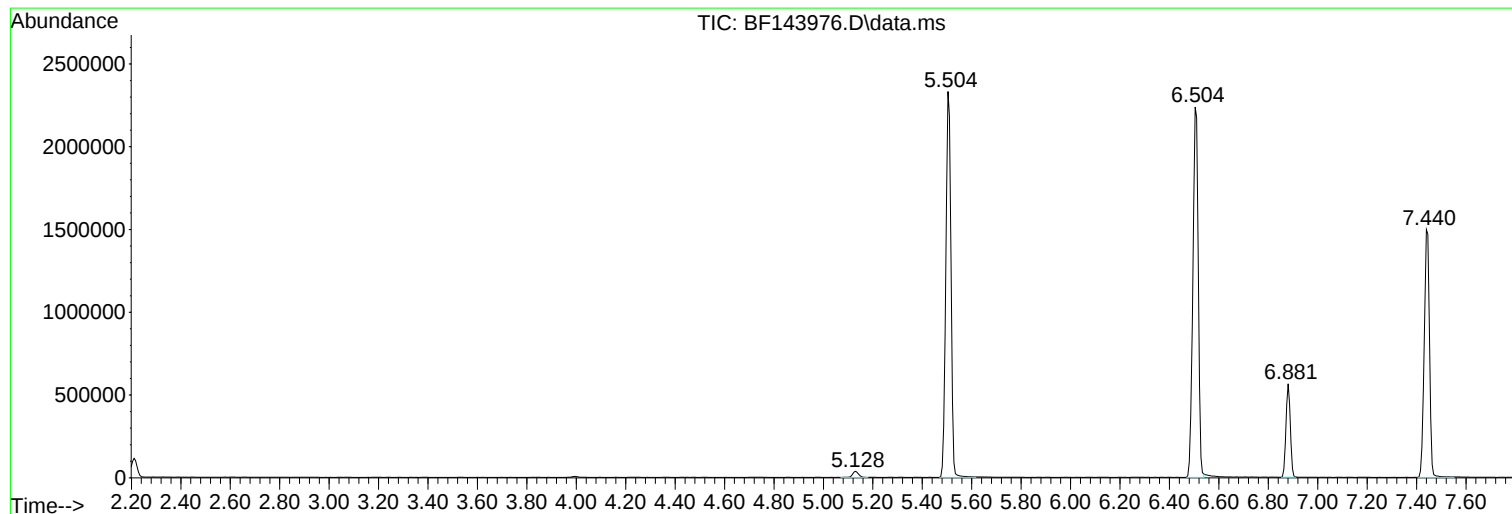

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143976.D
Acq On : 16 Oct 2025 13:14
Operator : RC/JU
Sample : PB170122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170122BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143976.D
Acq On : 16 Oct 2025 13:14
Operator : RC/JU
Sample : PB170122BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB170122BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------