


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143973.D
Acq On : 16 Oct 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 06 15:29:47 2025

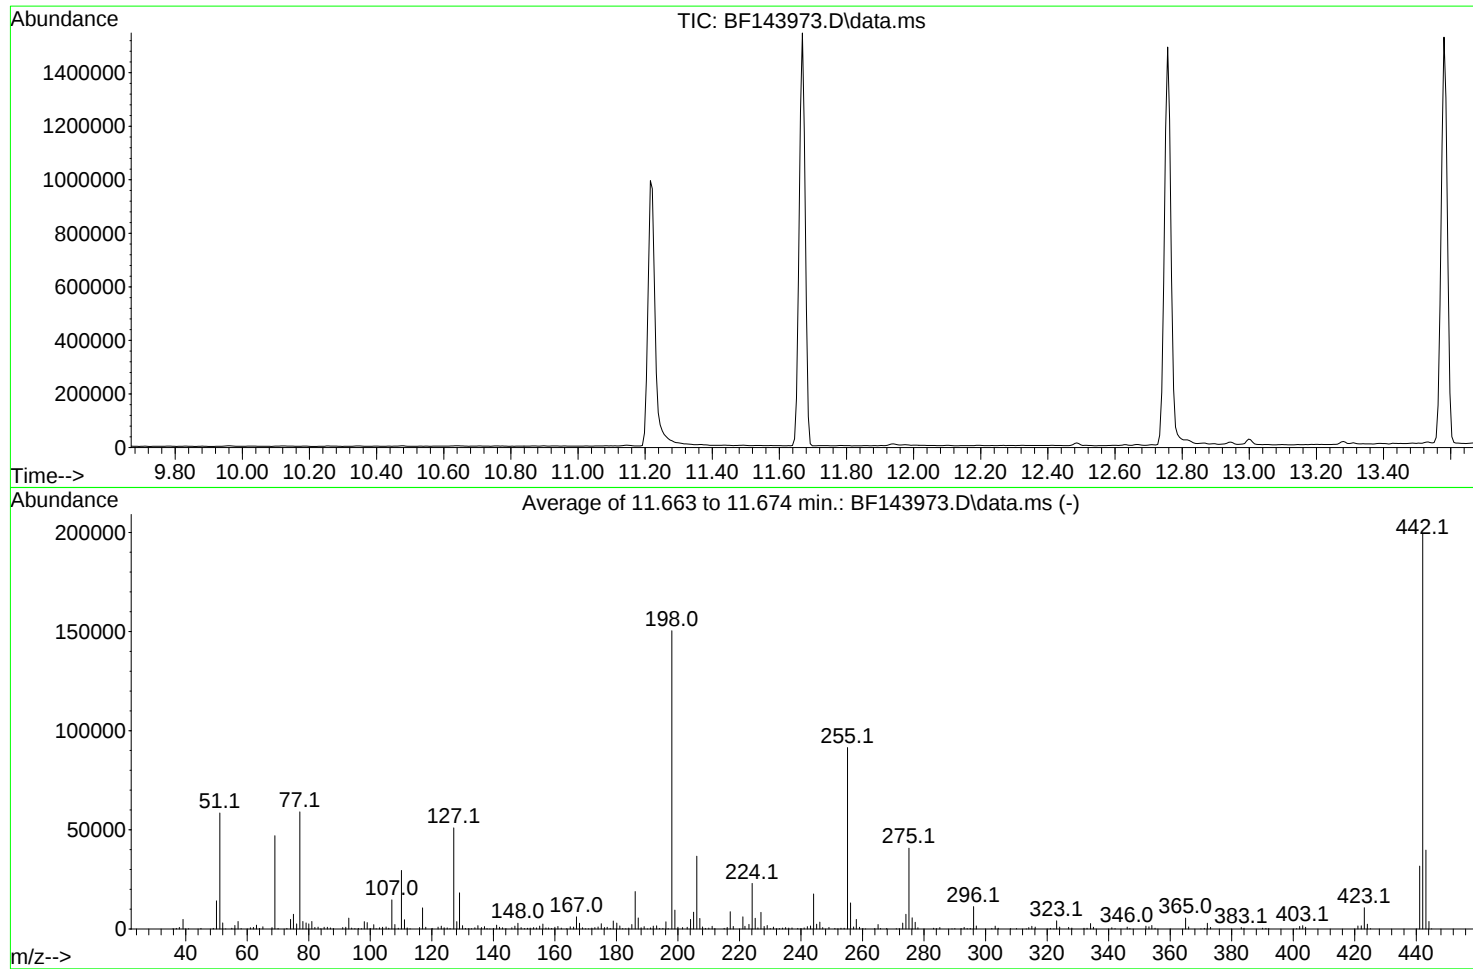




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	674	PASS
69	69	100	100	100.0	47061	PASS
70	69	0.00	2	0.6	295	PASS
197	198	0.00	2	0.1	181	PASS
198	198	100	100	100.0	150408	PASS
199	198	5	9	6.3	9452	PASS
365	198	1	100	3.6	5445	PASS
441	443	0.01	150	79.7	31669	PASS
442	442	100	100	100.0	199168	PASS
443	442	15	24	19.9	39733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143973.D
Acq On : 16 Oct 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 14:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

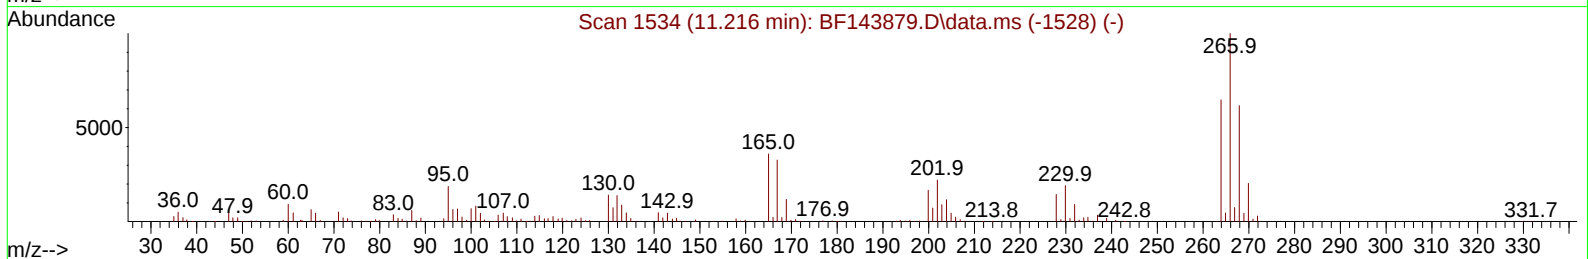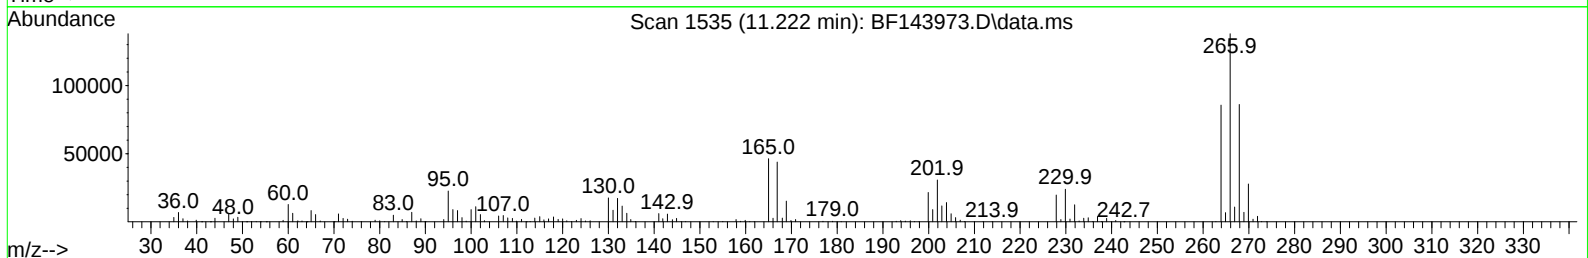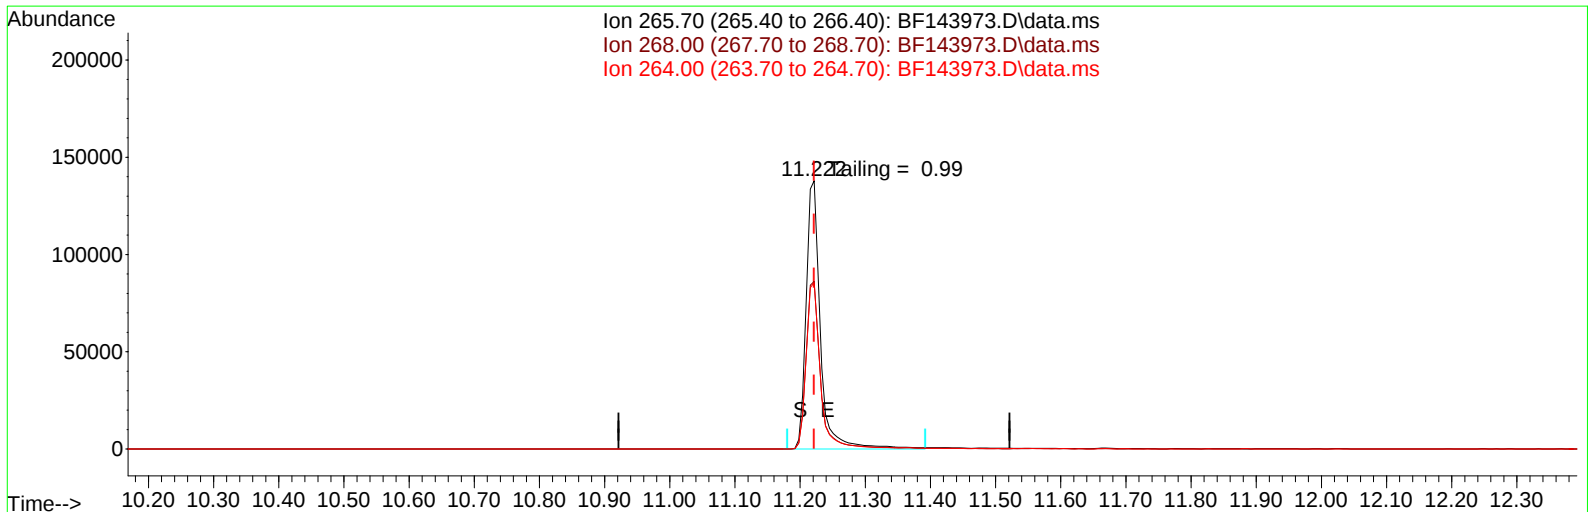

TIC: BF143973.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 33792.17 ng




response 211066

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	62.44
264.00	64.70	62.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101625\
Data File : BF143973.D
Acq On : 16 Oct 2025 10:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 16 14:46:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

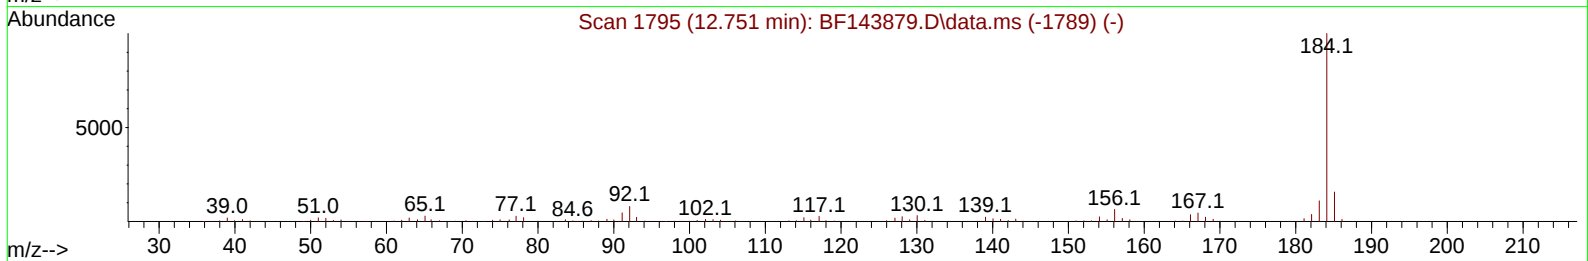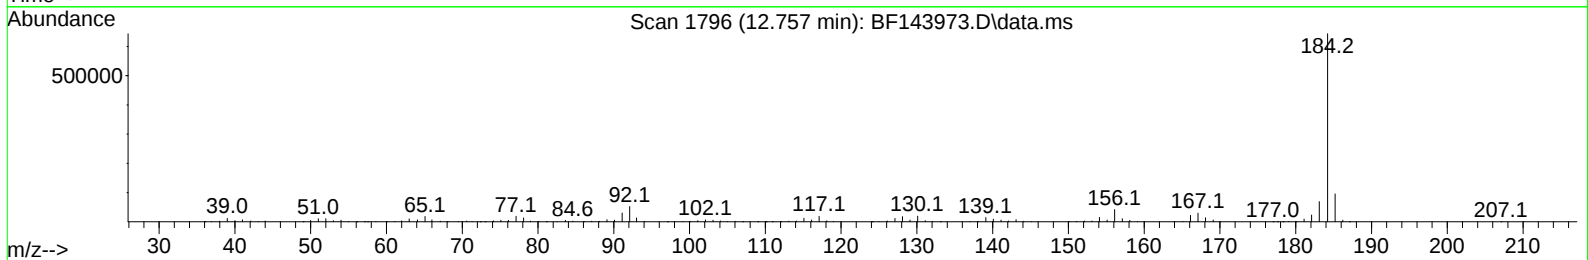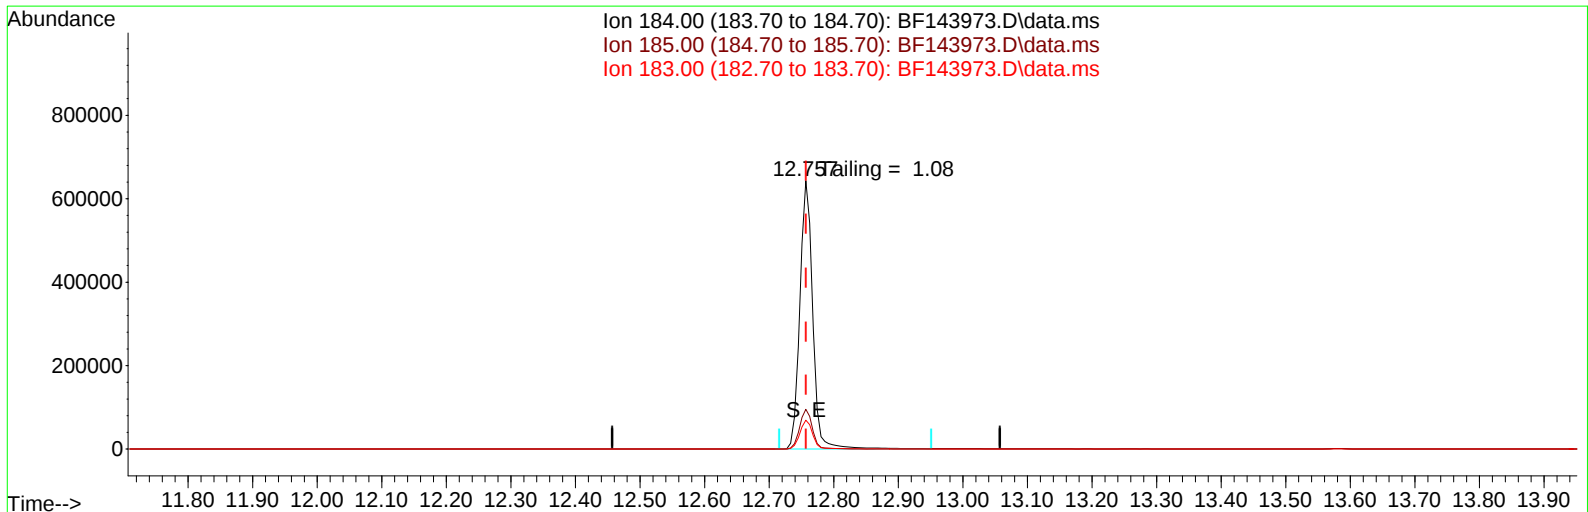

TIC: BF143973.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 895443

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.81
183.00	11.00	10.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/16/2025	BNA_F	<u>BF143973.D</u>
Compound Name	Response	Retention Time
DDT	417908	13.58
DDD	6331	13.28
DDE	2697	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9028	426936	2.11

Instrument :
BNA_F
ClientSampleId :
DFTPP