
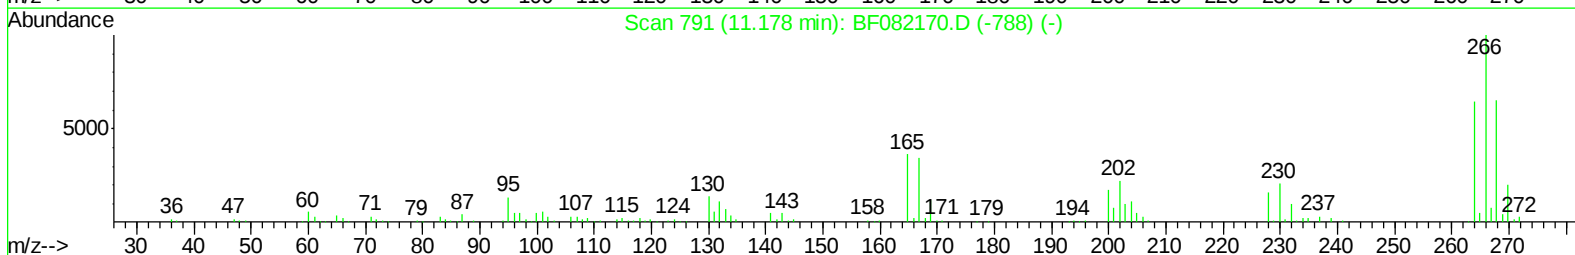
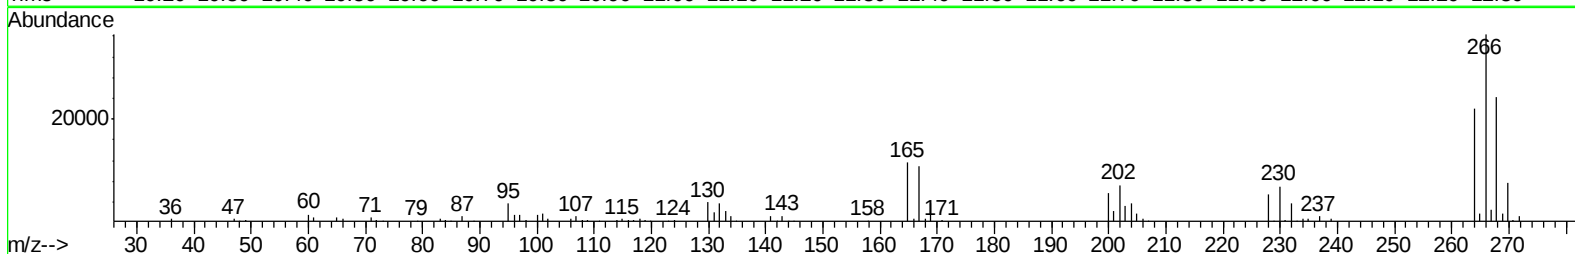


Data Path : Z:\HPCHEM1\BNA F\DATA\BF101715\
Data File : BF082342.D
Acq On : 17 Oct 2015 00:04
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 04:23:26 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

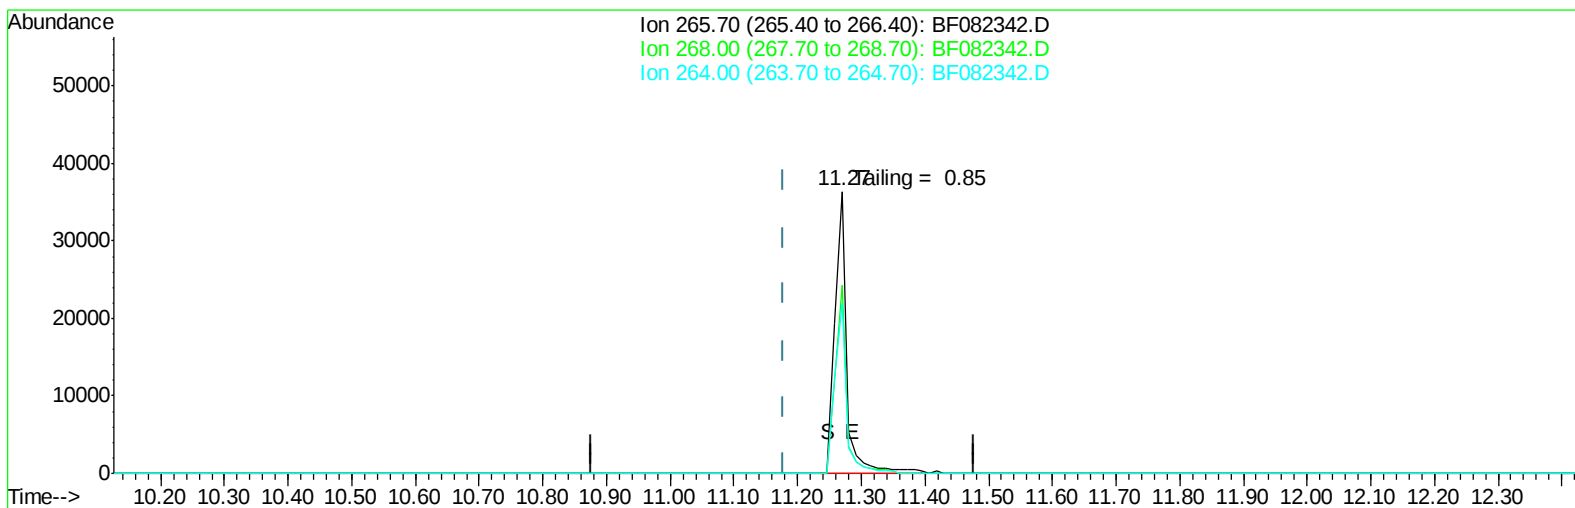

TIC: BF082342.D

(69) Pentachlorophenol (C)




11.269min (+0.091) 0.00ng

response 47531

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.02
264.00	64.20	60.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101715\
Data File : BF082342.D
Acq On : 17 Oct 2015 00:04
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 04:23:26 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 01:46:21 2015
Response via : Initial Calibration

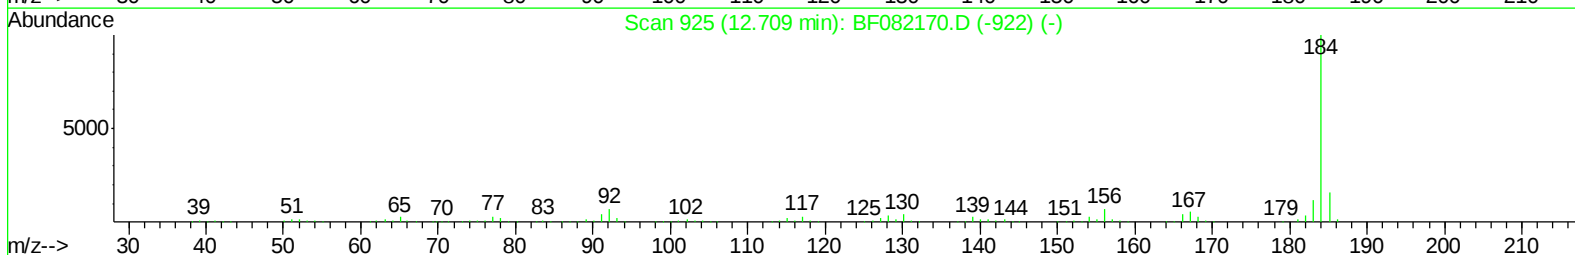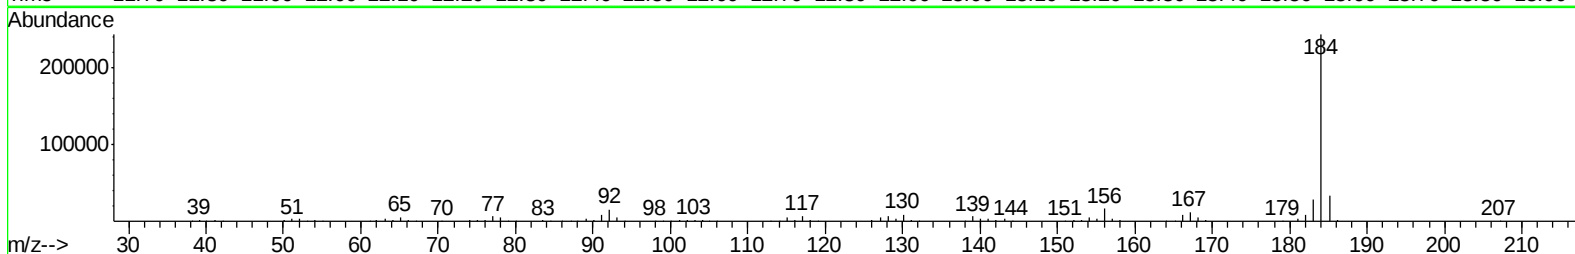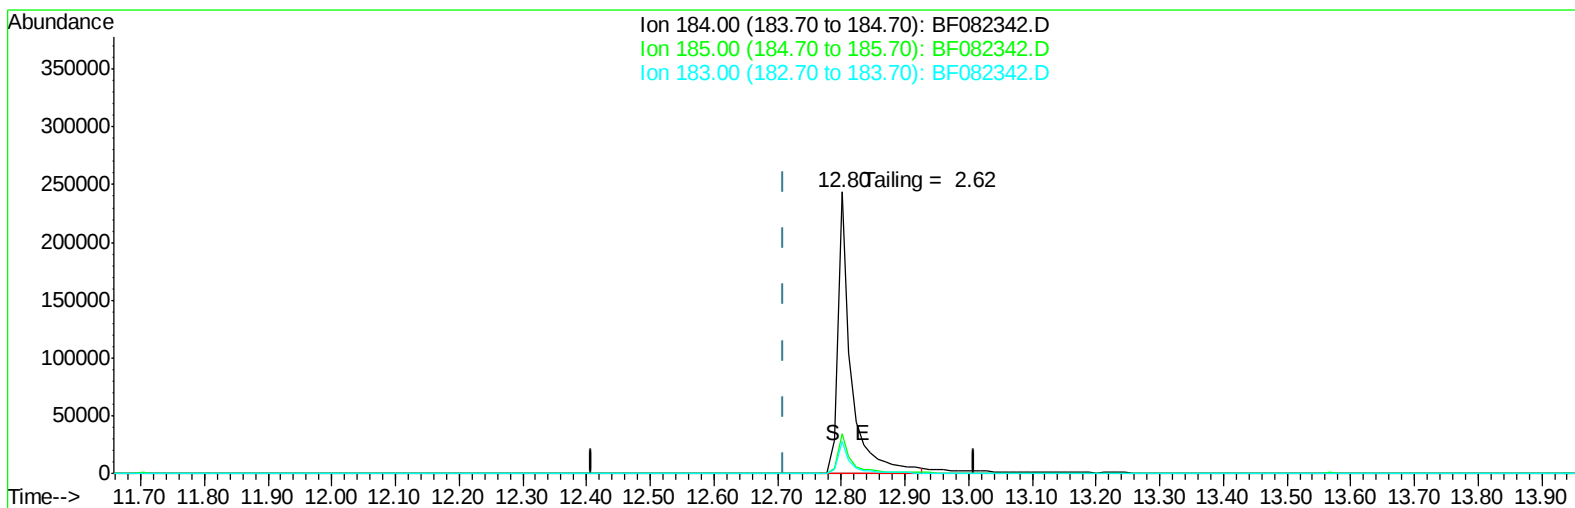

TIC: BF082342.D

(76) Benzidine

12.801min (+0.091) 0.00ng

response 360637

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.90
183.00	11.40	11.47
0.00	0.00	0.00