

Data Path : Z:\HPCHEM1\BNA F\Data\BF101715\
 Data File : BF082340.D
 Acq On : 16 Oct 2015 22:07
 Operator : UM/IZ
 Sample : G4046-05 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MANAHAWKENINSULATION

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.926	417	419	421	rBV	224483	271596	2.26%	0.148%
2	8.206	529	531	532	rBV	513827	466389	3.88%	0.255%
3	9.955	682	684	685	rBV	675669	560101	4.66%	0.306%
4	9.989	685	687	689	rVB	753725	625779	5.20%	0.342%
5	10.503	730	732	734	rBV	548788	475155	3.95%	0.259%
6	11.304	799	802	803	rBV2	469799	513811	4.27%	0.280%
7	11.338	803	805	808	rVB	437409	409696	3.41%	0.224%
8	11.486	812	818	819	rBV	4704941	7801321	64.85%	4.259%
9	11.521	819	821	823	rVB	1341466	1347809	11.20%	0.736%
10	11.681	831	835	839	rBV2	1546114	1792056	14.90%	0.978%
11	11.944	855	858	859	rBV	1036416	983043	8.17%	0.537%
12	11.978	859	861	863	rVV	1500209	1491467	12.40%	0.814%
13	12.024	863	865	866	rVV	526733	489503	4.07%	0.267%
14	12.058	866	868	872	rVV2	1774474	2759179	22.93%	1.506%
15	12.184	877	879	882	rVV3	154393	446271	3.71%	0.244%
16	12.241	882	884	885	rVV	852634	809189	6.73%	0.442%
17	12.275	885	887	889	rVV	664217	752393	6.25%	0.411%
18	12.389	894	897	898	rVV	375046	530166	4.41%	0.289%
19	12.424	898	900	901	rVV	238234	333554	2.77%	0.182%
20	12.492	904	906	908	rVV	446096	693658	5.77%	0.379%
21	12.538	908	910	911	rVV	362786	657857	5.47%	0.359%
22	12.629	913	918	919	rVV4	622743	1536411	12.77%	0.839%
23	12.687	919	923	925	rVV	5983442	11002445	91.46%	6.006%
24	12.767	928	930	932	rVV2	200043	367947	3.06%	0.201%
25	12.812	932	934	936	rVV	745925	994912	8.27%	0.543%
26	12.915	939	943	949	rVV2	5280332	12030437	100.00%	6.568%
27	13.018	949	952	954	rVV	814007	1531599	12.73%	0.836%
28	13.052	954	955	957	rVV	843043	792548	6.59%	0.433%
29	13.109	957	960	962	rVV2	881069	1693322	14.08%	0.924%
30	13.144	962	963	966	rVV	476814	707248	5.88%	0.386%
31	13.224	966	970	972	rVV	1967140	3845838	31.97%	2.099%
32	13.292	972	976	978	rVV	2110344	2824851	23.48%	1.542%
33	13.327	978	979	983	rVV2	1249018	2756000	22.91%	1.505%
34	13.418	986	987	989	rVV	579728	959346	7.97%	0.524%

Data Path : Z:\HPCHEM1\BNA F\Data\BF101715\
 Data File : BF082340.D
 Acq On : 16 Oct 2015 22:07
 Operator : UM/IZ
 Sample : G4046-05 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MANAHAWKENINSULATION

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.452	989	990	994	rVV2	902687	1329771	11.05%	0.726%
36	13.532	994	997	999	rVV4	244138	671989	5.59%	0.367%
37	13.578	999	1001	1002	rVV	227313	304668	2.53%	0.166%
38	13.624	1002	1005	1006	rVV3	564336	960903	7.99%	0.525%
39	13.658	1006	1008	1011	rVV	848270	1309117	10.88%	0.715%
40	13.749	1011	1016	1018	rVV2	948431	2364525	19.65%	1.291%
41	13.829	1018	1023	1024	rVV	459320	1217853	10.12%	0.665%
42	13.875	1024	1027	1029	rVV3	1798668	4125745	34.29%	2.252%
43	13.921	1029	1031	1034	rVV3	975956	2257538	18.77%	1.232%
44	13.967	1034	1035	1038	rVV	938052	1110795	9.23%	0.606%
45	14.035	1038	1041	1043	rVV	429338	872197	7.25%	0.476%
46	14.127	1044	1049	1050	rVV2	3664547	9118182	75.79%	4.978%
47	14.172	1050	1053	1055	rVV	4250118	7241700	60.19%	3.953%
48	14.218	1055	1057	1058	rVV2	400009	647629	5.38%	0.354%
49	14.241	1058	1059	1062	rVV2	1283173	1982429	16.48%	1.082%
50	14.298	1062	1064	1066	rVV3	727281	1324795	11.01%	0.723%
51	14.332	1066	1067	1068	rVV	763999	857077	7.12%	0.468%
52	14.367	1068	1070	1074	rVV4	745804	2326983	19.34%	1.270%
53	14.492	1077	1081	1083	rVV	1911271	3003163	24.96%	1.639%
54	14.527	1083	1084	1087	rVV2	1645364	2878460	23.93%	1.571%
55	14.572	1087	1088	1090	rVV	790092	1029869	8.56%	0.562%
56	14.641	1090	1094	1096	rVV3	657999	1906860	15.85%	1.041%
57	14.698	1096	1099	1101	rVV2	1040176	2151254	17.88%	1.174%
58	14.767	1101	1105	1107	rVV	3396637	4809258	39.98%	2.625%
59	14.801	1107	1108	1110	rVV	164249	271503	2.26%	0.148%
60	14.881	1112	1115	1119	rVV4	754474	2147488	17.85%	1.172%
61	14.950	1119	1121	1123	rVV	495366	850611	7.07%	0.464%
62	15.007	1125	1126	1128	rVV	338848	576541	4.79%	0.315%
63	15.064	1128	1131	1135	rVV3	528487	1670619	13.89%	0.912%
64	15.144	1135	1138	1141	rVV	1772740	2817933	23.42%	1.538%
65	15.258	1141	1148	1151	rVV2	2936924	10653940	88.56%	5.816%
66	15.304	1151	1152	1154	rVV	335164	571169	4.75%	0.312%
67	15.350	1154	1156	1157	rVV	697587	1044495	8.68%	0.570%
68	15.384	1157	1159	1161	rVV3	179371	428622	3.56%	0.234%
69	15.464	1161	1166	1168	rVV	2495142	5938856	49.37%	3.242%
70	15.555	1170	1174	1176	rVV	1994014	4172180	34.68%	2.278%
71	15.624	1176	1180	1182	rVV	2566739	4545683	37.78%	2.482%

Data Path : Z:\HPCHEM1\BNA F\Data\BF101715\
 Data File : BF082340.D
 Acq On : 16 Oct 2015 22:07
 Operator : UM/IZ
 Sample : G4046-05 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MANAHAWKENINSULATION

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	15.670	1182	1184	1185	rVV2	553733	905475	7.53%	0.494%
73	15.704	1185	1187	1191	rVV2	1220536	2328066	19.35%	1.271%
74	15.773	1191	1193	1196	rVV3	369491	826390	6.87%	0.451%
75	15.841	1196	1199	1201	rVV2	313141	859897	7.15%	0.469%
76	15.887	1201	1203	1207	rVV2	915770	2617418	21.76%	1.429%
77	15.990	1210	1212	1214	rVV	220510	438763	3.65%	0.240%
78	16.024	1214	1215	1219	rVB2	237667	387790	3.22%	0.212%
79	16.104	1219	1222	1224	rBV	145745	286066	2.38%	0.156%
80	16.230	1231	1233	1236	rVV	260202	474066	3.94%	0.259%
81	16.298	1236	1239	1243	rVB	1675013	2799182	23.27%	1.528%
82	16.378	1243	1246	1250	rBV4	115575	252029	2.09%	0.138%
83	16.561	1259	1262	1268	rVB4	80798	285409	2.37%	0.156%
84	16.664	1268	1271	1273	rBV	121829	250867	2.09%	0.137%
85	16.881	1288	1290	1293	rVB	311196	543359	4.52%	0.297%
86	16.961	1293	1297	1298	rBV2	186688	409724	3.41%	0.224%
87	17.178	1307	1316	1319	rBV	1083047	2861557	23.79%	1.562%
88	17.236	1319	1321	1326	rVB	142095	259531	2.16%	0.142%
89	17.338	1326	1330	1332	rBV	269089	649086	5.40%	0.354%
90	17.430	1332	1338	1346	rVB2	549155	1967696	16.36%	1.074%
91	17.624	1349	1355	1361	rVB	800997	2212889	18.39%	1.208%
92	17.853	1371	1375	1382	rVB2	274555	840032	6.98%	0.459%
93	18.550	1431	1436	1444	rVB6	58518	253534	2.11%	0.138%
94	18.779	1452	1456	1464	rVB4	48165	247306	2.06%	0.135%
95	19.887	1546	1553	1562	rVB	257983	985873	8.19%	0.538%
96	20.082	1563	1570	1574	rVV2	172934	730766	6.07%	0.399%
97	20.173	1574	1578	1590	rVB3	127373	583178	4.85%	0.318%
98	20.733	1622	1627	1637	rVB3	47297	241411	2.01%	0.132%
99	21.030	1647	1653	1657	rBV2	78604	378565	3.15%	0.207%
100	21.133	1658	1662	1673	rVB	135115	558032	4.64%	0.305%


Sum of corrected areas: 183179254

Data Path : Z:\HPCHEM1\BNA F\Data\BF101715\
Data File : BF082340.D
Acq On : 16 Oct 2015 22:07
Operator : UM/IZ
Sample : G4046-05 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MANAHAWKENINSULATION

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

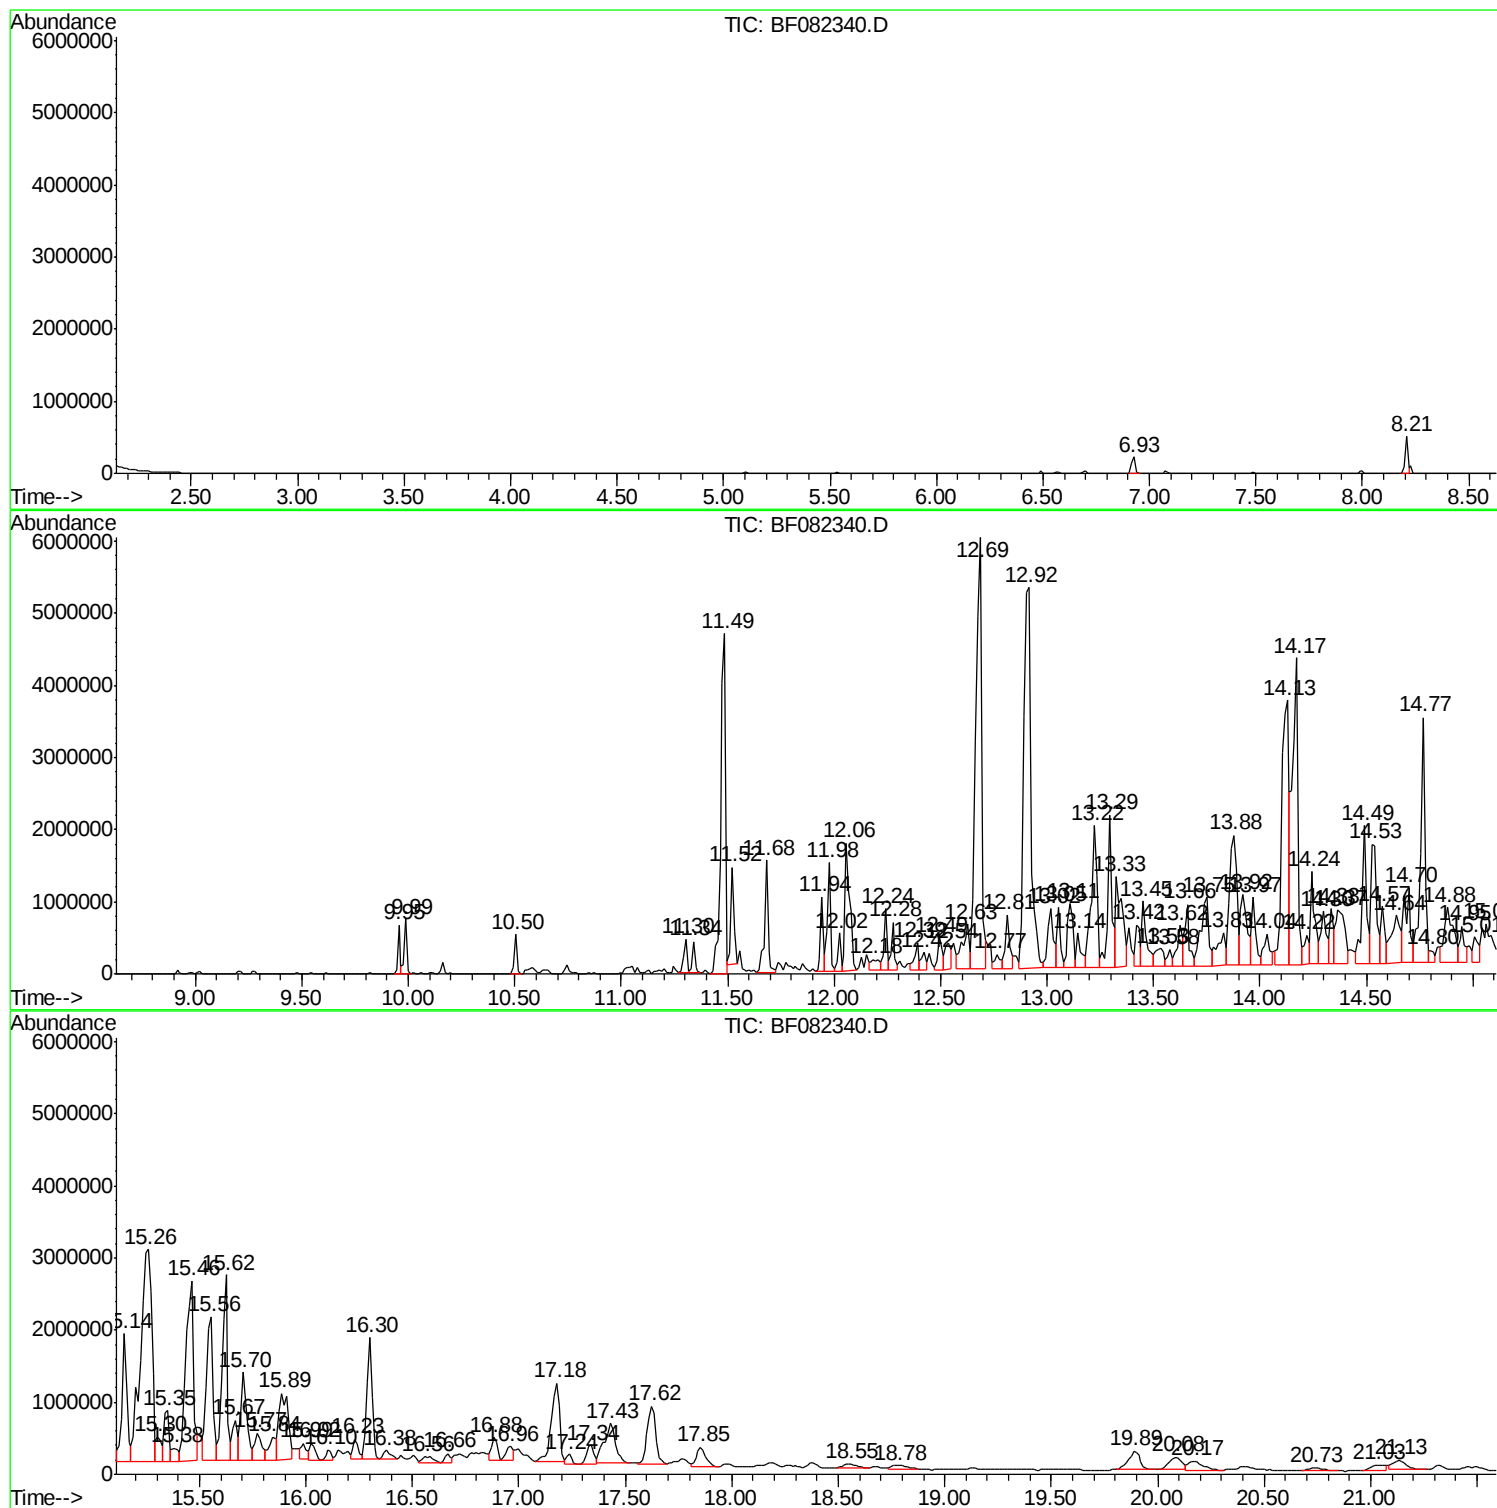

Data Path : Z:\HPCHEM1\BNA_F\Data\BF101715\
Data File : BF082340.D
Acq On : 16 Oct 2015 22:07
Operator : UM/IZ
Sample : G4046-05 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MANAHAWKENINSULATION

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\Data\BF101715\
Data File : BF082340.D
Acq On : 16 Oct 2015 22:07
Operator : UM/IZ
Sample : G4046-05 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MANAHAWKENINSULATION

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc