


Data Path : Z:\HPCHEM1\BNA F\Data\BF101715\
 Data File : BF082319.D
 Acq On : 16 Oct 2015 11:18
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 12 01:46:21 2015

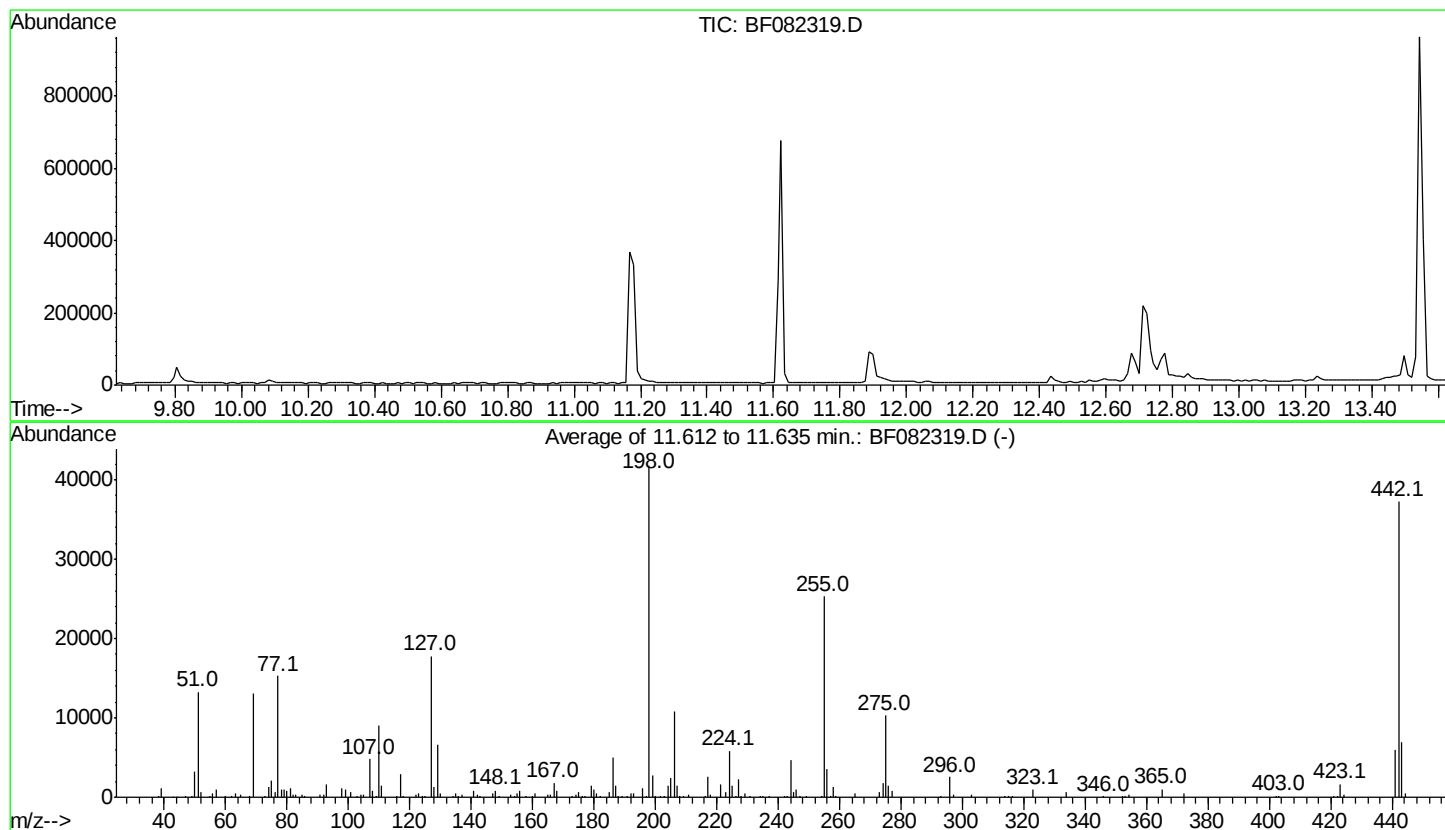

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	13246	PASS
68	69	0.00	2	1.7	225	PASS
69	198	0.00	100	31.2	13054	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	17787	PASS
197	198	0.00	2	0.4	187	PASS
198	198	100	100	100.0	41789	PASS
199	198	5	9	6.6	2750	PASS
275	198	10	60	24.6	10290	PASS
365	198	1	100	2.5	1035	PASS
441	442	0.01	24	15.9	5929	PASS
442	198	50	100	89.1	37233	PASS
443	442	15	24	18.5	6899	PASS