
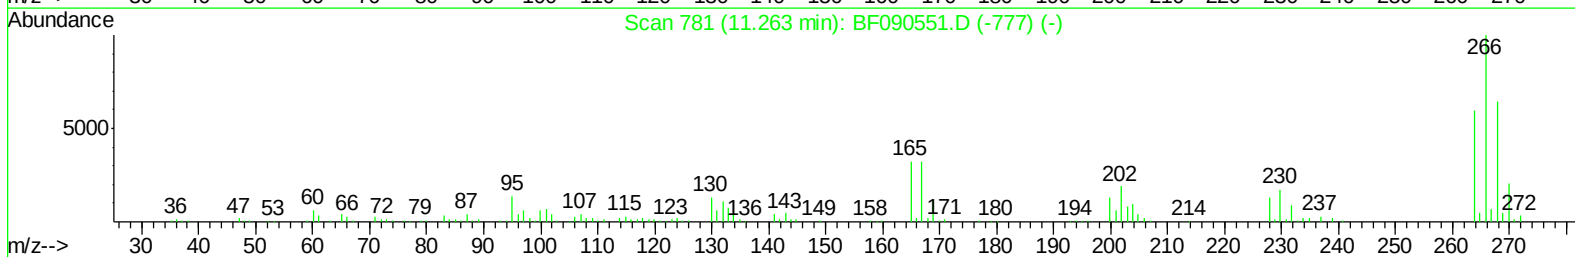
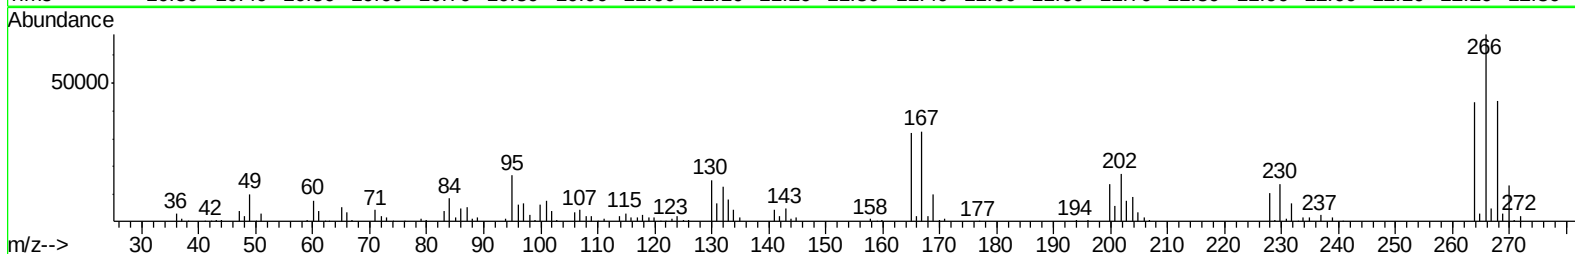


Data Path : Z:\HPCHEM1\BNA F\Data\BF101716\
Data File : BF090600.D
Acq On : 17 Oct 2016 10:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 18:55:32 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

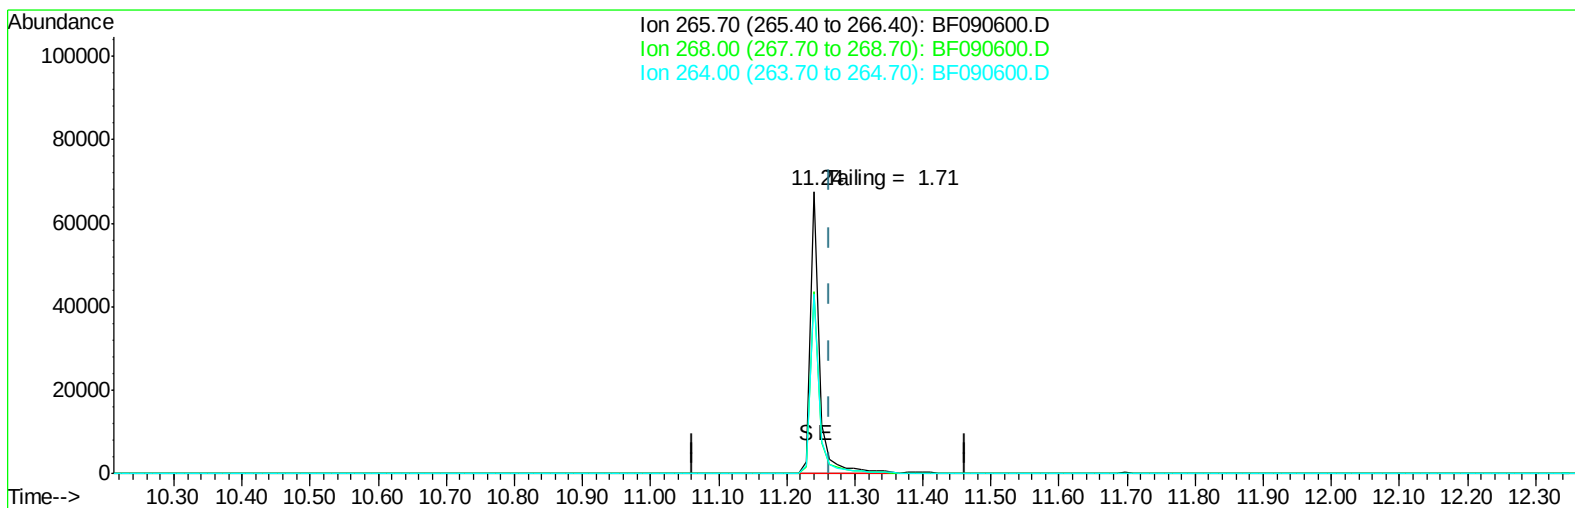

TIC: BF090600.D

(69) Pentachlorophenol (C)




11.240min (-0.023) 36279.40ng

response 63891

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.34
264.00	59.90	63.80
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF101716\
Data File : BF090600.D
Acq On : 17 Oct 2016 10:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 18:55:32 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

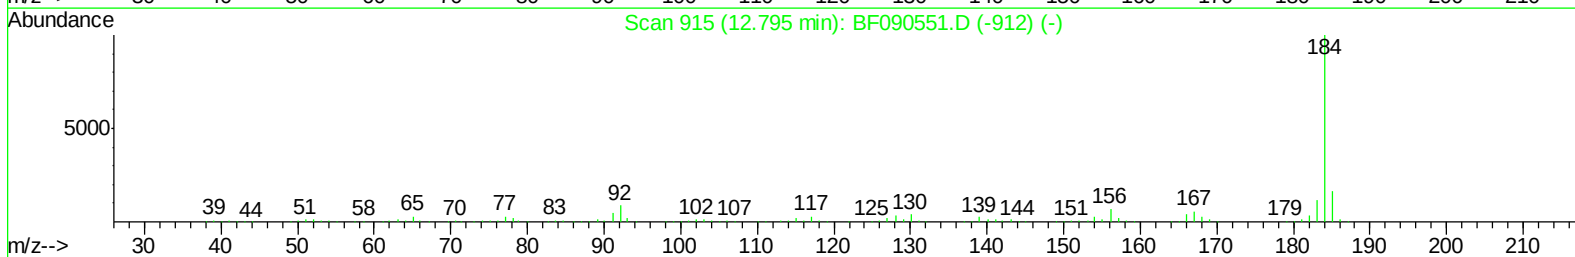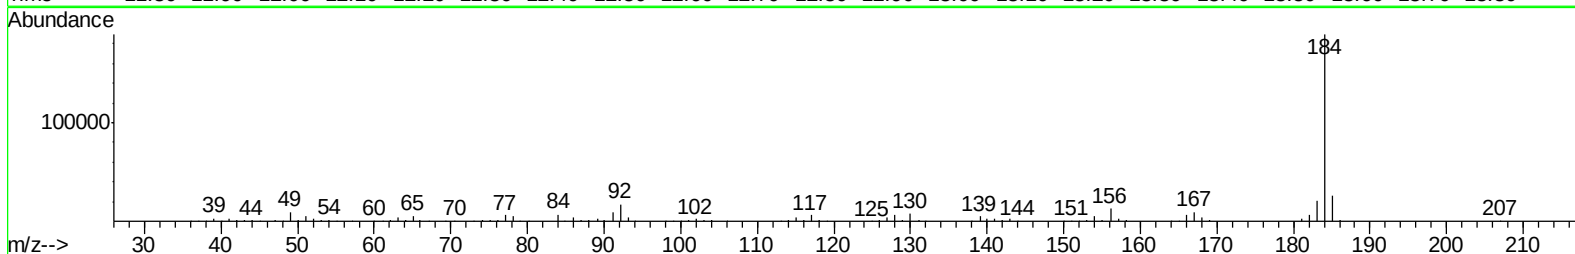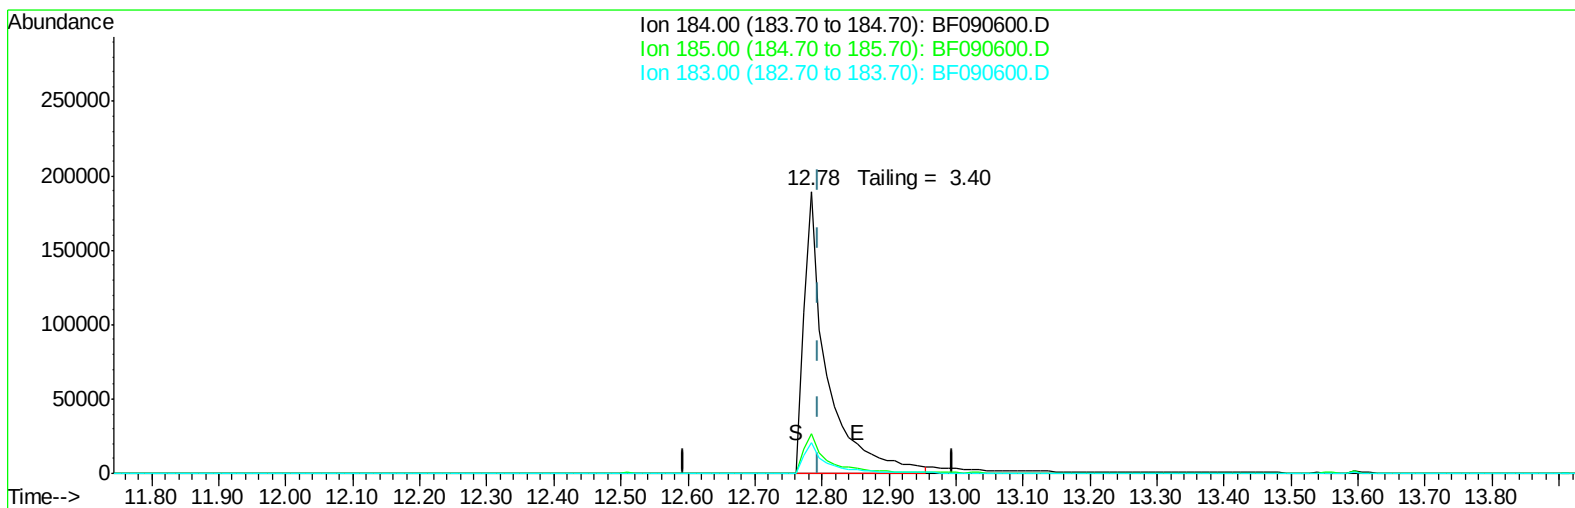

TIC: BF090600.D

(76) Benzidine

12.783min (-0.012) 78629.26ng m

response 449973

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.89
183.00	11.70	11.00
0.00	0.00	0.00