
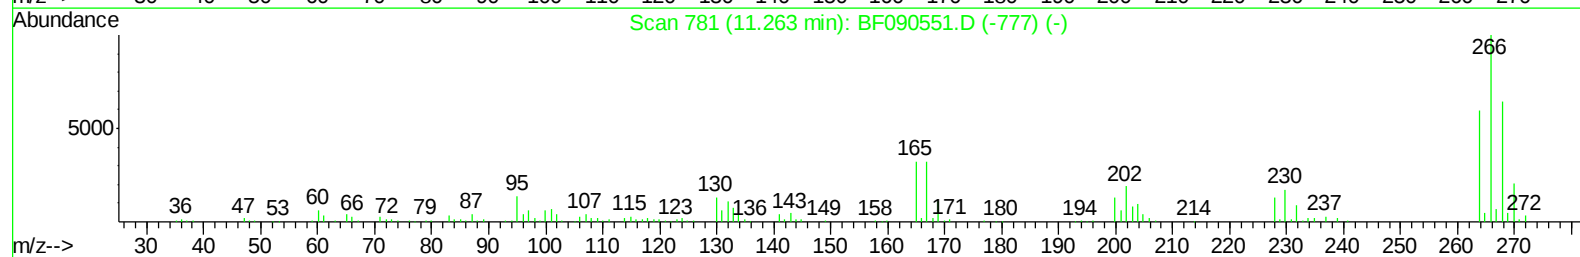
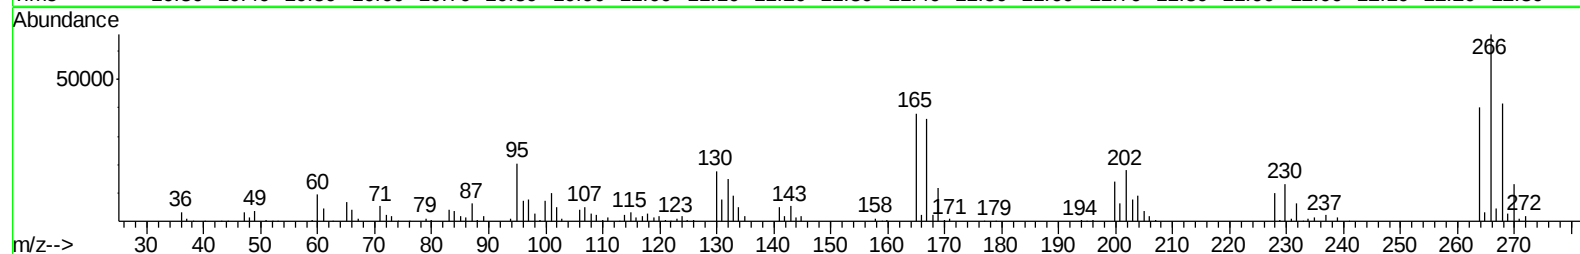


Data Path : Z:\HPCHEM1\BNA F\Data\BF101716\
Data File : BF090604.D
Acq On : 17 Oct 2016 13:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 18:59:29 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

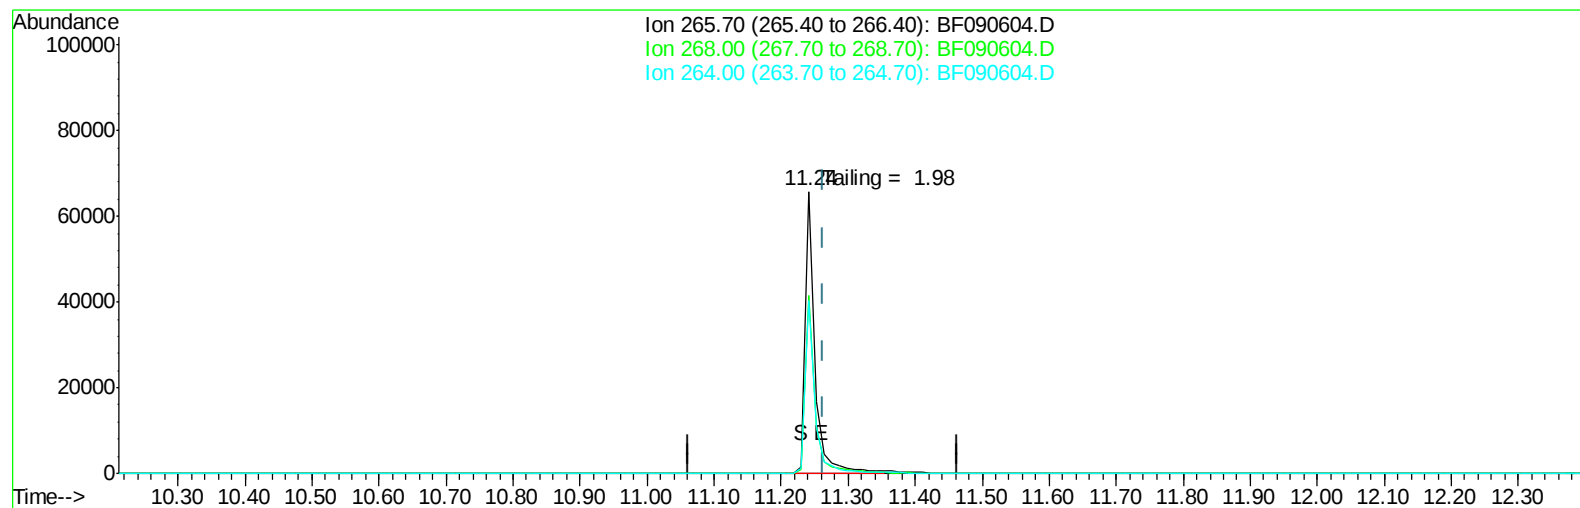

TIC: BF090604.D

(69) Pentachlorophenol (C)




11.240min (-0.023) 0.00ng m

response 67405

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	63.34
264.00	59.90	61.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF101716\
Data File : BF090604.D
Acq On : 17 Oct 2016 13:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 18:59:29 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 14 12:44:45 2016
Response via : Initial Calibration

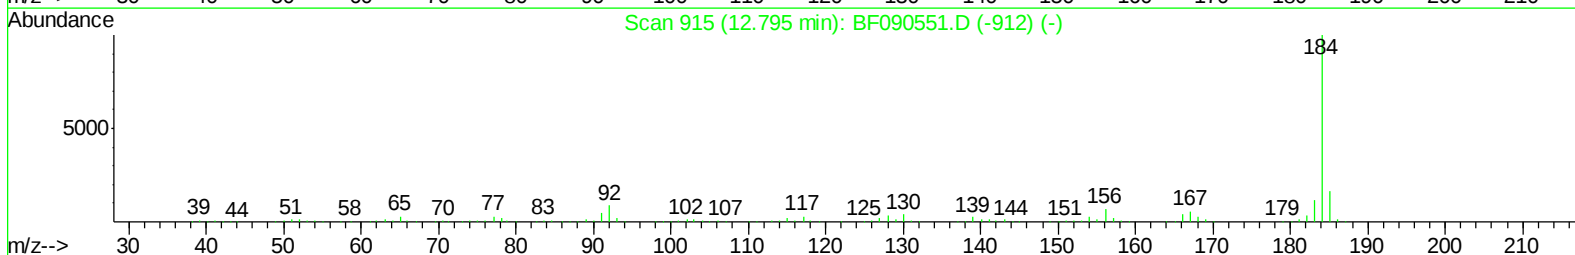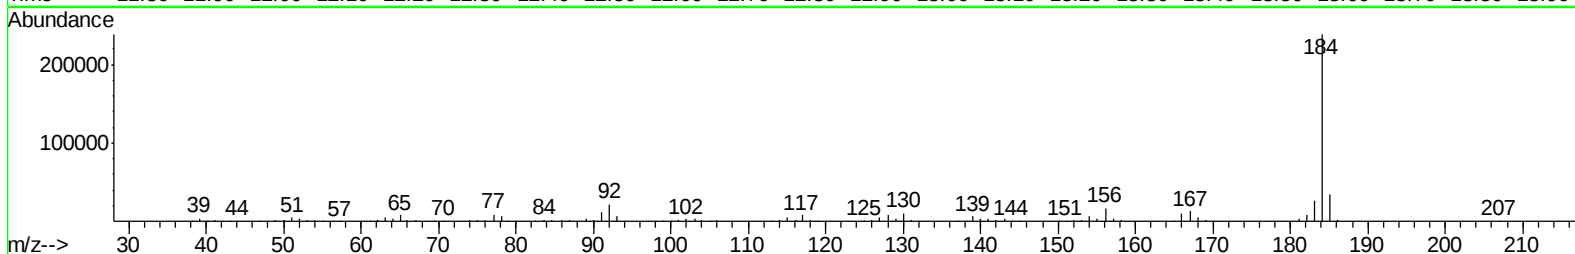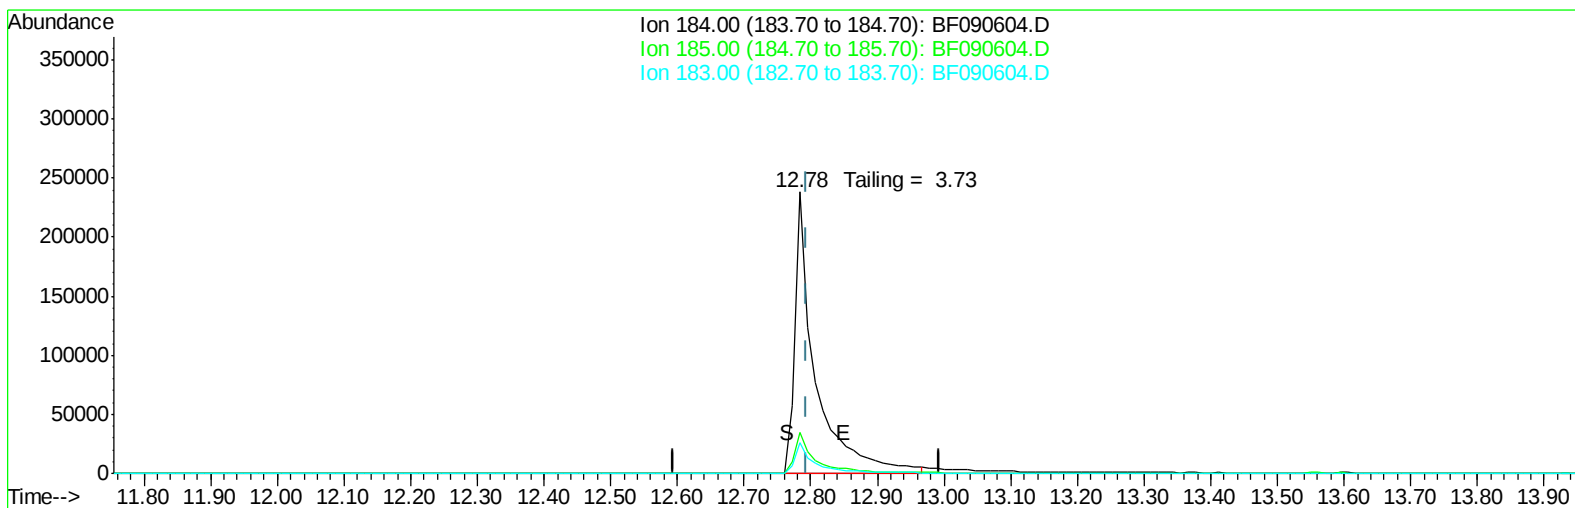

TIC: BF090604.D

(76) Benzidine

12.783min (-0.012) 0.00ng

response 502688

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.69
183.00	11.70	11.08
0.00	0.00	0.00