

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101716\
 Data File : BF090606.D
 Acq On : 17 Oct 2016 14:38
 Operator : UM/SJ
 Sample : H5263-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-02-001-A

Quant Time: Oct 17 16:12:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 17 15:58:48 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.91	152	166478	20.00	ng	0.00
21) Naphthalene-d8	8.19	136	720340	20.00	ng	-0.01
38) Acenaphthene-d10	9.95	164	398889	20.00	ng	-0.01
63) Phenanthrene-d10	11.43	188	639267	20.00	ng	-0.01
75) Chrysene-d12	14.08	240	566852	20.00	ng	-0.01
86) Perylene-d12	15.54	264	470317	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	1196829	131.79	ng	0.01
7) Phenol-d6	6.54	99	1803303	133.64	ng	0.00
23) Nitrobenzene-d5	7.47	82	1075859	82.97	ng	-0.01
41) 2,4,6-Tribromophenol	10.74	330	354598	99.71	ng	-0.01
44) 2-Fluorobiphenyl	9.27	172	1838532	75.94	ng	0.00
78) Terphenyl-d14	13.02	244	1804587	74.12	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.66	163	199879	7.72	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101716\
Data File : BF090606.D
Acq On : 17 Oct 2016 14:38
Operator : UM/SJ
Sample : H5263-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-001-A

Quant Time: Oct 17 16:12:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 15:58:48 2016
Response via : Initial Calibration

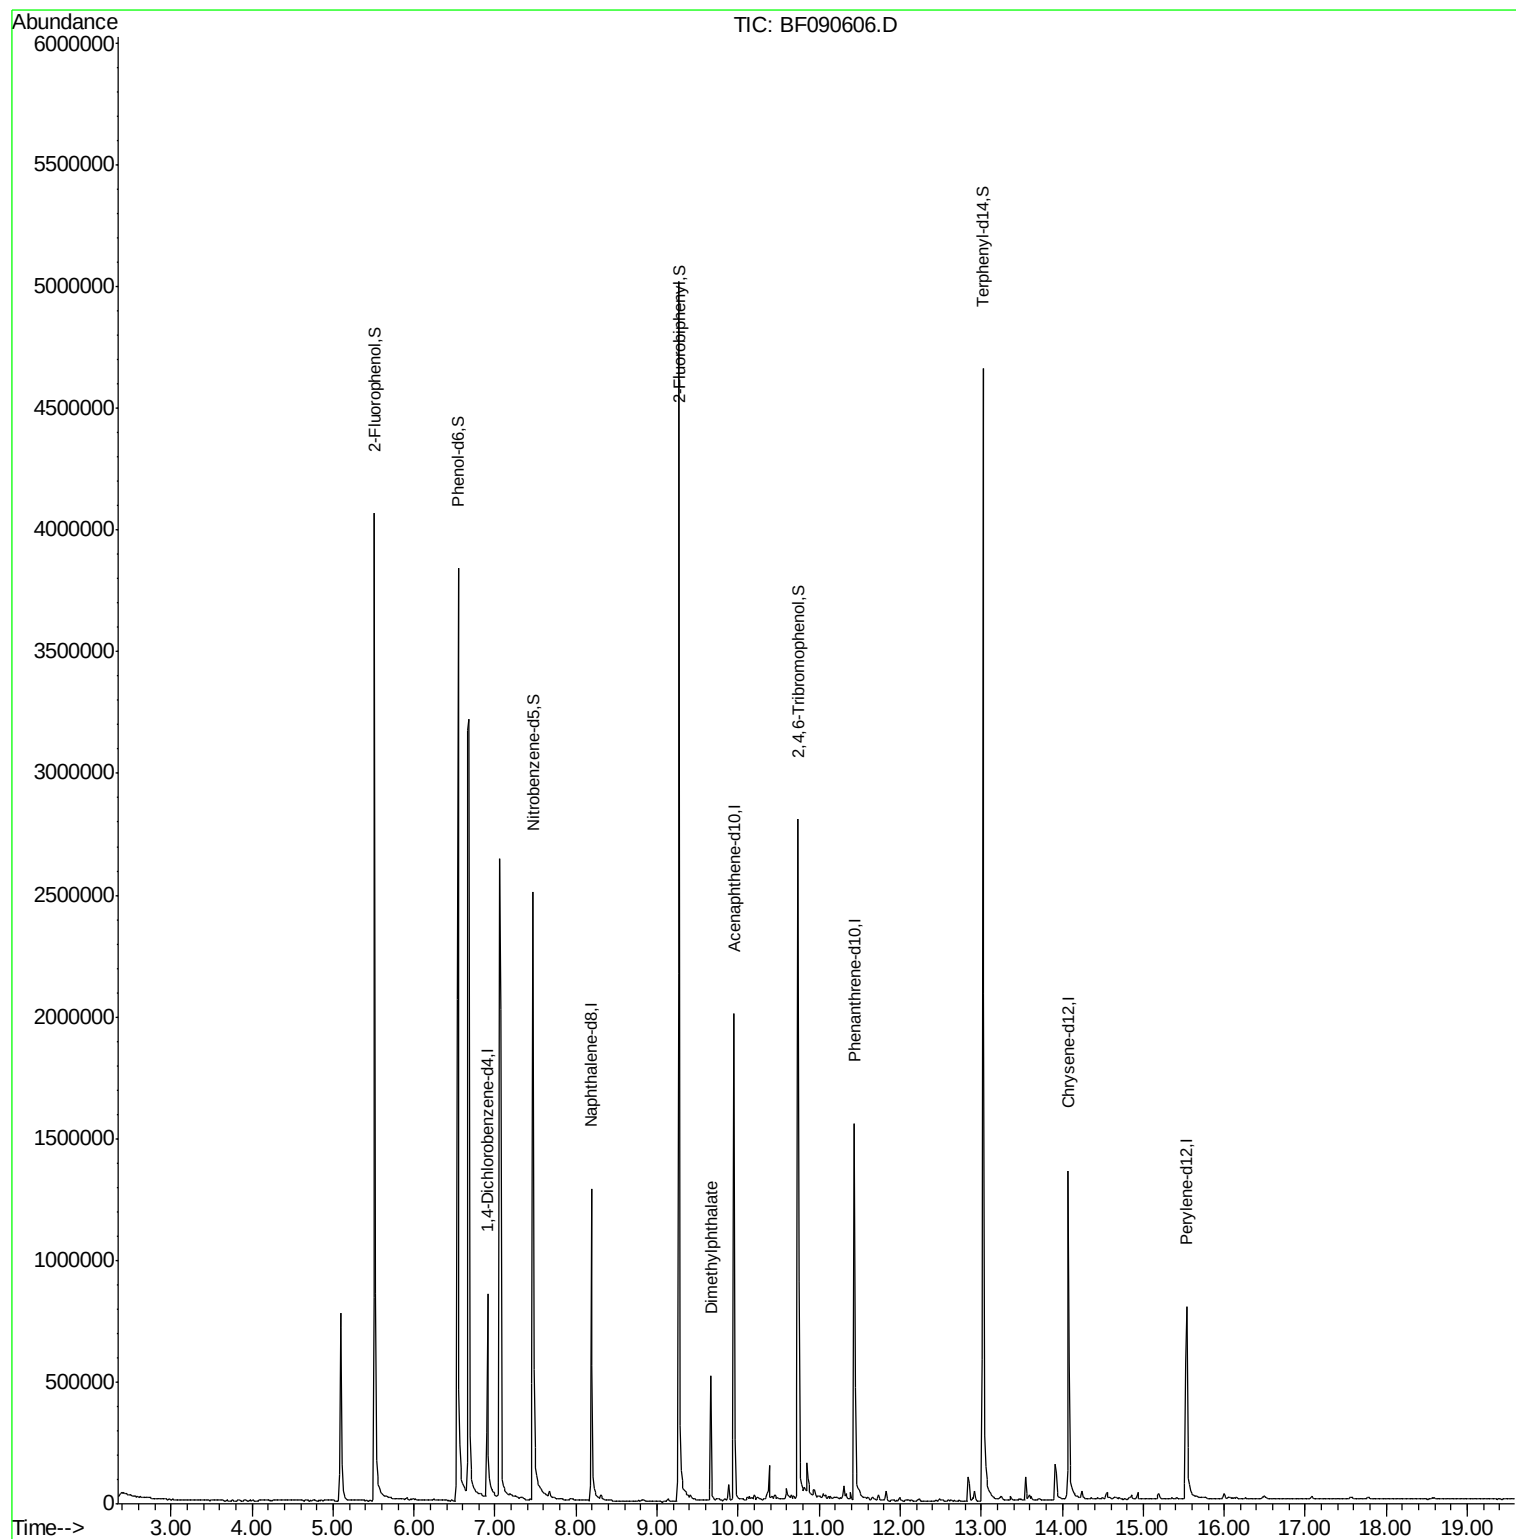

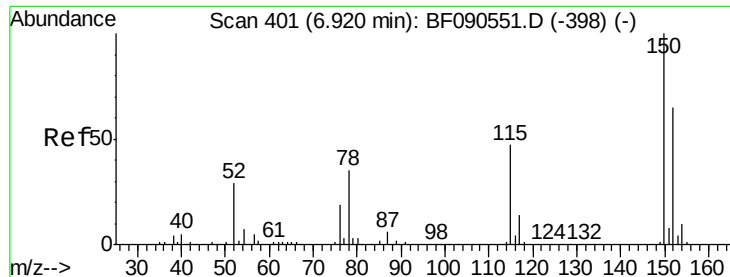

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.91 min Scan# 400

Delta R.T. -0.00 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38

Instrument :

BNA_F

ClientSampleId :

FK-BPM-02-001-A


Tot Ion:152 Resp: 166478

Ion Ratio Lower Upper

152 100

150 156.2 127.2 190.8




115 61.5 58.6 88.0

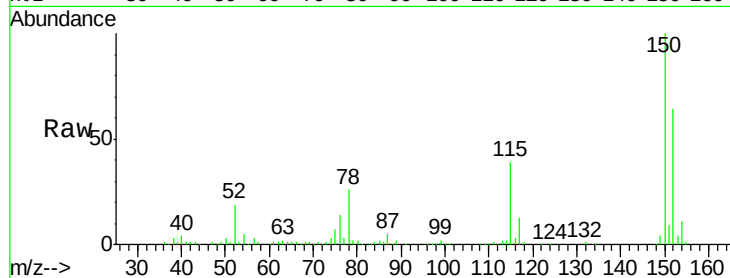

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

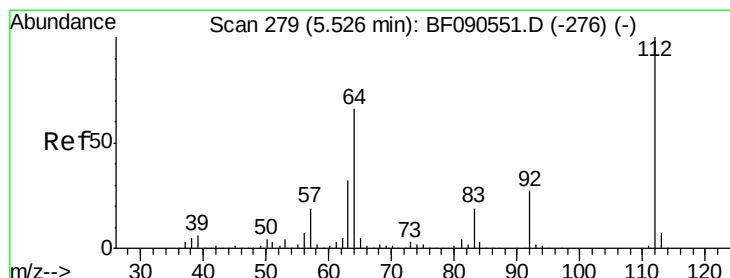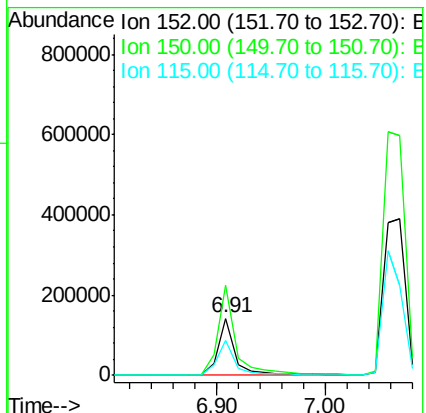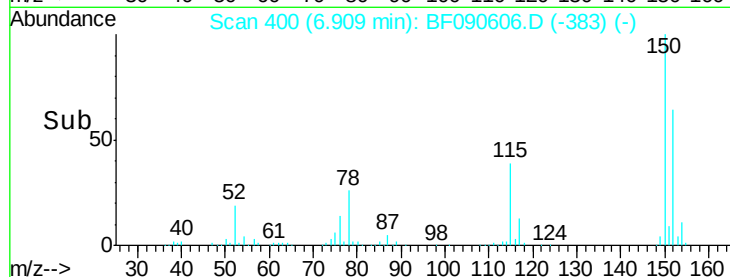

#5

2-Fluorophenol

Concen: 131.79 ng

RT: 5.51 min Scan# 278

Delta R.T. 0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38


Tgt Ion:112 Resp: 1196829

Ion Ratio Lower Upper

112 100

64 68.8 52.6 78.8



63 33.7 26.0 39.0

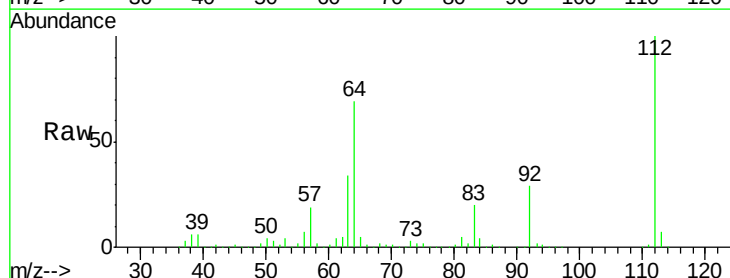


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

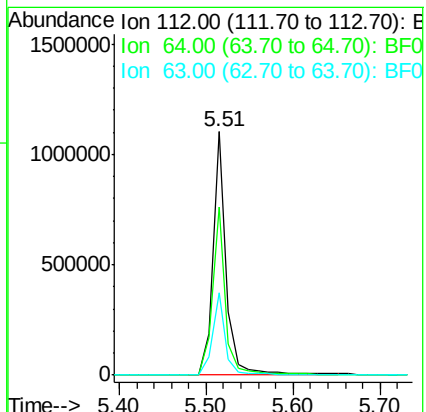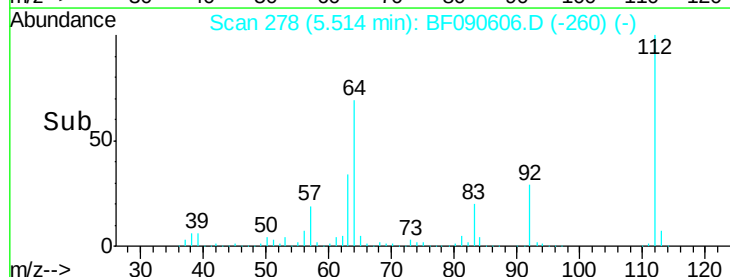

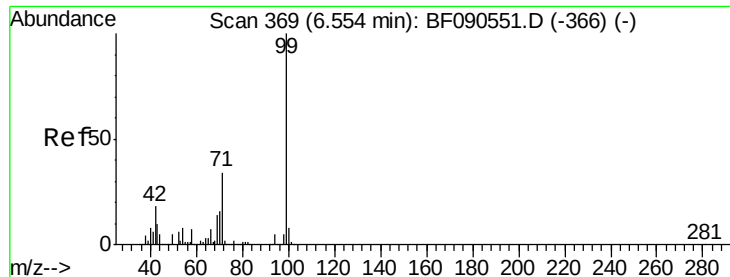

#7

Phenol-d6

Concen: 133.64 ng

RT: 6.54 min Scan# 368

Delta R.T. -0.00 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38

Instrument :

BNA_F

ClientSampleId :

FK-BPM-02-001-A


Tot Ion: 99 Resp: 1803303

Ion Ratio Lower Upper




99 100

42 15.0 14.7 22.1

71 31.7 27.6 41.4

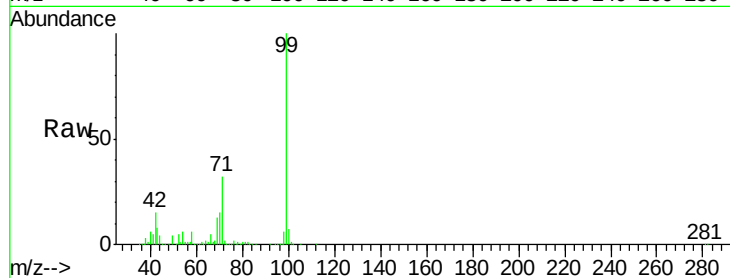

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

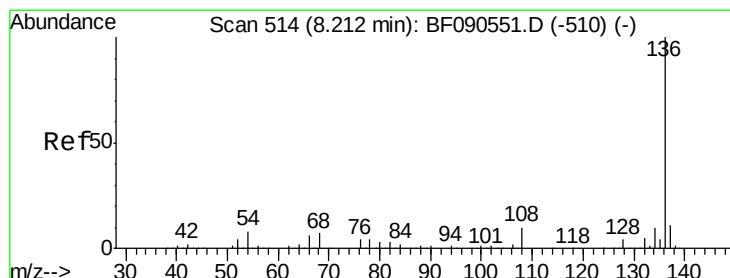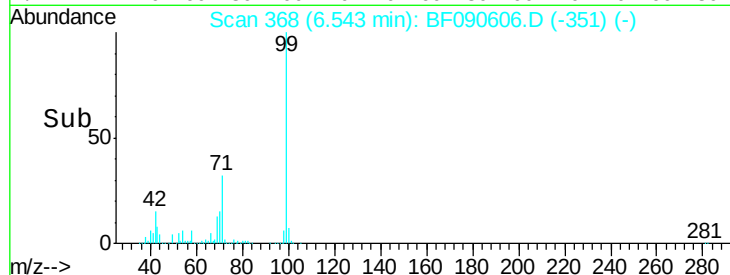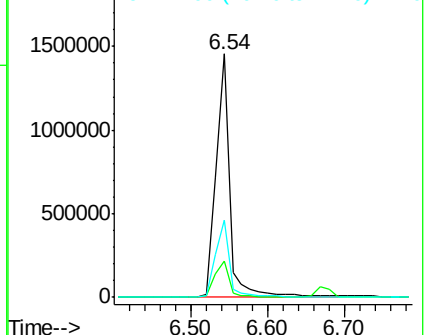

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.19 min Scan# 512

Delta R.T. -0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38

Tgt Ion: 136 Resp: 720340


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 11.0 6.8 10.2#

68 9.3 6.0 9.0#

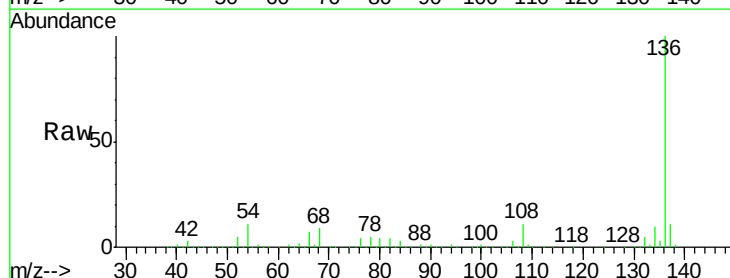

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

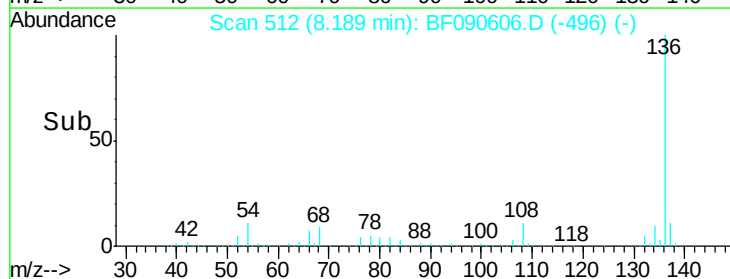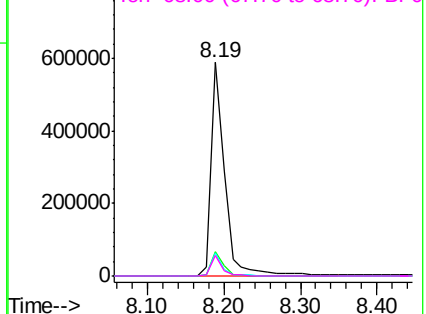

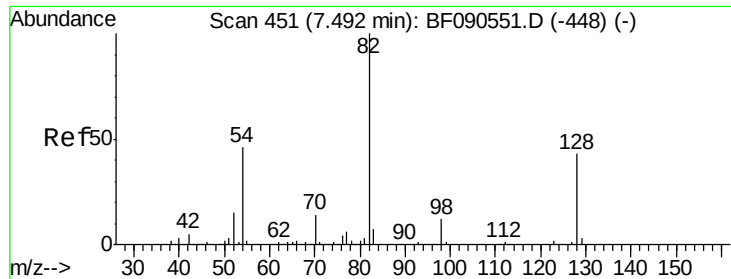


#23
 Nitrobenzene-d5
 Concen: 82.97 ng
 RT: 7.47 min Scan# 449
 Delta R.T. -0.01 min
 Lab File: BF090606.D
 Acq: 17 Oct 2016 14:38




Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-02-001-A

Tot Ion: 82 Resp: 1075859

Ion	Ratio	Lower	Upper
82	100		
128	40.2	34.3	51.5
54	48.2	37.0	55.6

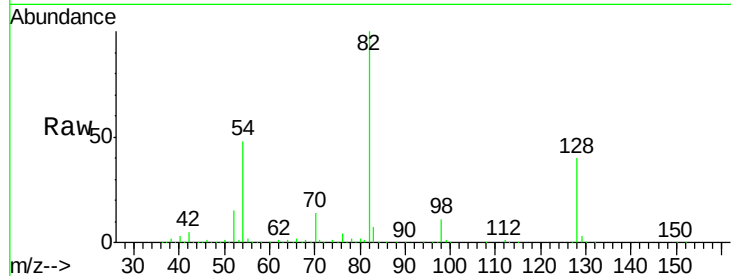


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

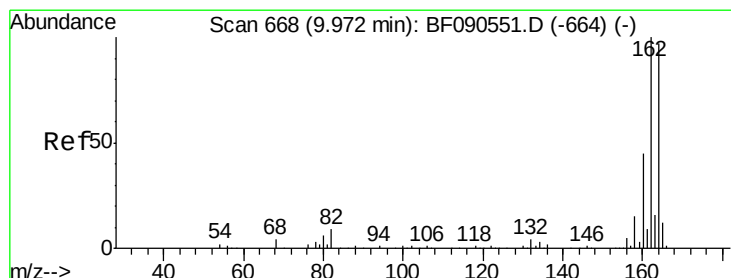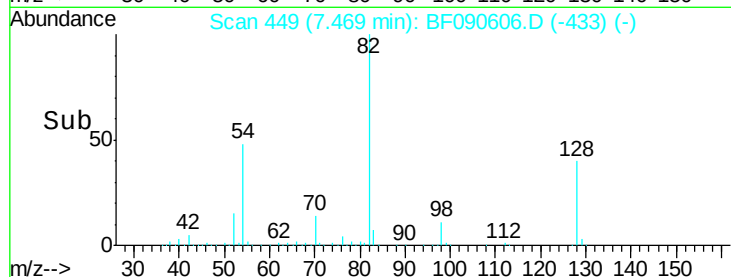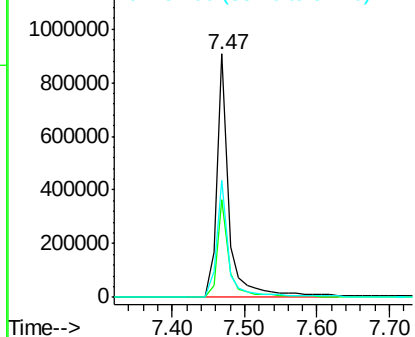



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.95 min Scan# 666
 Delta R.T. -0.01 min
 Lab File: BF090606.D
 Acq: 17 Oct 2016 14:38


Tgt Ion: 164 Resp: 398889

Ion	Ratio	Lower	Upper
164	100		
162	103.0	82.2	123.4
160	47.1	36.6	55.0

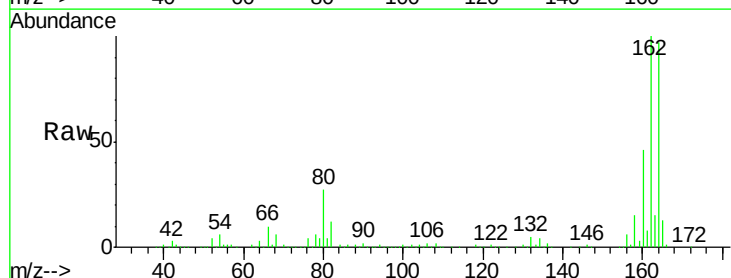

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



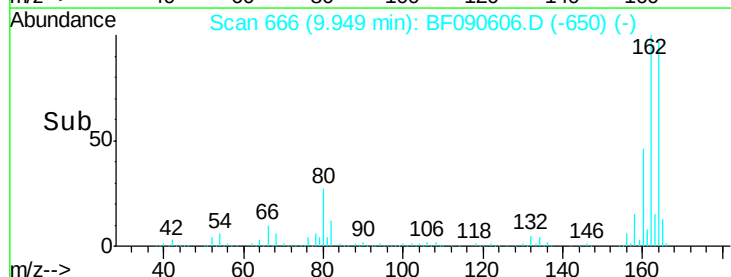
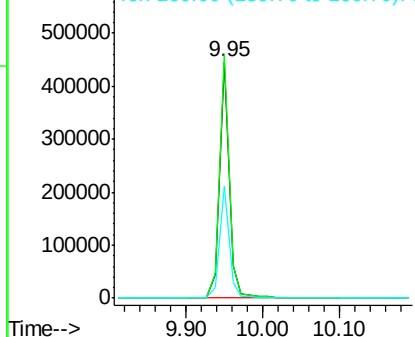


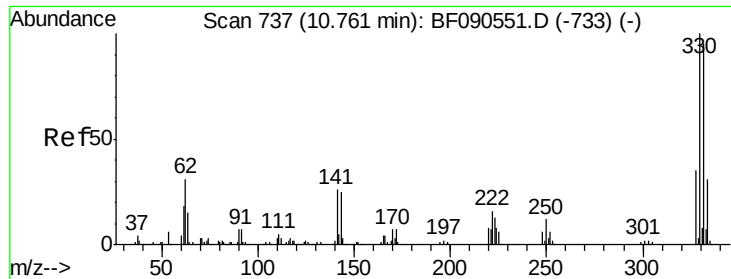

#41
 2,4,6-Tribromophenol
 Concen: 99.71 ng
 RT: 10.74 min Scan# 735
 Delta R.T. -0.01 min
 Lab File: BF090606.D
 Acq: 17 Oct 2016 14:38




Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-02-001-A


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	76.2	114.2
141	42.4	31.4	47.2

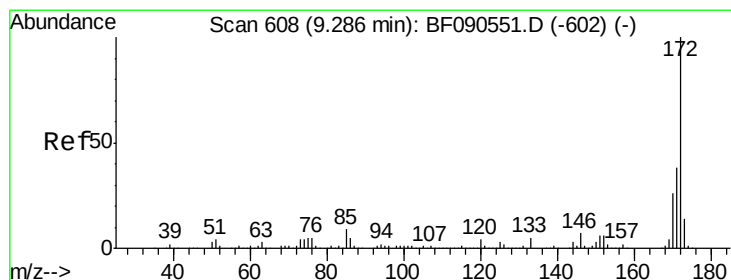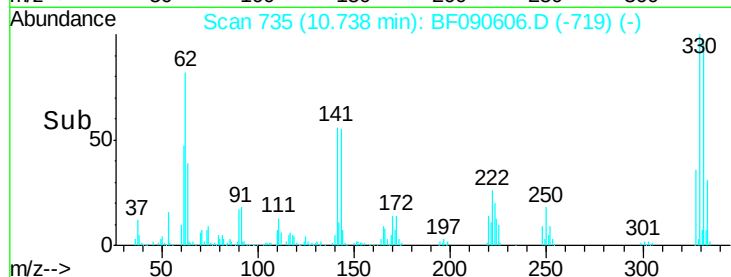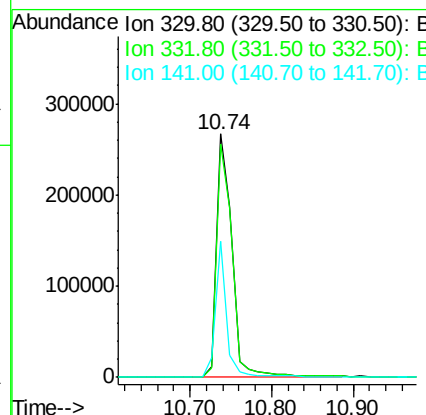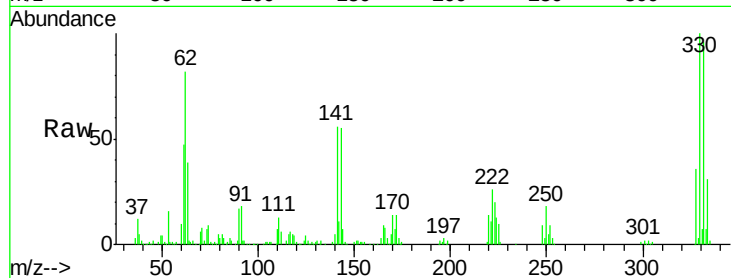

#44
 2-Fluorobiphenyl
 Concen: 75.94 ng
 RT: 9.27 min Scan# 607
 Delta R.T. -0.00 min
 Lab File: BF090606.D
 Acq: 17 Oct 2016 14:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	30.1	45.1
170	25.1	20.6	30.8

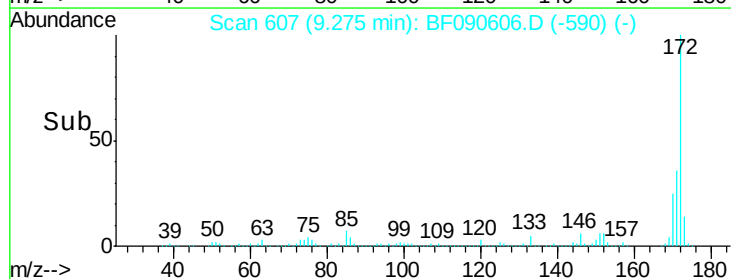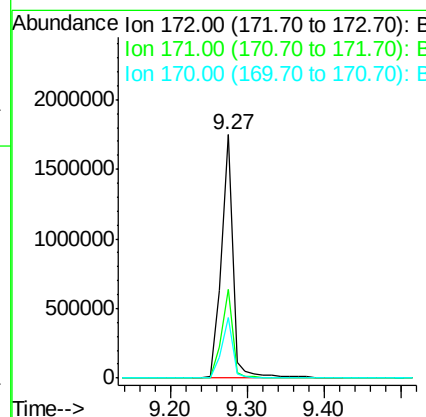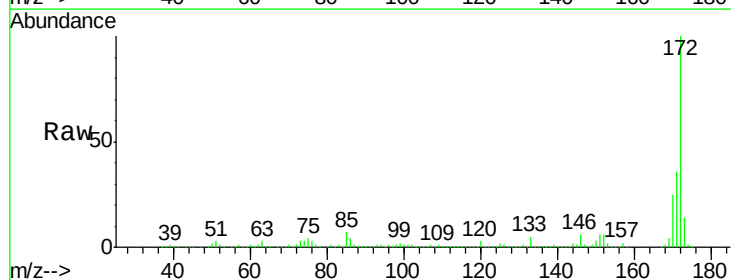

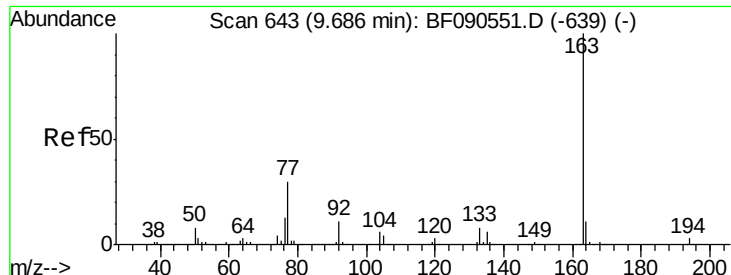

#49

Dimethylphthalate

Concen: 7.72 ng

RT: 9.66 min Scan# 641

Delta R.T. -0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38

Instrument :

BNA_F

ClientSampleId :

FK-BPM-02-001-A


Tot Ion:163 Resp: 199879

Ion Ratio Lower Upper

163 100

194 3.0 2.3 3.5




164 10.1 8.6 13.0

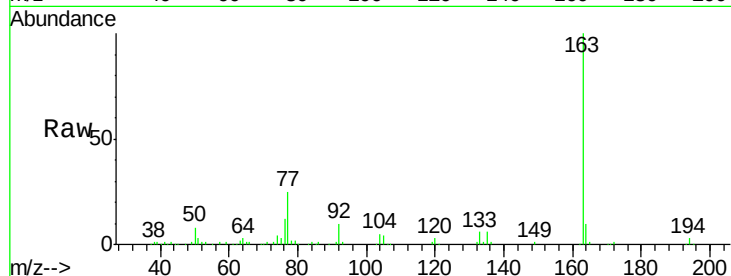

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

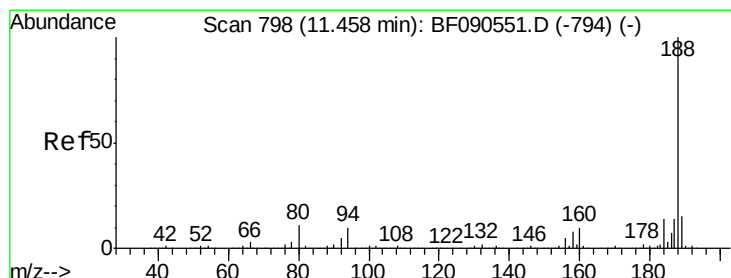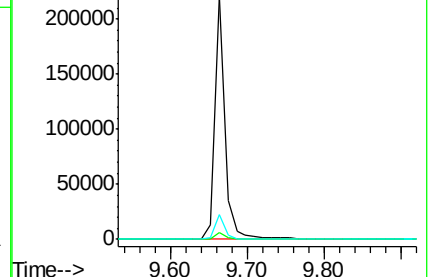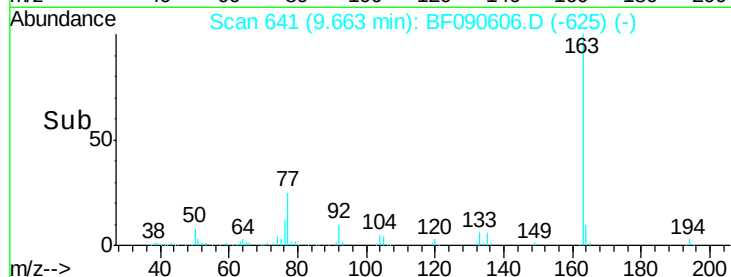

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.43 min Scan# 796

Delta R.T. -0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38


Tgt Ion:188 Resp: 639267

Ion Ratio Lower Upper

188 100

94 14.1 7.7 11.5#



80 16.2 8.6 12.8#

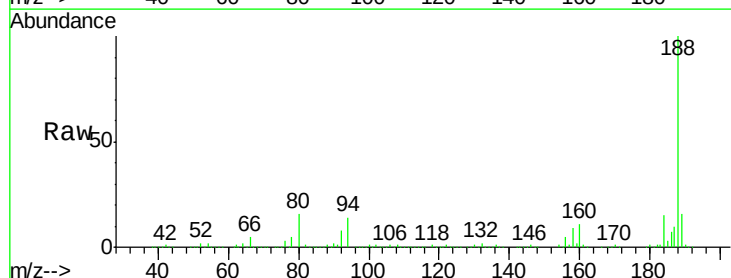


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

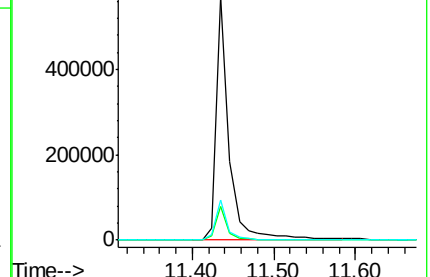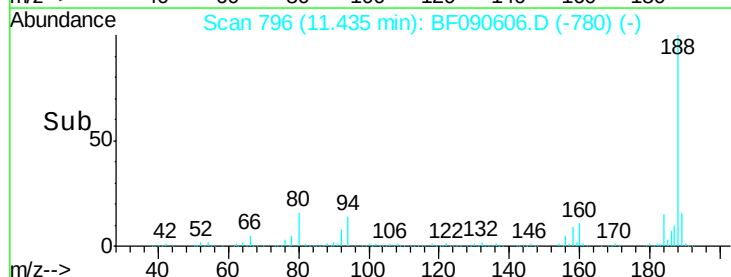

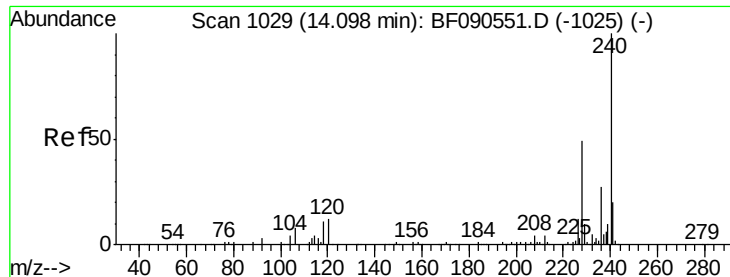

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.08 min Scan# 1027

Delta R.T. -0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38

Instrument :

BNA_F

ClientSampleId :

FK-BPM-02-001-A


Tot Ion:240 Resp: 566852

Ion Ratio Lower Upper

240 100

120 18.4 9.8 14.8#




236 26.8 21.7 32.5

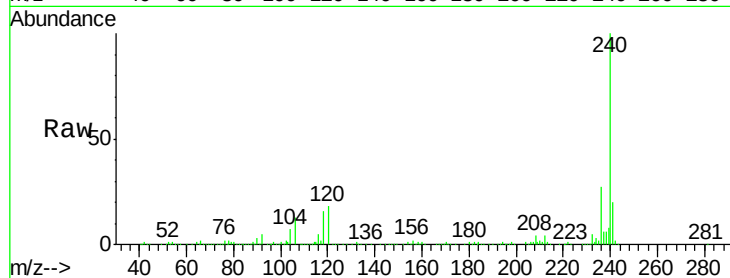

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

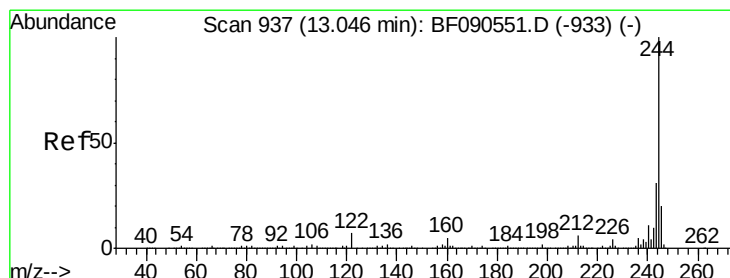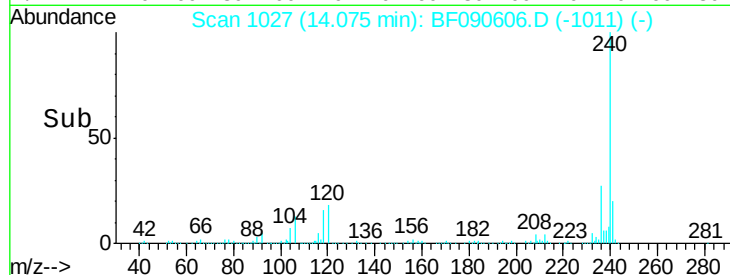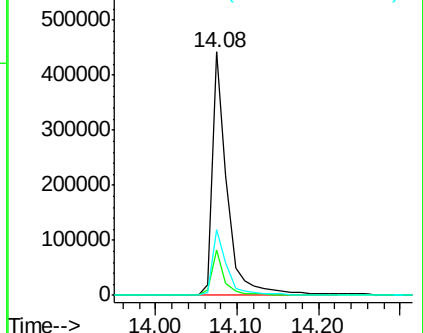

#78

Terphenyl-d14

Concen: 74.12 ng

RT: 13.02 min Scan# 935

Delta R.T. -0.01 min

Lab File: BF090606.D

Acq: 17 Oct 2016 14:38


Tgt Ion:244 Resp: 1804587

Ion Ratio Lower Upper

244 100

212 7.9 5.0 7.4#



122 16.9 5.6 8.4#

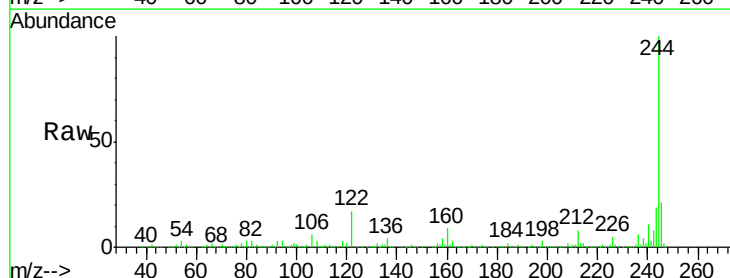


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

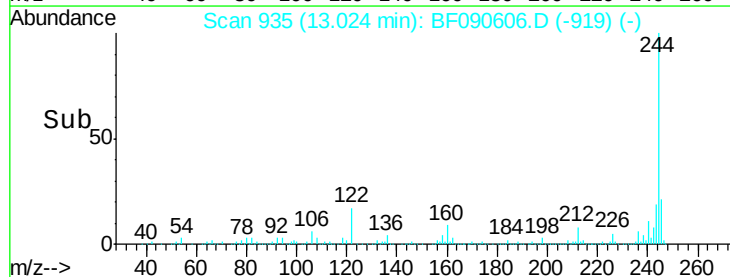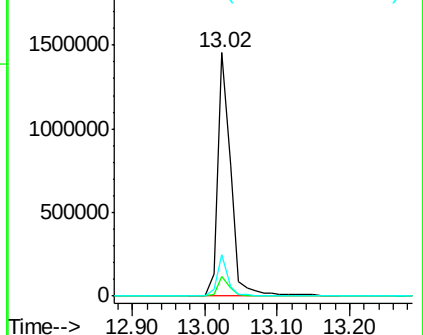


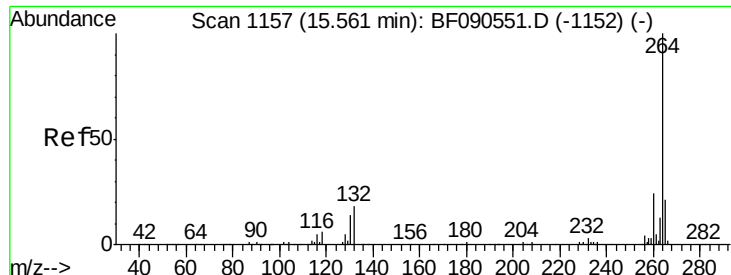

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.54 min Scan# 1155
Delta R.T. -0.00 min
Lab File: BF090606.D
Acq: 17 Oct 2016 14:38

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-001-A

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.3	28.9
265	21.2	16.7	25.1

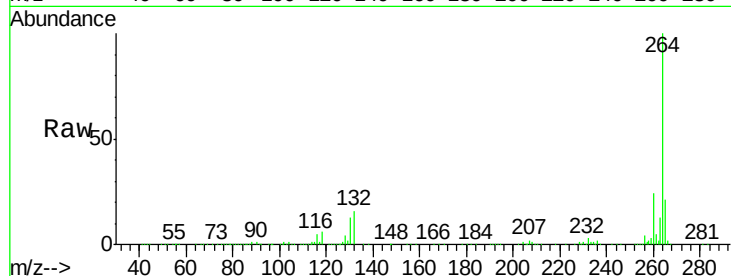

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

