


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101716\
 Data File : BF090600.D
 Acq On : 17 Oct 2016 10:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 17 19:19:58 2016

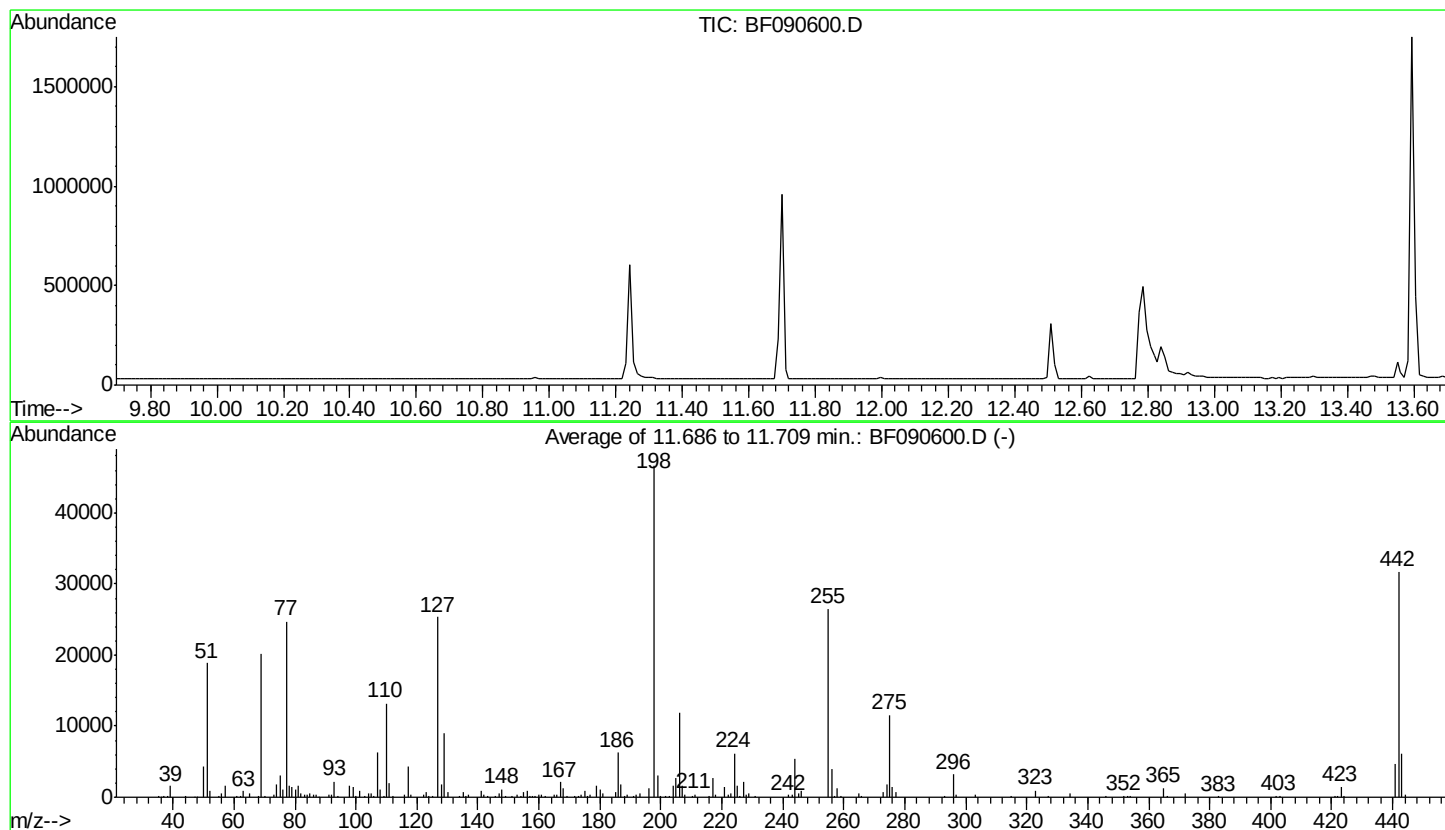

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	18855	PASS
68	69	0.00	2	1.0	211	PASS
69	198	0.00	100	43.2	20156	PASS
70	69	0.00	2	0.5	105	PASS
127	198	10	80	54.3	25320	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46644	PASS
199	198	5	9	6.5	3020	PASS
275	198	10	60	24.7	11529	PASS
365	198	1	100	2.7	1279	PASS
441	442	0.01	24	15.0	4753	PASS
442	198	50	100	68.1	31785	PASS
443	442	15	24	19.2	6114	PASS