


Data Path : Z:\HPCHEM1\BNA F\Data\BF101716\
 Data File : BF090604.D
 Acq On : 17 Oct 2016 13:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

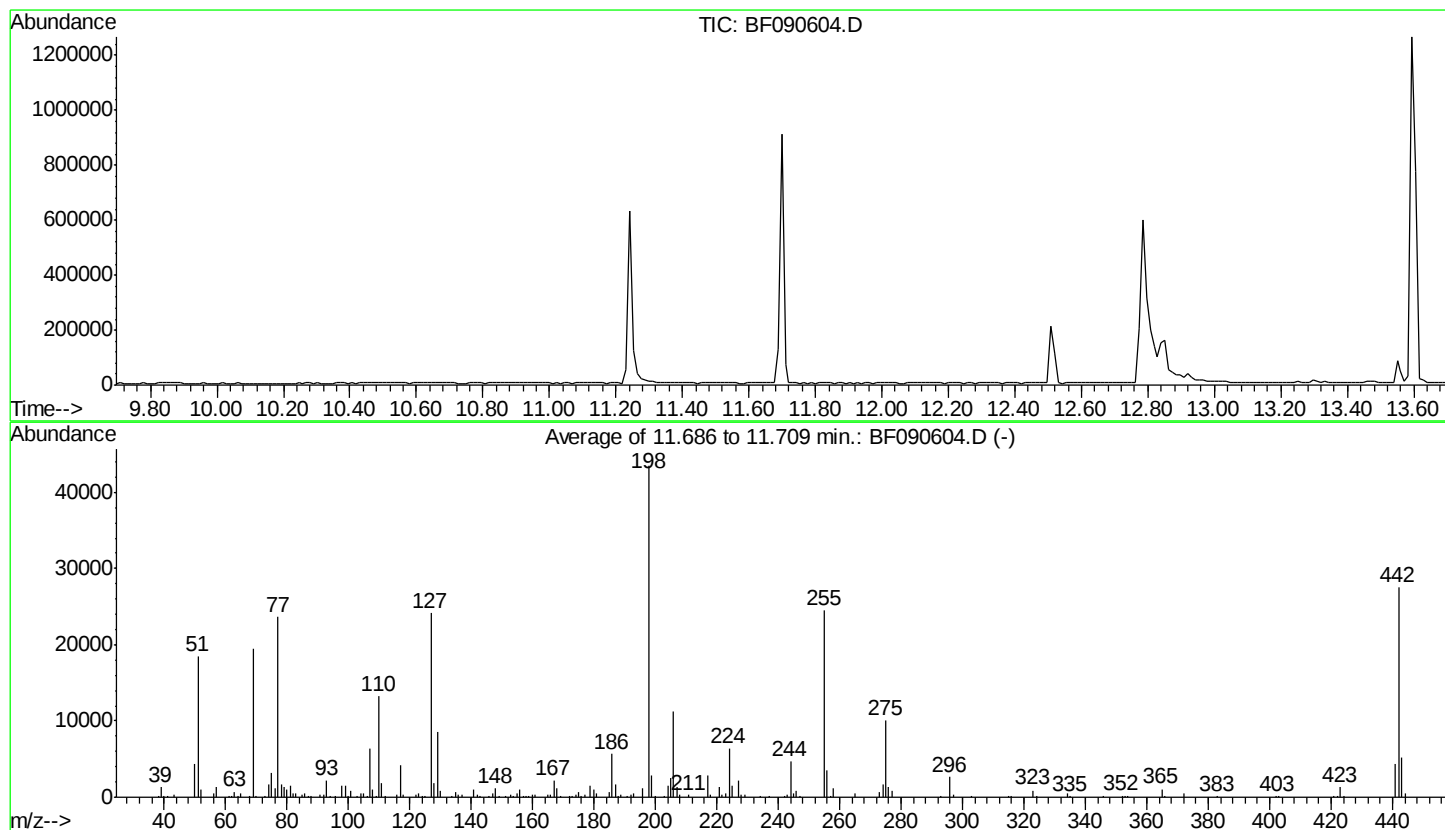

AutoFind: Scans 818, 819, 820; Background Corrected with Scan 815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	18405	PASS
68	69	0.00	2	1.0	203	PASS
69	198	0.00	100	44.7	19449	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	55.5	24157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43504	PASS
199	198	5	9	6.5	2819	PASS
275	198	10	60	23.1	10052	PASS
365	198	1	100	2.5	1088	PASS
441	442	0.01	24	16.1	4421	PASS
442	198	50	100	63.2	27504	PASS
443	442	15	24	19.0	5213	PASS