

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101717\
 Data File : BF099598.D
 Acq On : 17 Oct 2017 23:09
 Operator : SJ/JU
 Sample : I5869-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-7S-10-11-17

Quant Time: Oct 18 00:22:49 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 17 17:32:20 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	105002	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	422576	20.00	ng	0.00
38) Acenaphthene-d10	9.86	164	182582	20.00	ng	0.00
63) Phenanthrene-d10	11.35	188	267300	20.00	ng	0.00
75) Chrysene-d12	13.99	240	171063	20.00	ng	0.00
86) Perylene-d12	15.45	264	185441	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	408905	61.99	ng	0.01
7) Phenol-d6	6.47	99	301199	37.02	ng	0.00
23) Nitrobenzene-d5	7.40	82	612567	92.96	ng	0.00
41) 2,4,6-Tribromophenol	10.66	330	156329	104.64	ng	0.00
44) 2-Fluorobiphenyl	9.19	172	1118365	102.26	ng	0.00
78) Terphenyl-d14	12.93	244	665324	88.45	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.57	163	38836	2.818	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101717\
Data File : BF099598.D
Acq On : 17 Oct 2017 23:09
Operator : SJ/JU
Sample : I5869-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-7S-10-11-17

Quant Time: Oct 18 00:22:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 17 17:32:20 2017
Response via : Initial Calibration

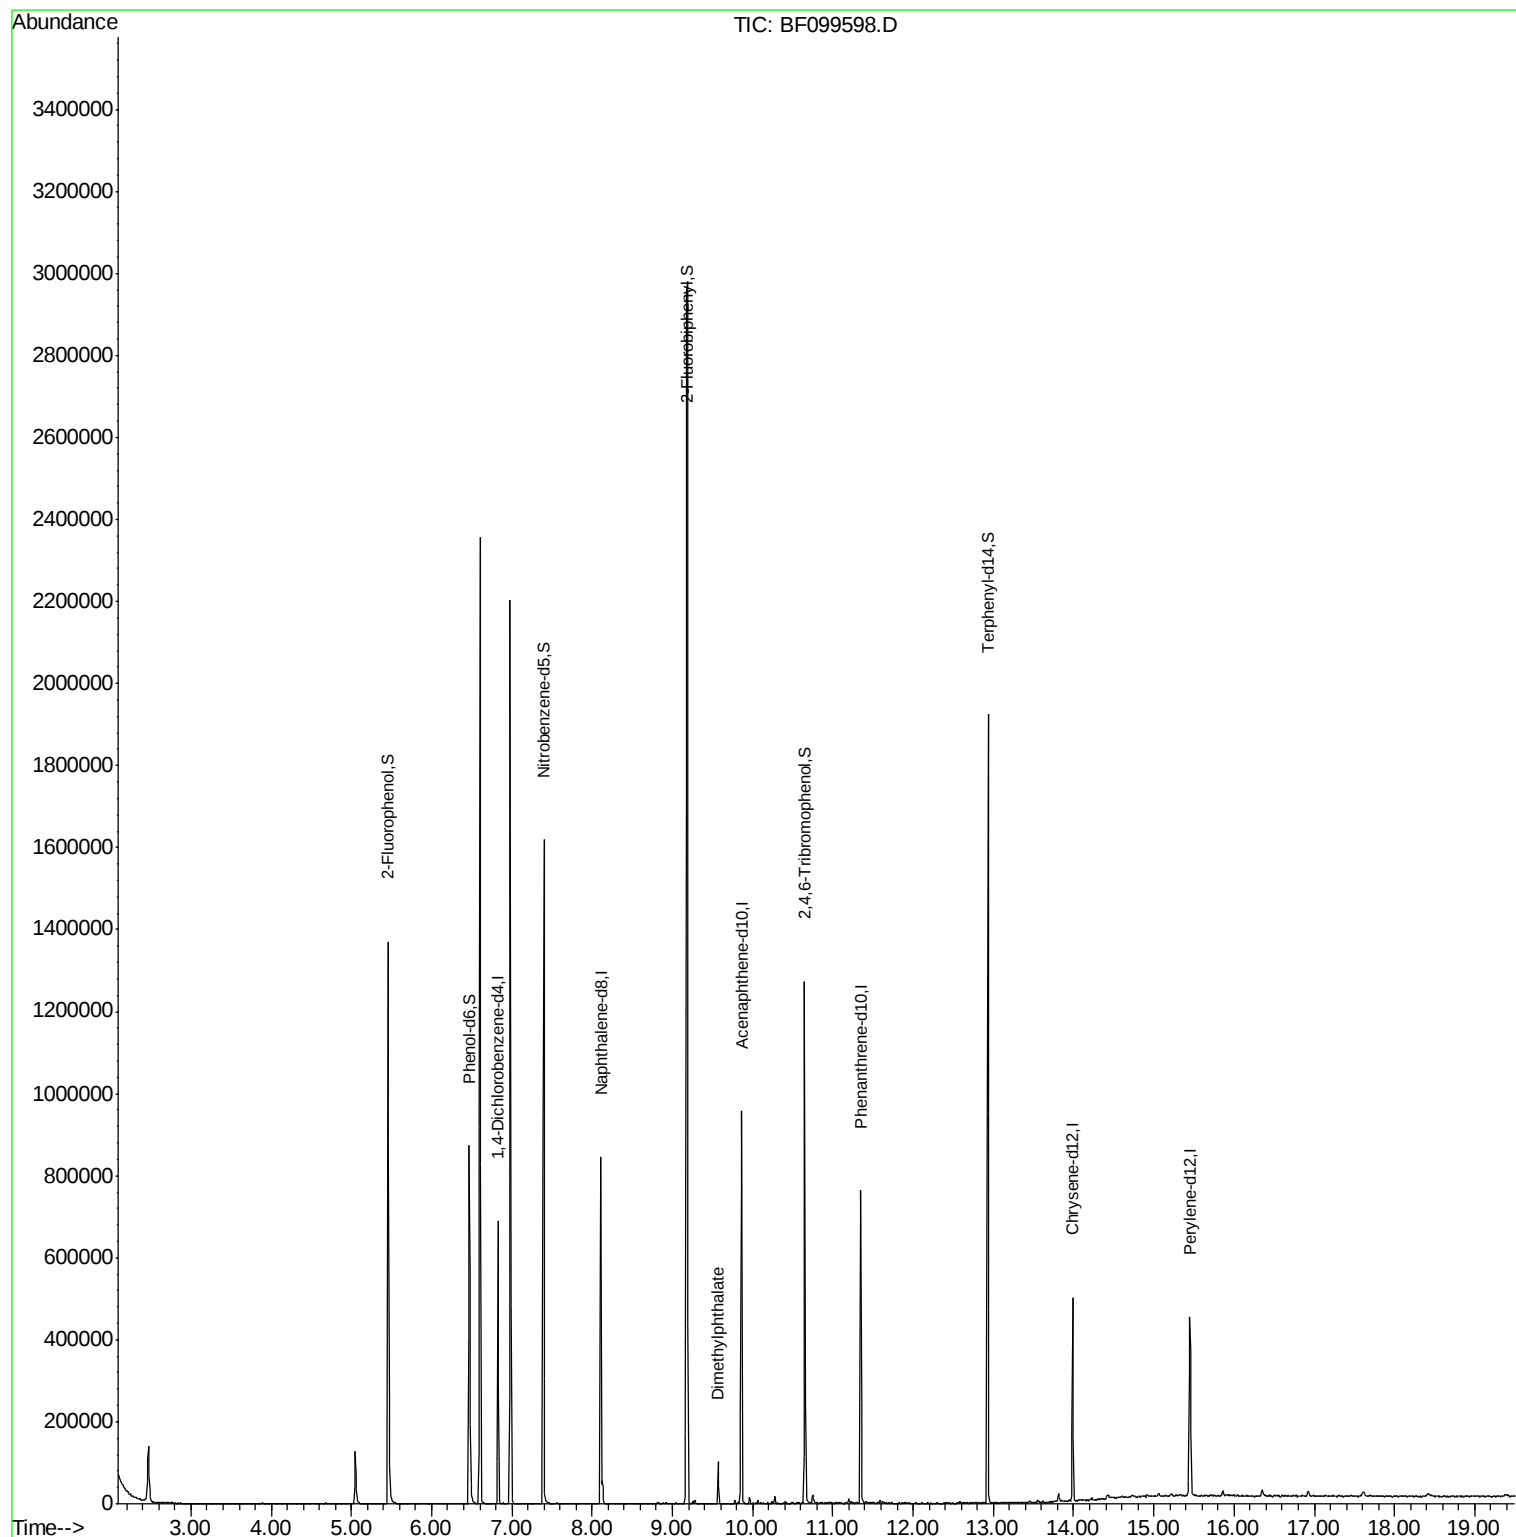

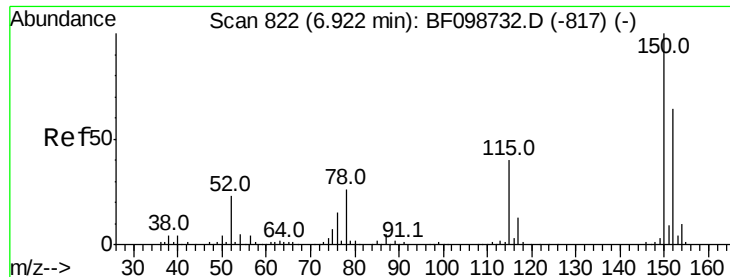


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 806
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09

Instrument :
 BNA_F
 ClientSampleId :
 MW-7S-10-11-17

Tot Ion:152 Resp: 105002
 Ion Ratio Lower Upper
 152 100
 150 157.2 124.6 186.8
 115 57.9 50.1 75.1

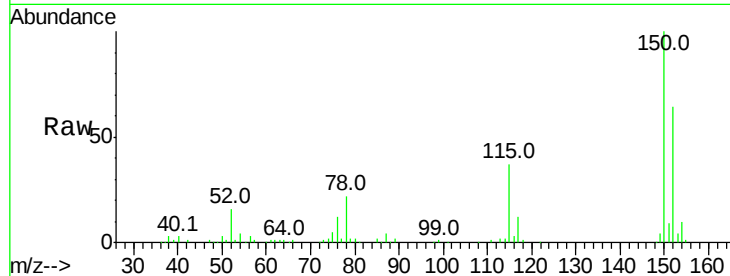


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

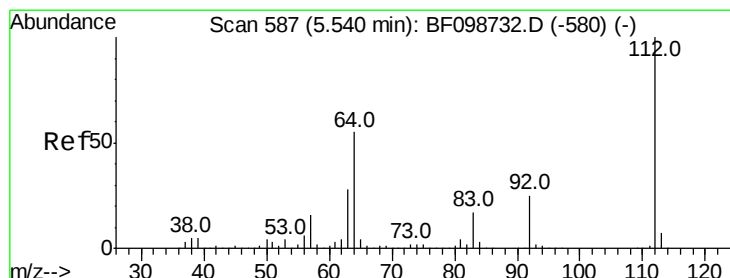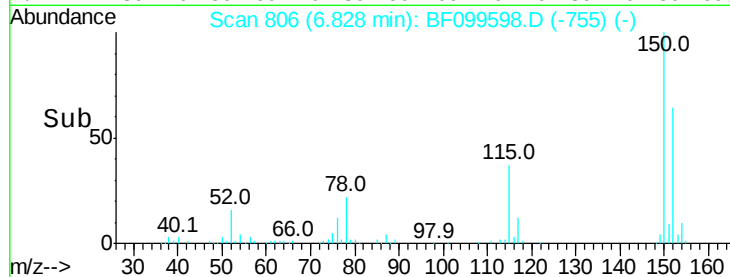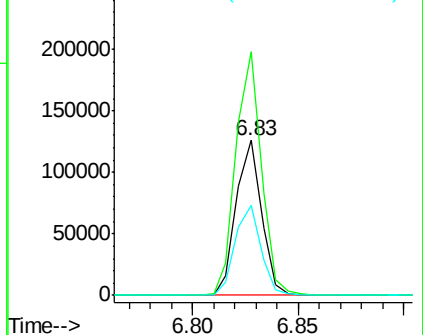



#5


2-Fluorophenol
 Concen: 61.993 ng
 RT: 5.46 min Scan# 573
 Delta R.T. 0.01 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09

Tgt Ion:112 Resp: 408905
 Ion Ratio Lower Upper
 112 100
 64 53.7 47.9 71.9
 63 26.1 23.7 35.5

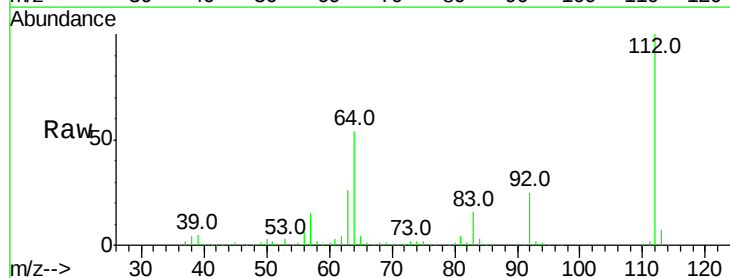

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

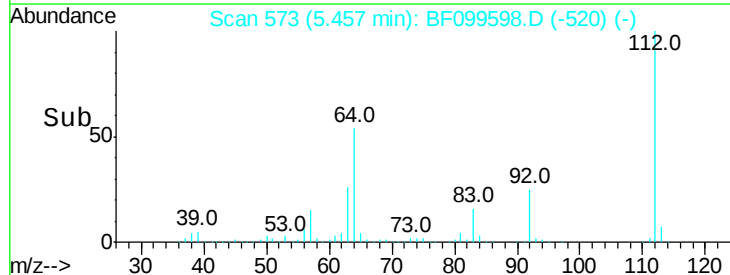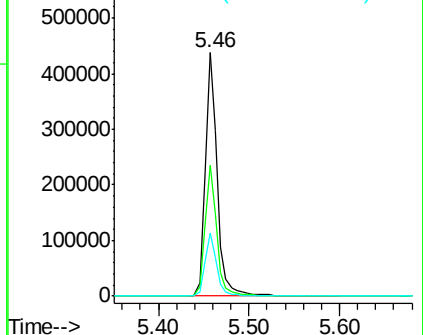

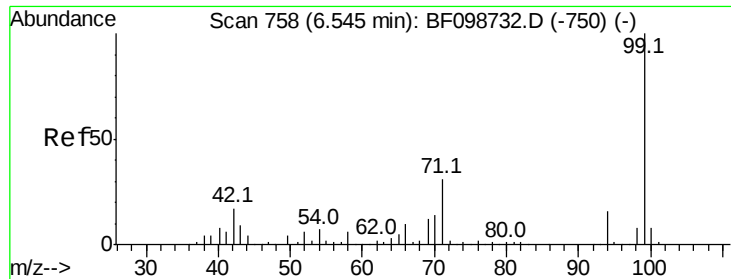

#7

Phenol-d6

Concen: 37.016 ng

RT: 6.47 min Scan# 745

Delta R.T. -0.00 min

Lab File: BF099598.D

Acq: 17 Oct 2017 23:09

Instrument :

BNA_F

ClientSampleId :

MW-7S-10-11-17


Tot Ion: 99 Resp: 301199

Ion Ratio Lower Upper

99 100

42 14.8 14.5 21.7




71 29.0 25.4 38.0

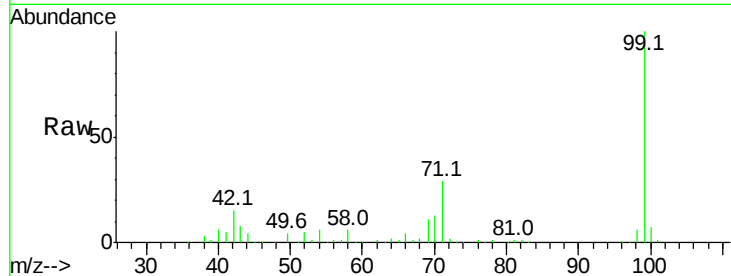

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

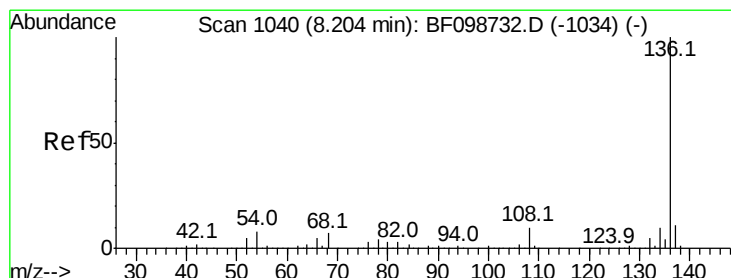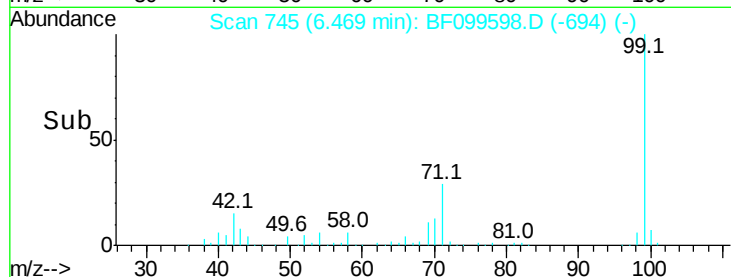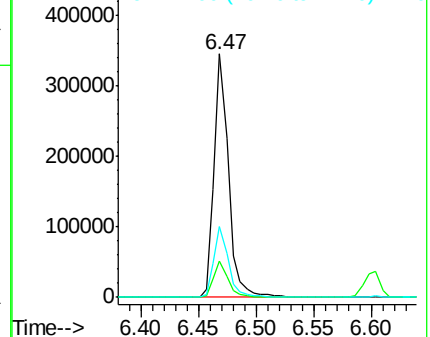

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.11 min Scan# 1024

Delta R.T. -0.00 min

Lab File: BF099598.D

Acq: 17 Oct 2017 23:09

Tgt Ion: 136 Resp: 422576


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 6.6 6.6 9.8

68 5.3 5.0 7.4


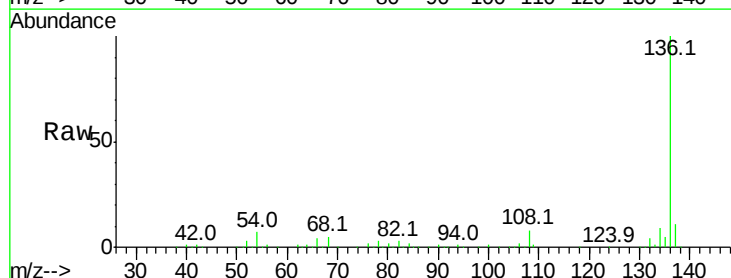



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



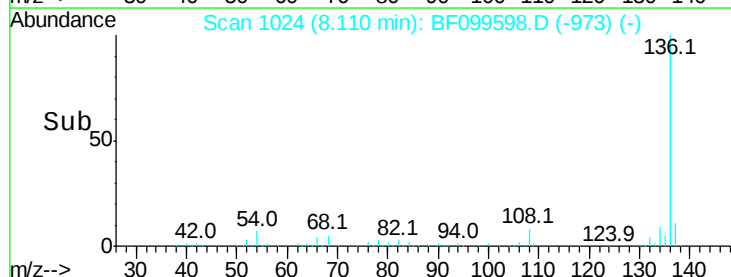
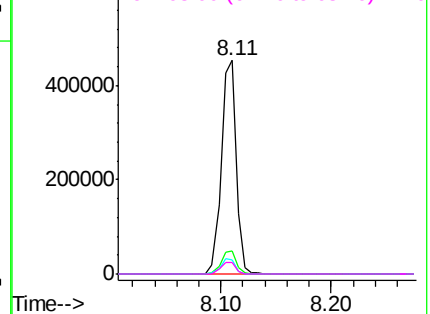


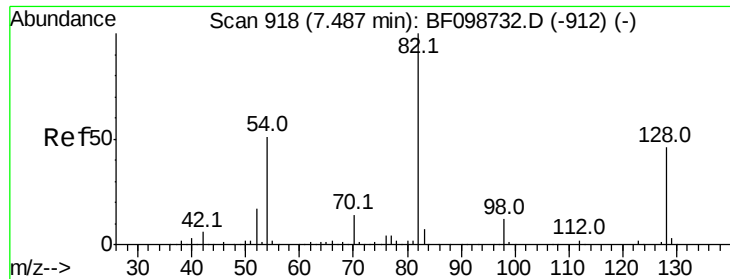

#23
 Nitrobenzene-d5
 Concen: 92.963 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09




Instrument :
 BNA_F
 ClientSampleId :
 MW-7S-10-11-17


Tot Ion	82	Resp	612567
Ion Ratio	100		
Lower	36.1		
Upper	54.1		
54	43.9	41.4	62.2

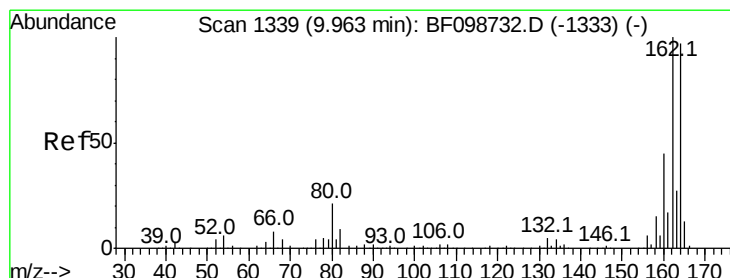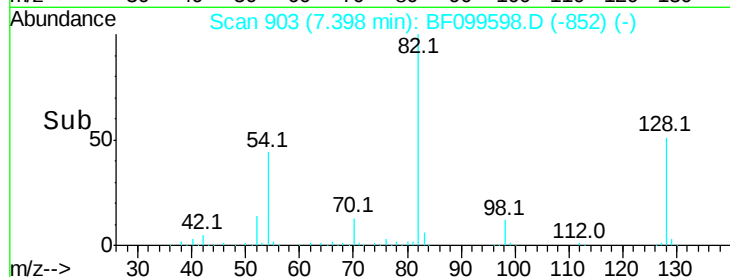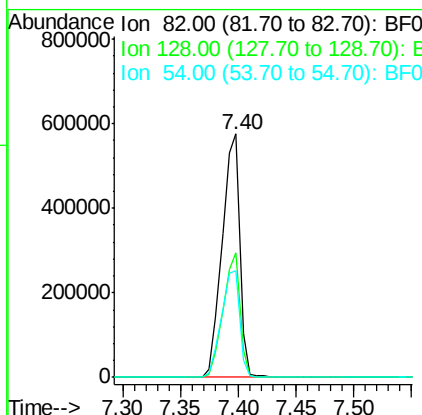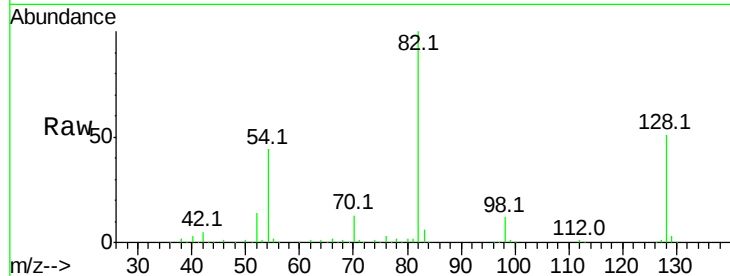

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.86 min Scan# 1322
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09

Tgt Ion	164	Resp	182582
Ion Ratio	100		
Lower	86.1		
Upper	129.1		
162	107.8	38.3	57.5
160	46.7		


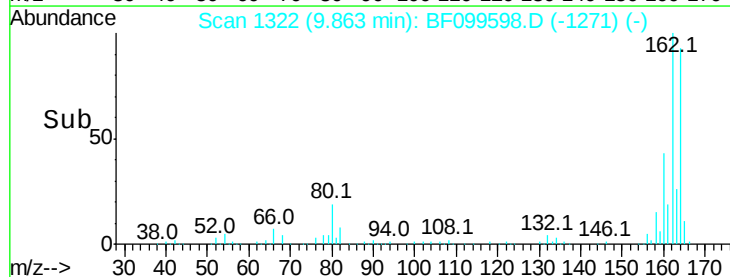
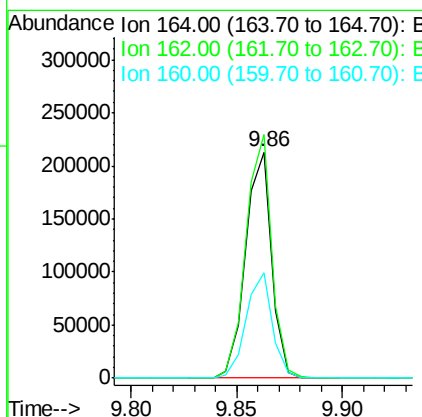
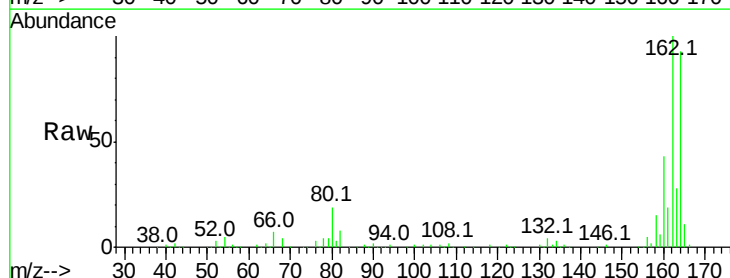


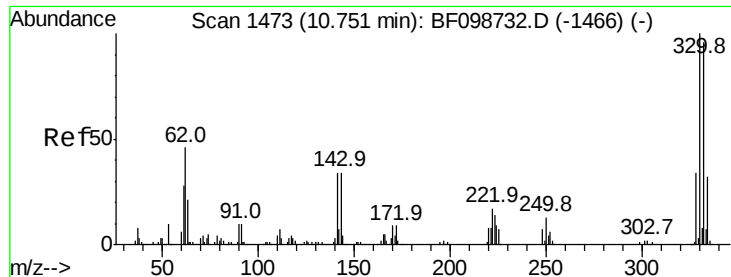

#41
 2,4,6-Tribromophenol
 Concen: 104.637 ng
 RT: 10.66 min Scan# 1457
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09




Instrument :
 BNA_F
 ClientSampleId :
 MW-7S-10-11-17


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.0	115.6
141	37.2	29.9	44.9

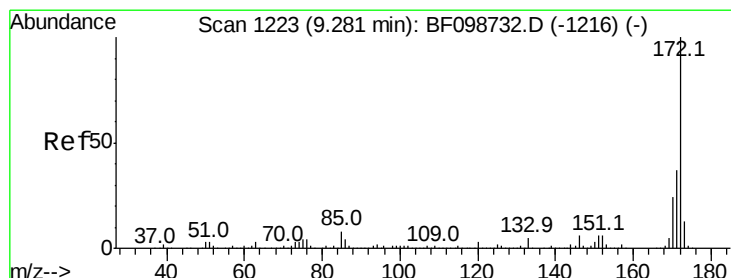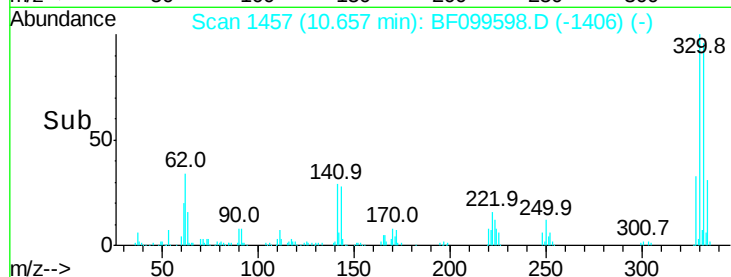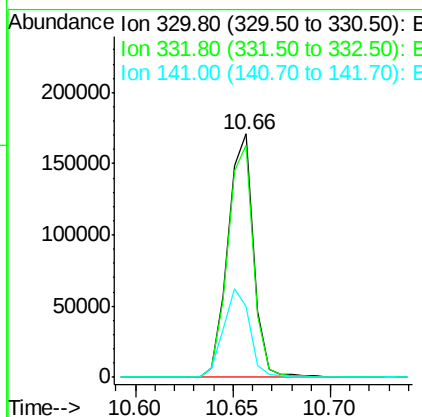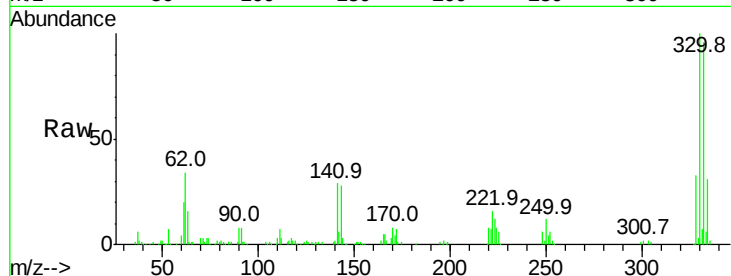

#44
 2-Fluorobiphenyl
 Concen: 102.256 ng
 RT: 9.19 min Scan# 1207
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.7	44.5
170	24.0	19.6	29.4

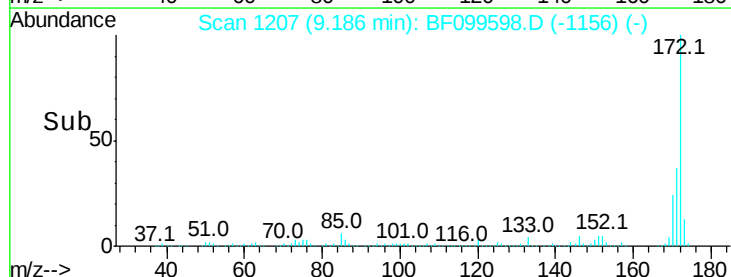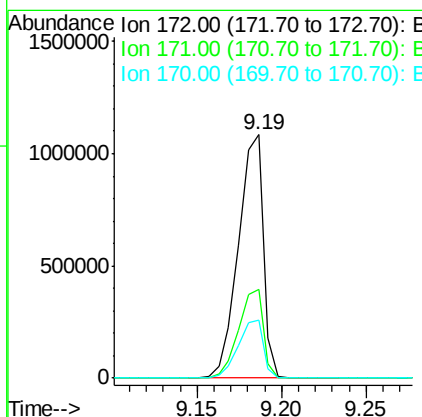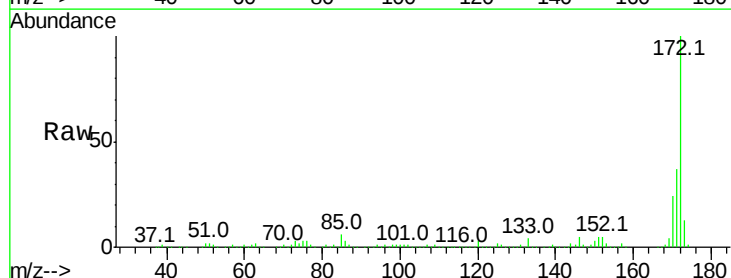


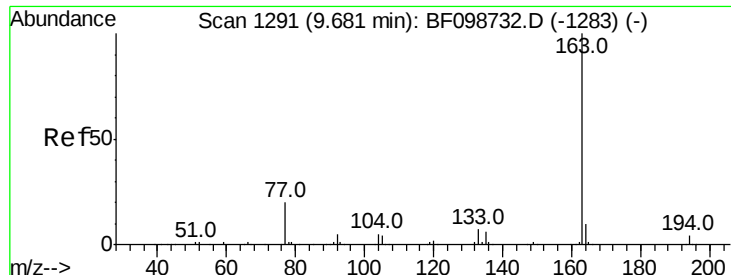




#49
Dimethylphthalate
Concen: 2.818 ng
RT: 9.57 min Scan# 1273
Delta R.T. -0.01 min
Lab File: BF099598.D
Acq: 17 Oct 2017 23:09

Instrument :
BNA_F
ClientSampleId :
MW-7S-10-11-17

Tot Ion:163 Resp: 38836
Ion Ratio Lower Upper
163 100
194 3.9 2.7 4.1
164 10.3 8.2 12.2

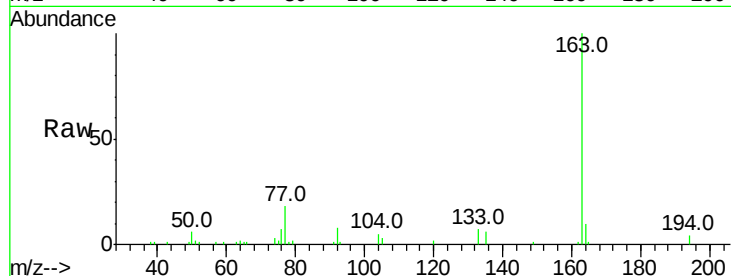


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

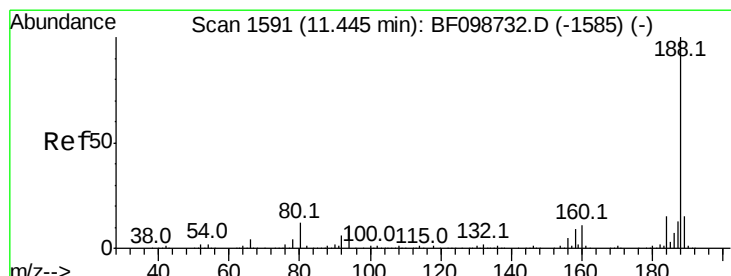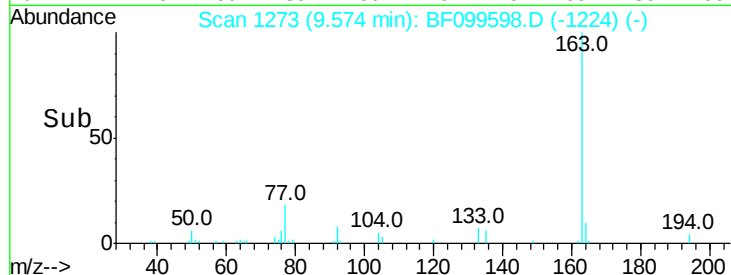
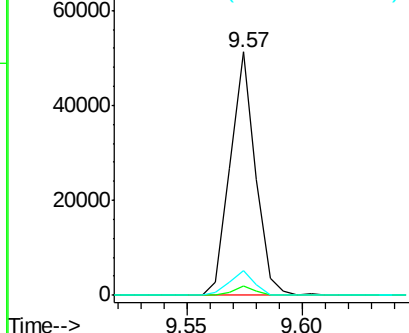



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.35 min Scan# 1575
Delta R.T. -0.00 min
Lab File: BF099598.D
Acq: 17 Oct 2017 23:09

Tgt Ion:188 Resp: 267300
Ion Ratio Lower Upper
188 100
94 10.1 8.5 12.7
80 10.6 9.2 13.8

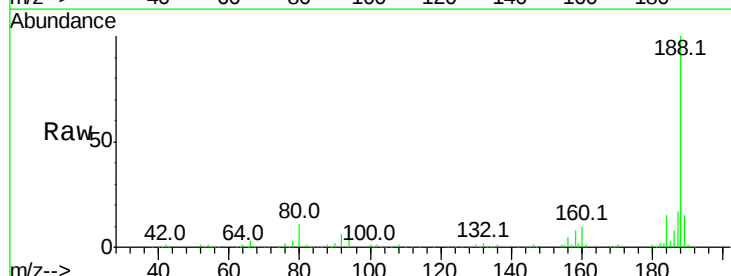

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

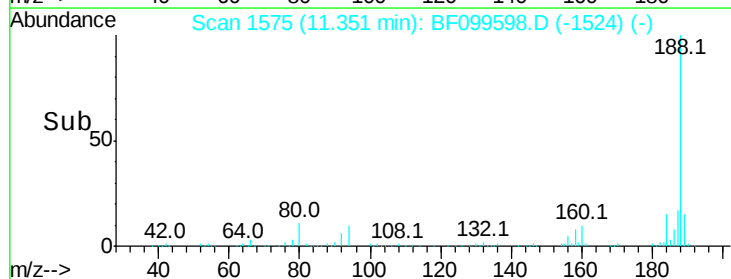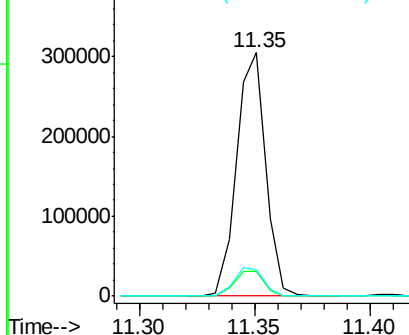

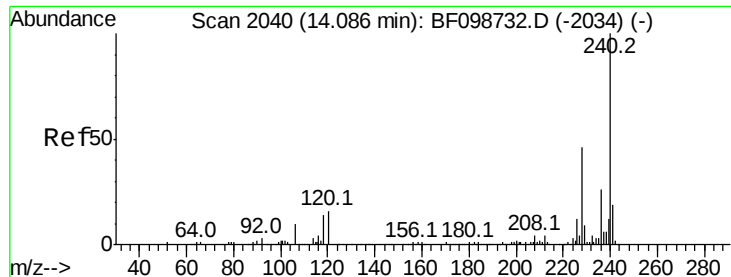

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.99 min Scan# 2024

Delta R.T. -0.01 min

Lab File: BF099598.D

Acq: 17 Oct 2017 23:09

Instrument :

BNA_F

ClientSampleId :

MW-7S-10-11-17


Tot Ion:240 Resp: 171063

Ion Ratio Lower Upper

240 100

120 12.1 9.5 14.3




236 25.8 20.7 31.1

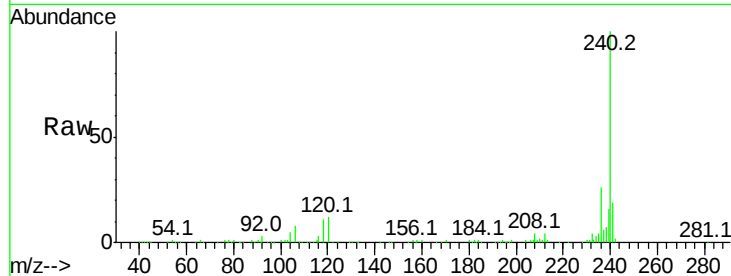

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

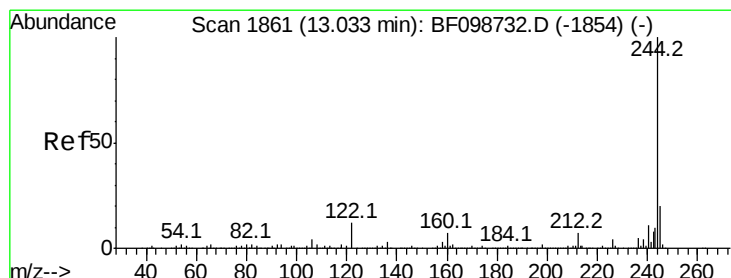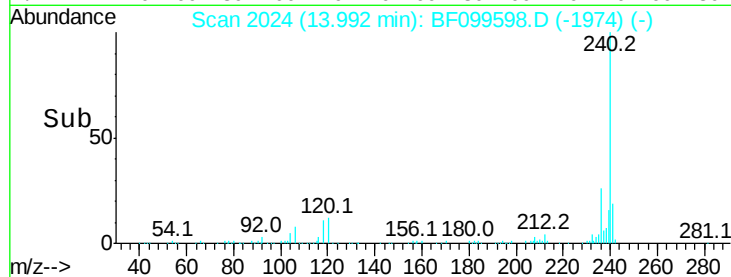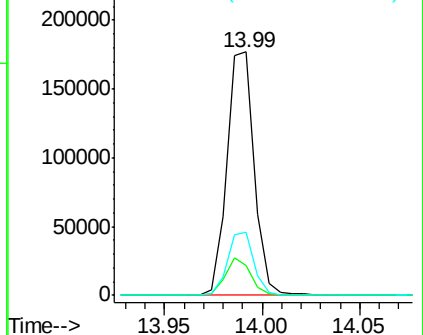

#78

Terphenyl-d14

Concen: 88.452 ng

RT: 12.93 min Scan# 1844

Delta R.T. -0.00 min

Lab File: BF099598.D

Acq: 17 Oct 2017 23:09


Tgt Ion:244 Resp: 665324

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0



122 12.5 11.0 16.4

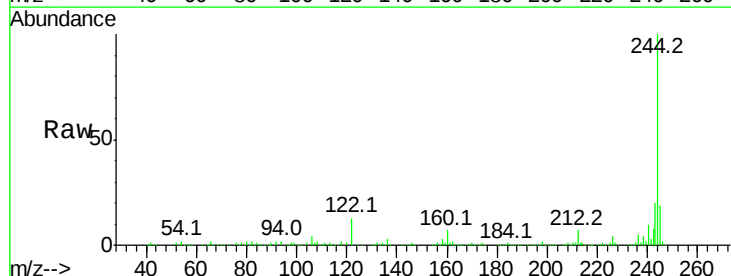


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

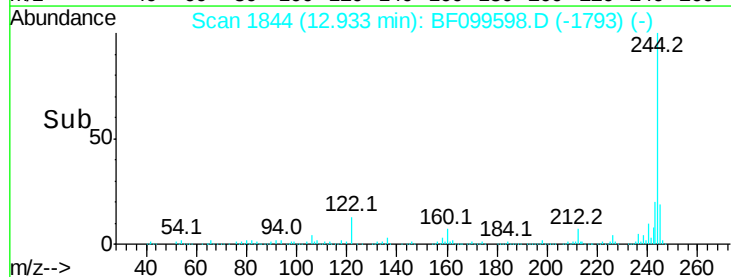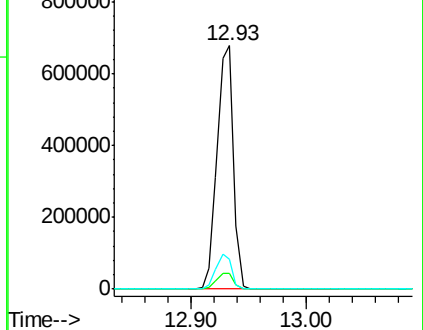


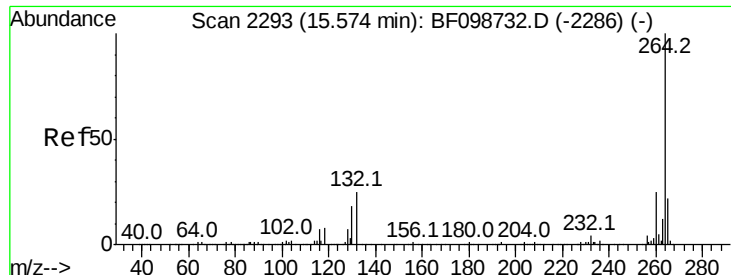

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.45 min Scan# 2272
 Delta R.T. -0.00 min
 Lab File: BF099598.D
 Acq: 17 Oct 2017 23:09

Instrument :
 BNA_F
 ClientSampleId :
 MW-7S-10-11-17

Tot Ion: 264 Resp: 185441
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.2 28.8
 265 21.8 17.5 26.3

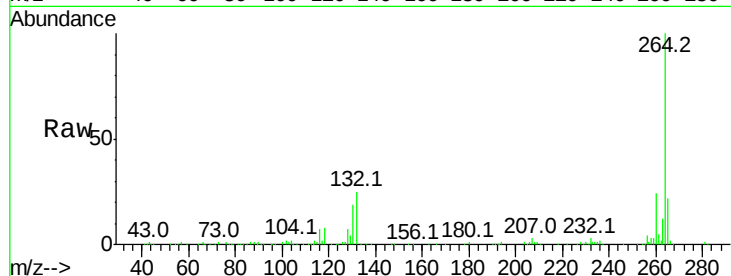

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

