

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101717\
 Data File : BF099584.D
 Acq On : 17 Oct 2017 16:42
 Operator : SJ/JU
 Sample : I5875-01RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TK2064L-T1-T2-T3RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.040	499	502	515	rBV	48084	59794	1.90%	0.414%
2	5.440	567	570	584	rVB	283489	327022	10.40%	2.266%
3	6.457	740	743	755	rBV	278754	305750	9.72%	2.118%
4	6.593	763	766	772	rBV	589721	485805	15.45%	3.366%
5	6.822	802	805	812	rBV	663829	611046	19.43%	4.234%
6	6.898	812	818	821	rVV	547212	514306	16.36%	3.563%
7	6.934	821	824	827	rVV	150514	120286	3.83%	0.833%
8	6.981	828	832	841	rVB	591894	521572	16.59%	3.614%
9	7.387	898	901	908	rBV	460458	399035	12.69%	2.765%
10	7.504	912	921	926	rBV	105061	161191	5.13%	1.117%
11	7.834	971	977	981	rBV	2685577	3144598	100.00%	21.787%
12	7.939	991	995	998	rVB	181070	155549	4.95%	1.078%
13	8.104	1019	1023	1025	rBV	919347	867740	27.59%	6.012%
14	8.128	1025	1027	1030	rVB	529550	401210	12.76%	2.780%
15	8.816	1140	1144	1151	rVB	295166	306425	9.74%	2.123%
16	8.916	1156	1161	1164	rBV	179086	149247	4.75%	1.034%
17	9.175	1200	1205	1209	rBV	891364	778641	24.76%	5.395%
18	9.439	1246	1250	1255	rBV2	38707	54751	1.74%	0.379%
19	9.516	1259	1263	1266	rVV	68501	69224	2.20%	0.480%
20	9.575	1270	1273	1278	rVB	91290	79996	2.54%	0.554%
21	9.857	1317	1321	1325	rVV	1033359	975108	31.01%	6.756%
22	9.998	1342	1345	1348	rBV	45955	39785	1.27%	0.276%
23	10.281	1386	1393	1395	rBV2	48074	52857	1.68%	0.366%
24	10.645	1452	1455	1465	rVB	373080	363155	11.55%	2.516%
25	10.751	1470	1473	1477	rBV	57932	69867	2.22%	0.484%
26	10.786	1477	1479	1483	rVB	53679	43229	1.37%	0.300%
27	11.227	1551	1554	1560	rVB2	27082	38272	1.22%	0.265%
28	11.345	1571	1574	1578	rBV	1075291	974774	31.00%	6.754%
29	11.863	1659	1662	1667	rBV	64277	69948	2.22%	0.485%
30	12.927	1839	1843	1846	rVB	785274	703941	22.39%	4.877%
31	13.480	1934	1937	1940	rBV4	25170	32848	1.04%	0.228%
32	13.810	1990	1993	1996	rBV2	66732	66191	2.10%	0.459%
33	13.951	2014	2017	2020	rVB	78119	66304	2.11%	0.459%
34	13.986	2020	2023	2027	rBV	791072	715797	22.76%	4.959%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101717\
Data File : BF099584.D
Acq On : 17 Oct 2017 16:42
Operator : SJ/JU
Sample : I5875-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TK2064L-T1-T2-T3RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.451	2266	2272	2281	rVB	479350	607584	19.32%	4.210%
36	15.857	2338	2341	2345	rVB	24609	33029	1.05%	0.229%
37	16.351	2421	2425	2432	rVB4	16982	31977	1.02%	0.222%
38	17.609	2634	2639	2648	rVB8	14957	35598	1.13%	0.247%


Sum of corrected areas: 14433452

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101717\
Data File : BF099584.D
Acq On : 17 Oct 2017 16:42
Operator : SJ/JU
Sample : I5875-01RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TK2064L-T1-T2-T3RE

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

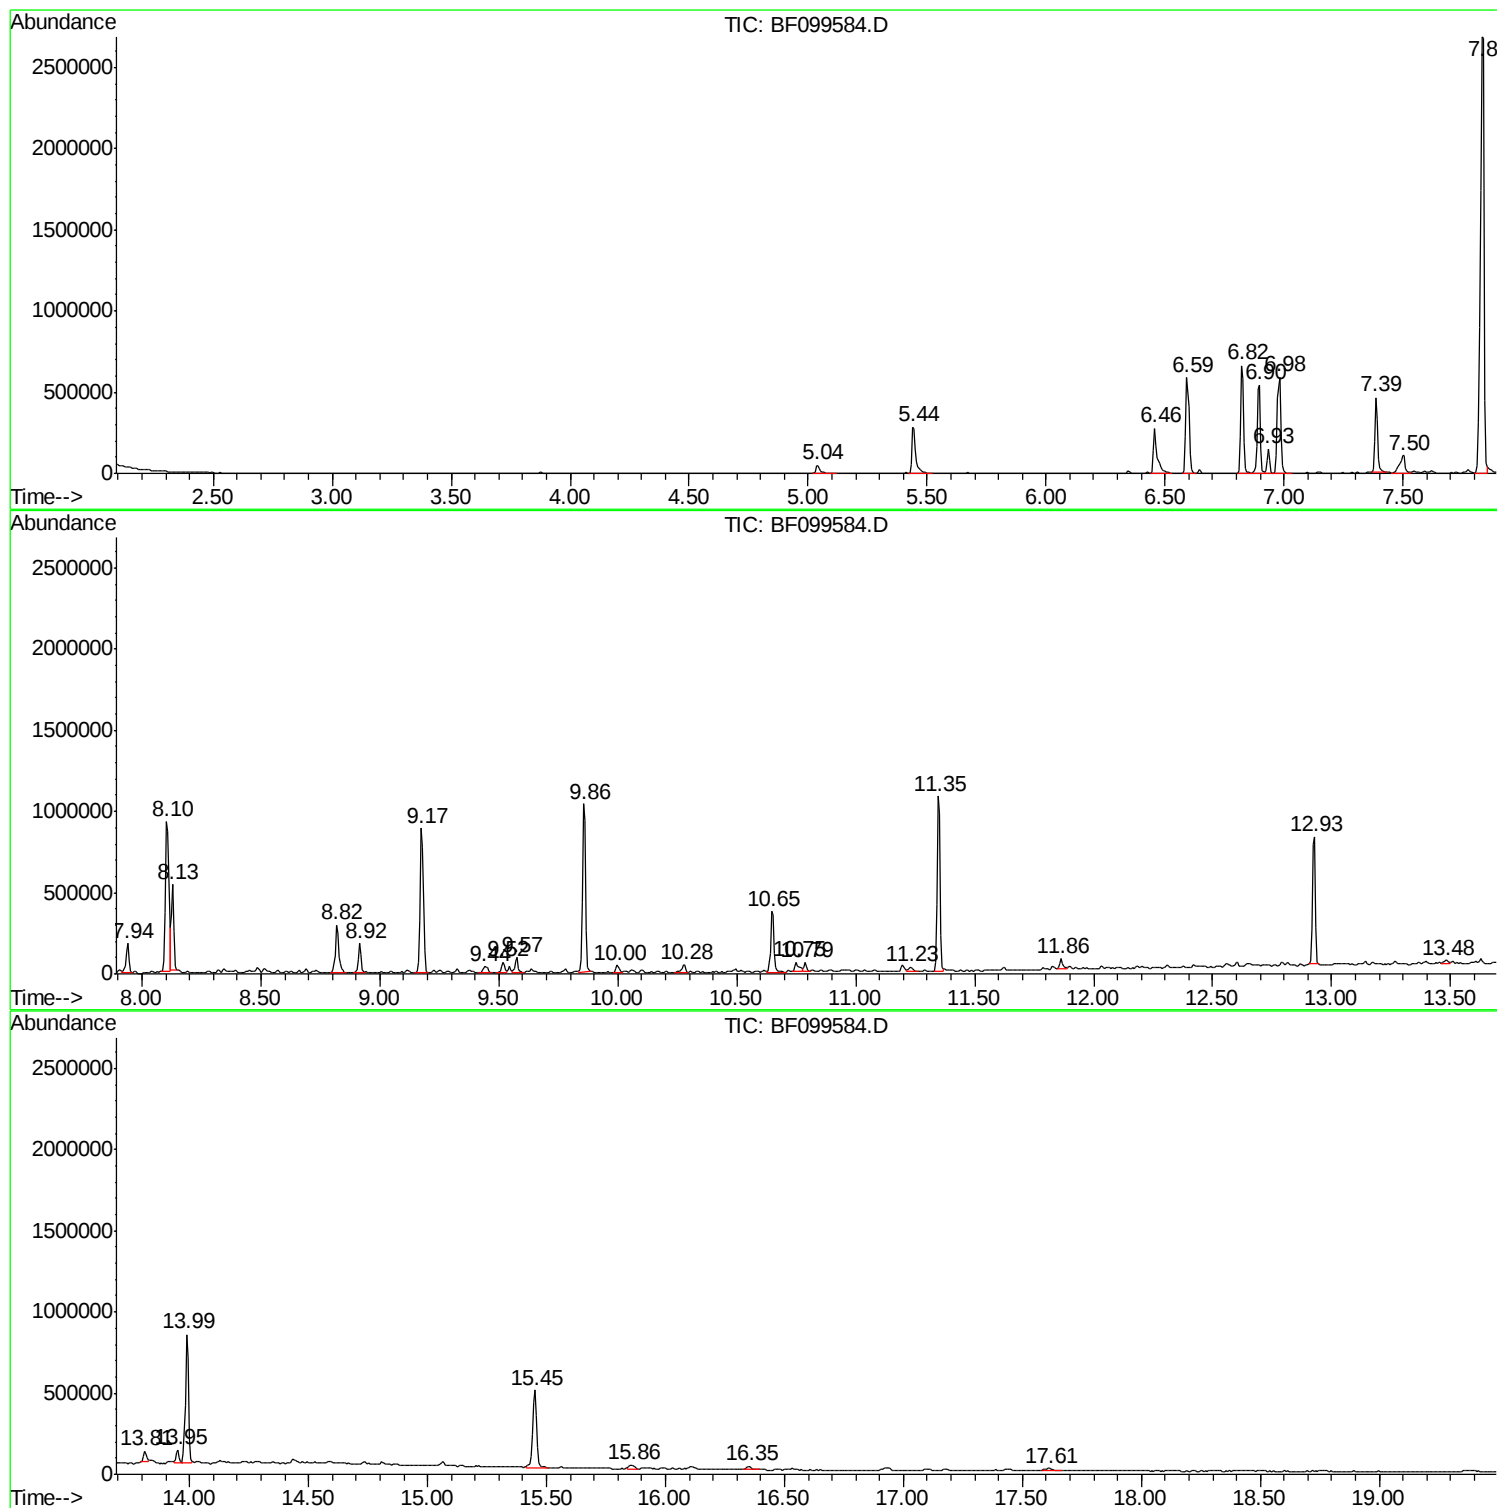

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF101717\
Data_File : BF099584.D
Acq_On : 17 Oct 2017 16:422
Operator : SJ/JUU
Sample : I5875-01REE
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
TK2064L-T1-T2-T3RE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
