


Data Path : Z:\HPCHEM1\BNA F\Data\BF101717\
 Data File : BF099580.D
 Acq On : 17 Oct 2017 14:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 17 17:32:20 2017

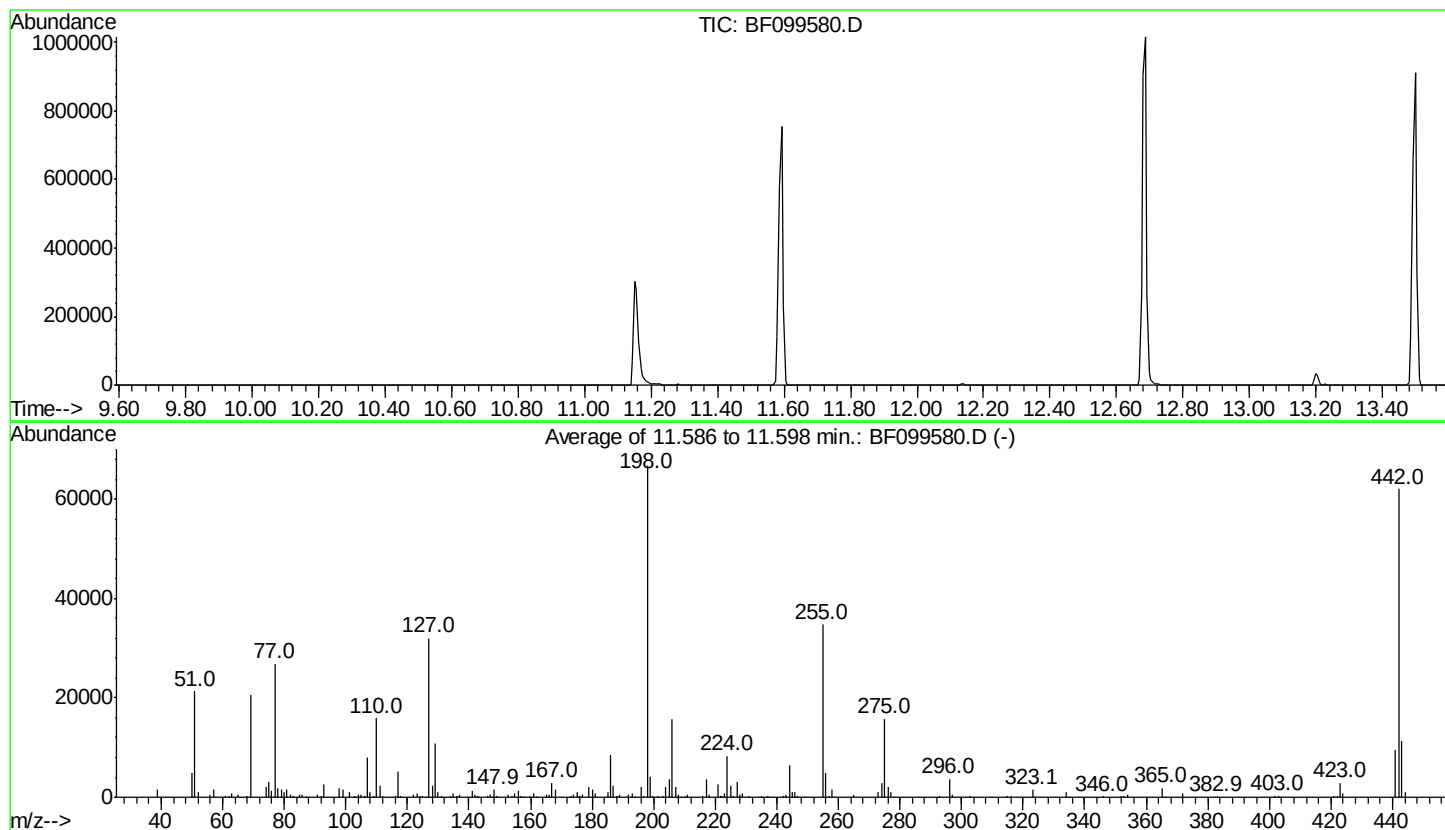

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	21260	PASS
68	69	0.00	2	1.8	364	PASS
69	198	0.00	100	31.0	20689	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	31962	PASS
197	198	0.00	2	0.4	250	PASS
198	198	100	100	100.0	66728	PASS
199	198	5	9	6.3	4209	PASS
275	198	10	60	23.7	15787	PASS
365	198	1	100	2.9	1937	PASS
441	442	0.01	24	15.5	9603	PASS
442	198	50	100	93.0	62069	PASS
443	442	15	24	18.3	11366	PASS