
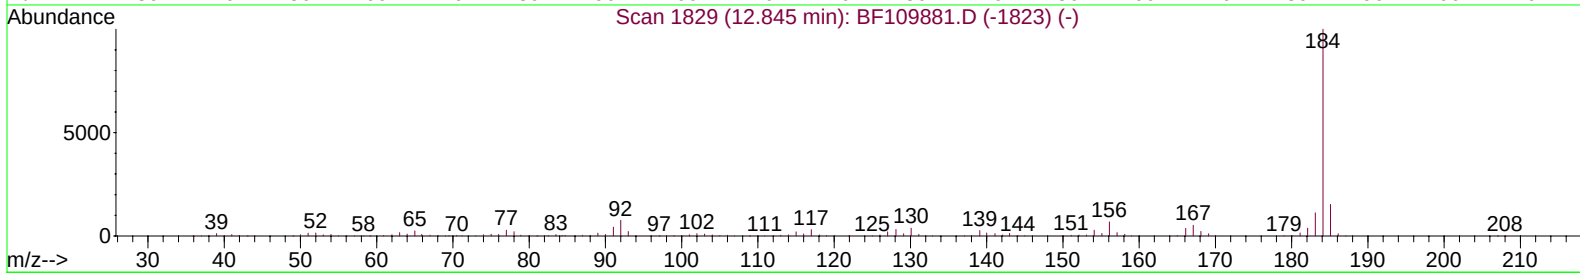
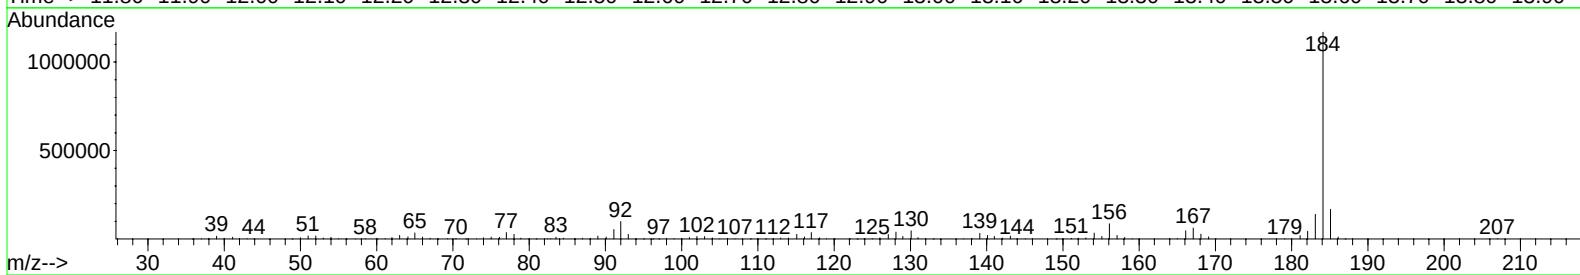


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101718\  
Data File   : BF109923.D  
Acq On      : 17 Oct 2018   16:43  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Oct 22 08:08:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

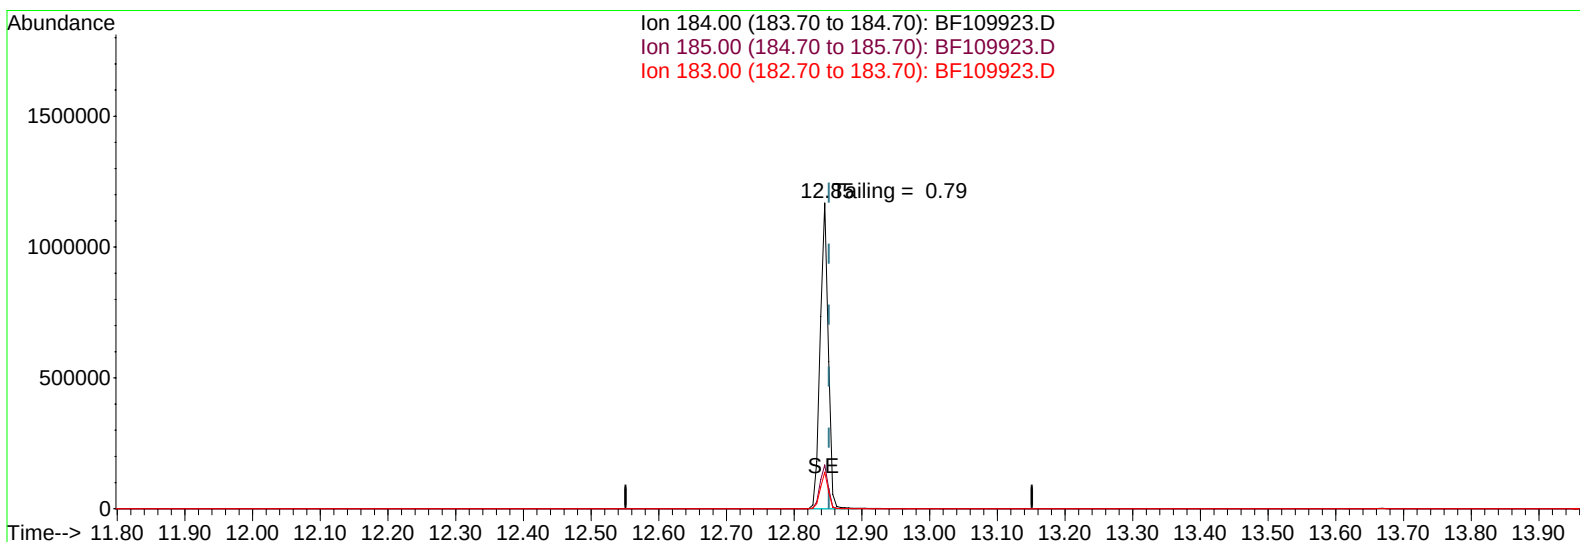

TIC: BF109923.D

(77) Benzidine




12.845min (-0.006) 0.00ng

response 970979

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.32
183.00	11.80	11.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101718\
Data File : BF109923.D
Acq On : 17 Oct 2018 16:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 08:08:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

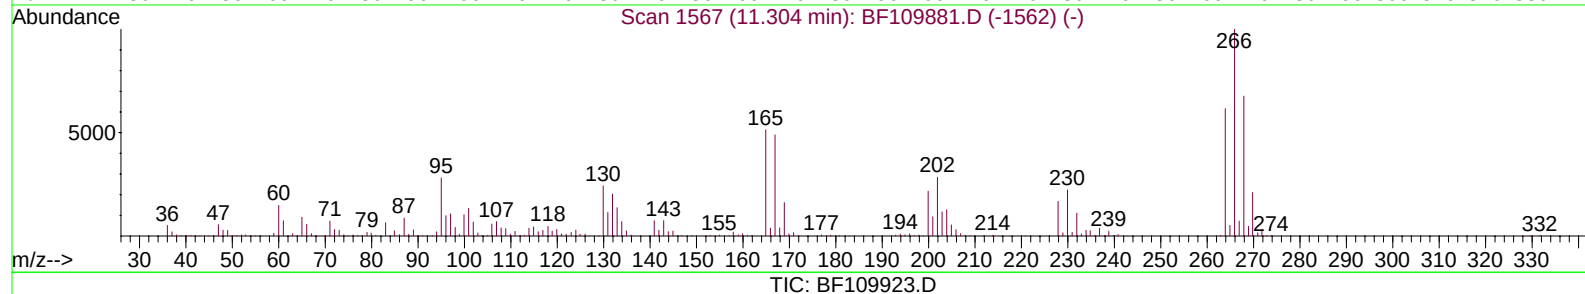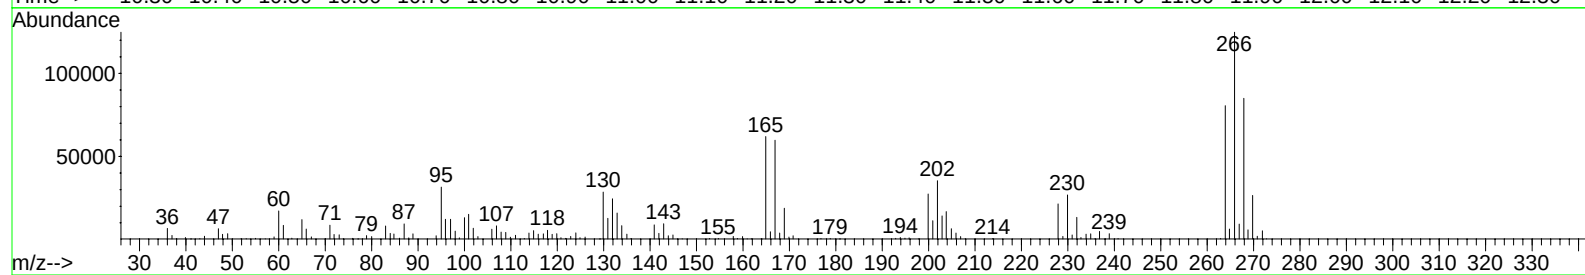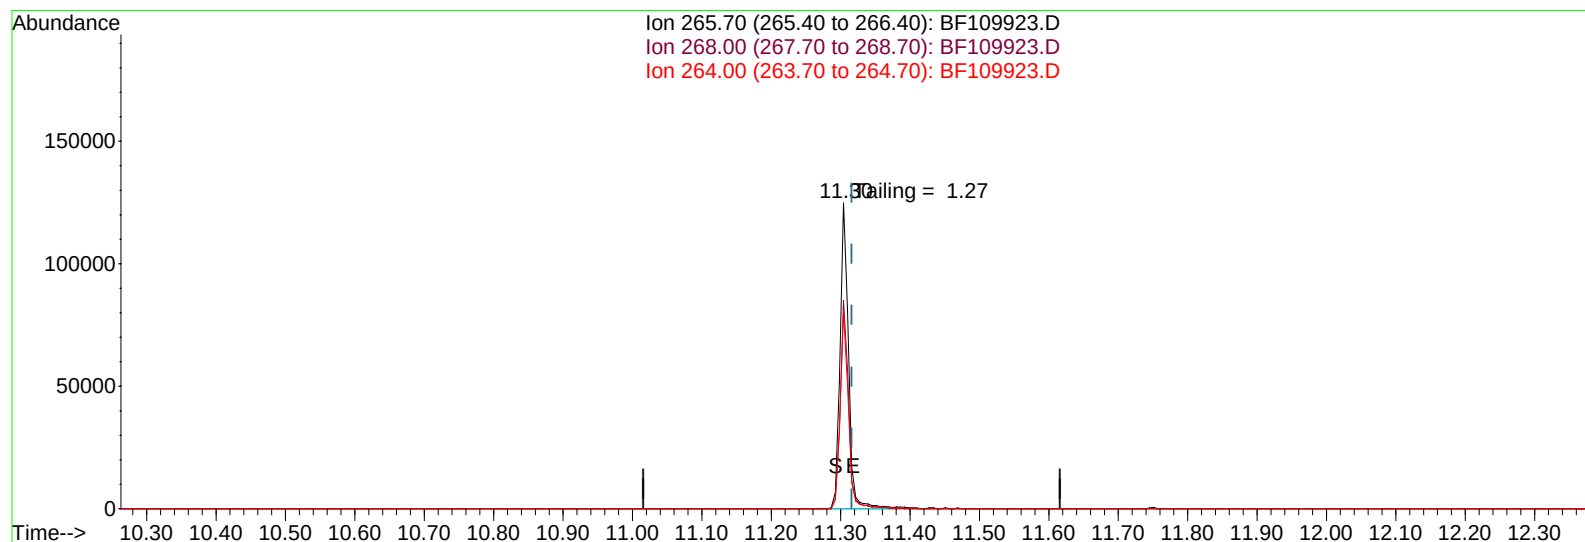

(70) Pentachlorophenol (C)

11.304min (-0.012) 19137.13ng

response 105474

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.09
264.00	63.20	64.59
0.00	0.00	0.00