


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101718\
 Data File : BF109914.D
 Acq On : 17 Oct 2018 10:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

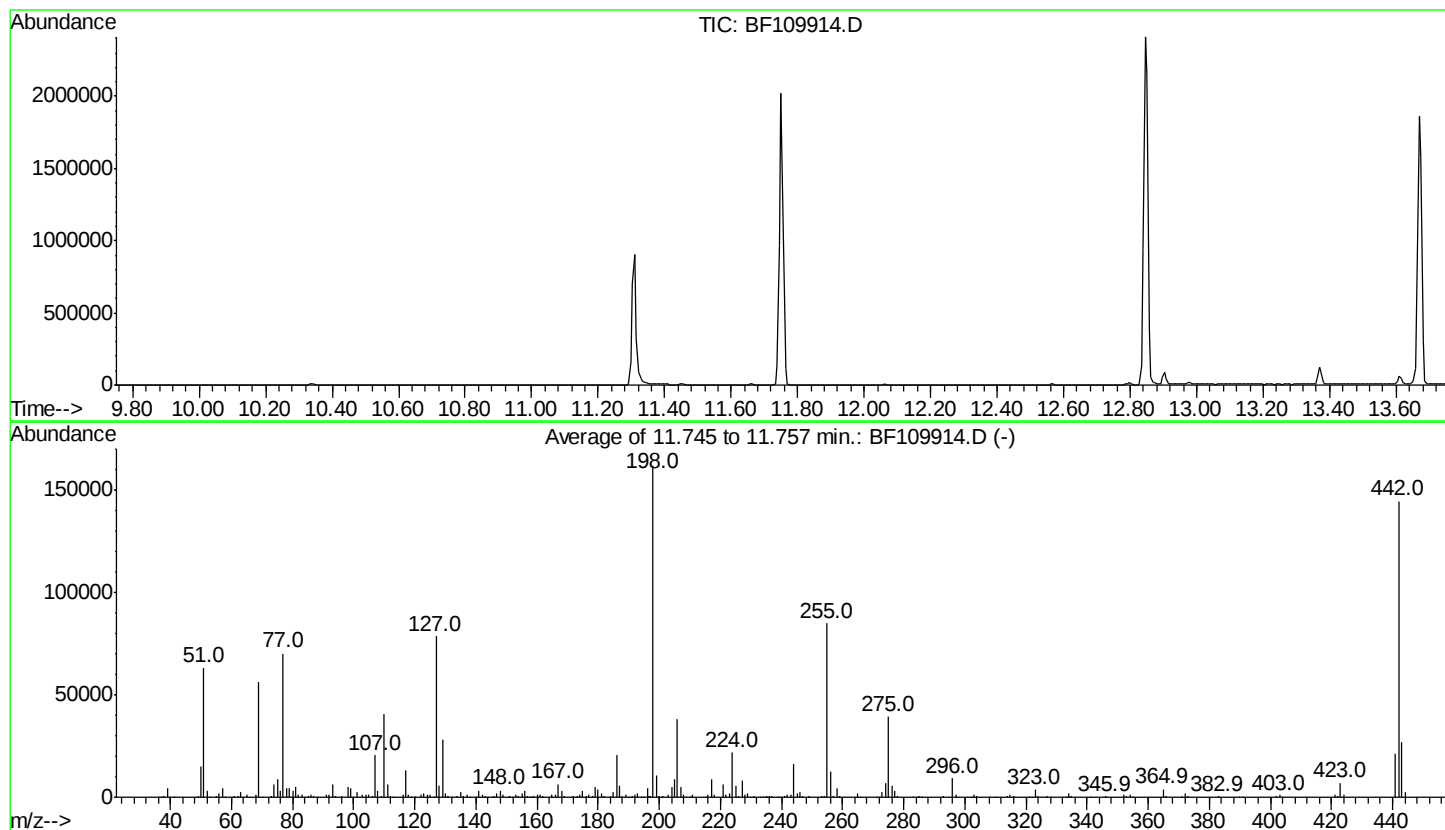

AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	63448	PASS
68	69	0.00	2	1.7	962	PASS
69	198	0.00	100	34.9	56514	PASS
70	69	0.00	2	0.6	327	PASS
127	198	10	80	48.5	78621	PASS
197	198	0.00	2	0.5	866	PASS
198	198	100	100	100.0	162037	PASS
199	198	5	9	6.5	10593	PASS
275	198	10	60	24.2	39282	PASS
365	198	1	100	2.5	4046	PASS
441	198	0.01	100	13.3	21581	PASS
442	198	50	100	89.2	144517	PASS
443	442	15	24	18.4	26641	PASS