


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF101718\  
 Data File : BF109923.D  
 Acq On : 17 Oct 2018 16:43  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF101518.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Oct 16 14:58:24 2018

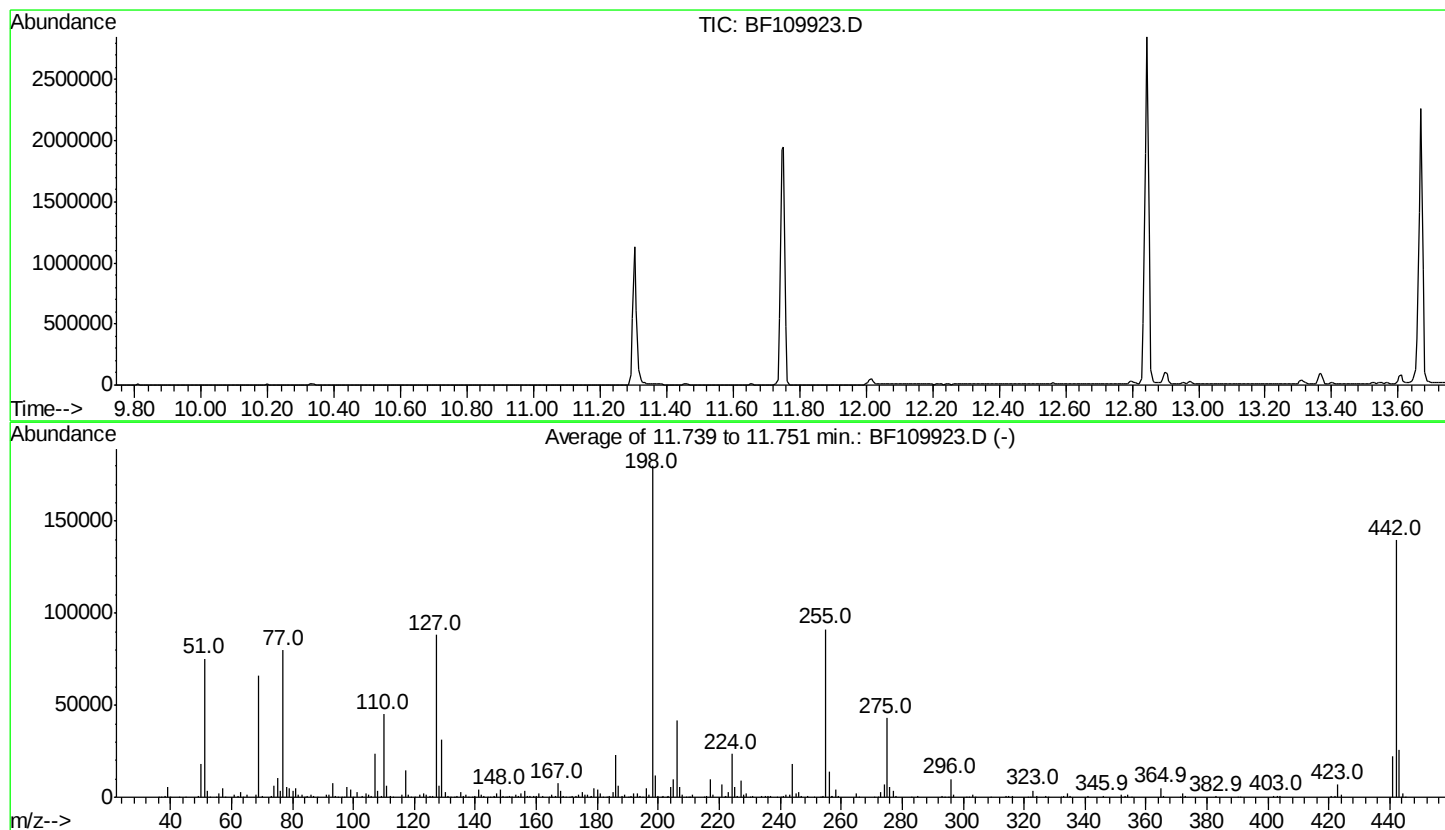

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 41.8      | 75392   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1181    | PASS             |
| 69          | 198          | 0.00         | 100          | 36.6      | 65976   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 467     | PASS             |
| 127         | 198          | 10           | 80           | 48.9      | 88120   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 1295    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 180154  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 11974   | PASS             |
| 275         | 198          | 10           | 60           | 23.8      | 42840   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 4893    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.4      | 22326   | PASS             |
| 442         | 198          | 50           | 100          | 77.5      | 139610  | PASS             |
| 443         | 442          | 15           | 24           | 18.4      | 25620   | PASS             |