

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
 Data File : BF130688.D
 Acq On : 17 Oct 2022 15:55
 Operator : CG\JU
 Sample : N5145-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-6-101322

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.740	447	451	462	rBV	128306	167493	5.53%	1.164%
2	5.175	522	525	542	rBV	898233	951272	31.38%	6.612%
3	6.222	700	703	719	rBV	531183	570320	18.81%	3.964%
4	6.569	759	762	771	rBV	539337	462466	15.26%	3.214%
5	7.146	855	860	863	rBV	1578222	1543621	50.92%	10.729%
6	7.851	976	980	988	rVB	632736	617692	20.38%	4.293%
7	8.934	1158	1164	1167	rBV	3401532	3031295	100.00%	21.070%
8	9.057	1181	1185	1193	rVB	60780	68037	2.24%	0.473%
9	9.604	1273	1278	1281	rBV	831743	705023	23.26%	4.900%
10	10.392	1408	1412	1422	rBV	2126887	1953400	64.44%	13.577%
11	11.081	1526	1529	1533	rBV	797528	683647	22.55%	4.752%
12	11.622	1616	1621	1626	rBV	43629	56737	1.87%	0.394%
13	12.669	1794	1799	1802	rBV	3016066	2748571	90.67%	19.104%
14	13.716	1973	1977	1984	rVB	436590	426362	14.07%	2.964%
15	15.086	2206	2210	2219	rBV	356680	401169	13.23%	2.788%




Sum of corrected areas: 14387105

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
Data File : BF130688.D
Acq On : 17 Oct 2022 15:55
Operator : CG\JU
Sample : N5145-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6-101322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

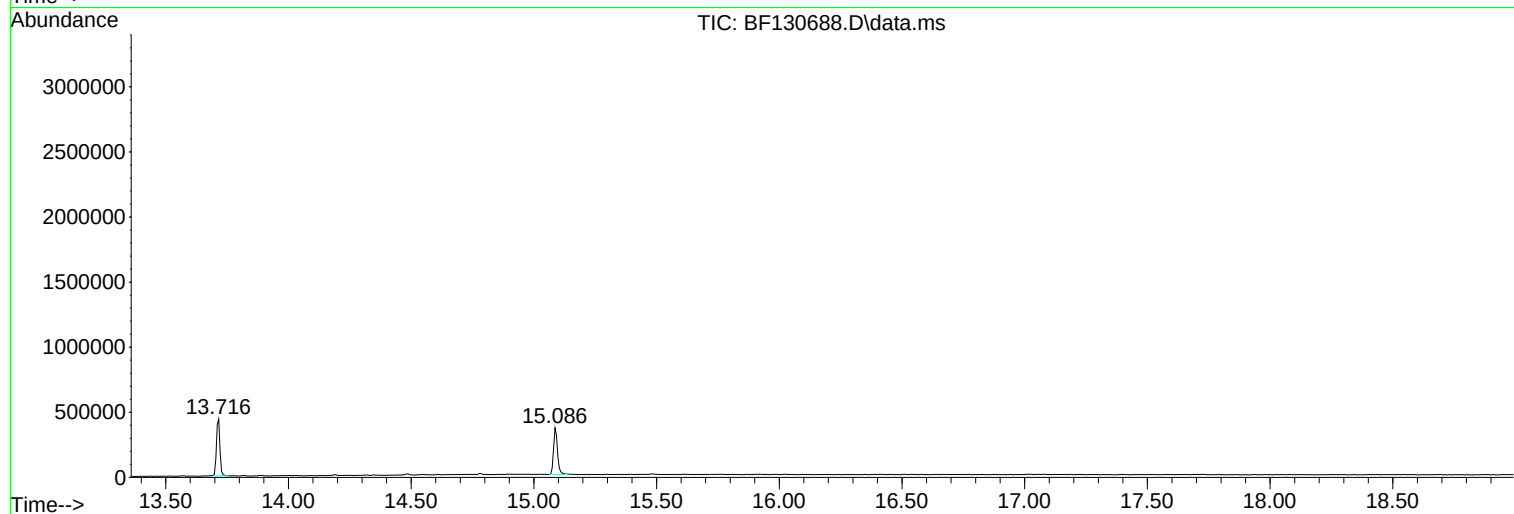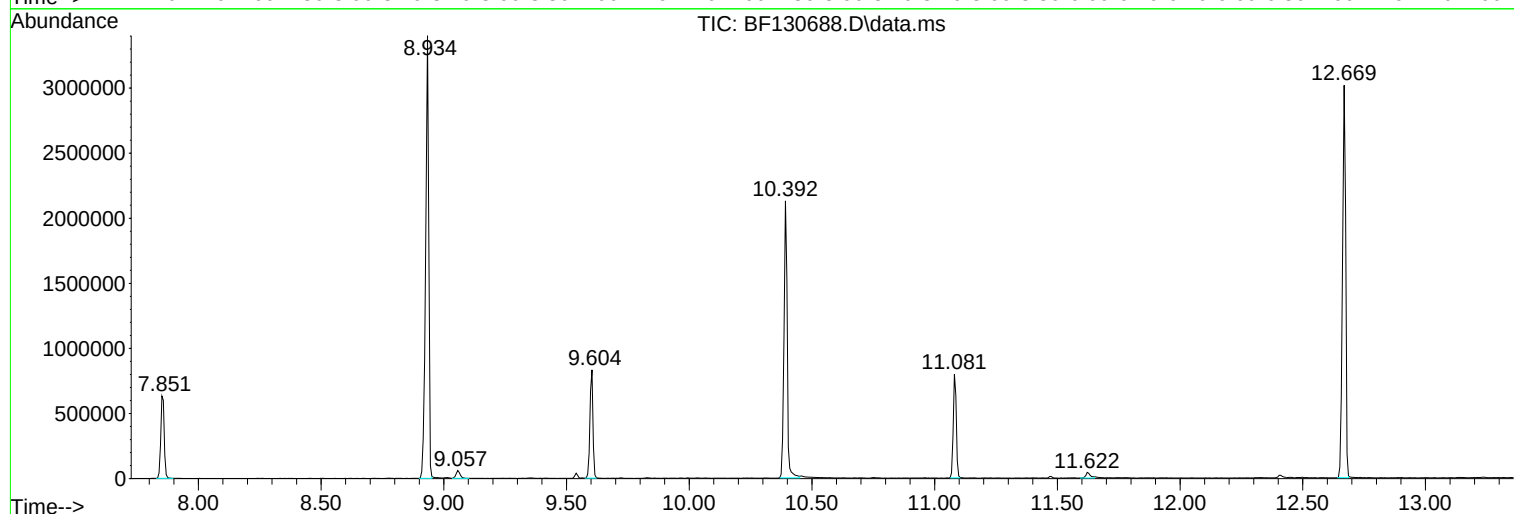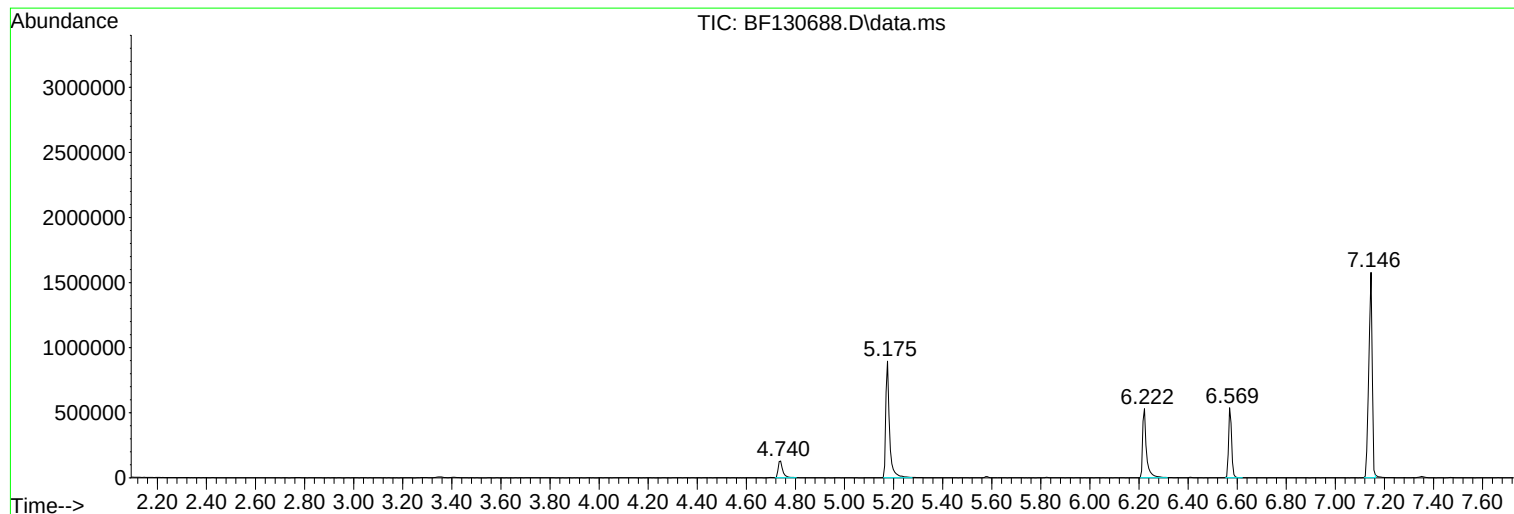

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
Data File : BF130688.D
Acq On : 17 Oct 2022 15:55
Operator : CG\JU
Sample : N5145-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6-101322










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.740	7.24 ng	167493	1,4-Dichlorobenzene-d4	6.569

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	40		
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	40		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		

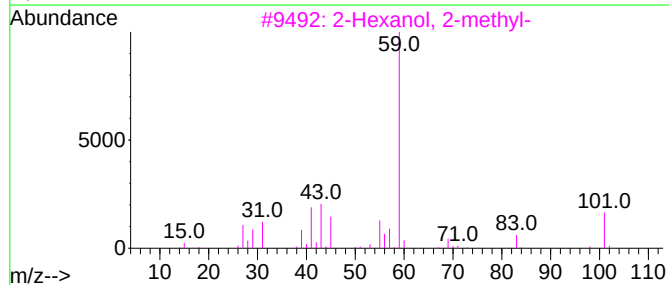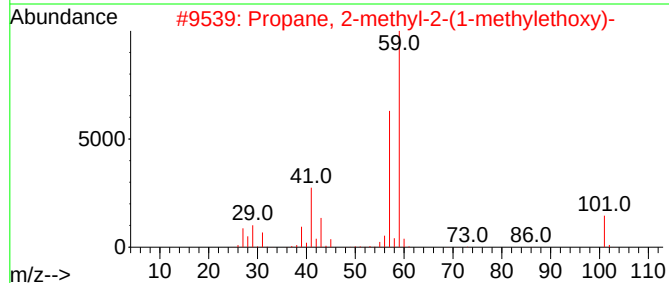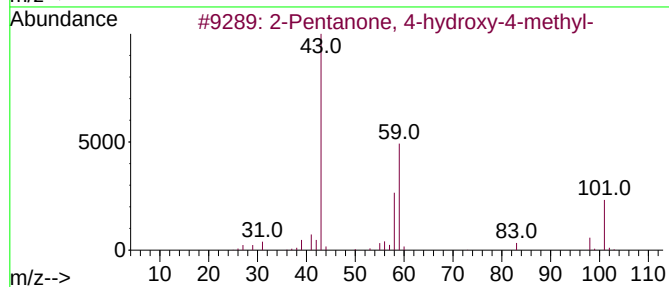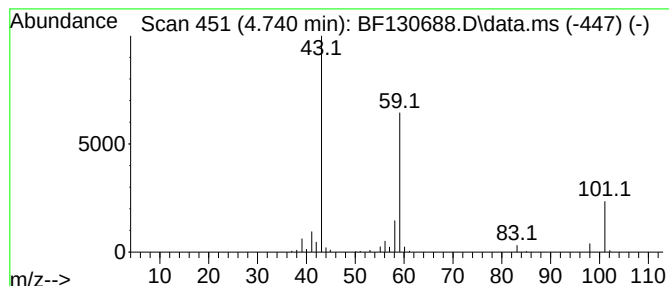

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
Data File : BF130688.D
Acq On : 17 Oct 2022 15:55
Operator : CG\JU
Sample : N5145-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-6-101322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.740	7.2	ng	167493	1	6.569	462466	20.0