


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
 Data File : BF130680.D
 Acq On : 17 Oct 2022 10:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 18 03:15:54 2022

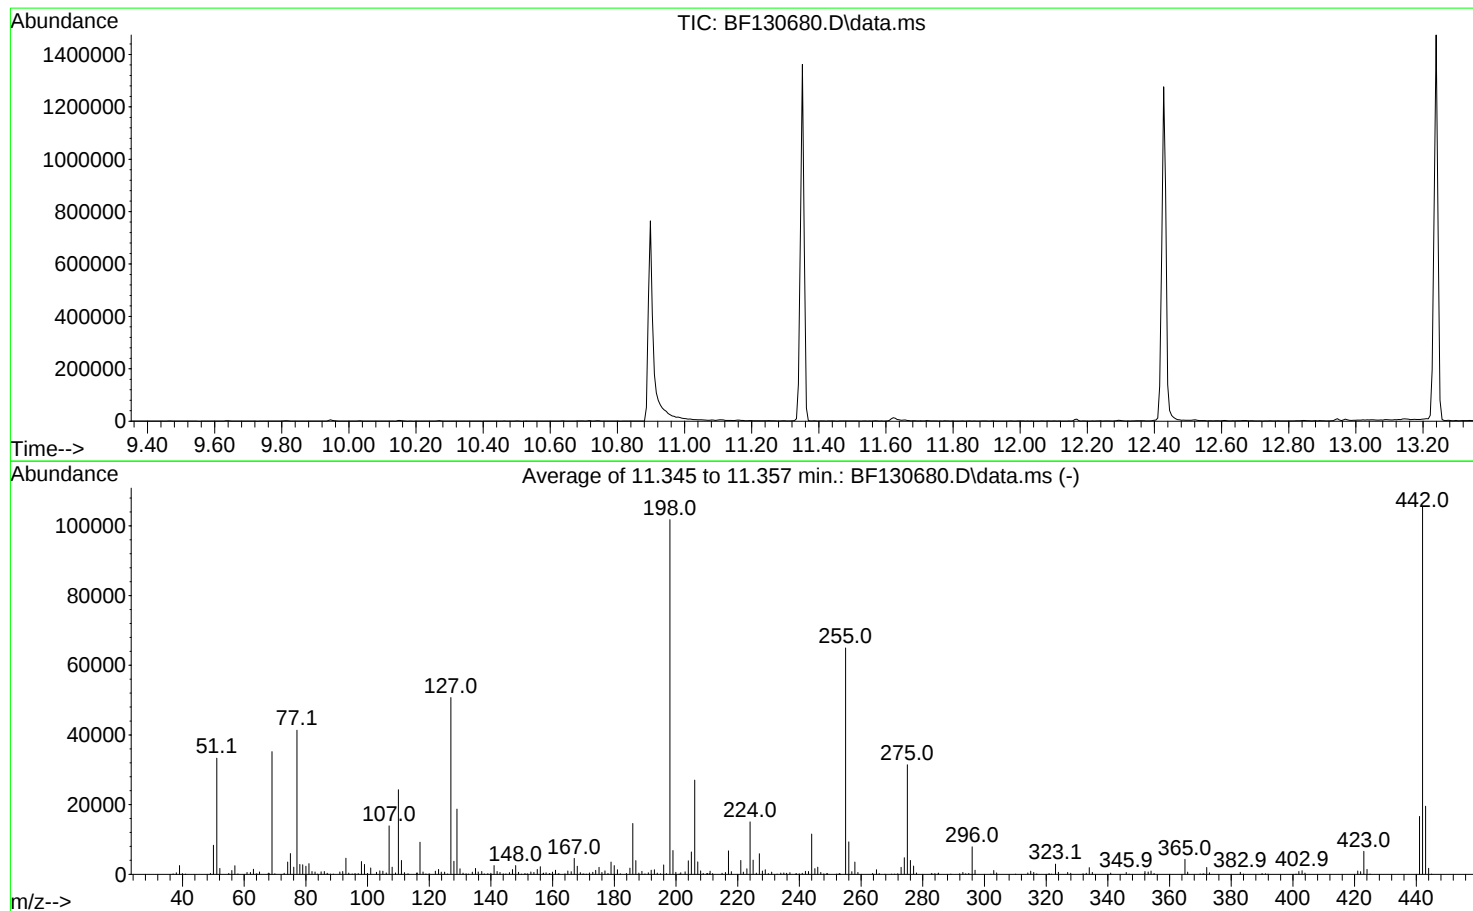




AutoFind: Scans 1574, 1575, 1576; Background Corrected with Scan 1569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	33316	PASS
68	69	0.00	2	1.0	358	PASS
69	198	0.00	100	34.6	35221	PASS
70	69	0.00	2	0.4	142	PASS
127	198	10	80	49.8	50725	PASS
197	198	0.00	2	0.2	204	PASS
198	198	100	100	100.0	101824	PASS
199	198	5	9	6.7	6827	PASS
275	198	10	60	30.9	31456	PASS
365	198	1	100	4.2	4293	PASS
441	198	0.01	100	16.3	16619	PASS
442	442	50	100	100.0	105592	PASS
443	442	15	24	18.5	19552	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
 Data File : BF130680.D
 Acq On : 17 Oct 2022 10:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 17 17:55:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 12 06:52:52 2022
 Response via : Initial Calibration

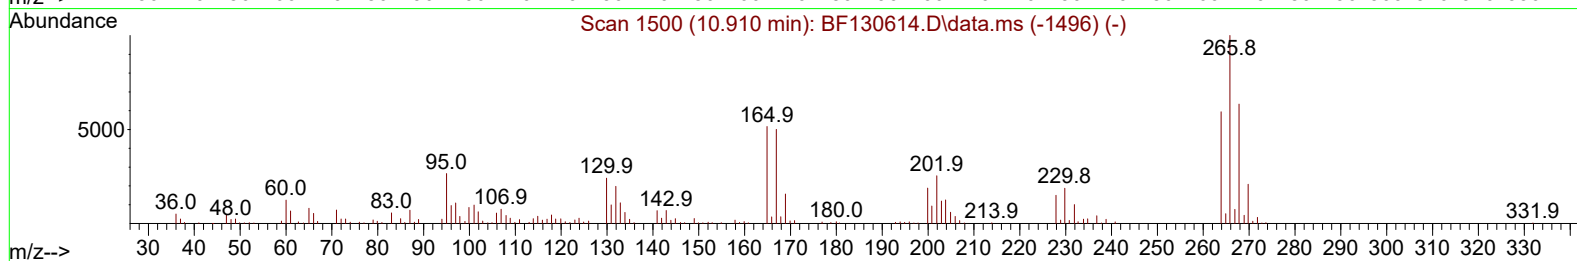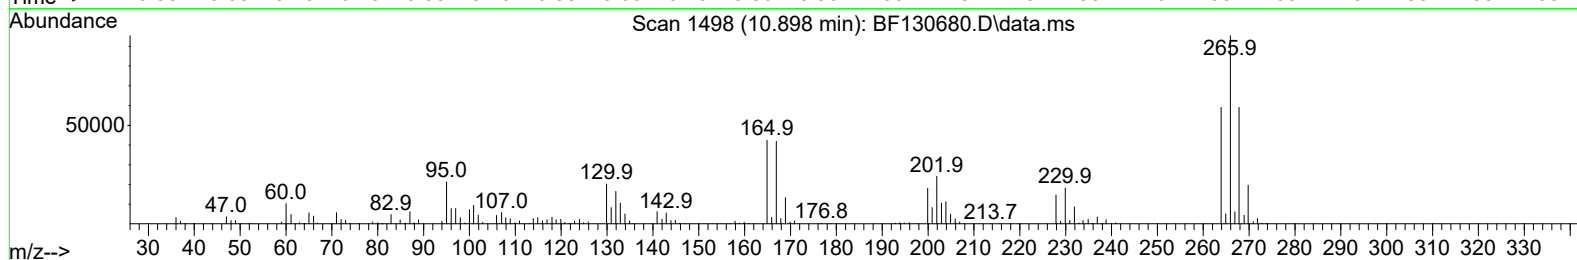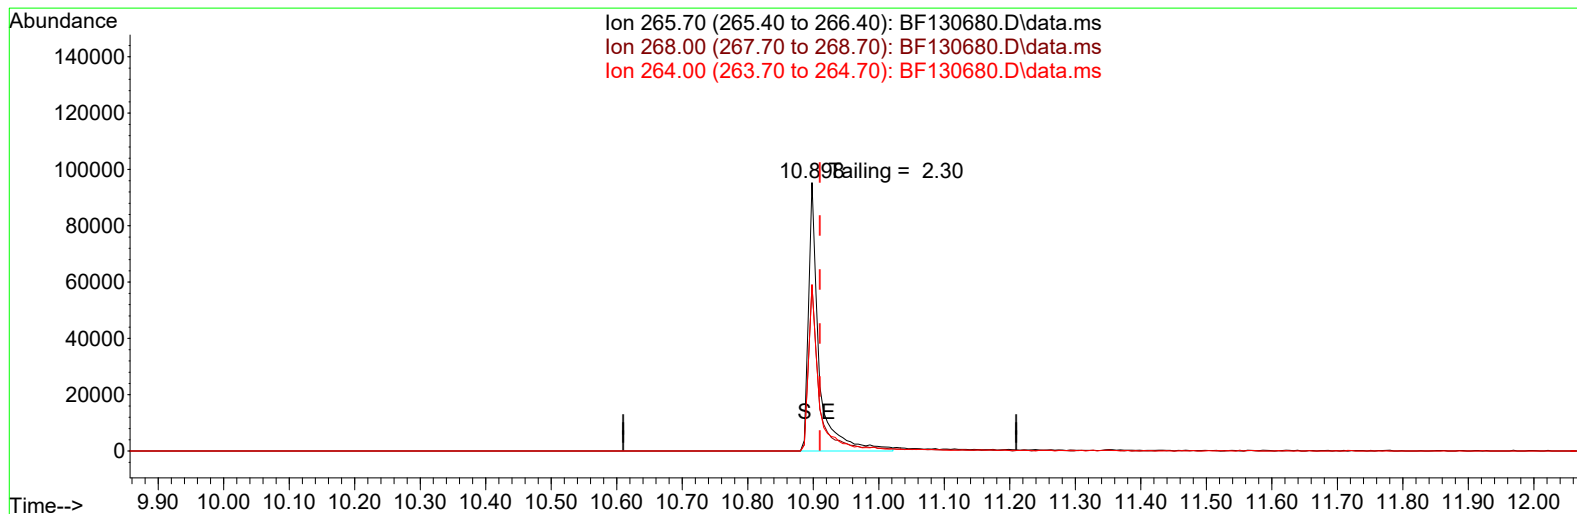

TIC: BF130680.D\data.ms

(70) Pentachlorophenol (C)

10.898min (-0.012) 298630.08 ng




response 108523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	61.90
264.00	59.40	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101722\
 Data File : BF130680.D
 Acq On : 17 Oct 2022 10:03
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 17 17:55:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 12 06:52:52 2022
 Response via : Initial Calibration

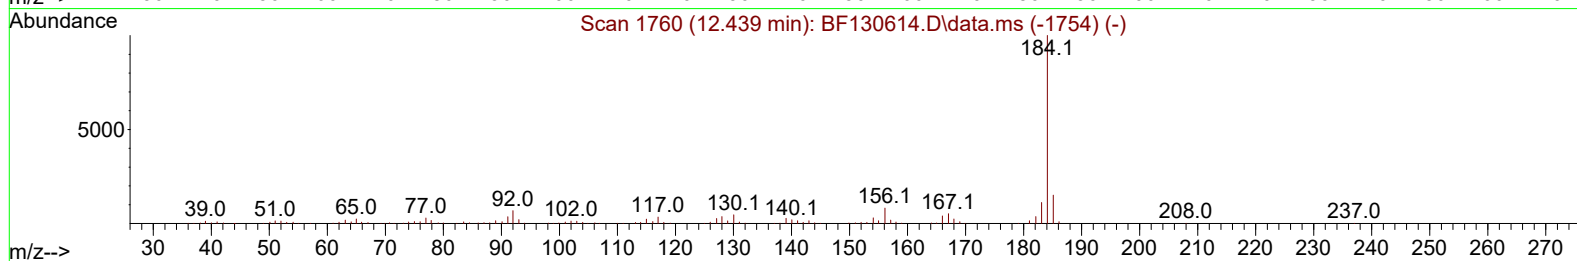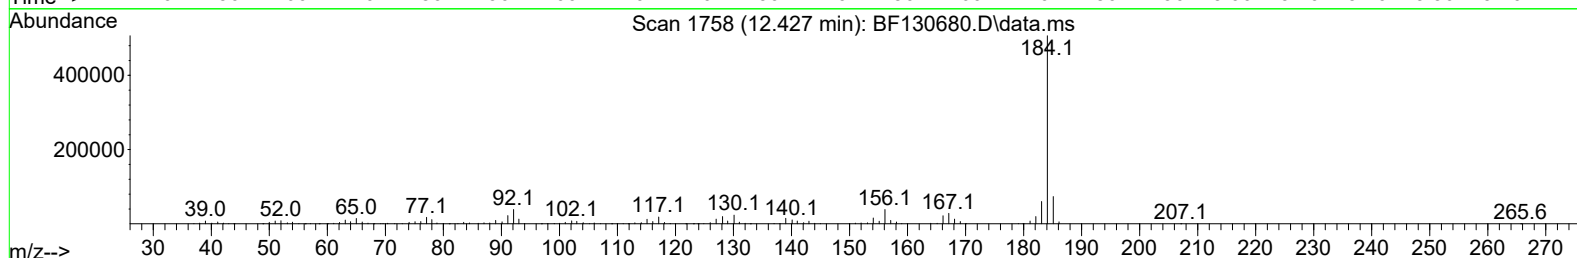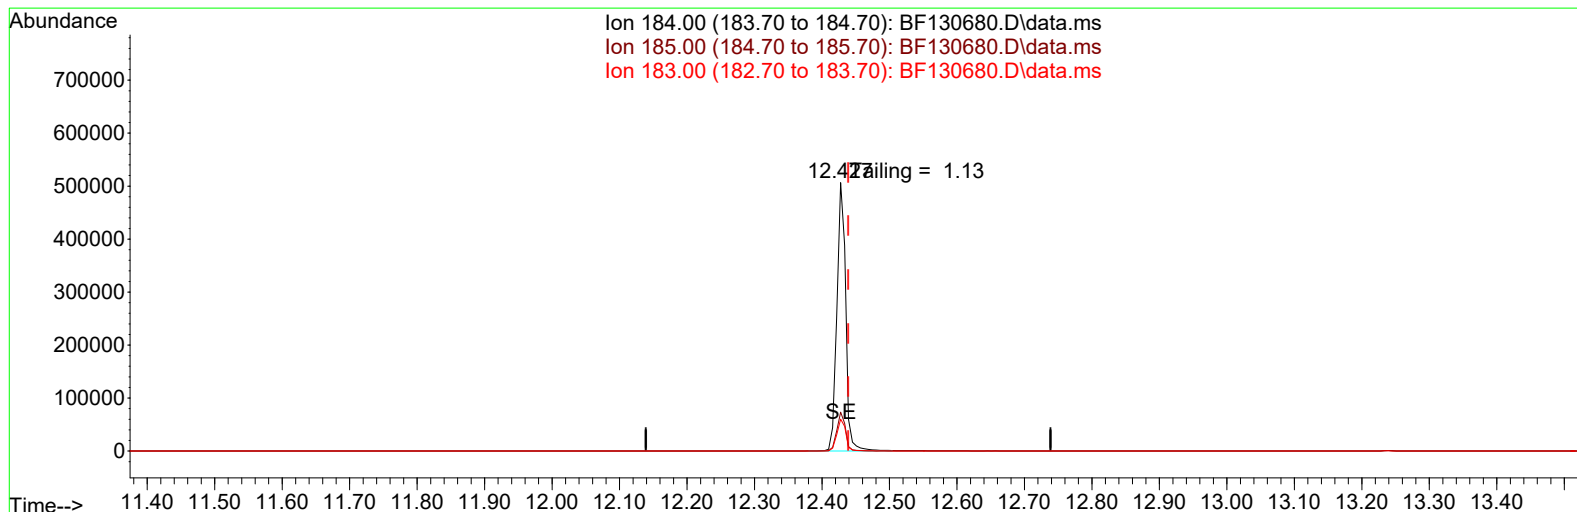

TIC: BF130680.D\data.ms

(77) Benzidine

12.427min (-0.012) 127684.96 ng

response 461519

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.49
183.00	11.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/17/2022	BNA_F	<u>BF130680.D</u>
Compound Name	Response	Retention Time
DDT	233225	13.239
DDD	3362	12.945
DDE	203	12.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3565	236790	1.51

Instrument :
BNA_F
ClientSampleId :
DFTPP