
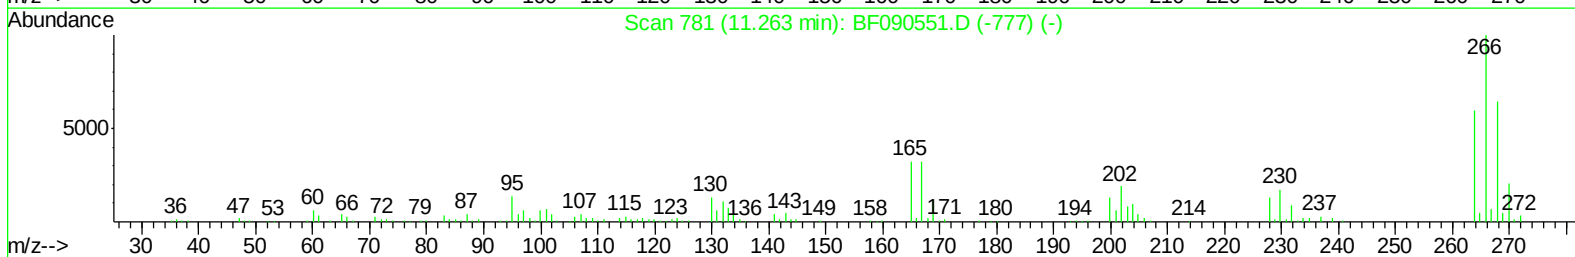
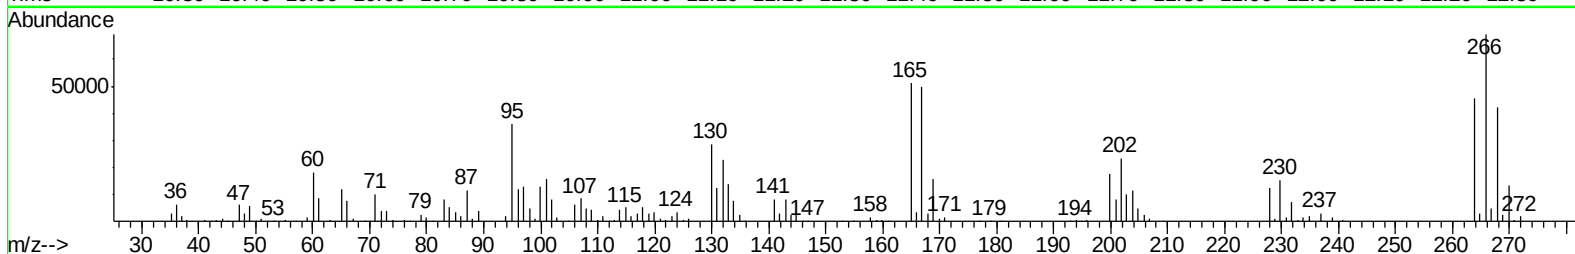


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101816\
Data File : BF090624.D
Acq On : 18 Oct 2016 10:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 07:46:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 19:19:58 2016
Response via : Initial Calibration

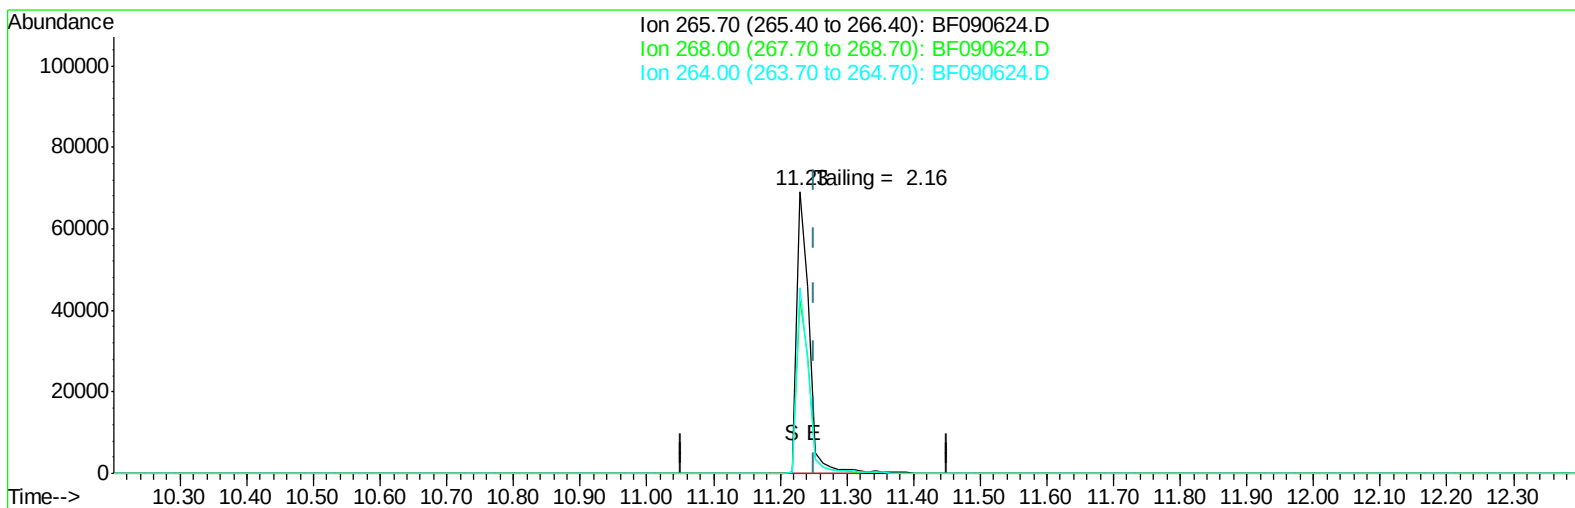

TIC: BF090624.D

(69) Pentachlorophenol (C)




11.229min (-0.023) 0.00ng

response 89927

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.44
264.00	59.90	65.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101816\
Data File : BF090624.D
Acq On : 18 Oct 2016 10:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 19 07:46:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 17 19:19:58 2016
Response via : Initial Calibration

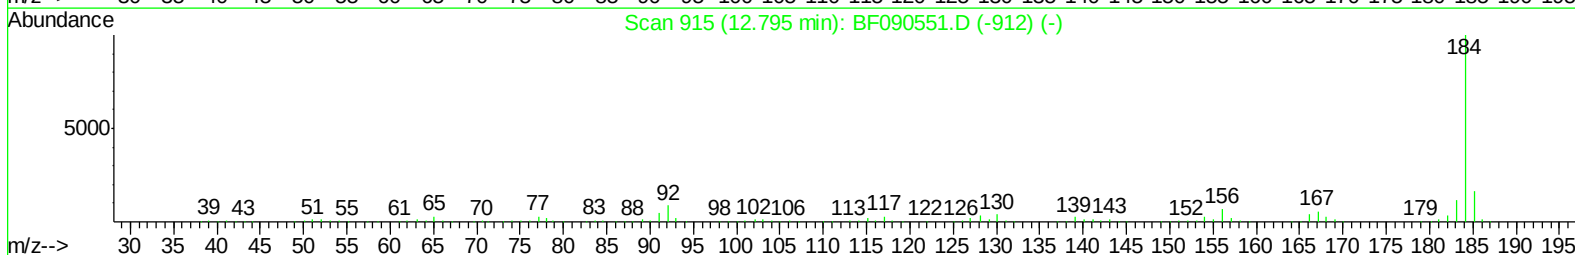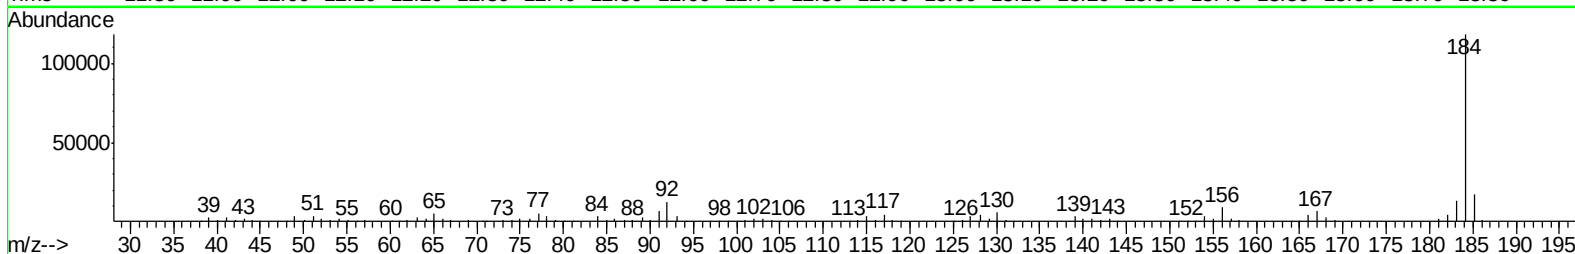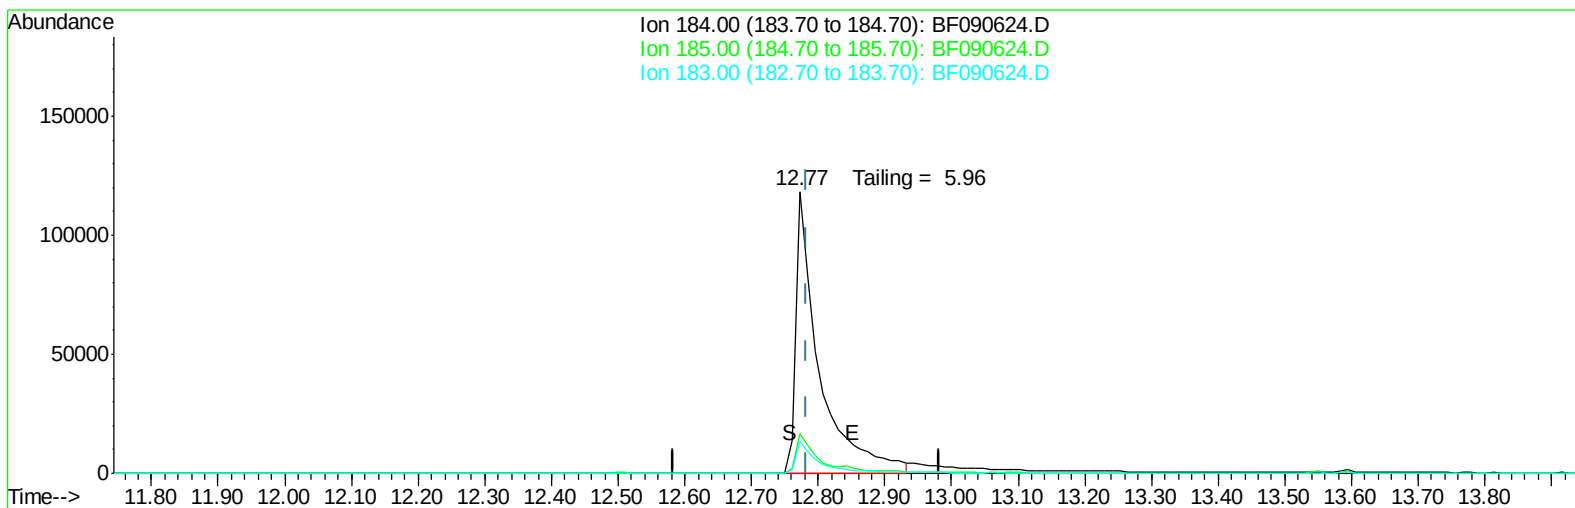

TIC: BF090624.D

(76) Benzidine

12.772min (-0.012) 0.00ng

response 289515

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.32
183.00	11.70	11.23
0.00	0.00	0.00