


Data Path : U:\HPCHEM1\BNA_F\DATA\BF101816\
 Data File : BF090624.D
 Acq On : 18 Oct 2016 10:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 19 15:13:23 2016

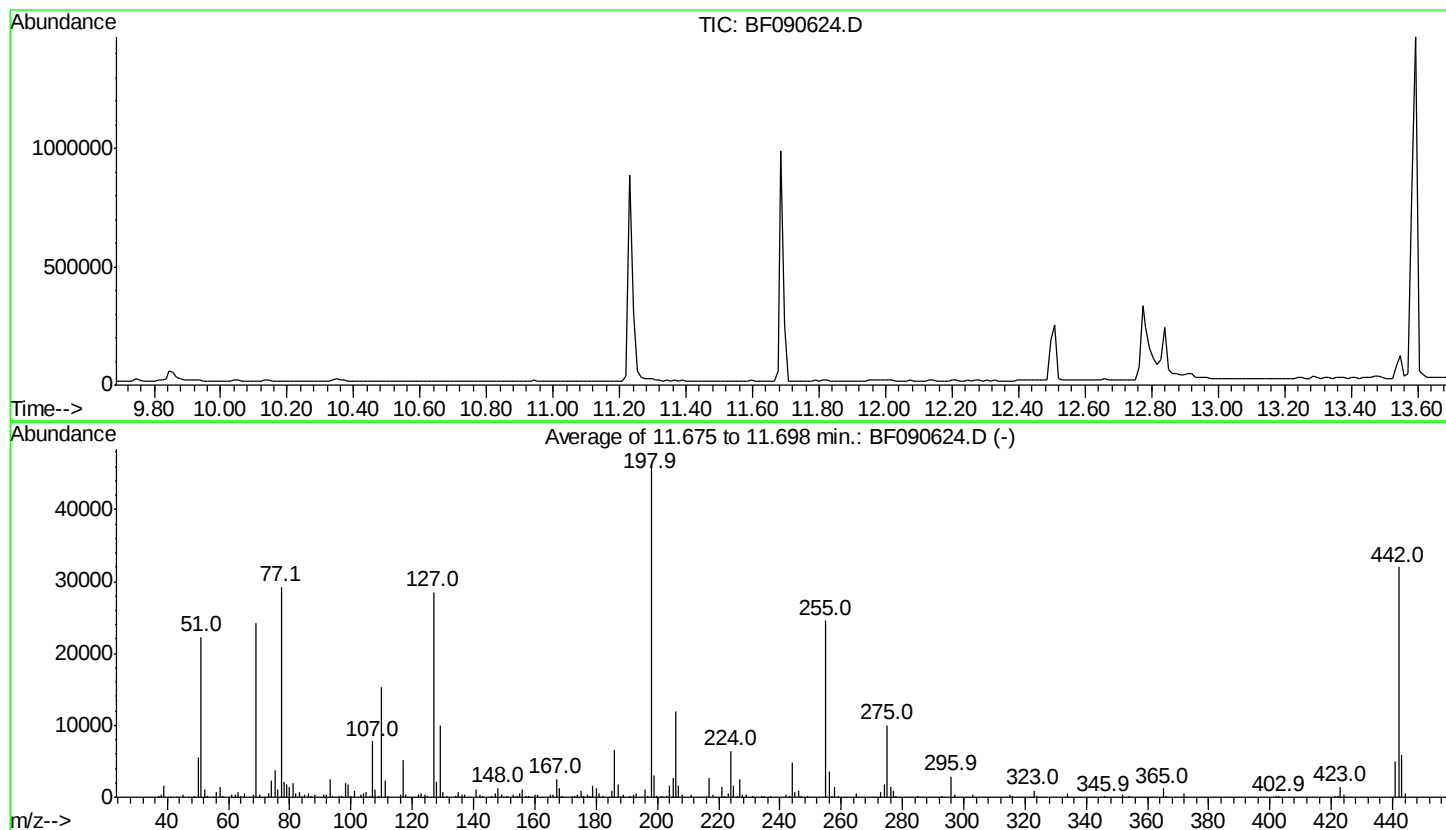

AutoFind: Scans 817, 818, 819; Background Corrected with Scan 814

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	22276	PASS
68	69	0.00	2	1.3	307	PASS
69	198	0.00	100	52.5	24192	PASS
70	69	0.00	2	1.2	279	PASS
127	198	10	80	61.9	28545	PASS
197	198	0.00	2	0.2	113	PASS
198	198	100	100	100.0	46116	PASS
199	198	5	9	6.5	3018	PASS
275	198	10	60	21.6	9975	PASS
365	198	1	100	2.6	1183	PASS
441	442	0.01	24	15.8	5047	PASS
442	198	50	100	69.4	32021	PASS
443	442	15	24	18.2	5827	PASS