

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101817\
 Data File : BF099627.D
 Acq On : 18 Oct 2017 19:51
 Operator : SJ/JU
 Sample : I5836-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ENV-125-11(10-15)

Quant Time: Oct 18 22:41:42 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 18 15:18:49 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	103861	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	428047	20.00	ng	0.00
38) Acenaphthene-d10	9.86	164	188582	20.00	ng	0.00
63) Phenanthrene-d10	11.35	188	305382	20.00	ng	0.00
75) Chrysene-d12	13.99	240	186029	20.00	ng	0.00
86) Perylene-d12	15.46	264	195688	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	602189	92.30	ng	0.00
7) Phenol-d6	6.47	99	720091	89.47	ng	-0.01
23) Nitrobenzene-d5	7.39	82	413628	61.97	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	141241	91.53	ng	0.00
44) 2-Fluorobiphenyl	9.18	172	745646	66.01	ng	0.00
78) Terphenyl-d14	12.93	244	484977	59.29	ng	0.00
Target Compounds						
10) Phenol	6.48	94	44046	4.893	ng	98
49) Dimethylphthalate	9.57	163	222099	15.604	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101817\
Data File : BF099627.D
Acq On : 18 Oct 2017 19:51
Operator : SJ/JU
Sample : I5836-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ENV-125-11(10-15)

Quant Time: Oct 18 22:41:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 18 15:18:49 2017
Response via : Initial Calibration

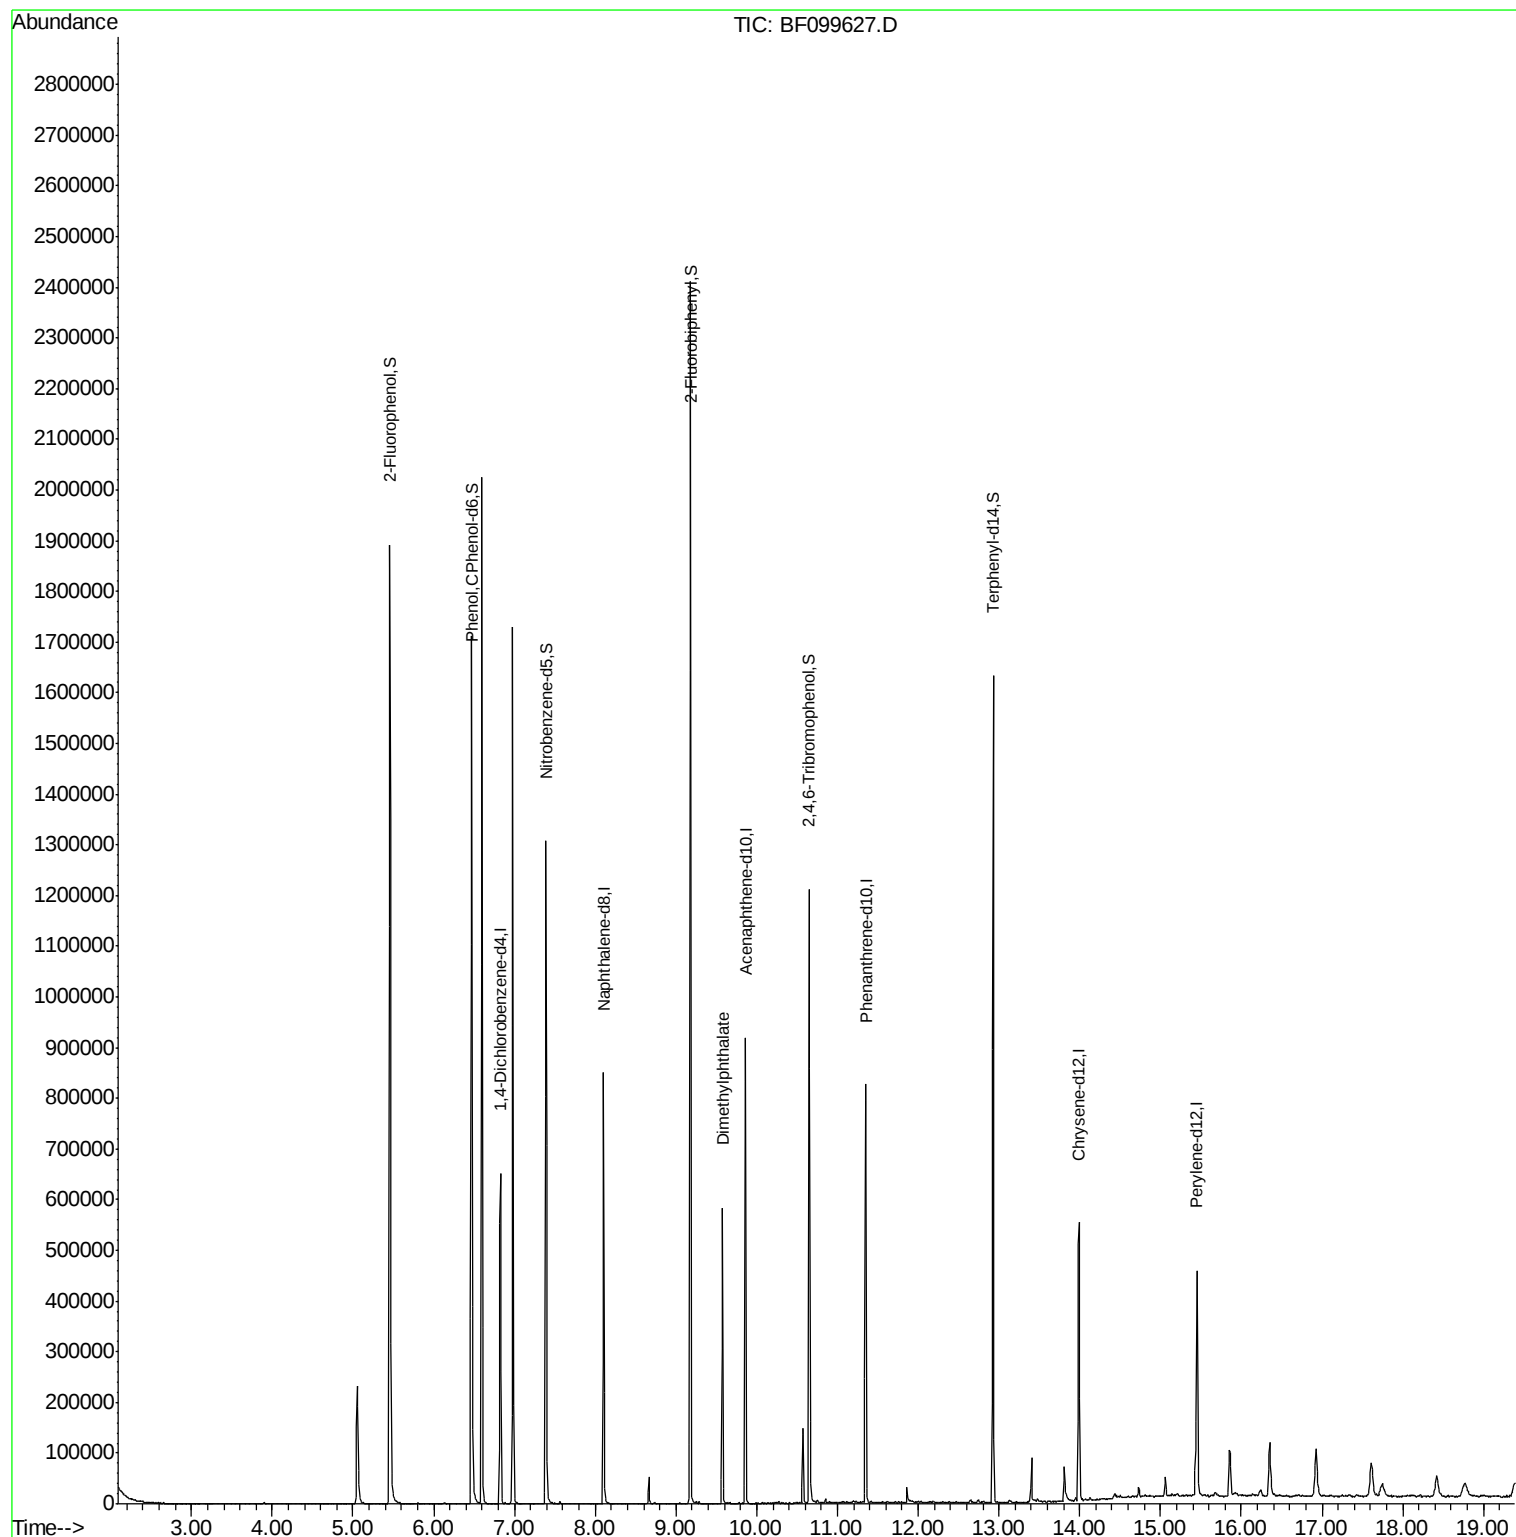




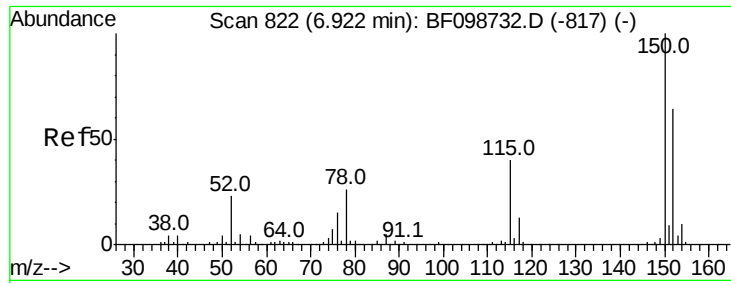


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.83 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: BF099627.D
 Acq: 18 Oct 2017 19:51

Instrument :
 BNA_F
 ClientSampleId :
 ENV-125-11(10-15)




Tot Ion:152 Resp: 103861
 Ion Ratio Lower Upper
 152 100
 150 154.3 124.6 186.8
 115 58.3 50.1 75.1

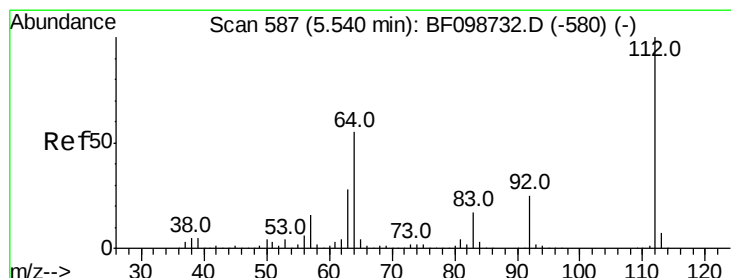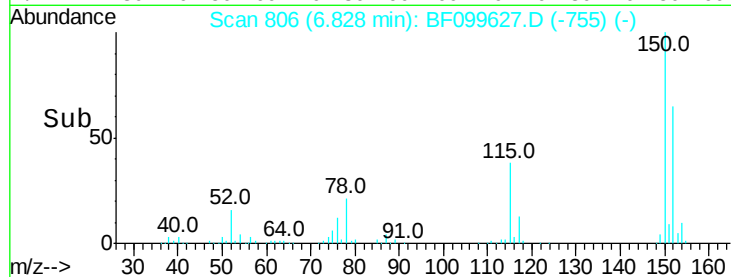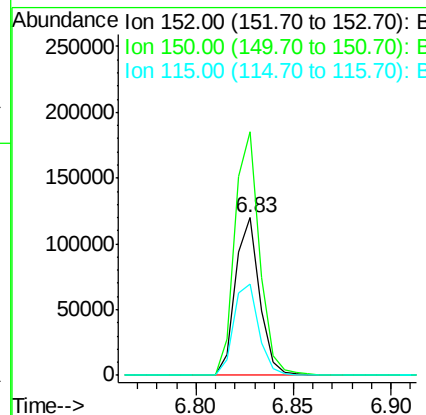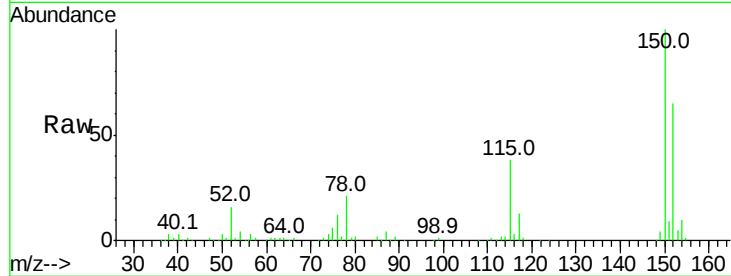


#5

2-Fluorophenol
 Concen: 92.299 ng
 RT: 5.46 min Scan# 573
 Delta R.T. 0.01 min
 Lab File: BF099627.D
 Acq: 18 Oct 2017 19:51

Tgt Ion:112 Resp: 602189
 Ion Ratio Lower Upper
 112 100
 64 54.8 47.9 71.9
 63 26.2 23.7 35.5

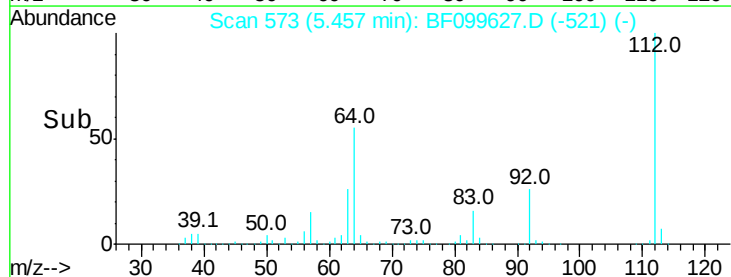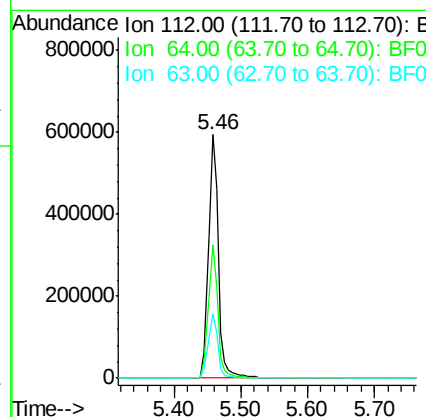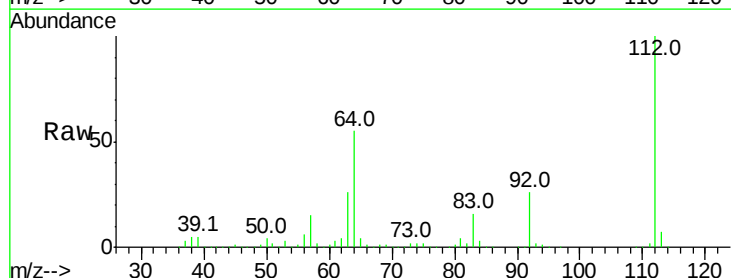

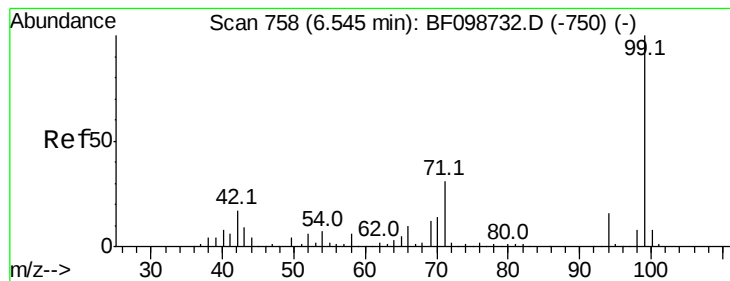

#7

Phenol-d6

Concen: 89.469 ng

RT: 6.47 min Scan# 745

Delta R.T. -0.01 min

Lab File: BF099627.D

Acq: 18 Oct 2017 19:51

Instrument :

BNA_F

ClientSampleId :

ENV-125-11(10-15)


Tot Ion: 99 Resp: 720091

Ion Ratio Lower Upper

99 100

42 14.7 14.5 21.7




71 30.1 25.4 38.0

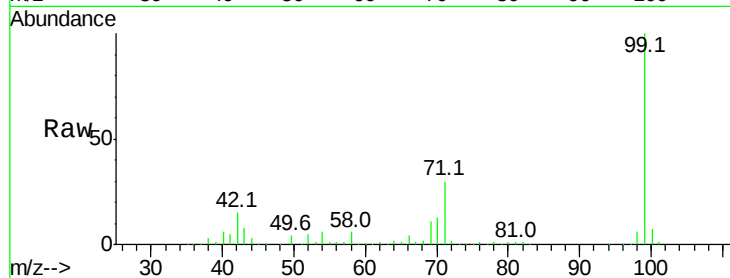

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

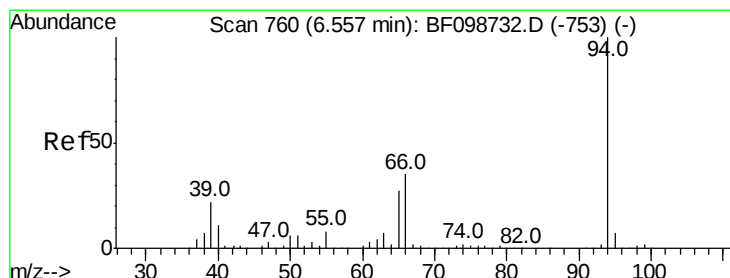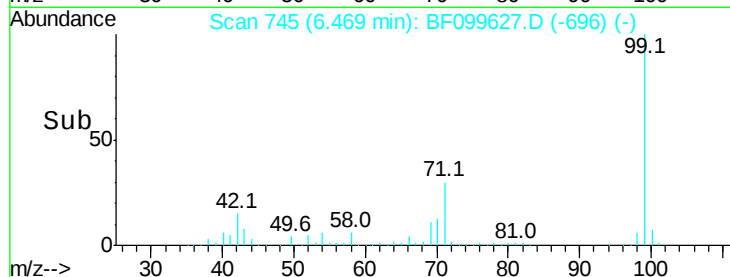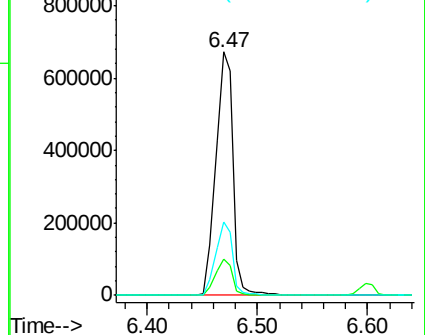

#10

Phenol

Concen: 4.893 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF099627.D

Acq: 18 Oct 2017 19:51


Tgt Ion: 94 Resp: 44046

Ion Ratio Lower Upper

94 100

65 26.3 7.9 47.9



66 36.8 16.2 56.2

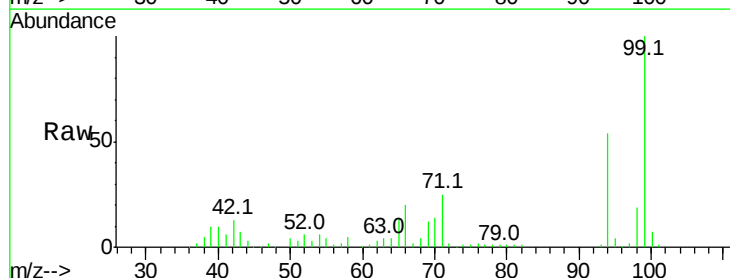


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0



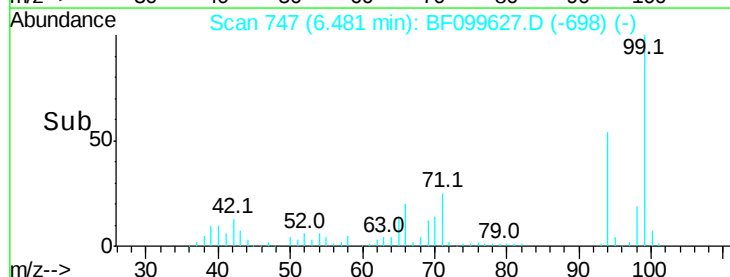
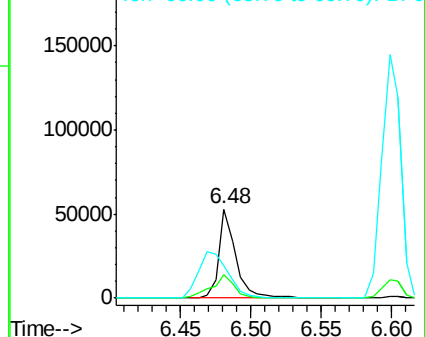


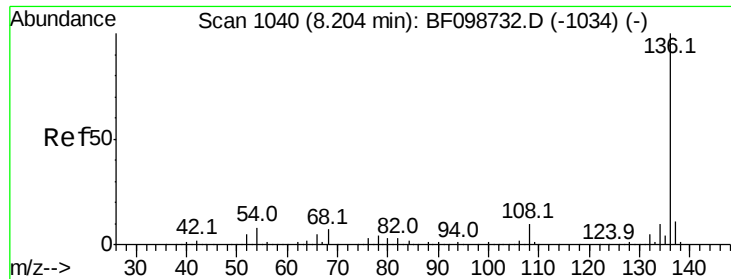

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.11 min Scan# 1024
Delta R.T. 0.00 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51




Instrument :
BNA_F
ClientSampleId :
ENV-125-11(10-15)


Tot Ion:	136	Resp:	428047
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.9	13.3
54	6.3	6.6	9.8#
68	5.3	5.0	7.4

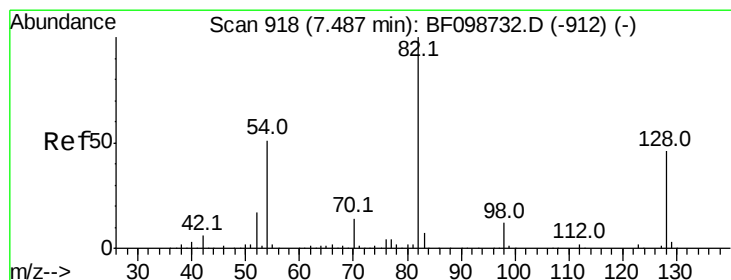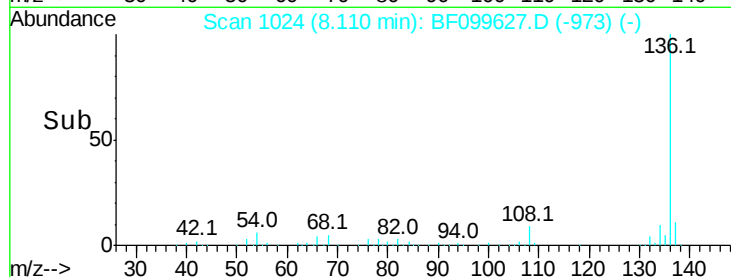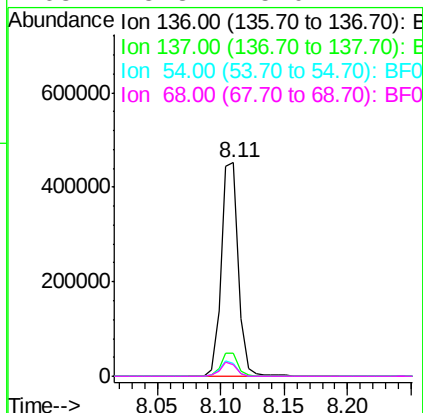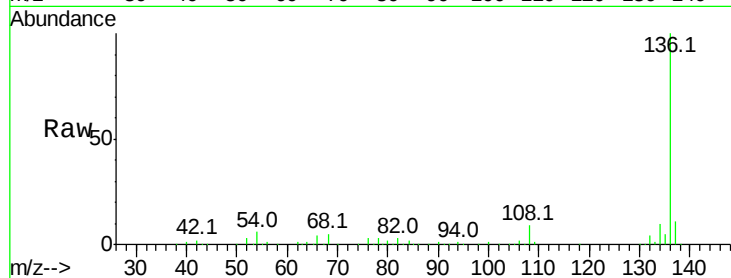

#23
Nitrobenzene-d5
Concen: 61.970 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.01 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51

Tgt Ion:	82	Resp:	413628
Ion	Ratio	Lower	Upper
82	100		
128	48.3	36.1	54.1
54	45.7	41.4	62.2

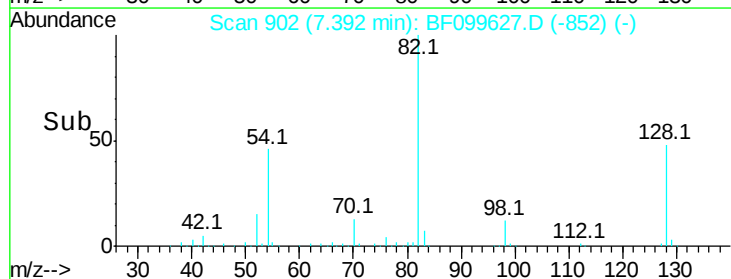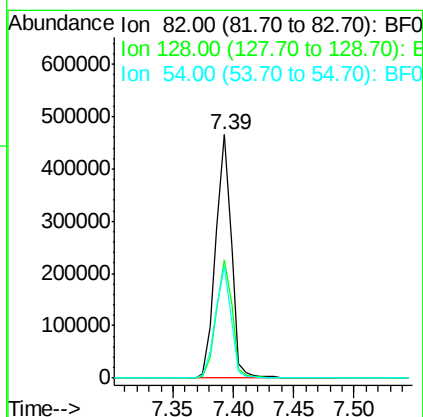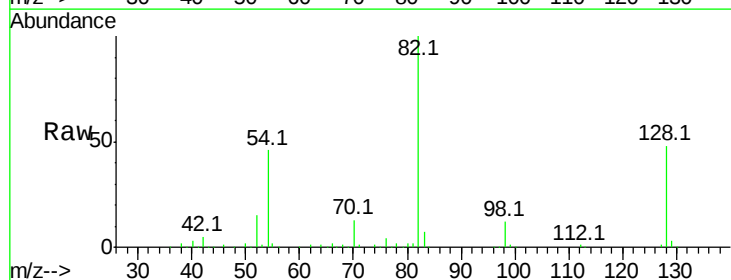


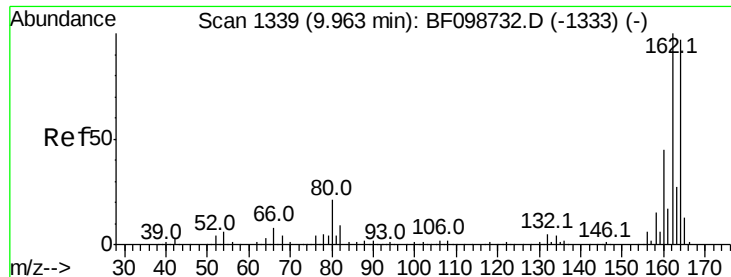




#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.86 min Scan# 1322
Delta R.T. -0.01 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51

Instrument :
BNA_F
ClientSampleId :
ENV-125-11(10-15)

Tot Ion:164 Resp: 188582
Ion Ratio Lower Upper
164 100
162 105.1 86.1 129.1
160 46.2 38.3 57.5

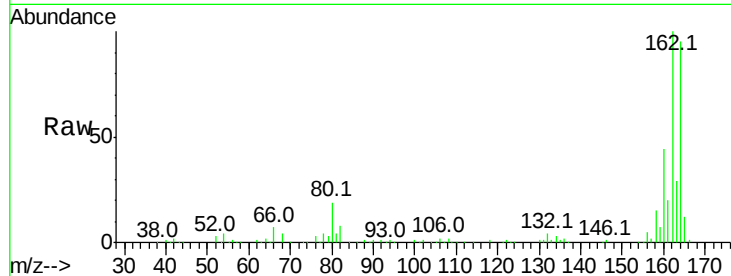


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

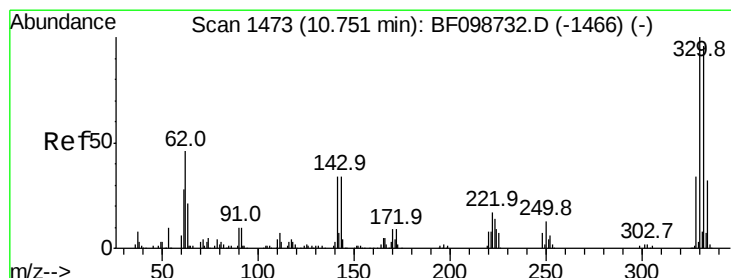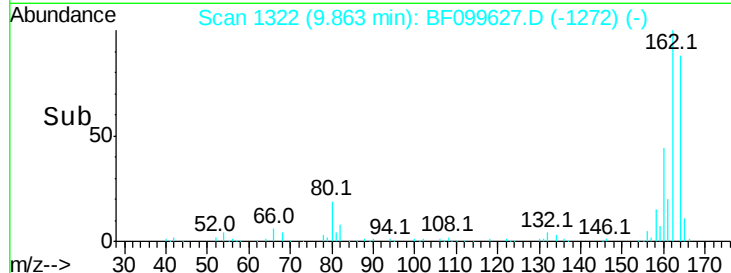
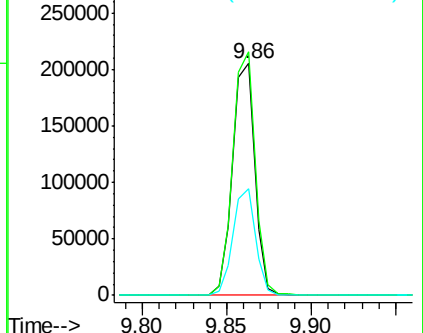



#41
2,4,6-Tribromophenol
Concen: 91.530 ng
RT: 10.65 min Scan# 1456
Delta R.T. -0.01 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51

Tgt Ion:330 Resp: 141241
Ion Ratio Lower Upper
330 100
332 96.7 77.0 115.6
141 37.6 29.9 44.9

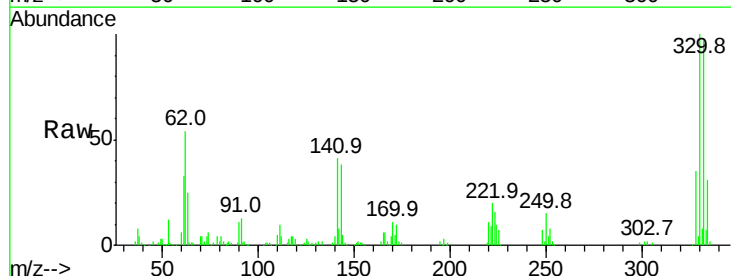

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

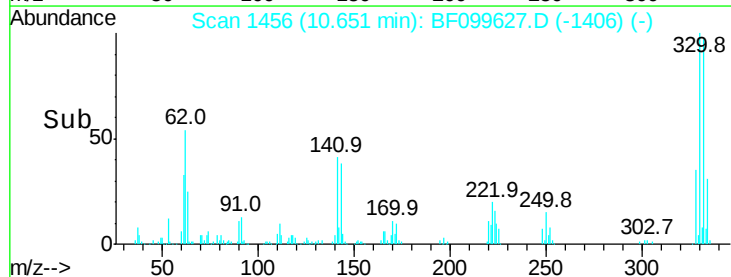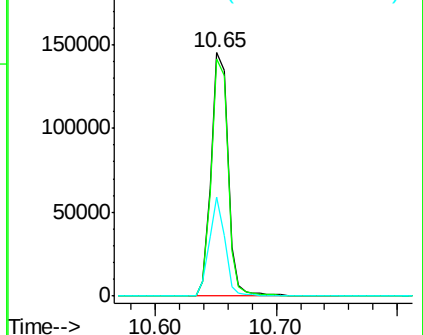


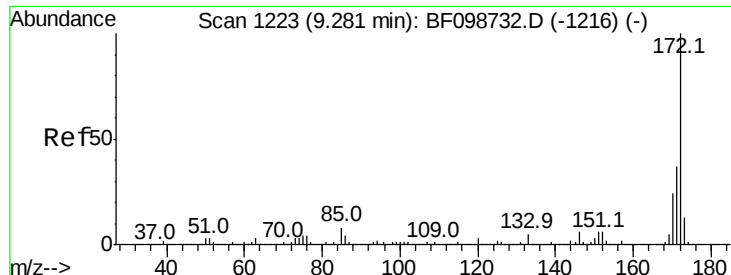




#44
2-Fluorobiphenyl
Concen: 66.008 ng
RT: 9.18 min Scan# 1206
Delta R.T. -0.01 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51

Instrument :
BNA_F
ClientSampleId :
ENV-125-11(10-15)

Tot Ion:172 Resp: 745646
Ion Ratio Lower Upper
172 100
171 36.4 29.7 44.5
170 24.0 19.6 29.4

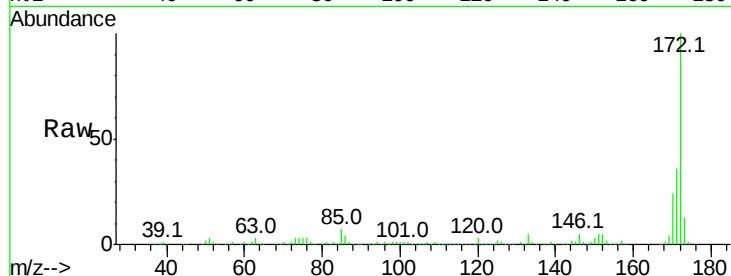


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

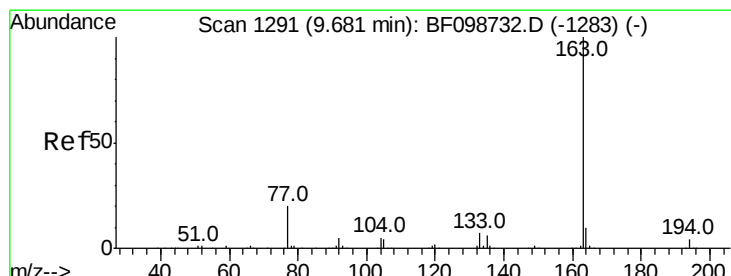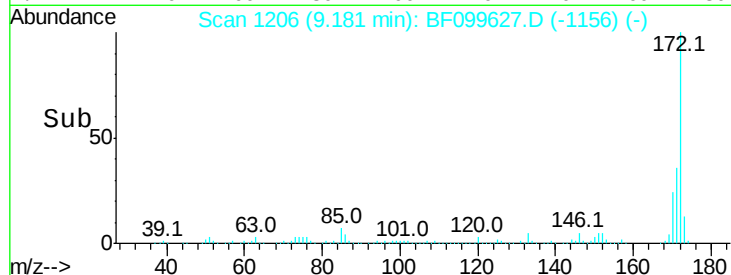
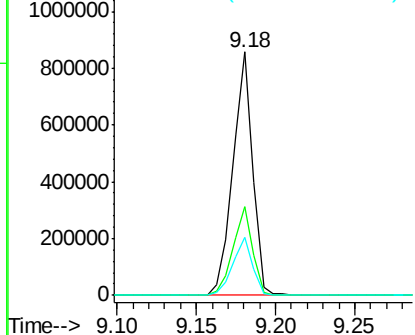



#49
Dimethylphthalate
Concen: 15.604 ng
RT: 9.57 min Scan# 1273
Delta R.T. -0.02 min
Lab File: BF099627.D
Acq: 18 Oct 2017 19:51

Tgt Ion:163 Resp: 222099
Ion Ratio Lower Upper
163 100
194 3.3 2.7 4.1
164 10.6 8.2 12.2

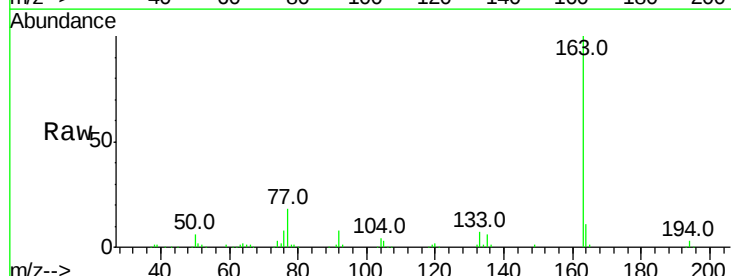

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

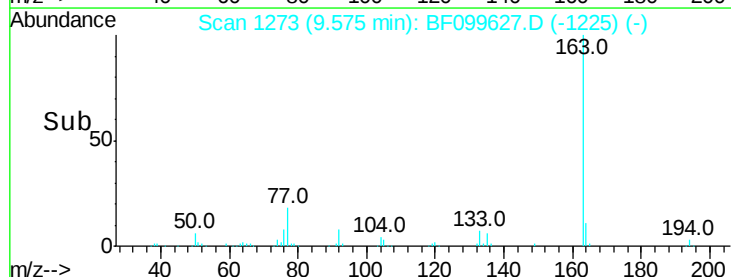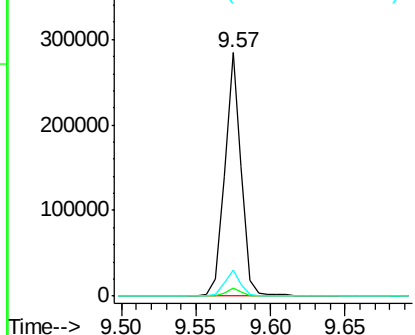


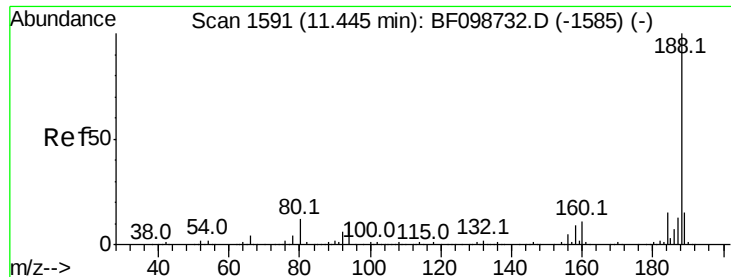




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.35 min Scan# 1575
 Delta R.T. 0.00 min
 Lab File: BF099627.D
 Acq: 18 Oct 2017 19:51

Instrument :
 BNA_F
 ClientSampleId :
 ENV-125-11(10-15)

Tot Ion:188 Resp: 305382
 Ion Ratio Lower Upper
 188 100
 94 9.0 8.5 12.7
 80 10.0 9.2 13.8

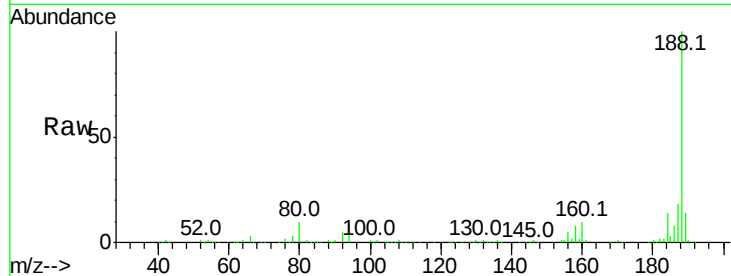


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

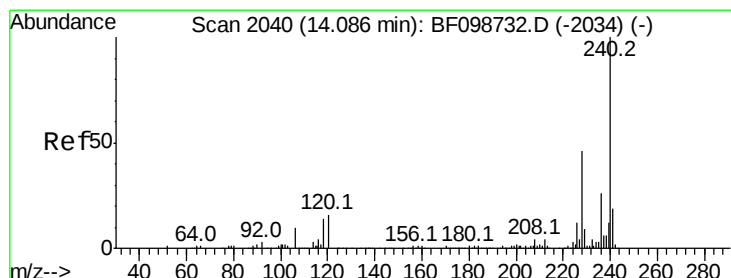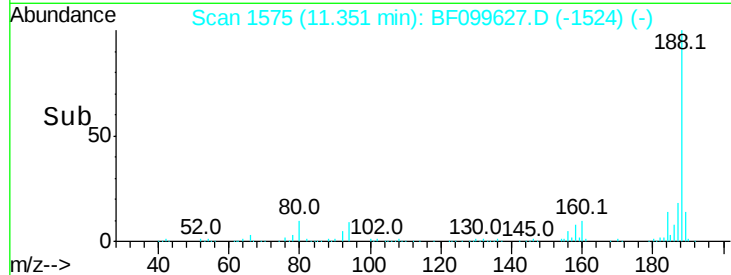
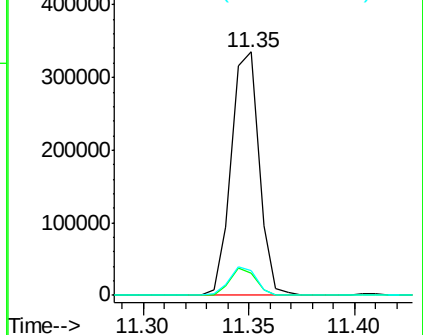



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.99 min Scan# 2024
 Delta R.T. -0.01 min
 Lab File: BF099627.D
 Acq: 18 Oct 2017 19:51

Tgt Ion:240 Resp: 186029
 Ion Ratio Lower Upper
 240 100
 120 12.7 9.5 14.3
 236 25.4 20.7 31.1

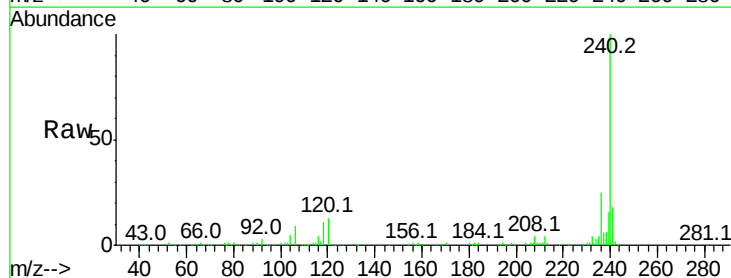

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

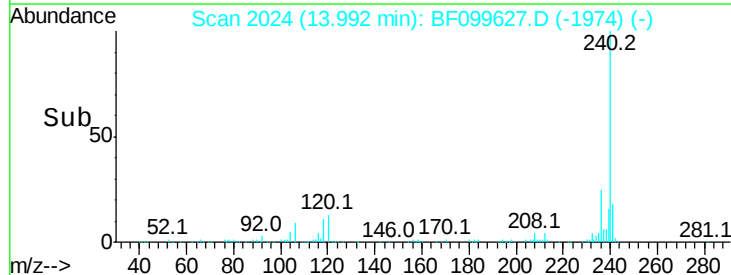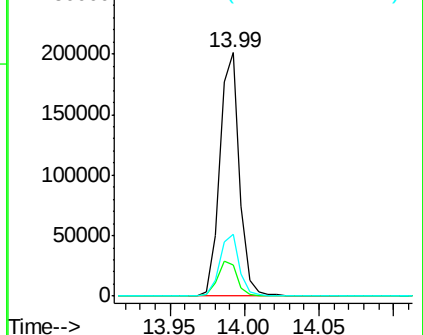

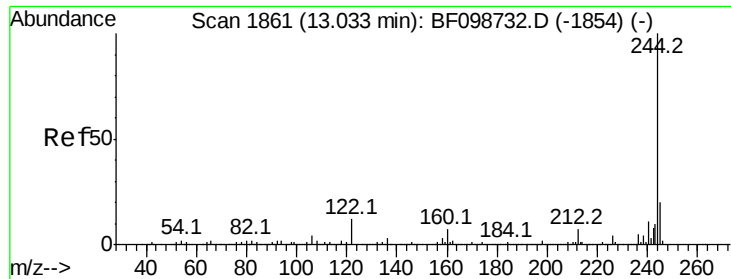

#78

Terphenyl-d14

Concen: 59.288 ng

RT: 12.93 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BF099627.D

Acq: 18 Oct 2017 19:51

Instrument :

BNA_F

ClientSampleId :

ENV-125-11(10-15)


Tot Ion:244 Resp: 484977

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 14.1 11.0 16.4

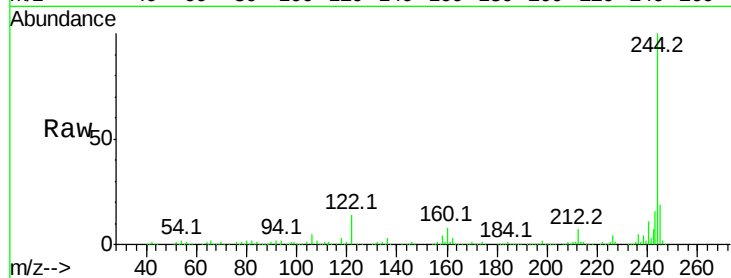

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

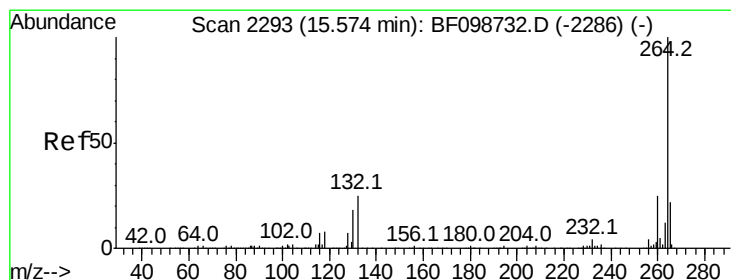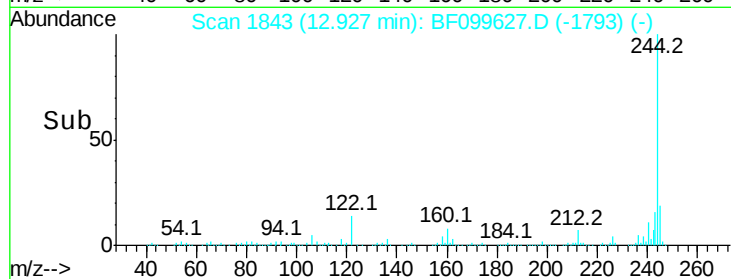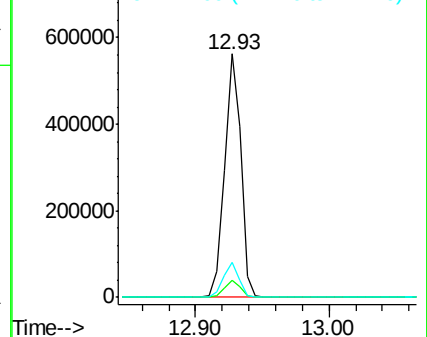

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2273

Delta R.T. 0.00 min

Lab File: BF099627.D

Acq: 18 Oct 2017 19:51


Tgt Ion:264 Resp: 195688

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 22.0 17.5 26.3

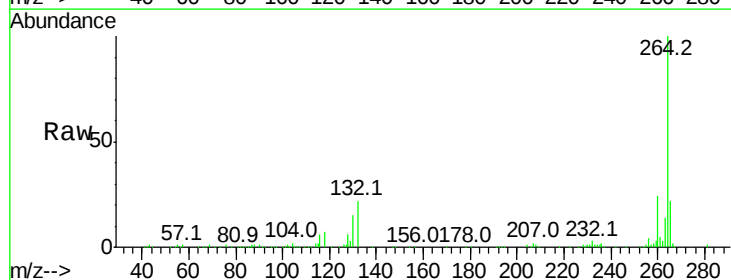

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

