

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101817\
 Data File : BF099613.D
 Acq On : 18 Oct 2017 13:17
 Operator : SJ/JU
 Sample : I5890-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ENGERT-COMP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	481	488	491	rBV2	101853	169231	4.78%	0.218%
2	5.040	497	502	503	rVV	210812	219948	6.22%	0.283%
3	5.063	503	506	517	rVV	294903	588916	16.65%	0.758%
4	5.234	530	535	539	rBV2	274038	353013	9.98%	0.455%
5	5.463	570	574	580	rVV	2401442	2571757	72.69%	3.312%
6	5.516	580	583	586	rVV	171012	167292	4.73%	0.215%
7	5.592	593	596	601	rVV3	279371	419334	11.85%	0.540%
8	5.639	601	604	607	rVV	452161	388799	10.99%	0.501%
9	5.681	607	611	617	rVB3	295516	412677	11.66%	0.531%
10	5.745	617	622	626	rVB	248569	215324	6.09%	0.277%
11	5.845	637	639	642	rVB	614649	583545	16.49%	0.752%
12	5.892	642	647	650	rBV4	478160	697375	19.71%	0.898%
13	5.981	658	662	665	rVB2	777230	1175687	33.23%	1.514%
14	6.022	665	669	672	rBV2	556152	647922	18.31%	0.834%
15	6.051	672	674	675	rBV	140484	122911	3.47%	0.158%
16	6.075	675	678	684	rBV3	1007474	1404801	39.71%	1.809%
17	6.128	684	687	689	rVB	1510253	1288685	36.42%	1.660%
18	6.163	689	693	695	rBV3	411440	577482	16.32%	0.744%
19	6.186	695	697	699	rVB	399766	298320	8.43%	0.384%
20	6.210	699	701	704	rVB2	341940	310436	8.77%	0.400%
21	6.263	704	710	713	rBV2	1329199	1789555	50.58%	2.305%
22	6.298	713	716	719	rBV3	166953	183297	5.18%	0.236%
23	6.357	722	726	734	rBV4	1720625	3001916	84.85%	3.866%
24	6.439	734	740	742	rBV3	502293	726651	20.54%	0.936%
25	6.475	742	746	748	rBV2	2248284	2670030	75.47%	3.439%
26	6.492	748	749	752	rVB3	901893	655036	18.51%	0.844%
27	6.522	752	754	756	rBV	548576	383931	10.85%	0.494%
28	6.569	756	762	765	rBV4	1176104	2235836	63.19%	2.880%
29	6.604	765	768	773	rVB	2985908	3538073	100.00%	4.557%
30	6.663	773	778	779	rBV2	743766	779082	22.02%	1.003%
31	6.681	779	781	784	rVB	889586	774476	21.89%	0.997%
32	6.710	784	786	788	rBV2	381390	345068	9.75%	0.444%
33	6.763	788	795	796	rBV5	469115	1069171	30.22%	1.377%
34	6.786	796	799	801	rBV3	569957	565236	15.98%	0.728%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101817\
 Data File : BF099613.D
 Acq On : 18 Oct 2017 13:17
 Operator : SJ/JU
 Sample : I5890-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ENGERT-COMP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	6.810	801	803	804	rBV2	316493	265077	7.49%	0.341%
36	6.839	804	808	811	rVB2	2724786	3172480	89.67%	4.086%
37	6.881	811	815	818	rVB2	801240	963964	27.25%	1.241%
38	6.916	818	821	822	rBV2	695863	736875	20.83%	0.949%
39	6.939	822	825	827	rVB	732470	754529	21.33%	0.972%
40	6.969	827	830	832	rBV	1843869	2162558	61.12%	2.785%
41	7.028	838	840	841	rVB2	241081	145127	4.10%	0.187%
42	7.051	841	844	846	rBV	826272	700082	19.79%	0.902%
43	7.092	846	851	855	rVB4	1123827	1882321	53.20%	2.424%
44	7.128	855	857	860	rVB3	230761	183220	5.18%	0.236%
45	7.169	860	864	866	rBV2	700197	699851	19.78%	0.901%
46	7.222	869	873	875	rVV3	1385601	1422958	40.22%	1.833%
47	7.245	875	877	883	rVB5	699974	916249	25.90%	1.180%
48	7.298	883	886	889	rBV2	315334	437005	12.35%	0.563%
49	7.345	889	894	895	rVV2	1146114	1291424	36.50%	1.663%
50	7.363	895	897	899	rVV	1230027	1096855	31.00%	1.413%
51	7.398	899	903	906	rVV	2019483	2208769	62.43%	2.845%
52	7.469	910	915	918	rVB3	1133047	1859826	52.57%	2.395%
53	7.522	918	924	927	rBV3	746511	1523407	43.06%	1.962%
54	7.598	934	937	940	rVV3	885603	771214	21.80%	0.993%
55	7.628	940	942	945	rVB2	674181	602197	17.02%	0.776%
56	7.704	951	955	956	rBV2	401126	500151	14.14%	0.644%
57	7.722	956	958	960	rVV	908225	808770	22.86%	1.042%
58	7.745	960	962	966	rVB3	952962	911916	25.77%	1.174%
59	7.845	976	979	988	rVB6	376103	756290	21.38%	0.974%
60	7.922	988	992	997	rVV4	349549	505789	14.30%	0.651%
61	7.975	997	1001	1004	rVV2	413994	456801	12.91%	0.588%
62	8.004	1004	1006	1008	rVV3	236002	229524	6.49%	0.296%
63	8.039	1008	1012	1013	rVV3	343685	453517	12.82%	0.584%
64	8.110	1017	1024	1029	rVV2	1104559	2105256	59.50%	2.711%
65	8.157	1029	1032	1035	rVV2	1061521	1087288	30.73%	1.400%
66	8.186	1035	1037	1043	rVV5	320424	379400	10.72%	0.489%
67	8.275	1050	1052	1054	rVV3	94879	90539	2.56%	0.117%
68	8.304	1055	1057	1059	rVB2	183444	140939	3.98%	0.182%
69	8.392	1064	1072	1076	rBV4	369079	570163	16.12%	0.734%
70	8.486	1085	1088	1090	rVB3	125321	129273	3.65%	0.166%
71	8.516	1090	1093	1095	rBV	449621	383467	10.84%	0.494%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF101817\
 Data File : BF099613.D
 Acq On : 18 Oct 2017 13:17
 Operator : SJ/JU
 Sample : I5890-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ENGERT-COMP-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	8.639	1111	1114	1116	rVV4	82294	109183	3.09%	0.141%
73	8.686	1120	1122	1126	rVV4	63734	90241	2.55%	0.116%
74	8.728	1126	1129	1131	rVV4	81434	115915	3.28%	0.149%
75	8.786	1135	1139	1143	rVB3	119204	187671	5.30%	0.242%
76	8.886	1151	1156	1160	rBV5	93778	150047	4.24%	0.193%
77	9.116	1192	1195	1201	rVB	293952	248013	7.01%	0.319%
78	9.180	1201	1206	1209	rBV	2413470	2159147	61.03%	2.781%
79	9.575	1268	1273	1276	rBV	924767	822360	23.24%	1.059%
80	9.863	1318	1322	1325	rVB	971898	857621	24.24%	1.105%
81	10.574	1440	1443	1448	rVB	128590	106455	3.01%	0.137%
82	10.657	1452	1457	1460	rBV	1425101	1476786	41.74%	1.902%
83	10.763	1470	1475	1478	rBV	131963	130470	3.69%	0.168%
84	11.351	1571	1575	1577	rBV	926332	868779	24.56%	1.119%
85	11.374	1577	1579	1583	rVB	127114	107266	3.03%	0.138%
86	11.921	1669	1672	1677	rVV6	60414	101466	2.87%	0.131%
87	11.980	1677	1682	1685	rVV5	103605	143420	4.05%	0.185%
88	12.080	1696	1699	1703	rVV3	268587	263943	7.46%	0.340%
89	12.192	1715	1718	1725	rVB	846812	823985	23.29%	1.061%
90	12.286	1730	1734	1736	rVV	317344	290869	8.22%	0.375%
91	12.363	1743	1747	1751	rVB	122741	146278	4.13%	0.188%
92	12.563	1778	1781	1783	rBV	260207	214210	6.05%	0.276%
93	12.592	1783	1786	1790	rVB	229038	194611	5.50%	0.251%
94	12.792	1815	1820	1826	rVV	243142	262728	7.43%	0.338%
95	12.898	1835	1838	1840	rBV2	128927	135168	3.82%	0.174%
96	12.927	1840	1843	1847	rVB	1613712	1504104	42.51%	1.937%
97	13.063	1863	1866	1869	rVB	377071	309368	8.74%	0.398%
98	13.992	2019	2024	2027	rBV2	570648	599273	16.94%	0.772%
99	15.456	2268	2273	2277	rVV	395429	495975	14.02%	0.639%
100	16.933	2521	2524	2531	rVB2	56854	93886	2.65%	0.121%


Sum of corrected areas: 77645122

Data Path : Z:\HPCHEM1\BNA F\DATA\BF101817\
Data File : BF099613.D
Acq On : 18 Oct 2017 13:17
Operator : SJ/JU
Sample : I5890-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ENGERT-COMP-1

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

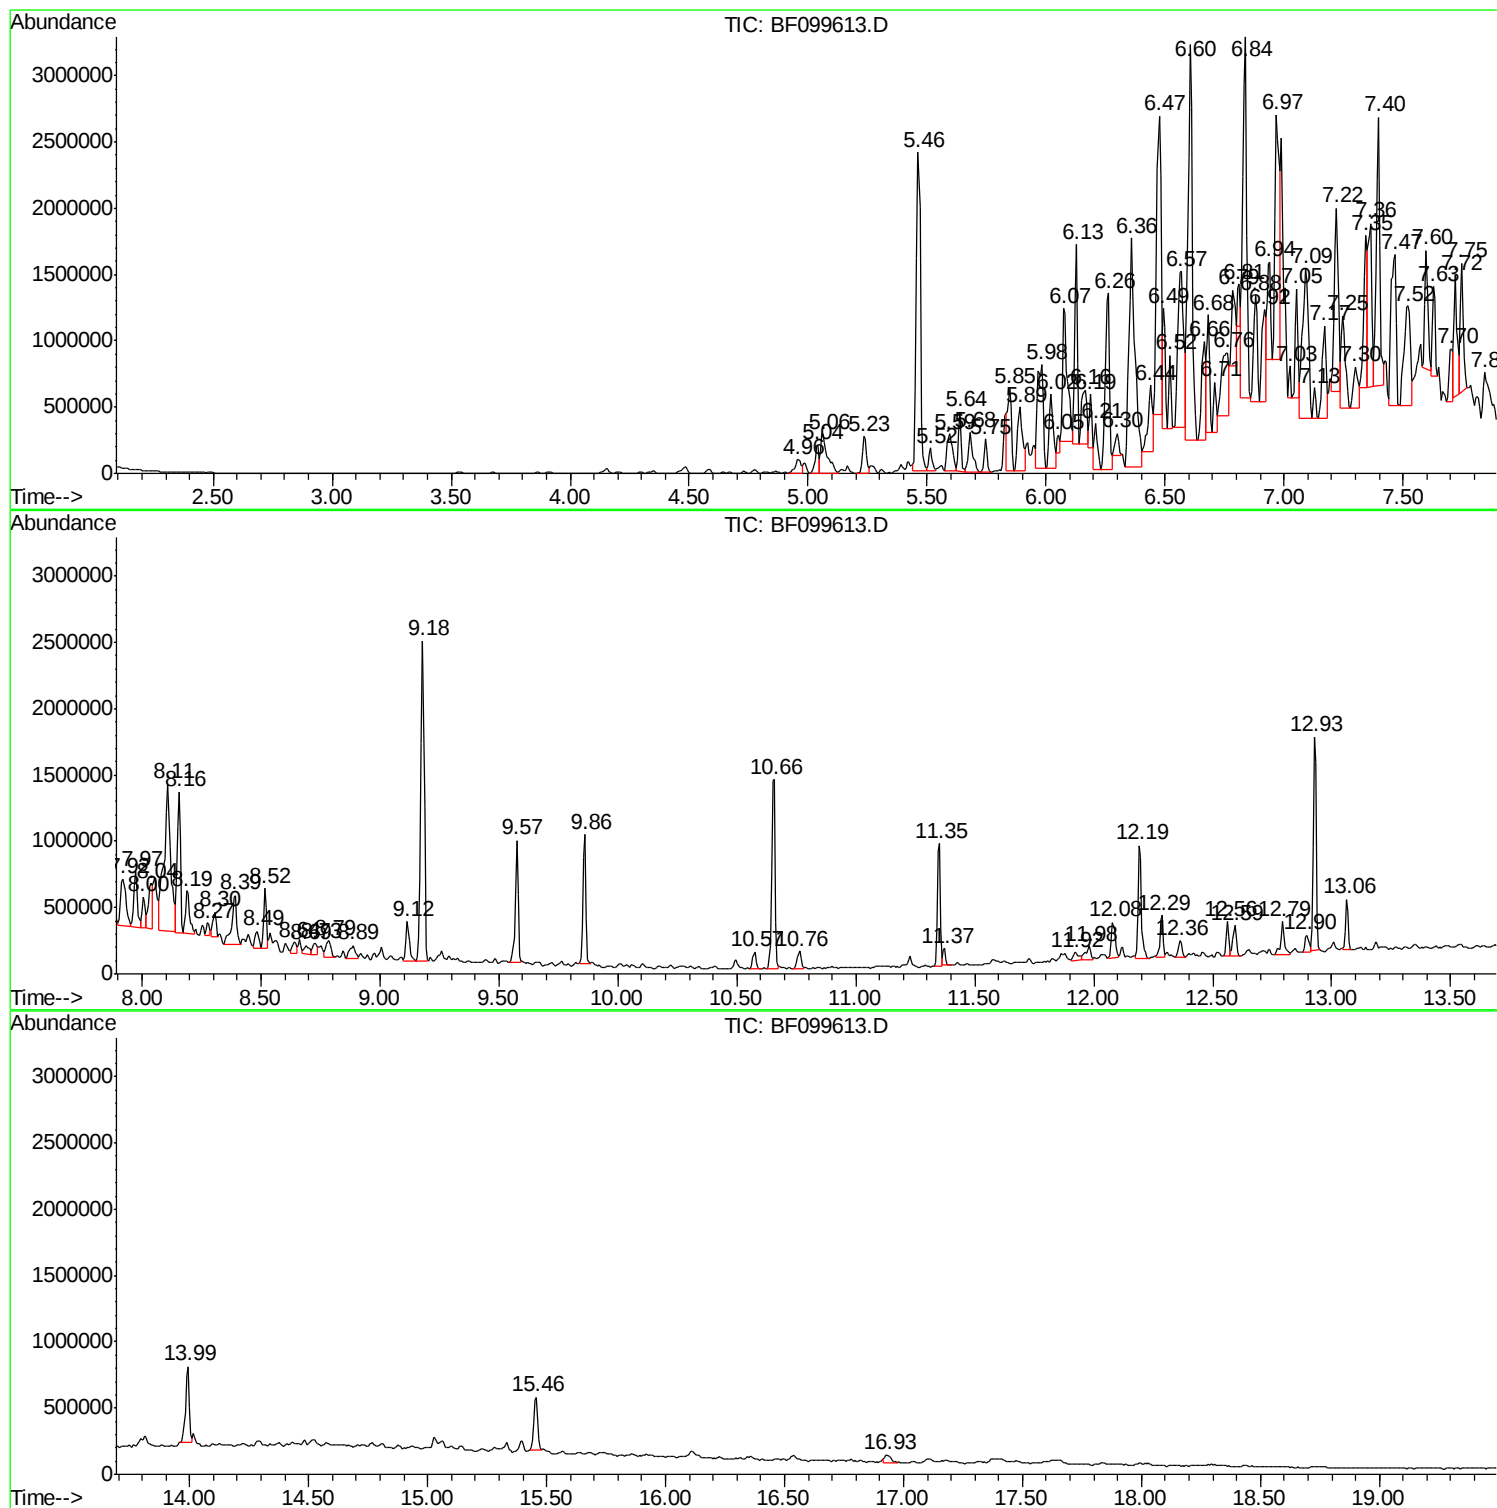

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF101817\
Data_File : BF099613.D
Acq_On : 18_Oct_2017. 13:177
Operator : SJ/JUU
Sample : I5890-166
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
ENGERT-COMP-1

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
