


Data Path : Z:\HPCHEM1\BNA F\Data\BF101817\
 Data File : BF099606.D
 Acq On : 18 Oct 2017 9:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 18 22:24:53 2017

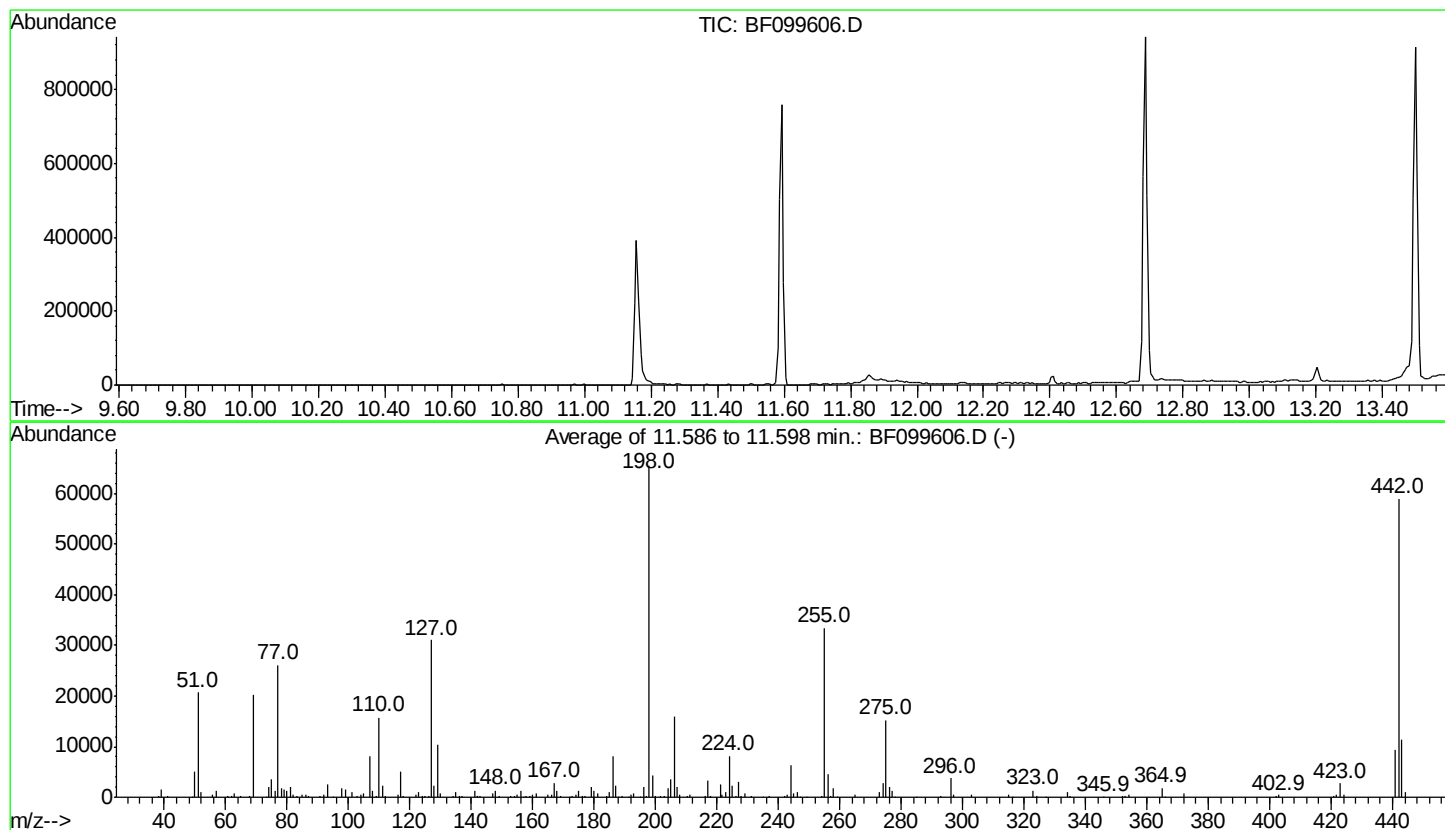

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	20678	PASS
68	69	0.00	2	1.4	291	PASS
69	198	0.00	100	30.9	20276	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	31115	PASS
197	198	0.00	2	0.4	292	PASS
198	198	100	100	100.0	65536	PASS
199	198	5	9	6.5	4243	PASS
275	198	10	60	23.2	15215	PASS
365	198	1	100	2.8	1830	PASS
441	442	0.01	24	15.8	9319	PASS
442	198	50	100	90.0	58968	PASS
443	442	15	24	19.2	11293	PASS