

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101818\
 Data File : BF109967.D
 Acq On : 18 Oct 2018 19:10
 Operator : JU/SJ
 Sample : J5565-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Oct 19 02:24:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 14:58:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	195100	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	756480	20.00	ng	-0.01
39) Acenaphthene-d10	10.02	164	353320	20.00	ng	-0.01
64) Phenanthrene-d10	11.51	188	646126	20.00	ng	0.00
76) Chrysene-d12	14.15	240	436945	20.00	ng	-0.01
87) Perylene-d12	15.67	264	369905	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	1391085	113.02	ng	0.00
7) Phenol-d6	6.60	99	1756584	114.93	ng	0.00
23) Nitrobenzene-d5	7.54	82	1098836	97.85	ng	-0.01
42) 2,4,6-Tribromophenol	10.81	330	420476	137.46	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	1868897	84.40	ng	0.00
79) Terphenyl-d14	13.09	244	1699564	81.68	ng	-0.01
Target Compounds						
10) Phenol	6.60	94	99351	6.021	ng	# 69
19) n-Nitroso-di-n-propylamine	7.54	70	147296	15.010	ng	# 78
25) Isophorone	7.54	82	1098823	49.799	ng	# 67
50) Dimethylphthalate	9.72	163	312263	12.481	ng	# 99
57) 2,4-Dinitrotoluene	10.02	165	43865	11.193	ng	# 19
65) 4,6-Dinitro-2-methylphenol	10.81	198	854	8.209	ng	# 1
67) 4-Bromophenyl-phenylether	10.81	248	26418	3.773	ng	# 1
84) Bis(2-ethylhexyl)phthalate	14.01	149	139229	8.155	ng	# 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101818\
Data File : BF109967.D
Acq On : 18 Oct 2018 19:10
Operator : JU/SJ
Sample : J5565-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Oct 19 02:24:25 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

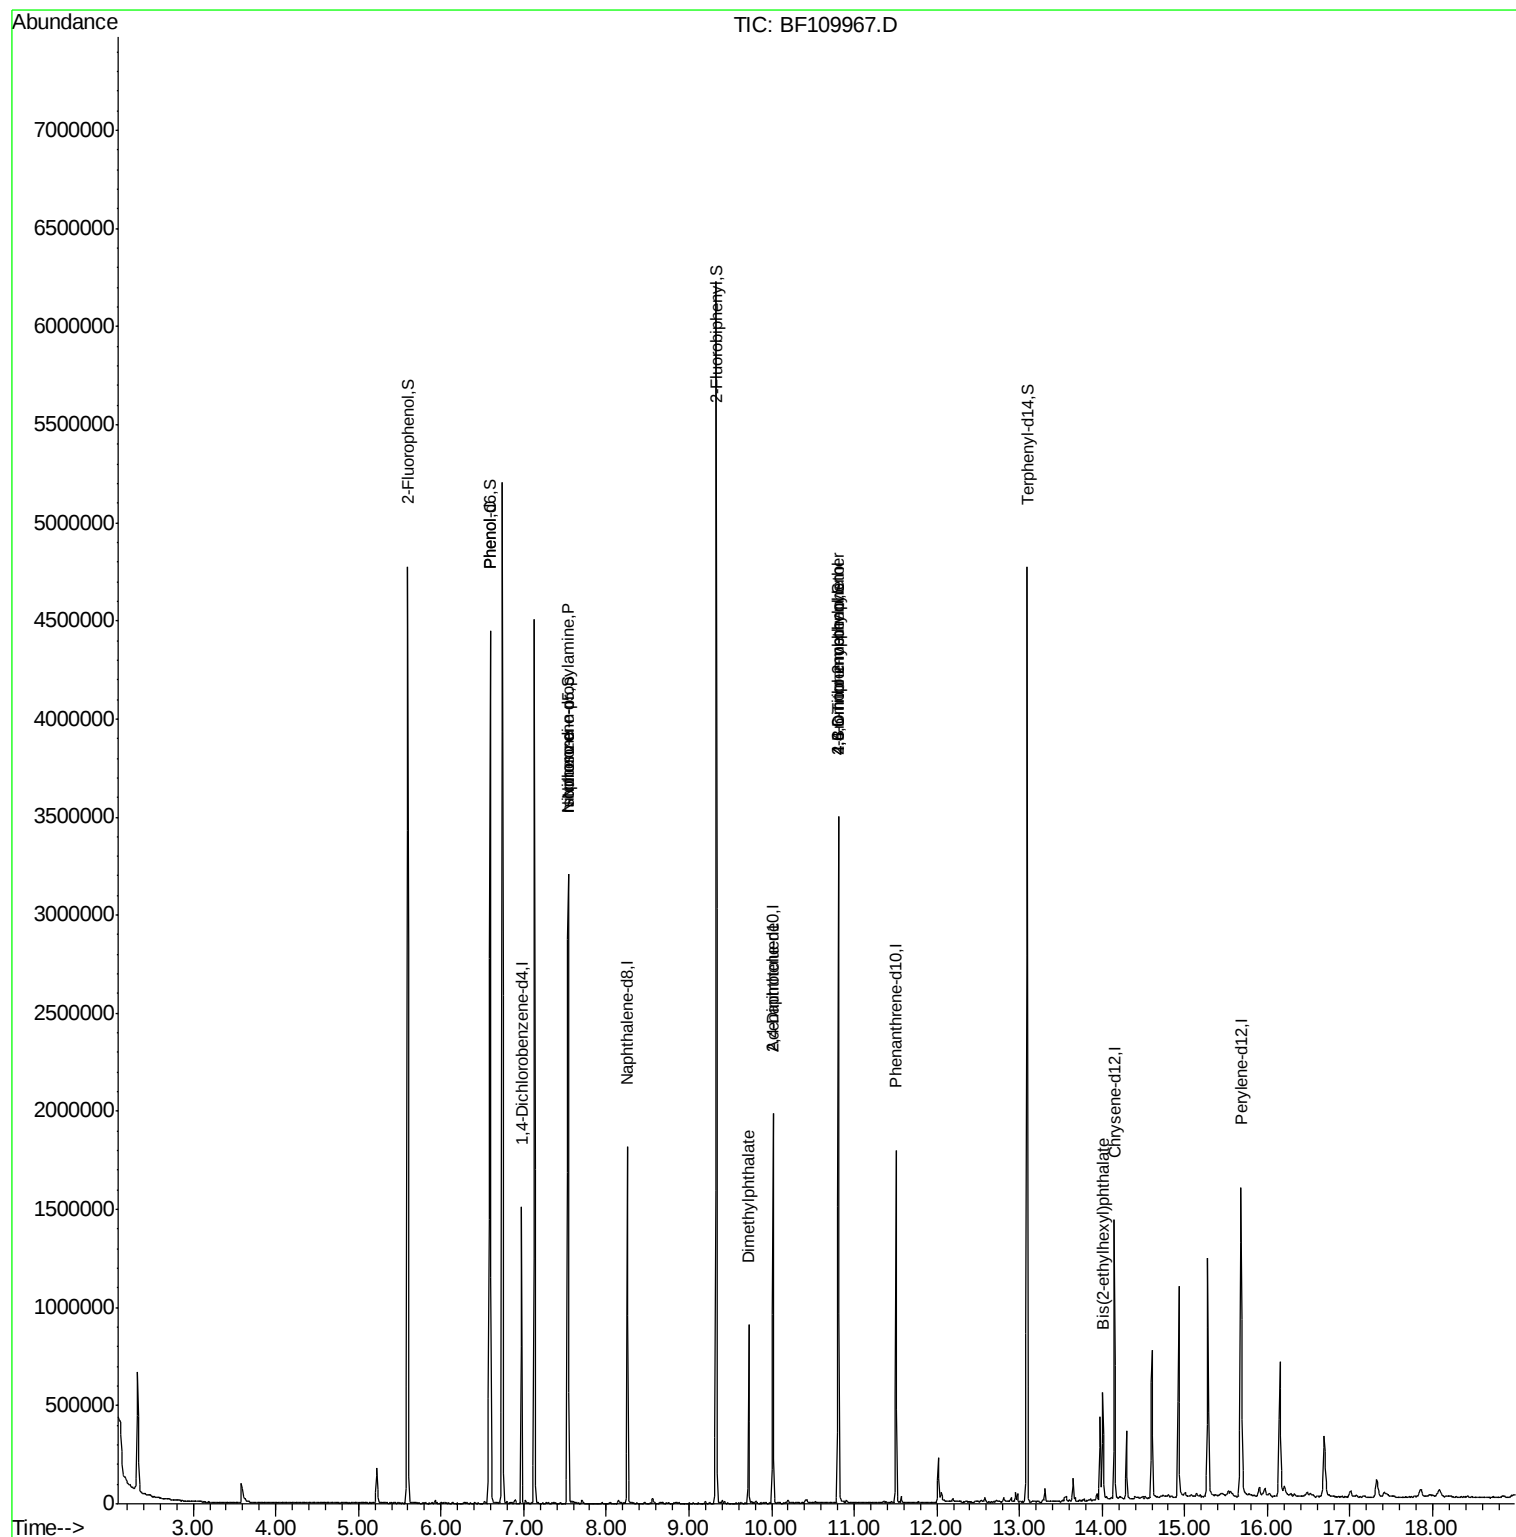

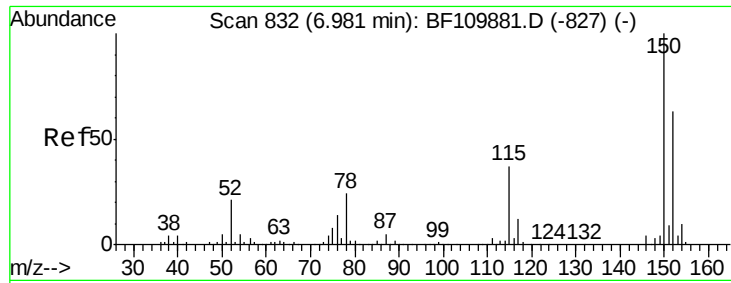


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 831
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 195100
Ion Ratio Lower Upper
152 100
150 155.4 122.7 184.1
115 60.6 49.1 73.7




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

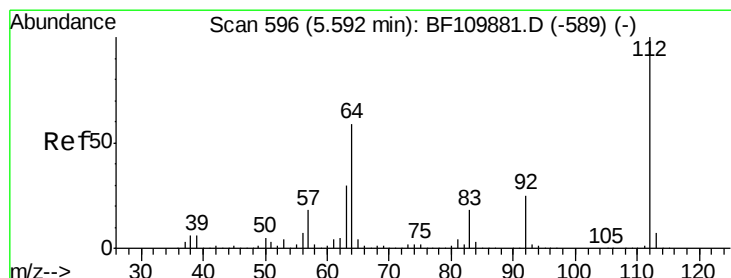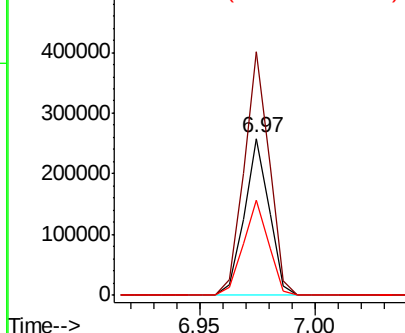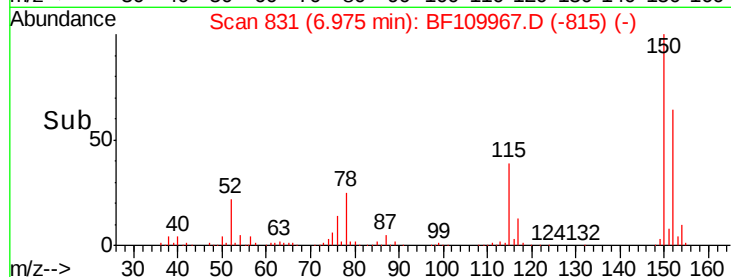



#5


2-Fluorophenol
Concen: 113.022 ng
RT: 5.60 min Scan# 597
Delta R.T. -0.00 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:112 Resp: 1391085
Ion Ratio Lower Upper
112 100
64 61.8 44.1 66.1
63 32.7 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

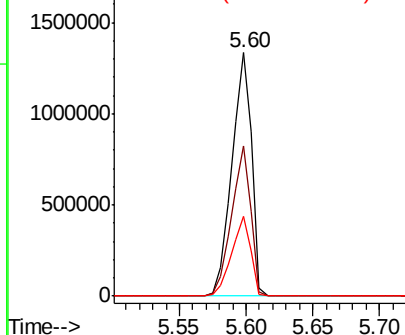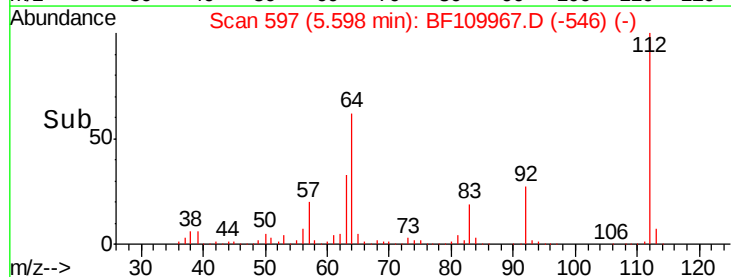

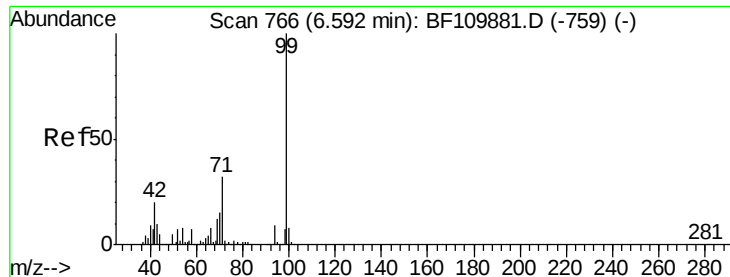

#7

Phenol-d6

Concen: 114.934 ng

RT: 6.60 min Scan# 767

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10


Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 1756584

Ion	Ratio	Lower	Upper
99	100		
42	18.6	15.8	23.6
71	34.2	28.0	42.0






Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

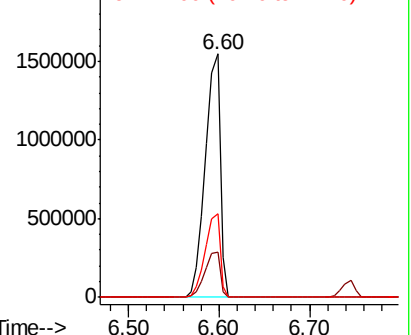

#10

Phenol

Concen: 6.021 ng

RT: 6.60 min Scan# 768


Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Tgt Ion: 94 Resp: 99351

Ion	Ratio	Lower	Upper
94	100		
65	30.2	25.3	65.3
66	43.4	54.5	94.5#






Abundance

Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1



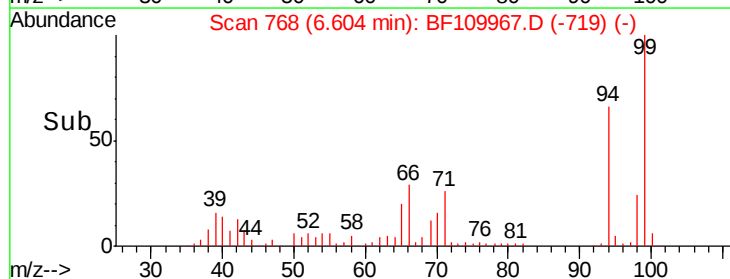
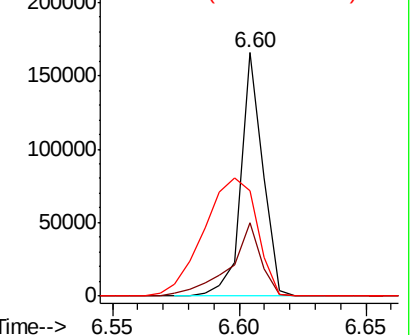


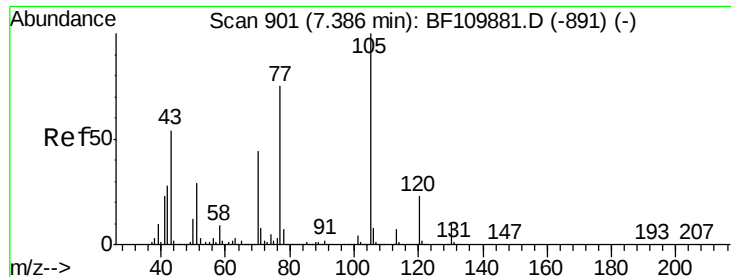

#19
n-Nitroso-di-n-propylamine
Concen: 15.010 ng
RT: 7.54 min Scan# 927
Delta R.T. 0.15 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 70 Resp: 147296
Ion Ratio Lower Upper
70 100
42 47.8 47.4 71.2
101 0.0 7.3 10.9#
130 2.4 16.2 24.2#

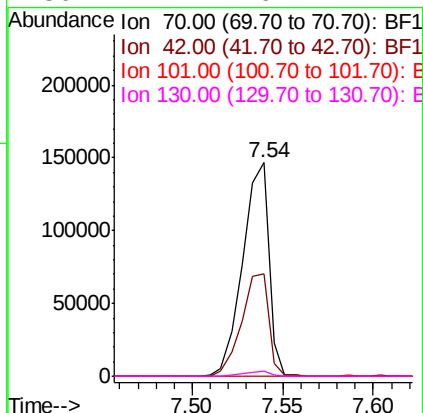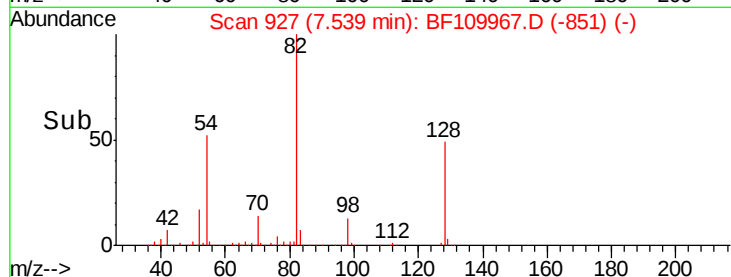

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.26 min Scan# 1049
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:136 Resp: 756480
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 8.2 5.4 8.2#
68 5.8 4.2 6.2

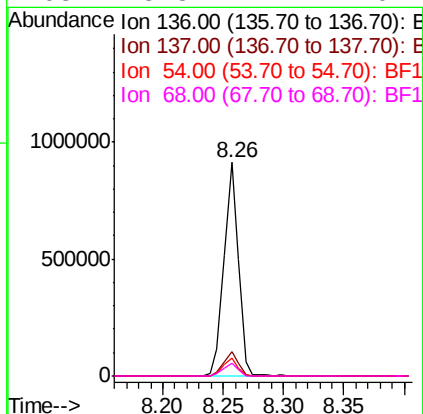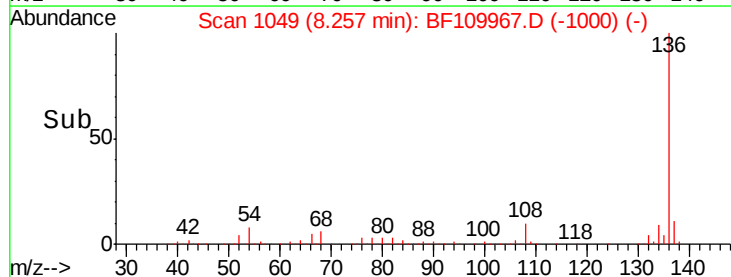


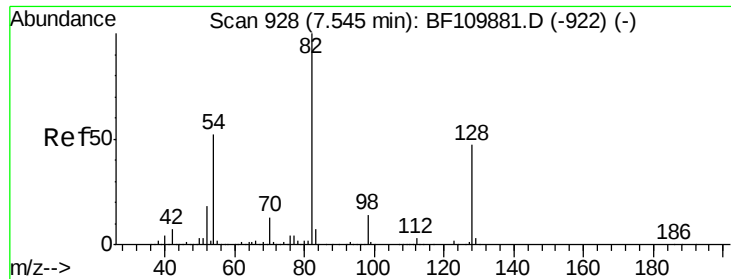




#23
Nitrobenzene-d5
Concen: 97.850 ng
RT: 7.54 min Scan# 927
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion	82	Resp	1098836
Ion	Ratio	Lower	Upper
82	100		
128	49.0	34.2	51.2
54	52.0	38.6	58.0




Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

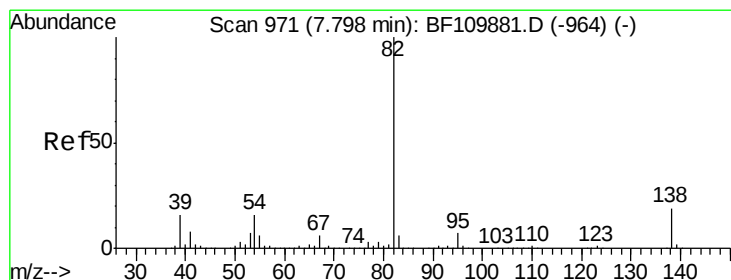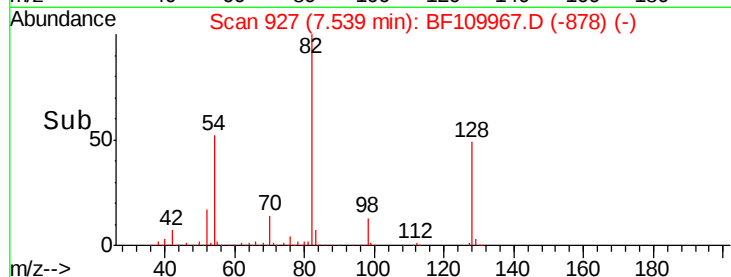
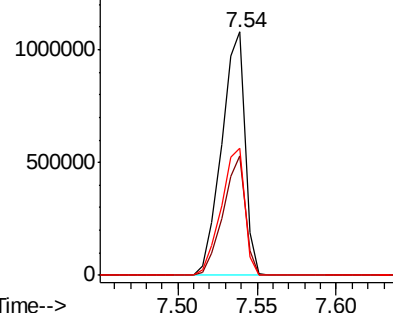



#25
Isophorone
Concen: 49.799 ng
RT: 7.54 min Scan# 927
Delta R.T. -0.26 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion	82	Resp	1098823
Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.7	8.5#
138	0.0	13.2	19.8#

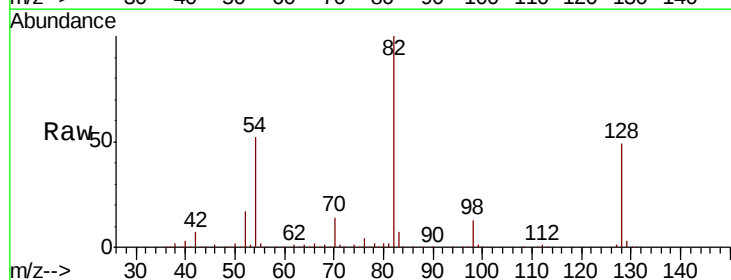

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

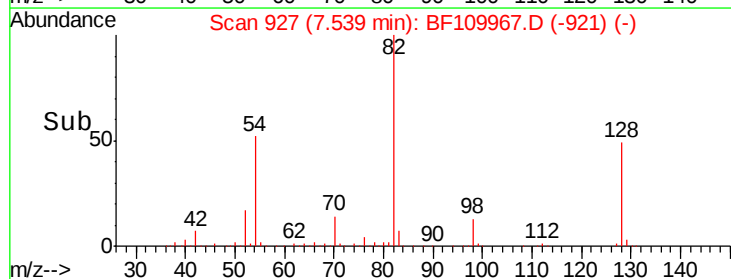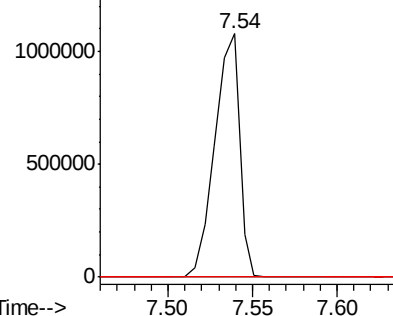


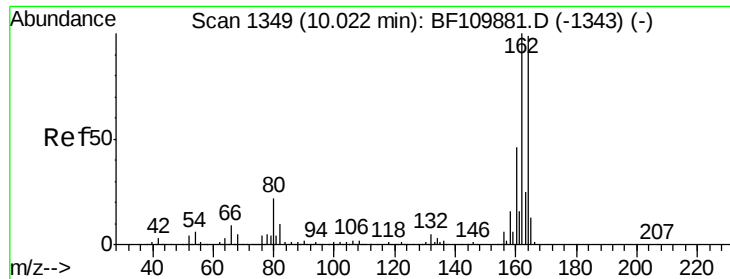




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.02 min Scan# 1348
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 353320
Ion Ratio Lower Upper
164 100
162 104.3 83.0 124.6
160 47.1 37.0 55.6




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


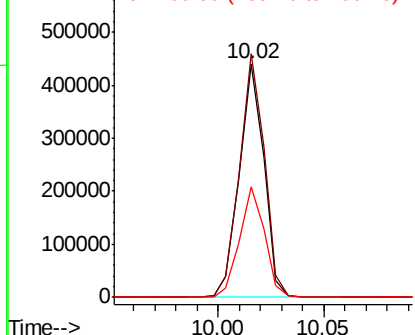



#42
2,4,6-Tribromophenol
Concen: 137.458 ng
RT: 10.81 min Scan# 1483
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:330 Resp: 420476
Ion Ratio Lower Upper
330 100
332 96.1 77.1 115.7
141 36.5 27.0 40.4



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

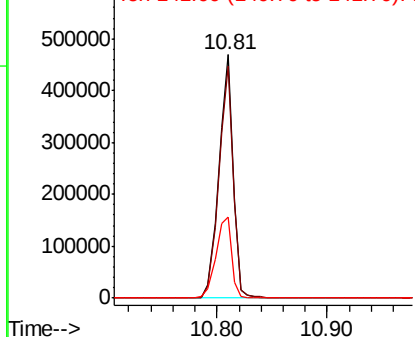


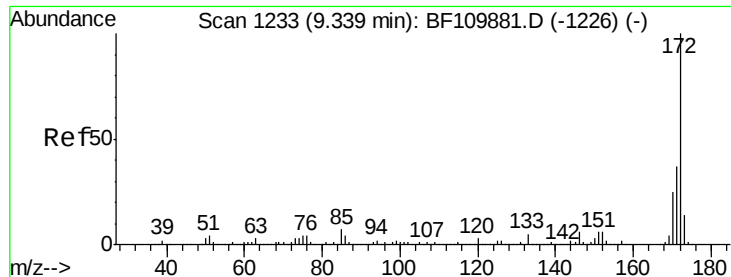




#45
2-Fluorobiphenyl
Concen: 84.403 ng
RT: 9.33 min Scan# 1232
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 1868897
Ion Ratio Lower Upper
172 100
171 37.3 28.6 43.0
170 24.6 19.7 29.5




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

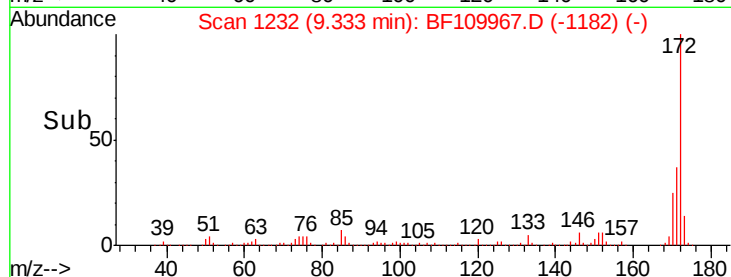
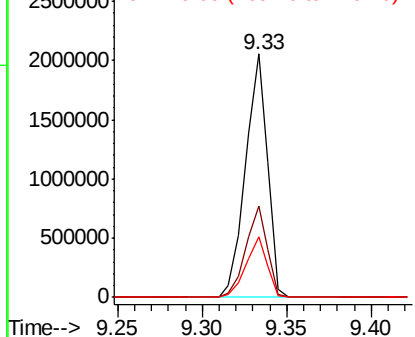



#50
Dimethylphthalate
Concen: 12.481 ng
RT: 9.72 min Scan# 1298
Delta R.T. -0.02 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:163 Resp: 312263
Ion Ratio Lower Upper
163 100
194 3.4 3.2 4.8
164 10.2 8.1 12.1



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

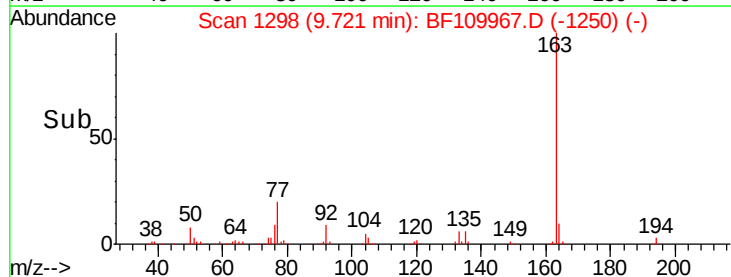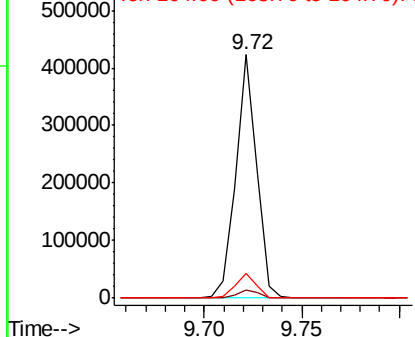

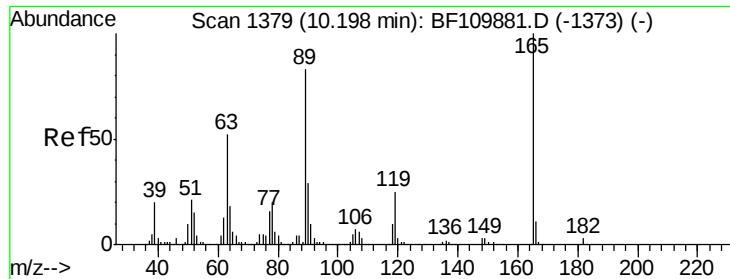

#57

2,4-Dinitrotoluene

Concen: 11.193 ng

RT: 10.02 min Scan# 1348

Delta R.T. -0.19 min


Lab File: BF109967.D

Acq: 18 Oct 2018 19:10




Instrument :

BNA_F

ClientSampleId :

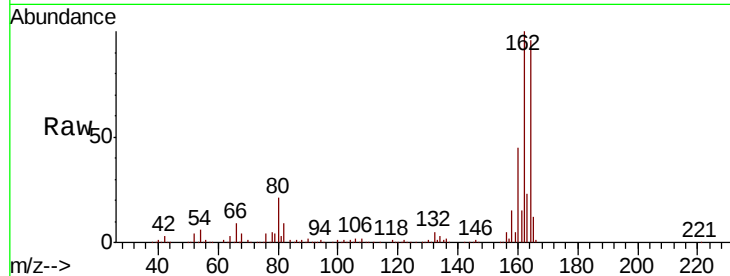

Tot Ion:	165	Resp:	43865
Ion	Ratio	Lower	Upper
165	100		
63	1.3	44.8	67.2#
89	1.3	62.2	93.4#
182	0.0	2.1	3.1#

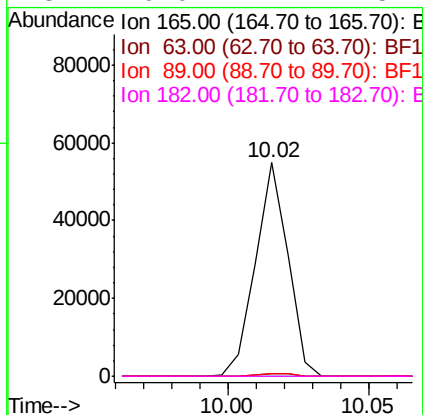

#64

Phenanthrene-d10

Concen: 20.000 ng




RT: 11.51 min Scan# 1602


Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Tgt Ion:	188	Resp:	646126
Ion	Ratio	Lower	Upper
188	100		
94	9.5	7.2	10.8
80	10.0	7.9	11.9

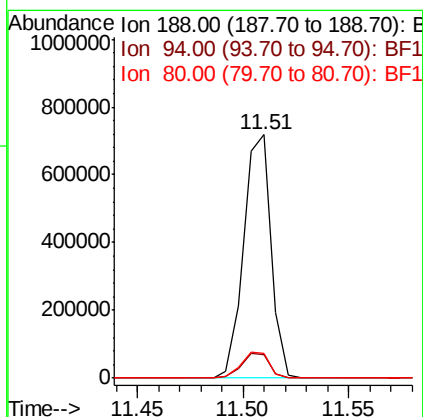


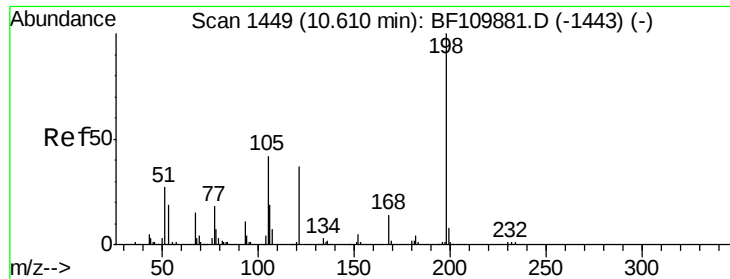




#65
 4,6-Dinitro-2-methylphenol
 Concen: 8.209 ng
 RT: 10.81 min Scan# 1483
 Delta R.T. 0.19 min
 Lab File: BF109967.D
 Acq: 18 Oct 2018 19:10

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
198	100		
51	169.8	22.8	62.8#
105	176.4	23.6	63.6#




Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E


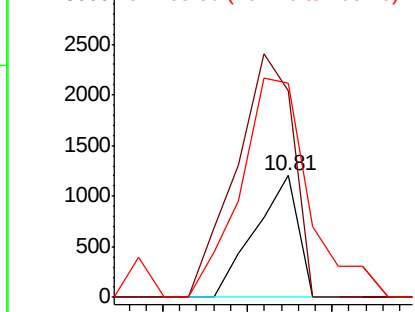



#67
 4-Bromophenyl-phenylether
 Concen: 3.773 ng
 RT: 10.81 min Scan# 1483
 Delta R.T. -0.25 min
 Lab File: BF109967.D
 Acq: 18 Oct 2018 19:10

Tgt Ion	Ratio	Lower	Upper
248	100		
250	196.2	79.4	119.2#
141	508.3	55.9	83.9#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

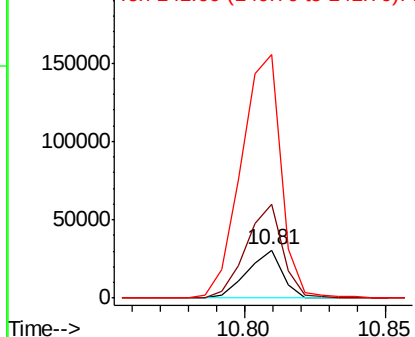



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2051

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 436945

Ion Ratio Lower Upper

240 100

120 12.2 8.3 12.5




236 25.8 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

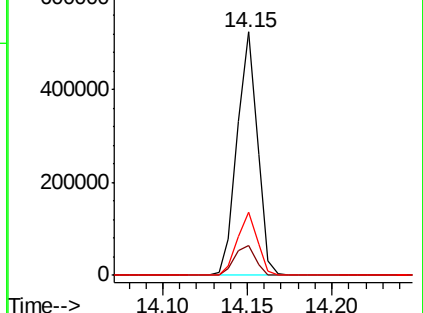

#79

Terphenyl-d14

Concen: 81.680 ng

RT: 13.09 min Scan# 1871

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10


Tgt Ion:244 Resp: 1699564

Ion Ratio Lower Upper

244 100

212 7.3 5.8 8.8



122 13.6 8.7 13.1#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

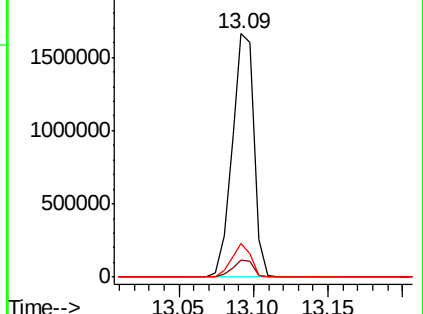



#84

Bis(2-ethylhexyl)phthalate

Concen: 8.155 ng

RT: 14.01 min Scan# 2027

Delta R.T. -0.12 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Instrument :

BNA_F

ClientSampleId :


Tot Ion:149 Resp: 139229

Ion Ratio Lower Upper

149 100

167 0.0 19.8 29.8#

279 0.0 2.7 4.1#






Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

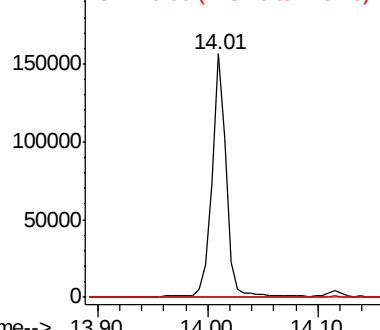

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2310

Delta R.T. -0.02 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10


Tgt Ion:264 Resp: 369905

Ion Ratio Lower Upper

264 100

260 22.2 18.7 28.1

265 21.3 16.7 25.1



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

