
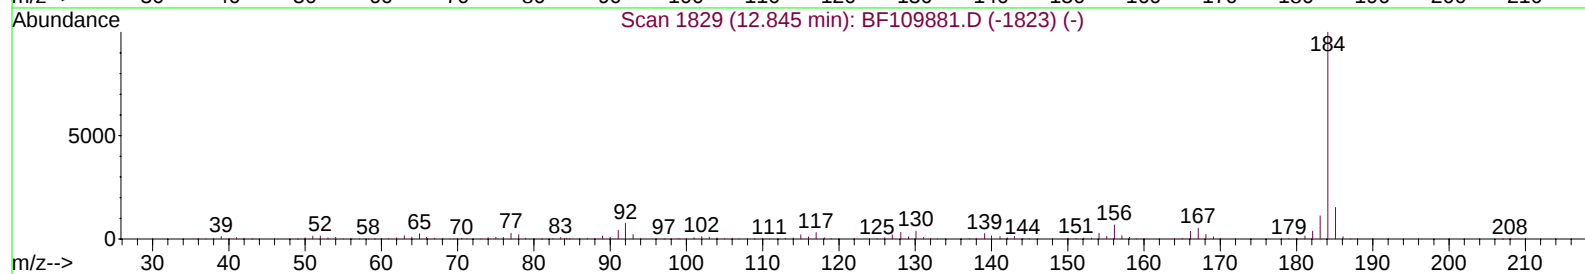
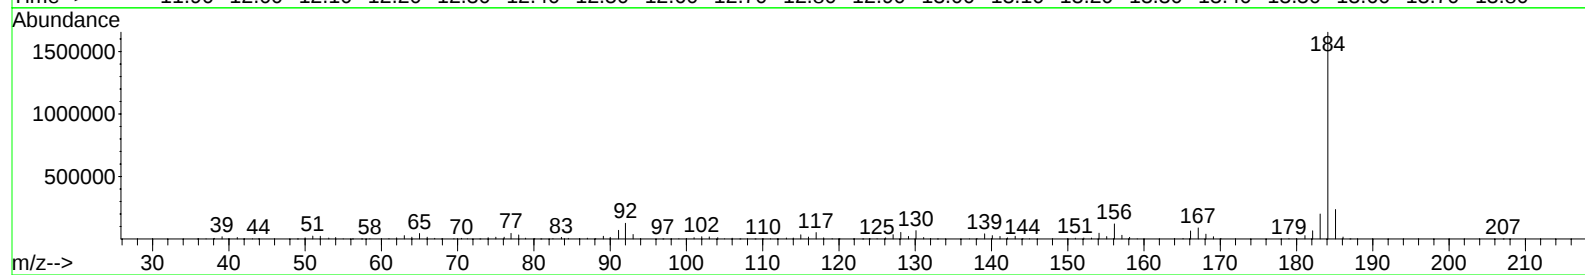


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101818\
 Data File : BF109950.D
 Acq On : 18 Oct 2018 10:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 07:34:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 14:58:24 2018
 Response via : Initial Calibration

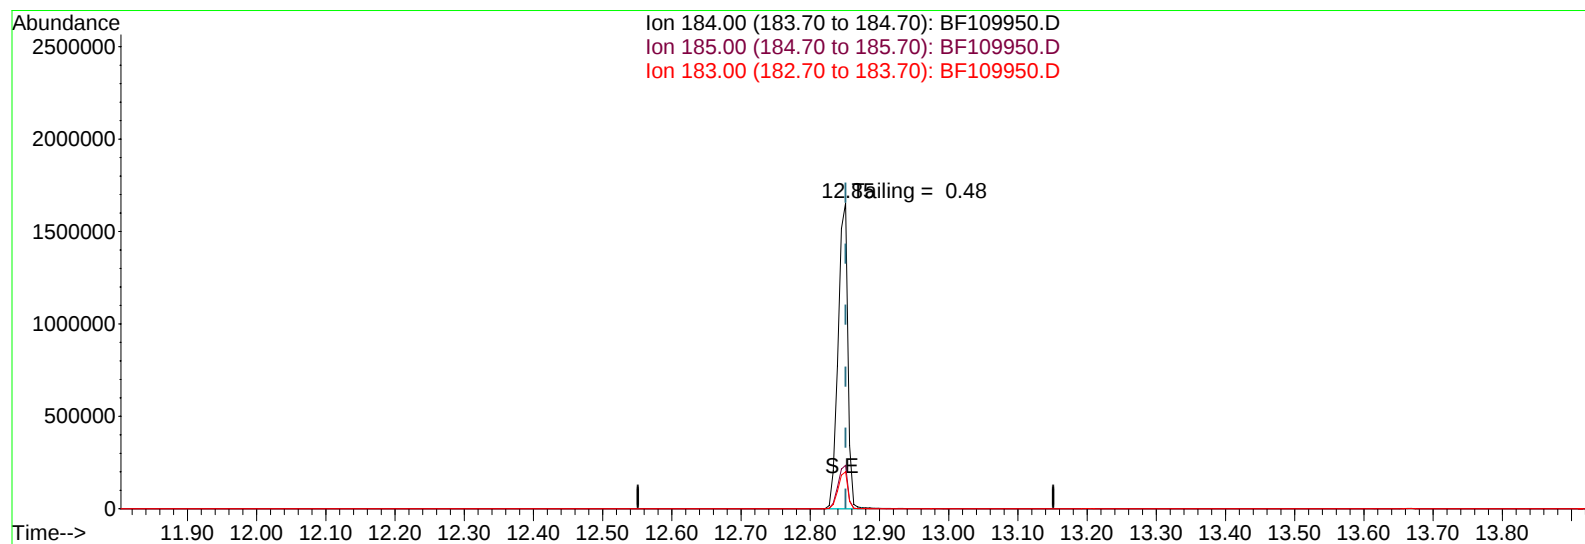

TIC: BF109950.D

(77) Benzidine




12.851min (-0.000) 0.00ng

response 1612071

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.24
183.00	11.80	12.08
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF101818\  
Data File   : BF109950.D  
Acq On      : 18 Oct 2018   10:15  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Oct 22 07:34:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

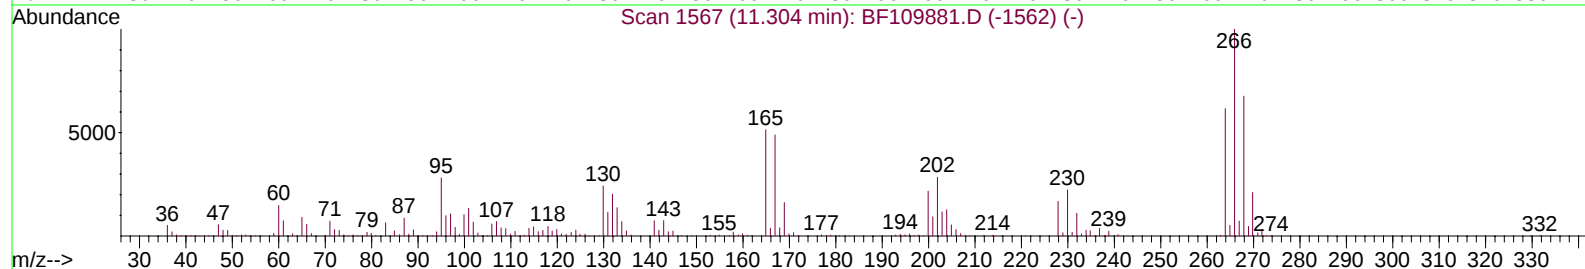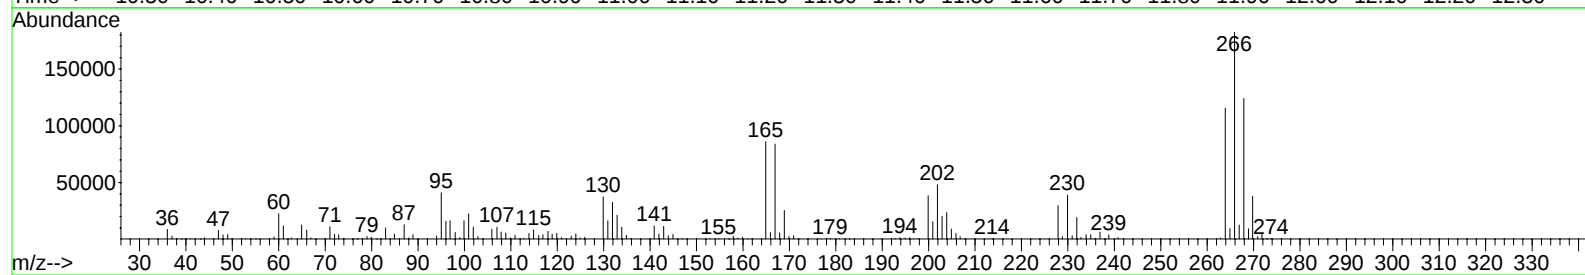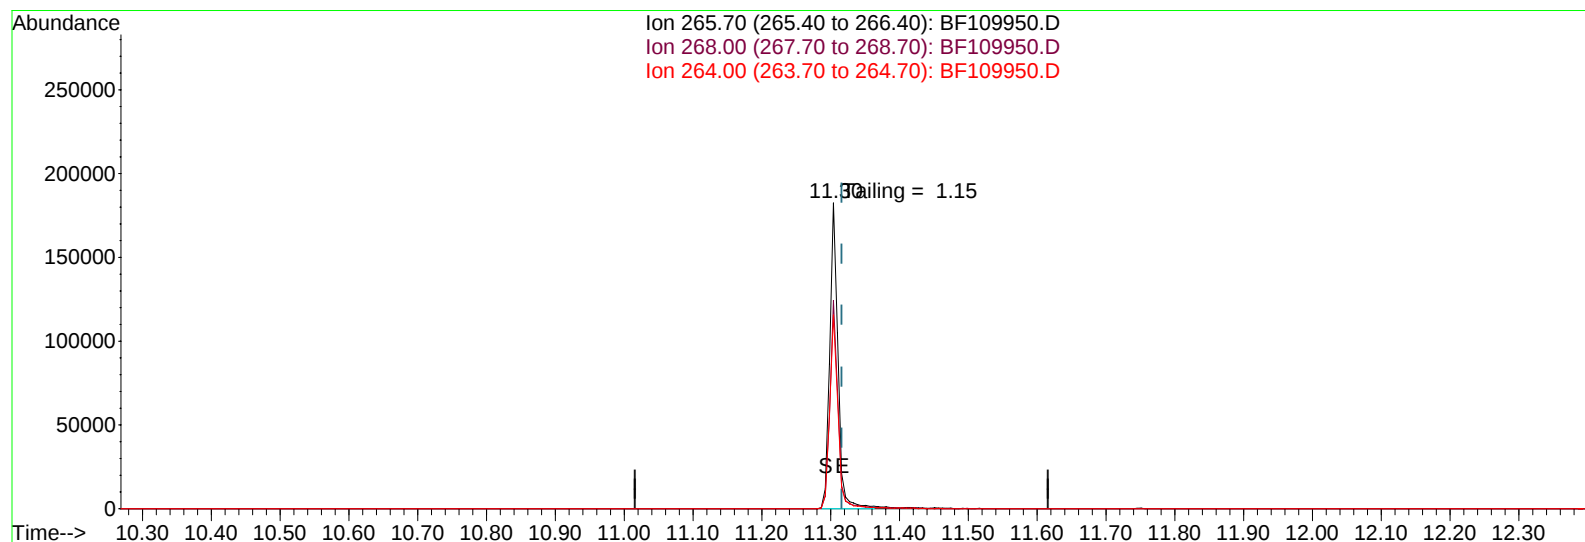

(70) Pentachlorophenol (C)

11.304min (-0.012) 34802.98ng

```
response 154048
```

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	68.13
264.00	63.20	63.37
0.00	0.00	0.00