

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101818\
 Data File : BF109967.D
 Acq On : 18 Oct 2018 19:10
 Operator : JU/SJ
 Sample : J5565-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RLF-SD-3

Quant Time: Oct 19 04:07:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 16 14:58:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	195100	20.00	ng	0.00
21) Naphthalene-d8	8.26	136	756480	20.00	ng	-0.01
39) Acenaphthene-d10	10.02	164	353320	20.00	ng	-0.01
64) Phenanthrene-d10	11.51	188	646126	20.00	ng	0.00
76) Chrysene-d12	14.15	240	436945	20.00	ng	-0.01
87) Perylene-d12	15.67	264	369905	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	1391085	113.02	ng	0.00
7) Phenol-d6	6.60	99	1756584	114.93	ng	0.00
23) Nitrobenzene-d5	7.54	82	1098836	97.85	ng	-0.01
42) 2,4,6-Tribromophenol	10.81	330	420476	137.46	ng	0.00
45) 2-Fluorobiphenyl	9.33	172	1868897	84.40	ng	0.00
79) Terphenyl-d14	13.09	244	1699564	81.68	ng	-0.01
Target Compounds						
10) Phenol	6.60	94	99351	6.021	ng	Qvalue # 69
50) Dimethylphthalate	9.72	163	312263	12.481	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101818\
Data File : BF109967.D
Acq On : 18 Oct 2018 19:10
Operator : JU/SJ
Sample : J5565-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RLF-SD-3

Quant Time: Oct 19 04:07:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 16 14:58:24 2018
Response via : Initial Calibration

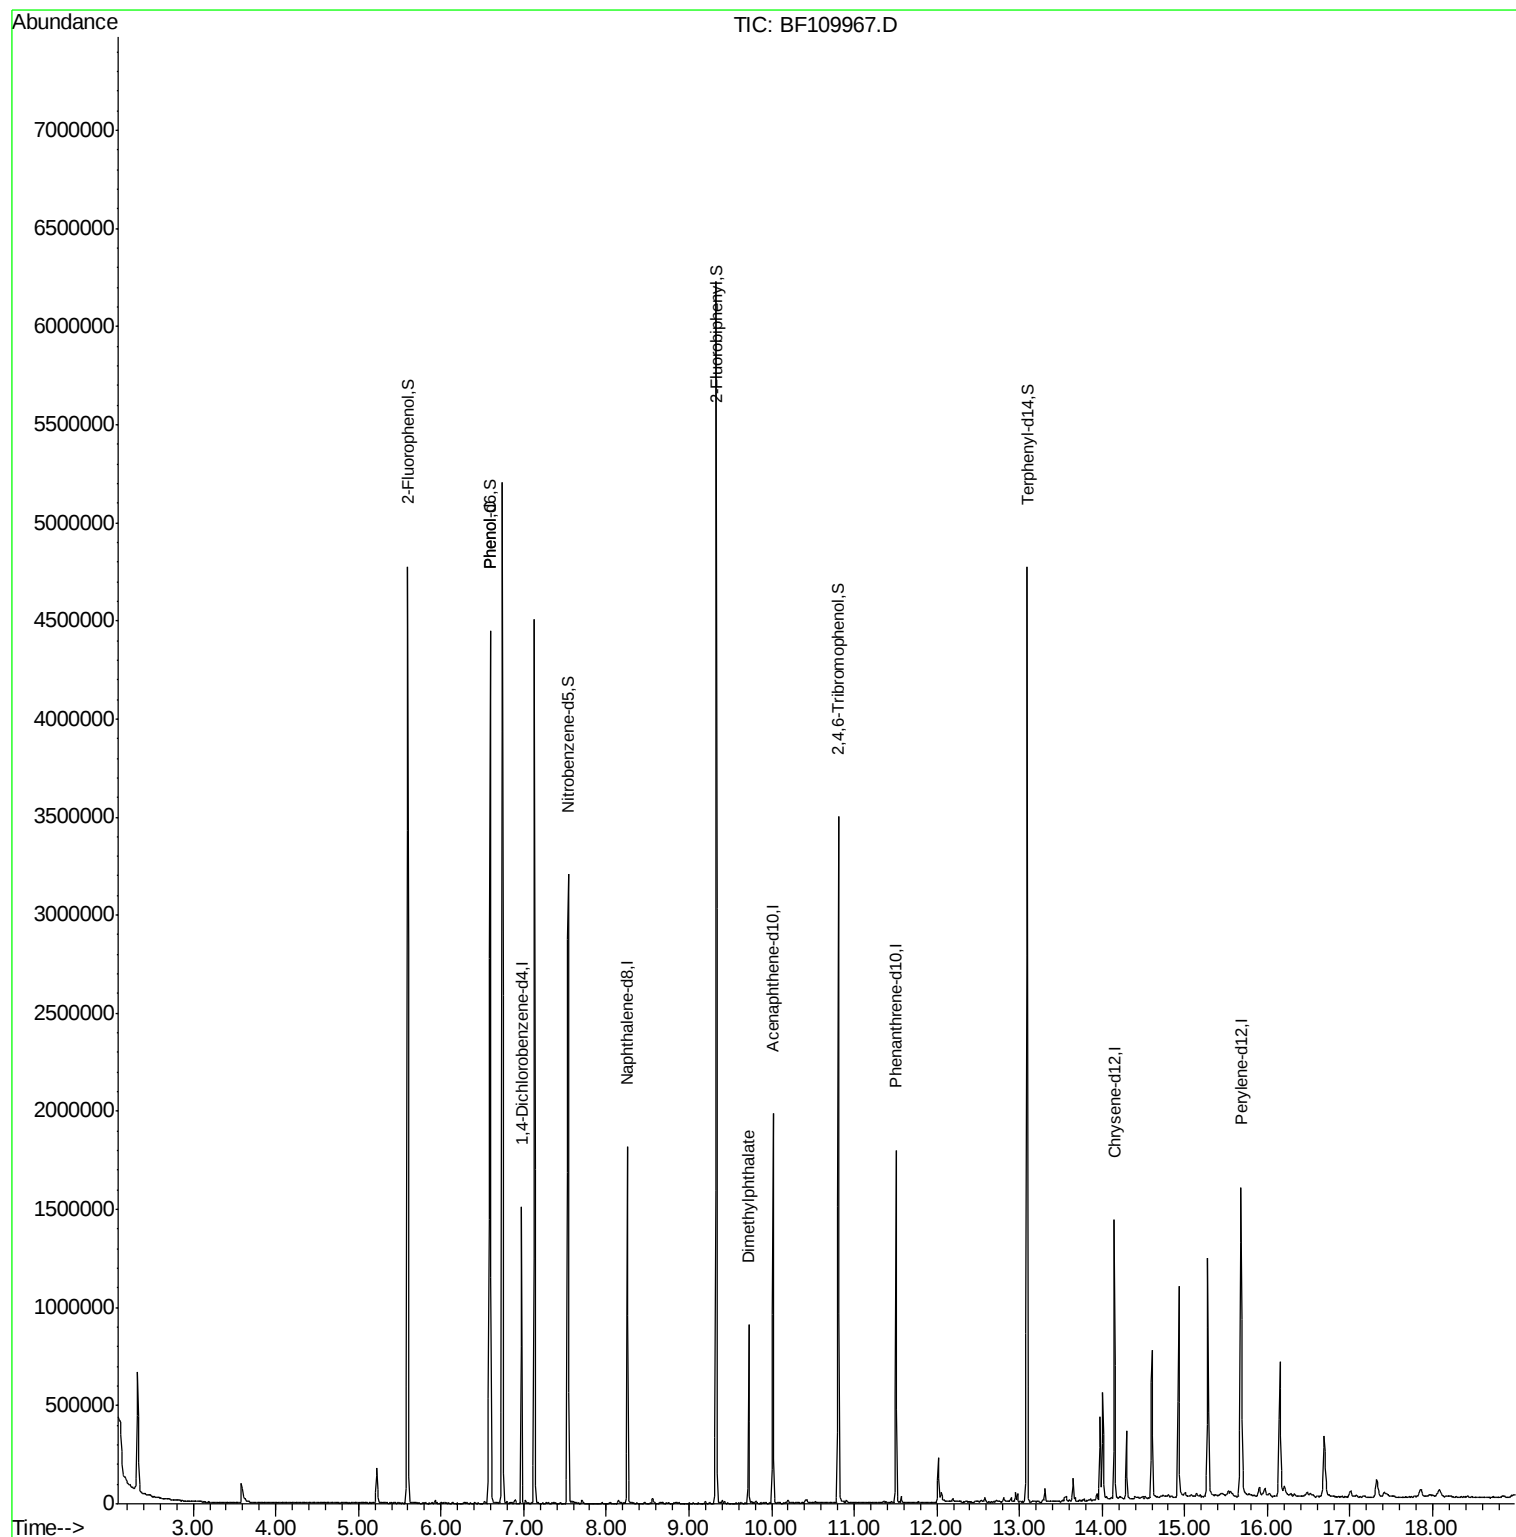

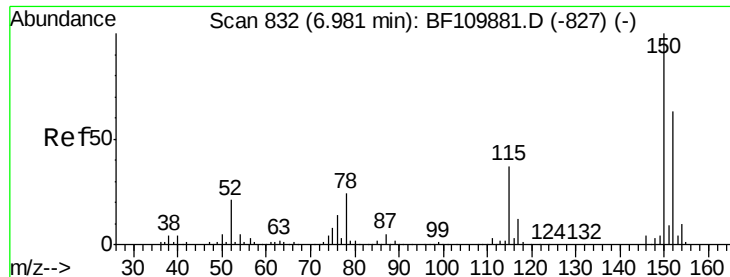


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 831
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :
RLF-SD-3

Tot Ion:152 Resp: 195100
Ion Ratio Lower Upper
152 100
150 155.4 122.7 184.1
115 60.6 49.1 73.7

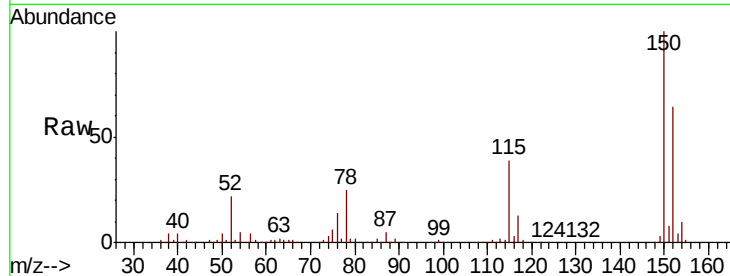


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

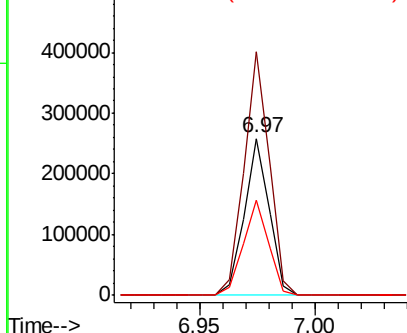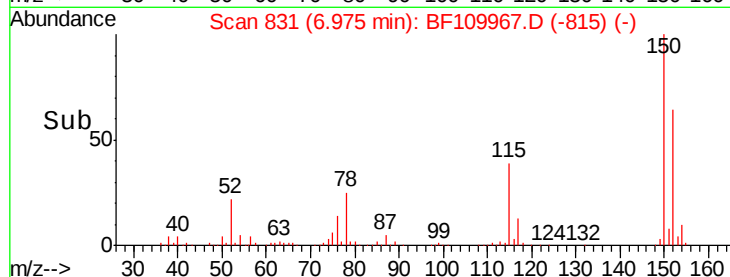



#5


2-Fluorophenol
Concen: 113.022 ng
RT: 5.60 min Scan# 597
Delta R.T. -0.00 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:112 Resp: 1391085
Ion Ratio Lower Upper
112 100
64 61.8 44.1 66.1
63 32.7 23.7 35.5

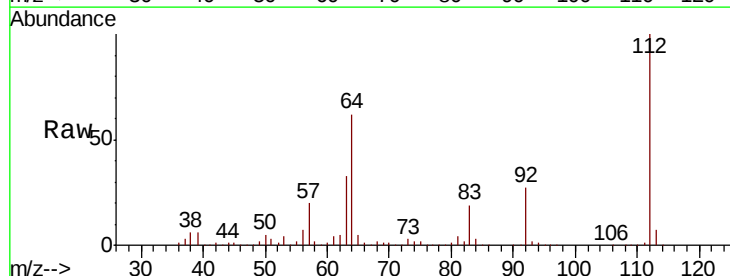

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

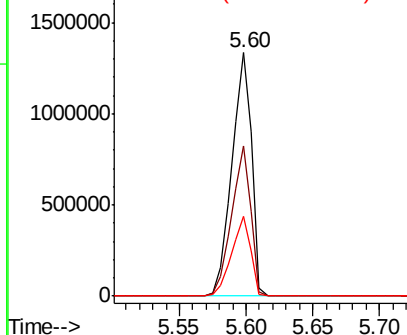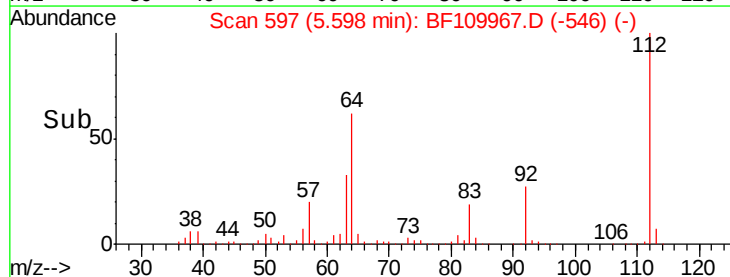

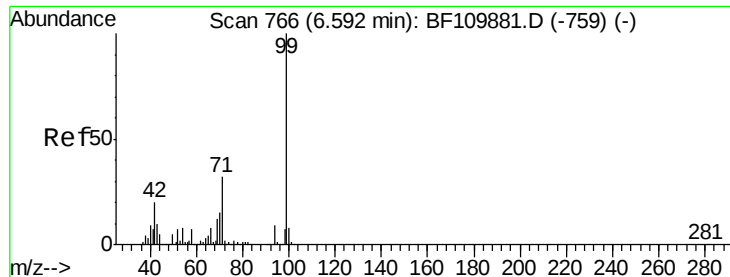

#7

Phenol-d6

Concen: 114.934 ng

RT: 6.60 min Scan# 767

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Instrument :

BNA_F

ClientSampleId :

RLF-SD-3


Tot Ion: 99 Resp: 1756584

Ion Ratio Lower Upper




99 100

42 18.6 15.8 23.6

71 34.2 28.0 42.0

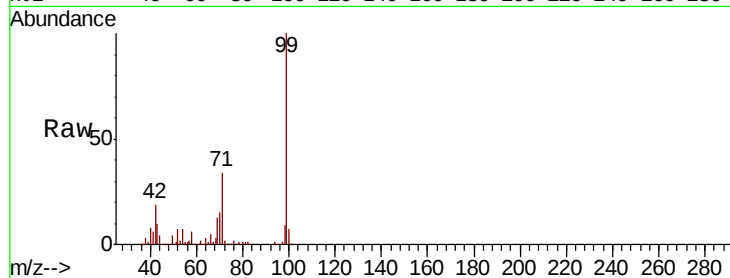

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

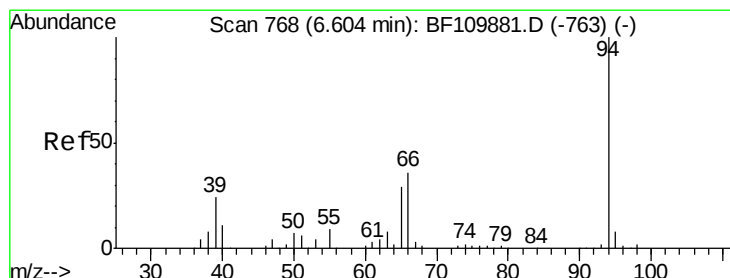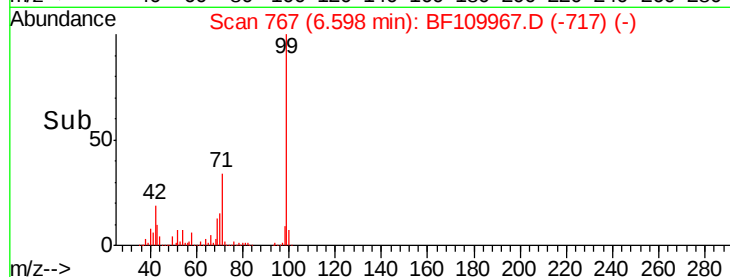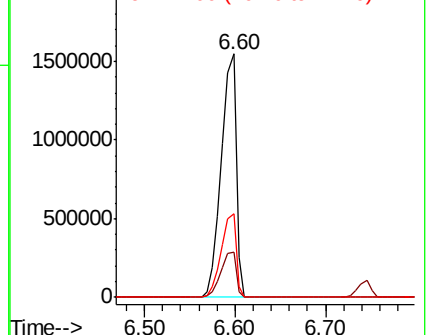

#10

Phenol

Concen: 6.021 ng

RT: 6.60 min Scan# 768

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10


Tgt Ion: 94 Resp: 99351

Ion Ratio Lower Upper



94 100


65 30.2 25.3 65.3

66 43.4 54.5 94.5#

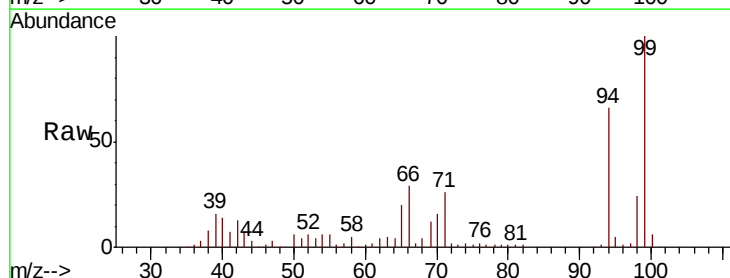

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

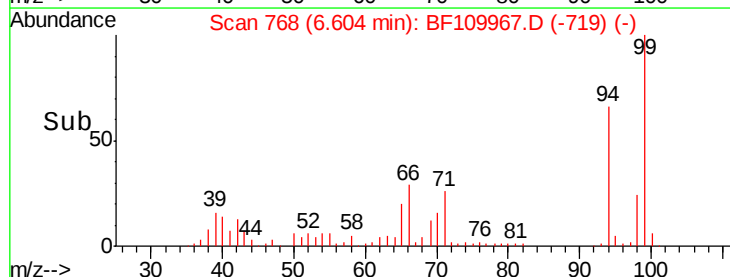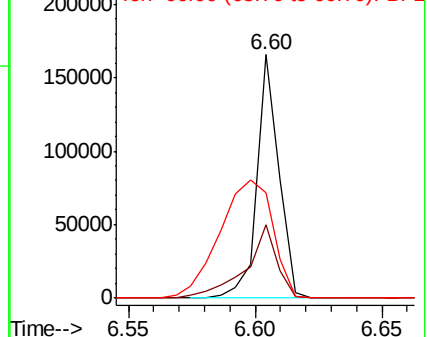


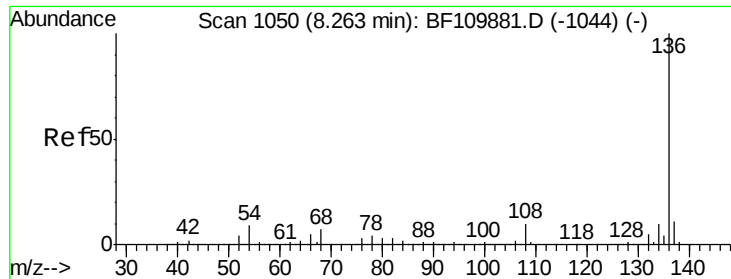




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.26 min Scan# 1049
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :
RLF-SD-3

Tot Ion:136	Resp:	756480
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.8 13.2
54	8.2	5.4 8.2#
68	5.8	4.2 6.2

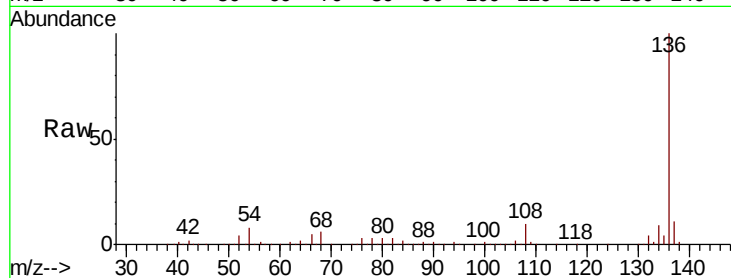


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

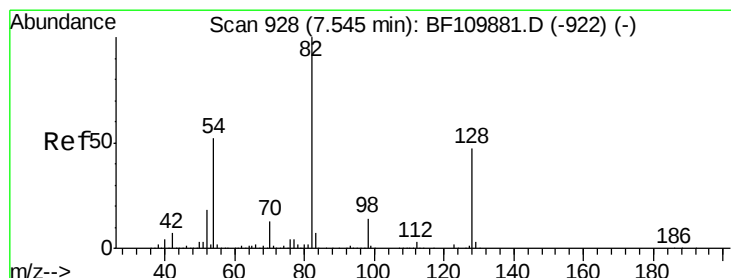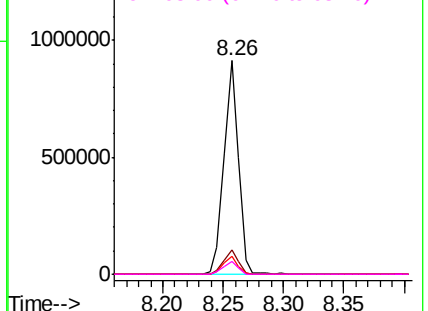
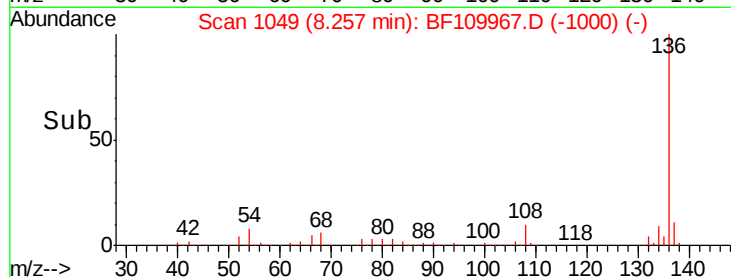



#23
Nitrobenzene-d5
Concen: 97.850 ng
RT: 7.54 min Scan# 927
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion: 82	Resp:	1098836
Ion Ratio	Lower	Upper
82	100	
128	49.0	34.2 51.2
54	52.0	38.6 58.0

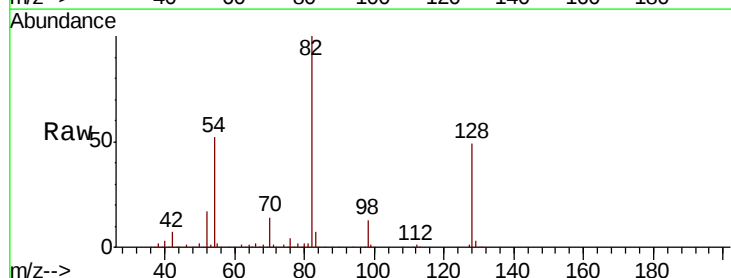

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



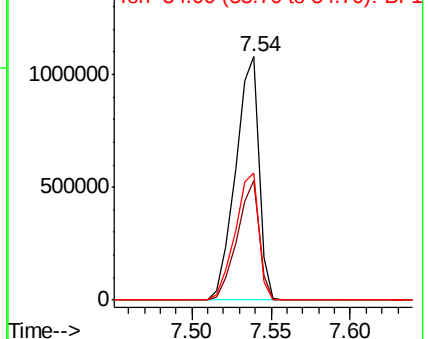
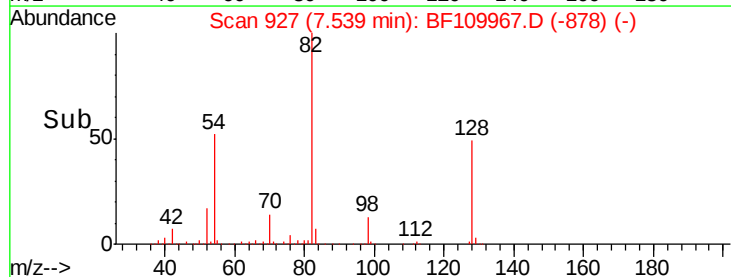


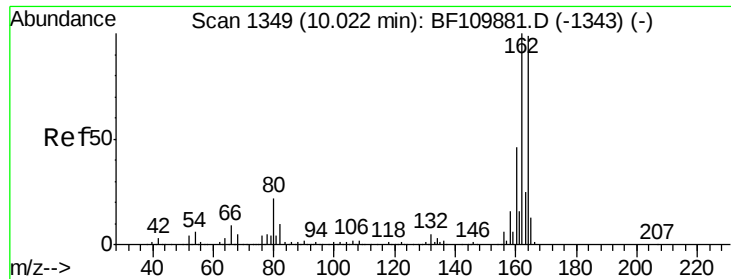

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.02 min Scan# 1348
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10




Instrument :
BNA_F
ClientSampleId :
RLF-SD-3


Tot Ion:164 Resp: 353320
Ion Ratio Lower Upper
164 100
162 104.3 83.0 124.6
160 47.1 37.0 55.6

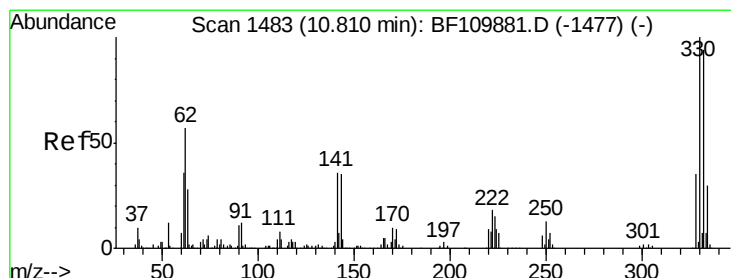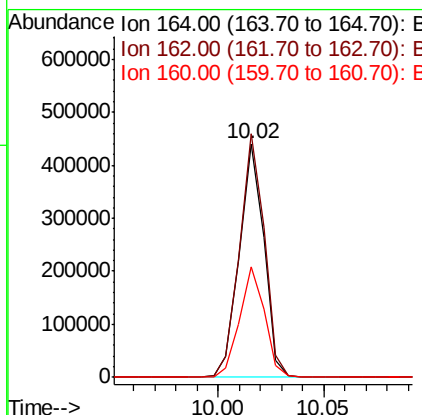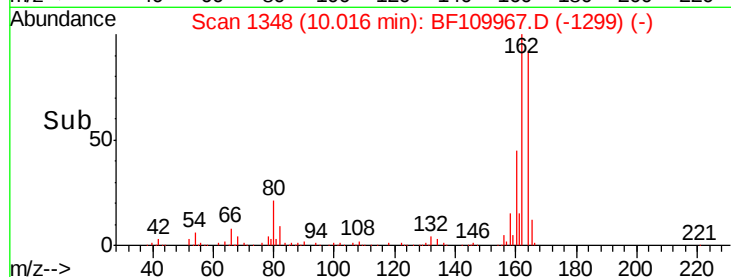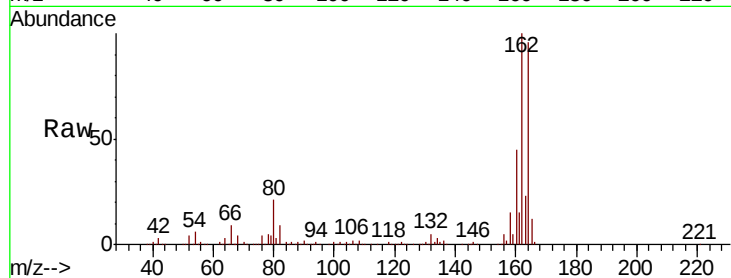

#42
2,4,6-Tribromophenol
Concen: 137.458 ng
RT: 10.81 min Scan# 1483
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:330 Resp: 420476
Ion Ratio Lower Upper
330 100
332 96.1 77.1 115.7
141 36.5 27.0 40.4

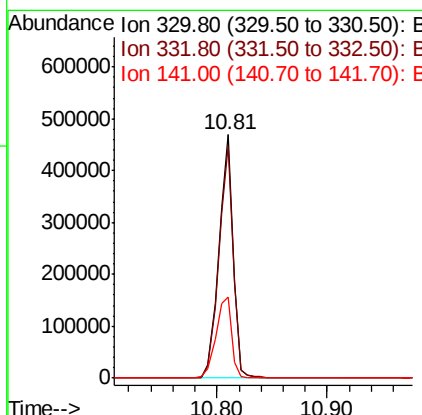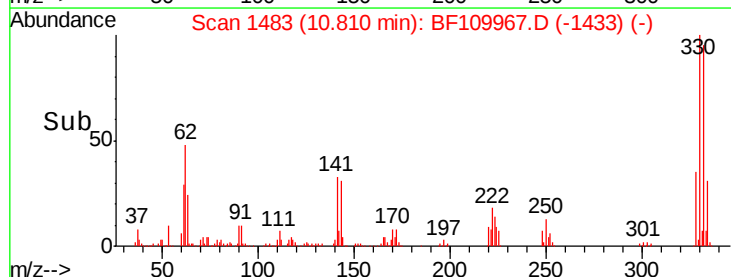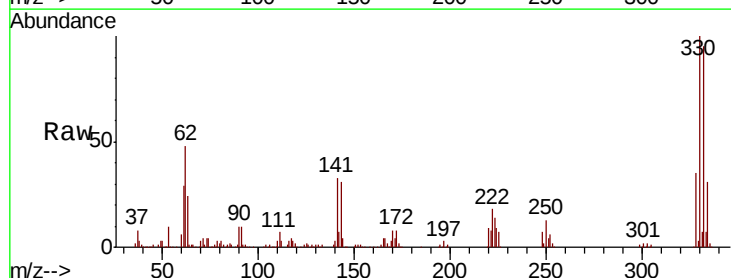


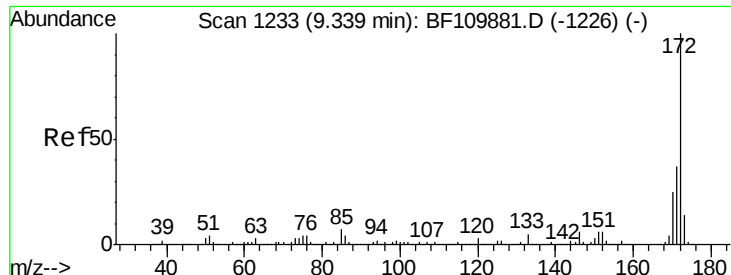




#45
2-Fluorobiphenyl
Concen: 84.403 ng
RT: 9.33 min Scan# 1232
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :
RLF-SD-3

Tot Ion:172 Resp: 1868897
Ion Ratio Lower Upper
172 100
171 37.3 28.6 43.0
170 24.6 19.7 29.5

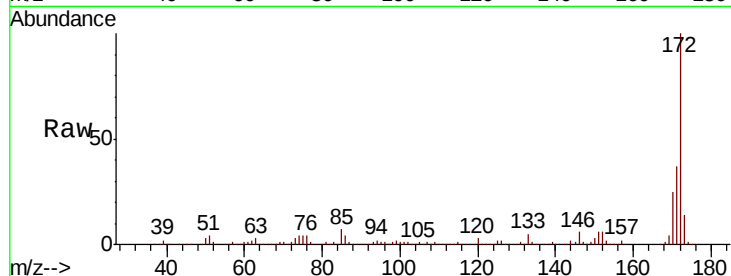


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

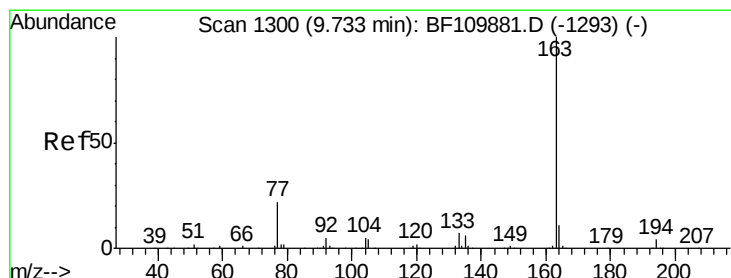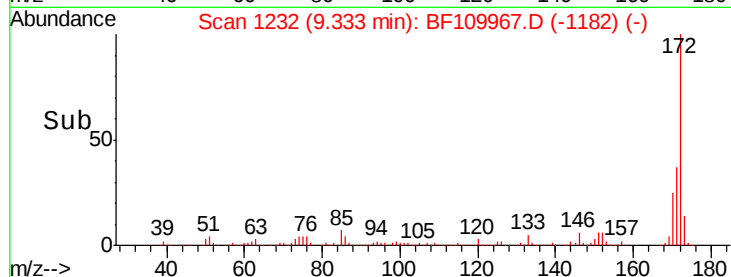
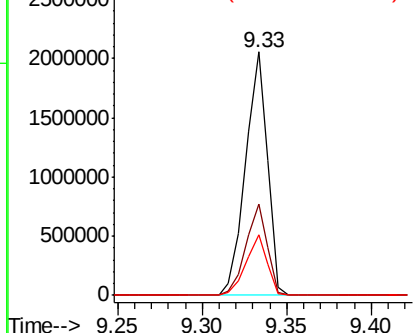



#50
Dimethylphthalate
Concen: 12.481 ng
RT: 9.72 min Scan# 1298
Delta R.T. -0.02 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:163 Resp: 312263
Ion Ratio Lower Upper
163 100
194 3.4 3.2 4.8
164 10.2 8.1 12.1

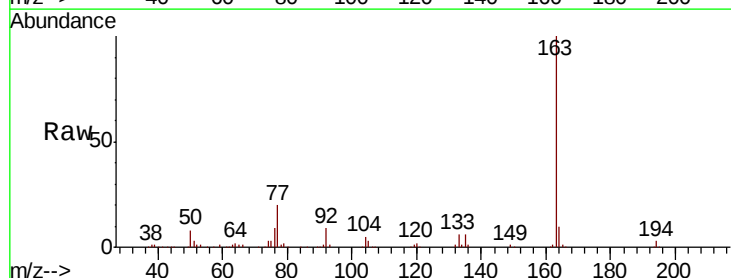

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

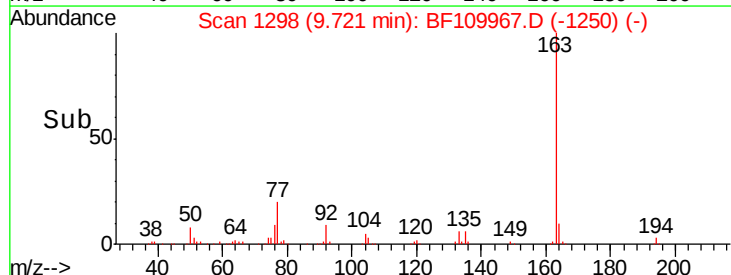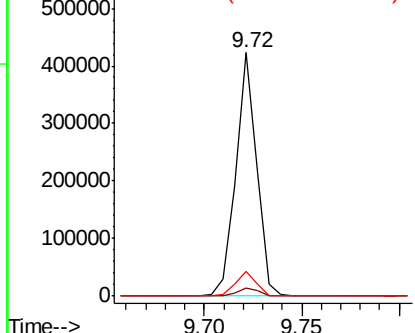


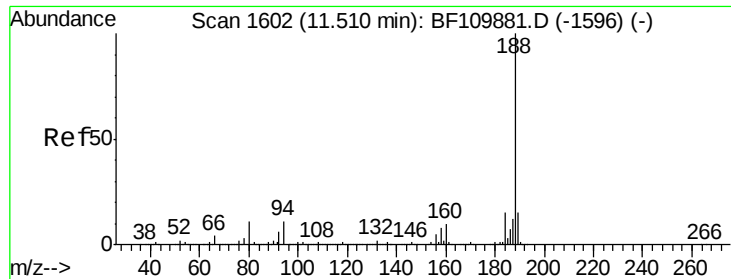




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.51 min Scan# 1602
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Instrument :
BNA_F
ClientSampleId :
RLF-SD-3

Tot Ion:188 Resp: 646126
Ion Ratio Lower Upper
188 100
94 9.5 7.2 10.8
80 10.0 7.9 11.9

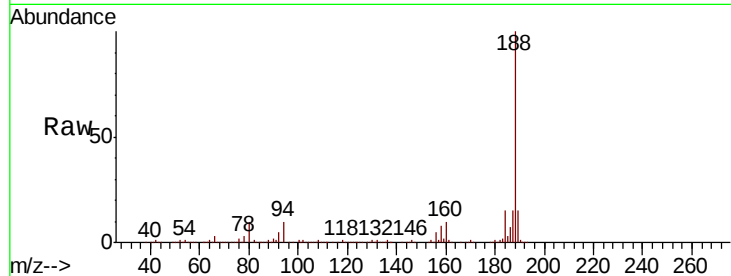


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

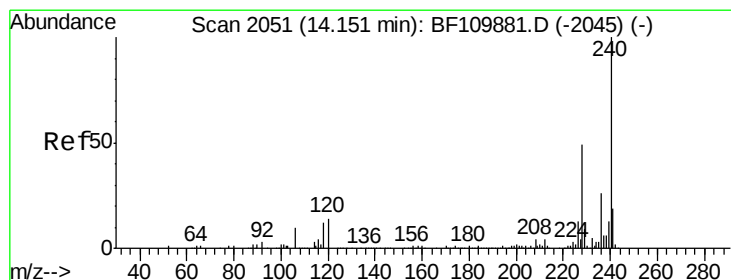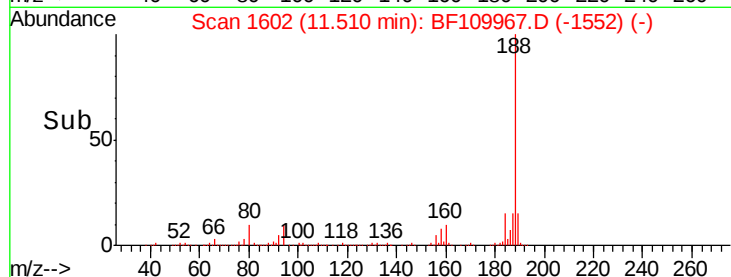
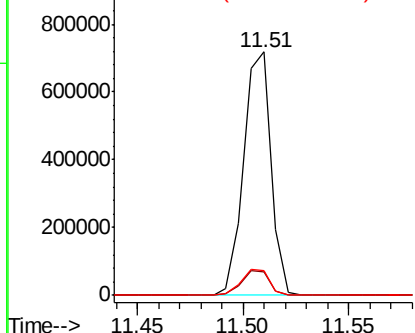



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2051
Delta R.T. -0.01 min
Lab File: BF109967.D
Acq: 18 Oct 2018 19:10

Tgt Ion:240 Resp: 436945
Ion Ratio Lower Upper
240 100
120 12.2 8.3 12.5
236 25.8 21.2 31.8

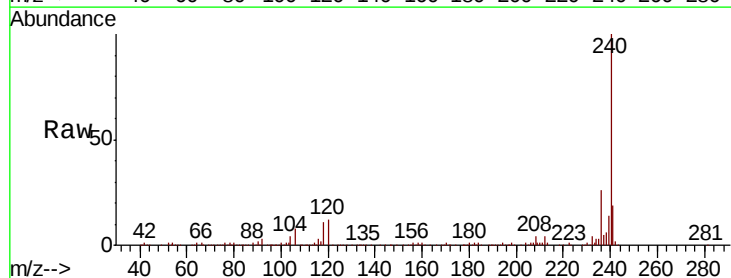

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

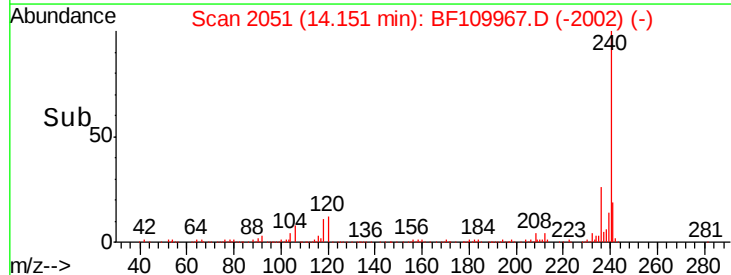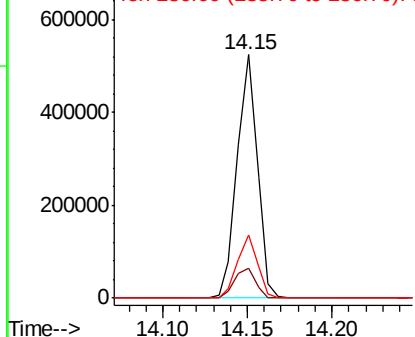

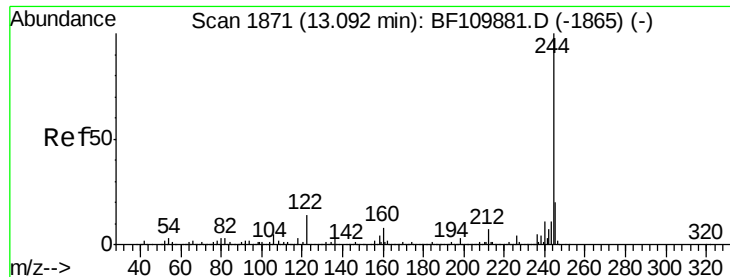

#79

Terphenyl-d14

Concen: 81.680 ng

RT: 13.09 min Scan# 1871

Delta R.T. -0.01 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10

Instrument :

BNA_F

ClientSampleId :

RLF-SD-3


Tot Ion:244 Resp: 1699564

Ion Ratio Lower Upper




244 100

212 7.3 5.8 8.8

122 13.6 8.7 13.1#

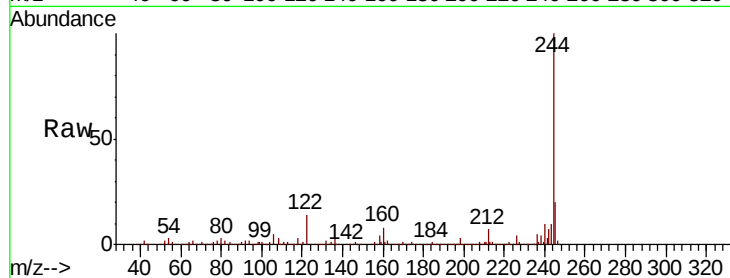

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

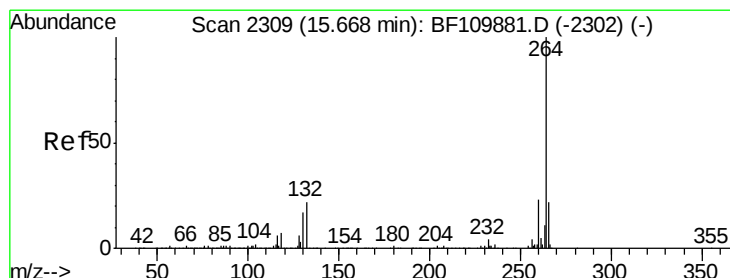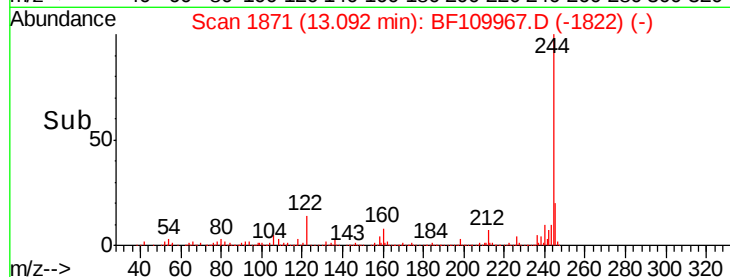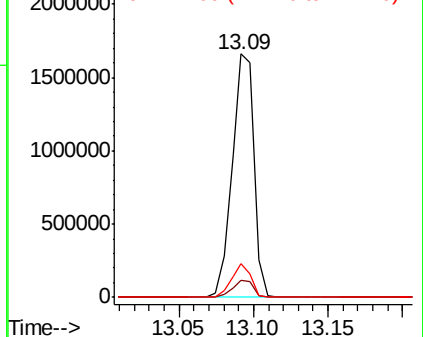

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2310

Delta R.T. -0.02 min

Lab File: BF109967.D

Acq: 18 Oct 2018 19:10


Tgt Ion:264 Resp: 369905

Ion Ratio Lower Upper

264 100

260 22.2 18.7 28.1

265 21.3 16.7 25.1

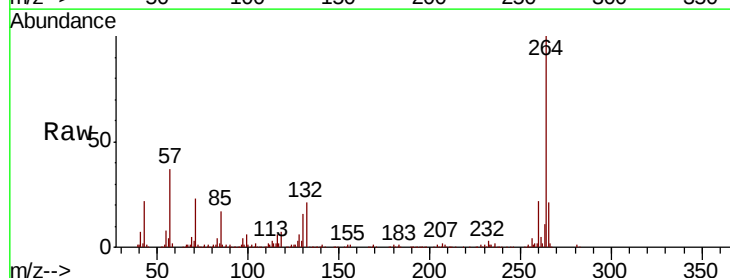

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

