

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101818\
 Data File : BF109966.D
 Acq On : 18 Oct 2018 18:43
 Operator : JU/SJ
 Sample : J5565-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RLF-SD-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.334	37	42	53	rVB	756966	1055769	20.10%	1.618%
2	3.593	253	256	265	rBV	83797	138252	2.63%	0.212%
3	5.222	529	533	544	rVB	174453	223660	4.26%	0.343%
4	5.598	592	597	600	rBV	4662272	4925099	93.78%	7.546%
5	6.598	760	767	771	rBV	4545362	5251536	100.00%	8.046%
6	6.745	787	792	795	rBV	5136721	5105271	97.21%	7.822%
7	6.975	827	831	834	rBV	1526819	1189003	22.64%	1.822%
8	7.134	853	858	861	rBV	4580048	3902164	74.31%	5.979%
9	7.539	921	927	930	rBV	3316706	3253949	61.96%	4.986%
10	8.257	1045	1049	1052	rBV	1864989	1498407	28.53%	2.296%
11	9.333	1227	1232	1235	rBV	5814484	5232237	99.63%	8.017%
12	9.722	1294	1298	1301	rBV	1095343	825739	15.72%	1.265%
13	10.016	1344	1348	1352	rBV2	1961746	1679716	31.99%	2.574%
14	10.198	1375	1379	1387	rBV2	41379	59144	1.13%	0.091%
15	10.810	1478	1483	1486	rBV	3429440	3326686	63.35%	5.097%
16	11.510	1598	1602	1605	rBV	1801180	1659504	31.60%	2.543%
17	12.016	1683	1688	1693	rBV	470965	526322	10.02%	0.806%
18	12.804	1818	1822	1831	rBV	90106	116557	2.22%	0.179%
19	13.092	1867	1871	1875	rBV	4512253	4222727	80.41%	6.470%
20	13.310	1896	1908	1911	rBV	85800	149572	2.85%	0.229%
21	13.651	1960	1966	1969	rBV2	143293	177721	3.38%	0.272%
22	13.933	2009	2014	2017	rBV	344185	463394	8.82%	0.710%
23	13.974	2017	2021	2024	rVV	940253	1192487	22.71%	1.827%
24	14.010	2024	2027	2031	rVV	2225809	2592496	49.37%	3.972%
25	14.057	2032	2035	2040	rVB	95553	104219	1.98%	0.160%
26	14.151	2047	2051	2055	rBV	1425372	1243207	23.67%	1.905%
27	14.292	2071	2075	2084	rVB	784571	840704	16.01%	1.288%
28	14.604	2122	2128	2138	rBV	1479272	1615282	30.76%	2.475%
29	14.927	2176	2183	2191	rBV	1854710	2378371	45.29%	3.644%
30	15.280	2236	2243	2256	rBV	1953682	2790190	53.13%	4.275%
31	15.527	2280	2285	2289	rBV	45811	73804	1.41%	0.113%
32	15.680	2304	2311	2324	rVB2	2129261	3570558	67.99%	5.471%
33	15.968	2355	2360	2365	rVB	49429	80865	1.54%	0.124%
34	16.151	2383	2391	2397	rBV	1069609	1931655	36.78%	2.960%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101818\
Data File : BF109966.D
Acq On : 18 Oct 2018 18:43
Operator : JU/SJ
Sample : J5565-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RLF-SD-1

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	16.204	2397	2400	2412	rVB8	50268	96957	1.85%	0.149%
36	16.692	2475	2483	2498	rVB	503525	1033511	19.68%	1.583%
37	17.321	2583	2590	2598	rVB	151683	343457	6.54%	0.526%
38	17.851	2675	2680	2690	rVB9	57249	133191	2.54%	0.204%
39	18.080	2711	2719	2727	rVB3	53353	146457	2.79%	0.224%
40	18.480	2780	2787	2795	rVB10	46597	118354	2.25%	0.181%


Sum of corrected areas: 65268194

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF101818\
Data File : BF109966.D
Acq On : 18 Oct 2018 18:43
Operator : JU/SJ
Sample : J5565-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RLF-SD-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

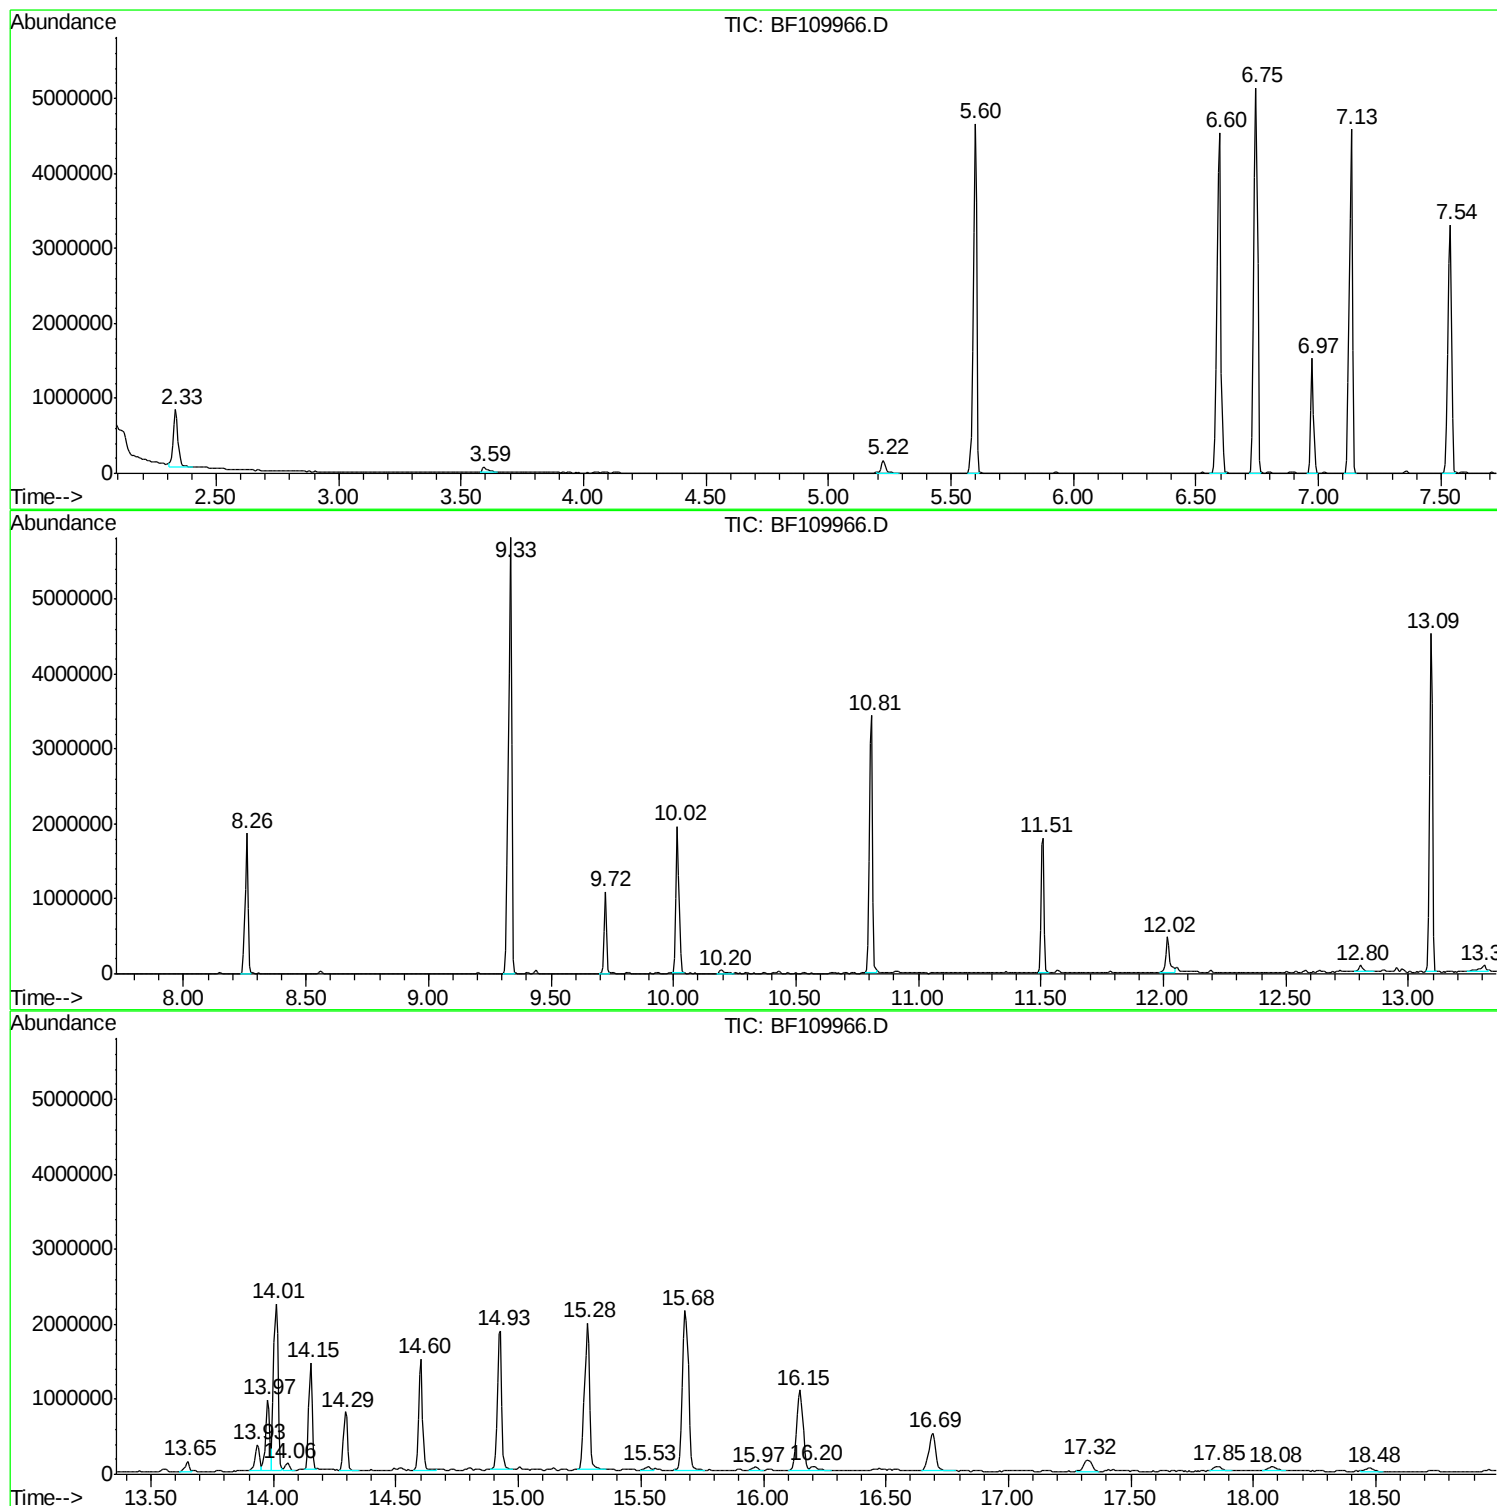

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101818\
Data_File : BF109966.D
Acq_On : 18_Oct_2018_ 18:433
Operator : JU/SJJ
Sample : J5565-011
Misc :
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
RLF-SD-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
