


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101818\
 Data File : BF109964.D
 Acq On : 18 Oct 2018 17:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

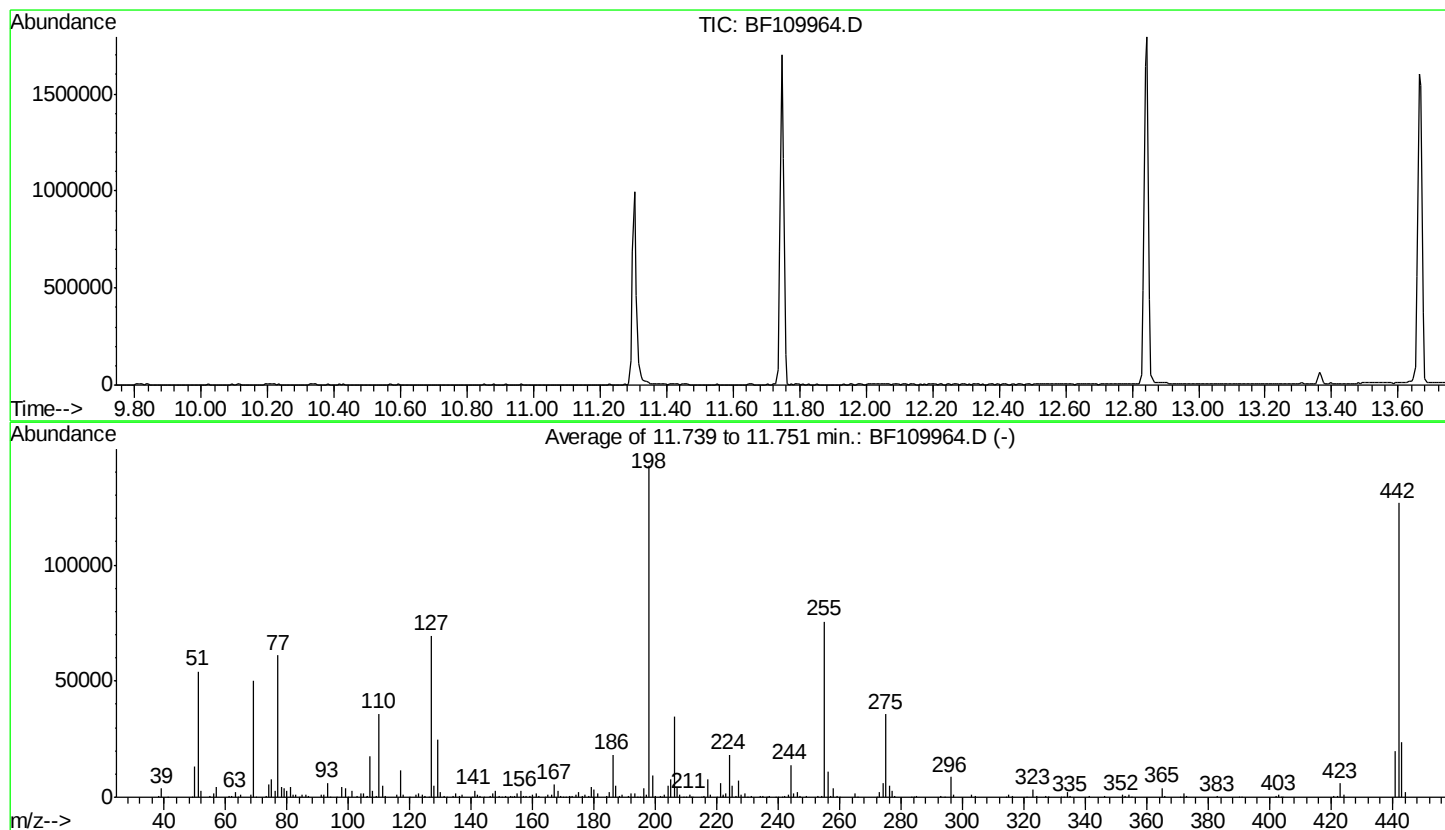

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	54106	PASS
68	69	0.00	2	1.8	897	PASS
69	198	0.00	100	35.2	50226	PASS
70	69	0.00	2	0.3	171	PASS
127	198	10	80	48.7	69520	PASS
197	198	0.00	2	0.8	1206	PASS
198	198	100	100	100.0	142789	PASS
199	198	5	9	6.6	9390	PASS
275	198	10	60	25.0	35640	PASS
365	198	1	100	2.8	3954	PASS
441	198	0.01	100	14.0	20032	PASS
442	198	50	100	88.7	126629	PASS
443	442	15	24	18.6	23591	PASS