


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF101818\
 Data File : BF109991.D
 Acq On : 19 Oct 2018 6:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 16 14:58:24 2018

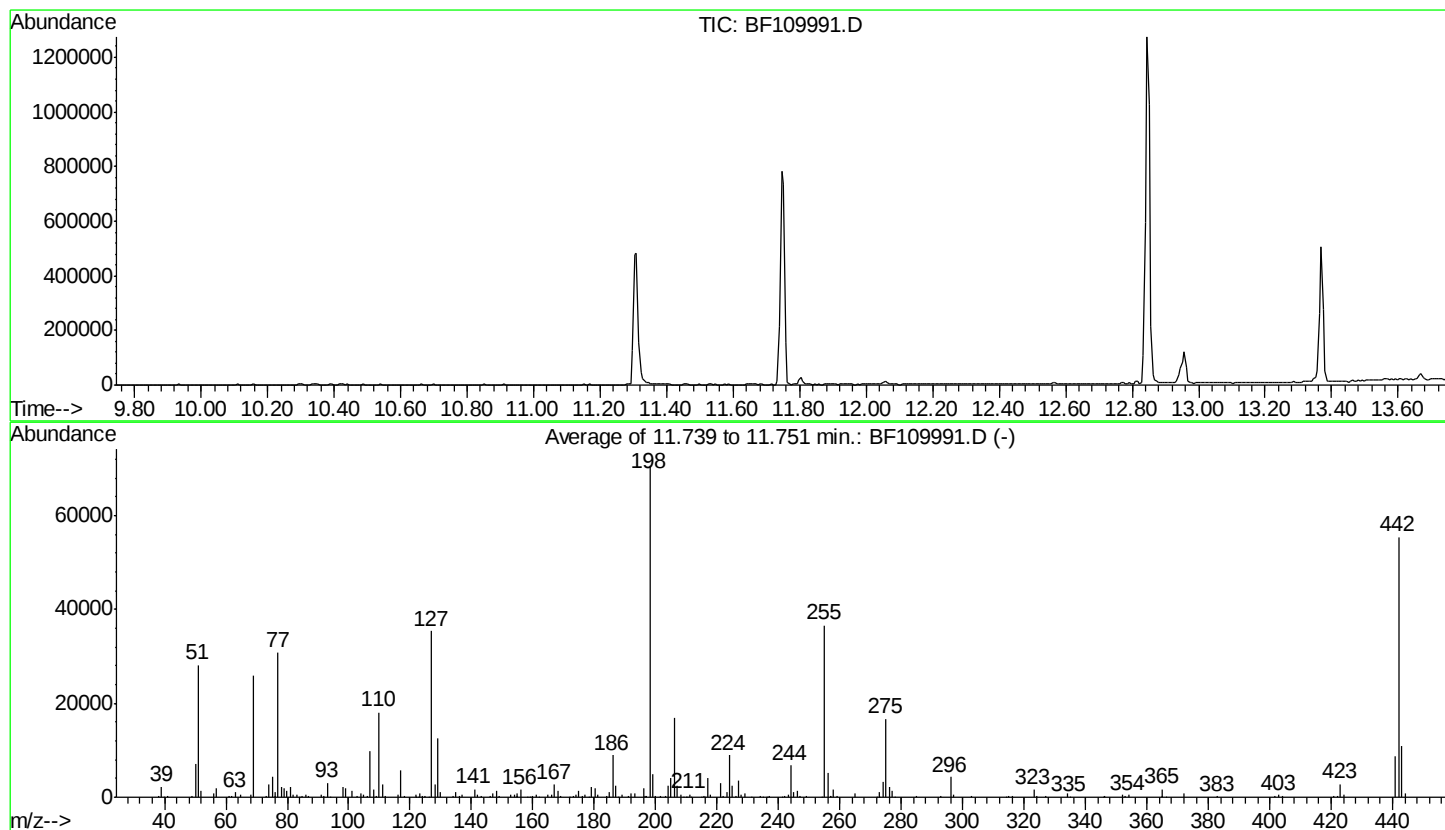

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	28171	PASS
68	69	0.00	2	1.7	449	PASS
69	198	0.00	100	36.7	25914	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	35306	PASS
197	198	0.00	2	0.6	415	PASS
198	198	100	100	100.0	70597	PASS
199	198	5	9	7.0	4936	PASS
275	198	10	60	23.7	16727	PASS
365	198	1	100	2.4	1680	PASS
441	198	0.01	100	12.2	8643	PASS
442	198	50	100	78.4	55338	PASS
443	442	15	24	19.7	10925	PASS