
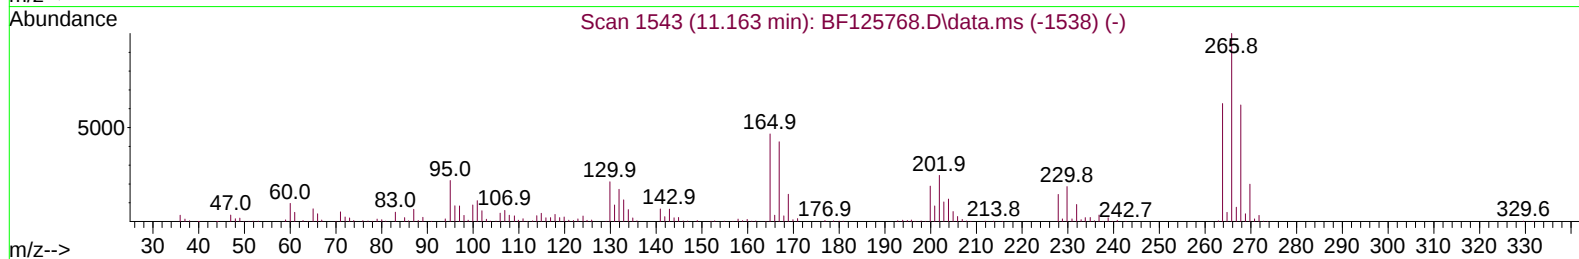
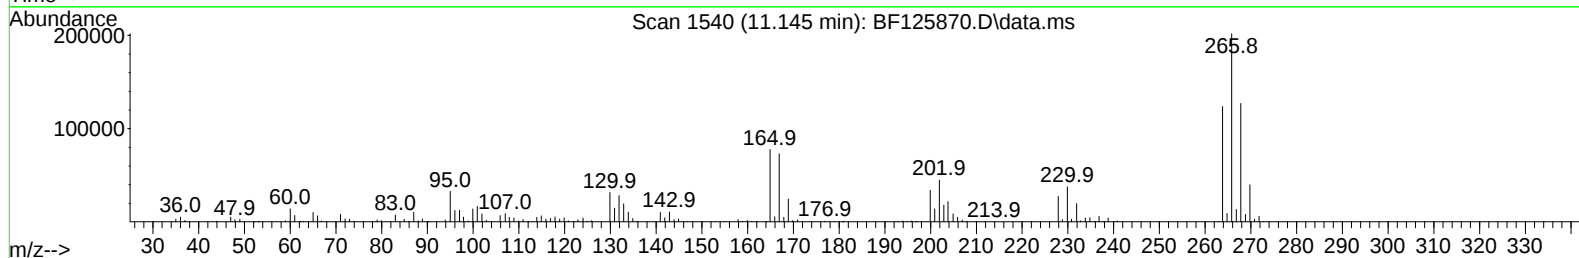


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125870.D
Acq On : 18 Oct 2021 11:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 12:36:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 15:00:46 2021
Response via : Initial Calibration

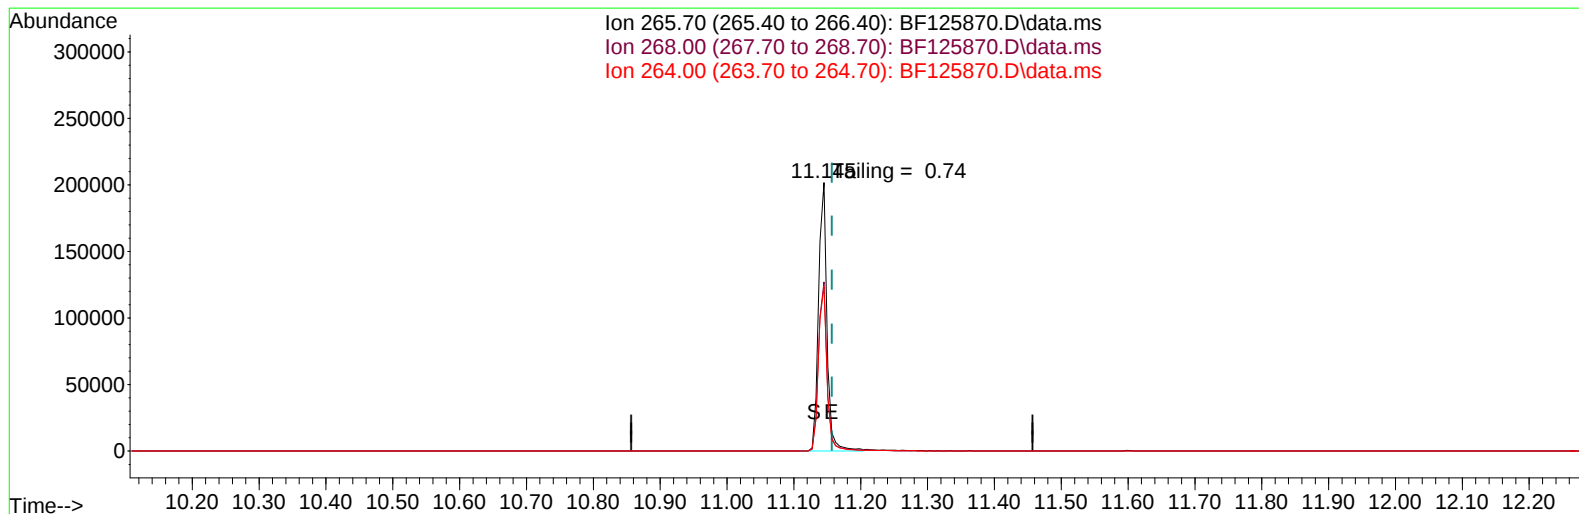

TIC: BF125870.D\data.ms

(70) Pentachlorophenol (C)




11.145min (-0.012) 39466.11 ng

response 179256

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.96
264.00	69.90	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125870.D
Acq On : 18 Oct 2021 11:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 18 12:36:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 15 15:00:46 2021
Response via : Initial Calibration

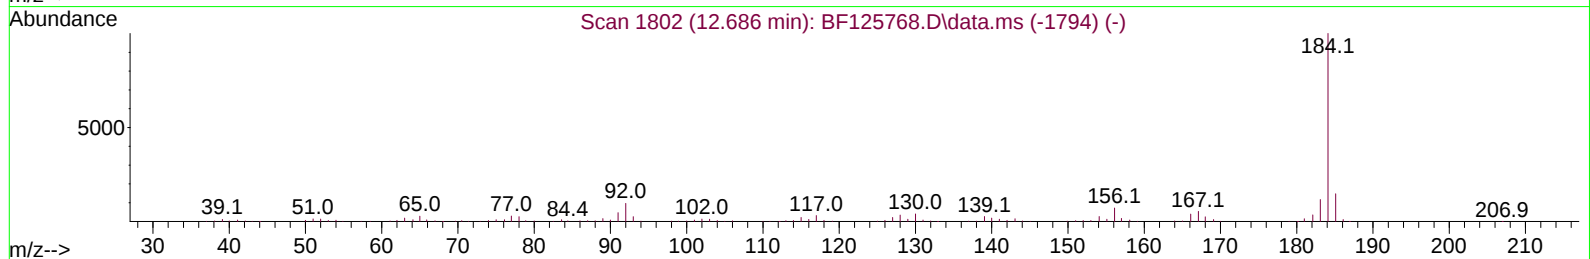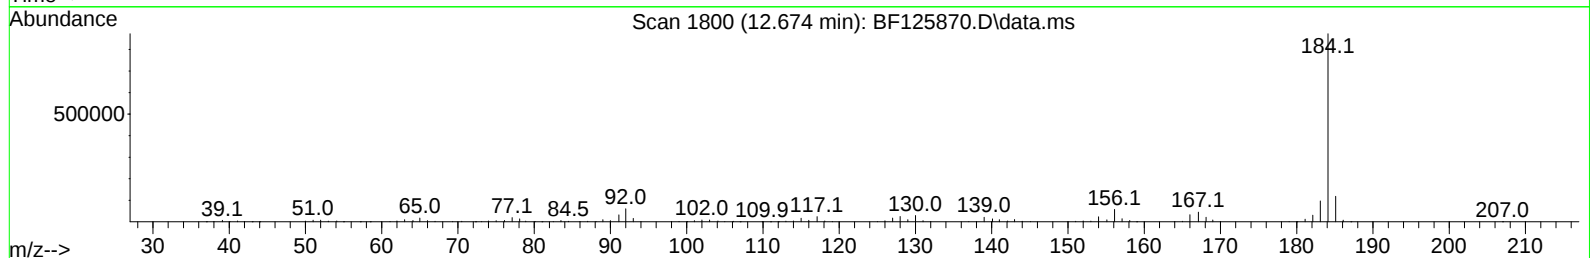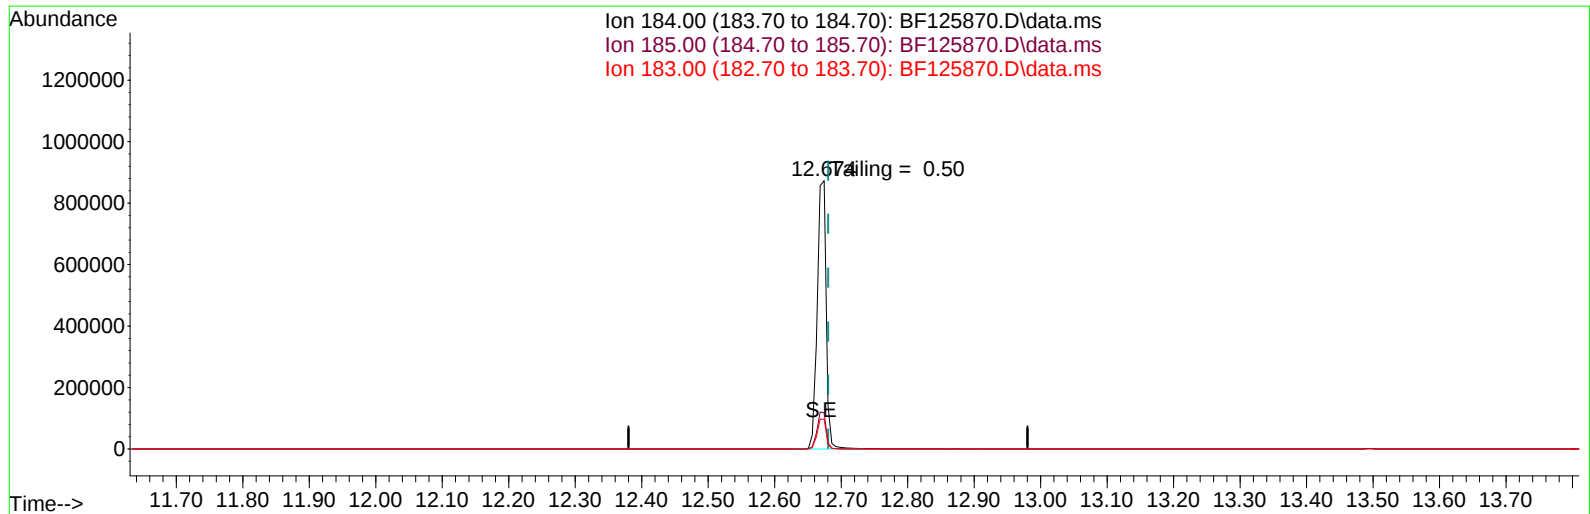

TIC: BF125870.D\data.ms

(77) Benzidine

12.674min (-0.006) 0.00 ng

response 817813

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.57
183.00	10.10	11.13
0.00	0.00	0.00