

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
 Data File : BF125875.D
 Acq On : 18 Oct 2021 14:06
 Operator : JU/CG
 Sample : M4260-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEST-DA-(1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	565	570	573	rBV	2802737	2681687	82.74%	12.844%
2	6.451	736	742	745	rBV	2667346	2685498	82.86%	12.862%
3	6.822	802	805	808	rBV	1149956	864730	26.68%	4.142%
4	7.381	895	900	903	rBV	2020287	1726527	53.27%	8.269%
5	8.004	1003	1006	1016	rBV	197312	168424	5.20%	0.807%
6	8.104	1019	1023	1026	rBV	1507743	1189854	36.71%	5.699%
7	9.175	1201	1205	1209	rBV	3638250	3241192	100.00%	15.524%
8	9.857	1317	1321	1324	rBV	1520791	1288827	39.76%	6.173%
9	10.639	1450	1454	1457	rBV	2107909	1744909	53.84%	8.357%
10	11.339	1569	1573	1576	rBV	1192485	1092794	33.72%	5.234%
11	11.863	1656	1662	1667	rBV2	93054	101200	3.12%	0.485%
12	12.921	1838	1842	1845	rBV	2417190	2121736	65.46%	10.162%
13	13.821	1990	1995	2005	rBV4	55356	108702	3.35%	0.521%
14	13.968	2016	2020	2024	rBV	1067687	927534	28.62%	4.442%
15	15.421	2262	2267	2271	rBV	766190	935121	28.85%	4.479%




Sum of corrected areas: 20878735

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125875.D
Acq On : 18 Oct 2021 14:06
Operator : JU/CG
Sample : M4260-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-DA-(1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

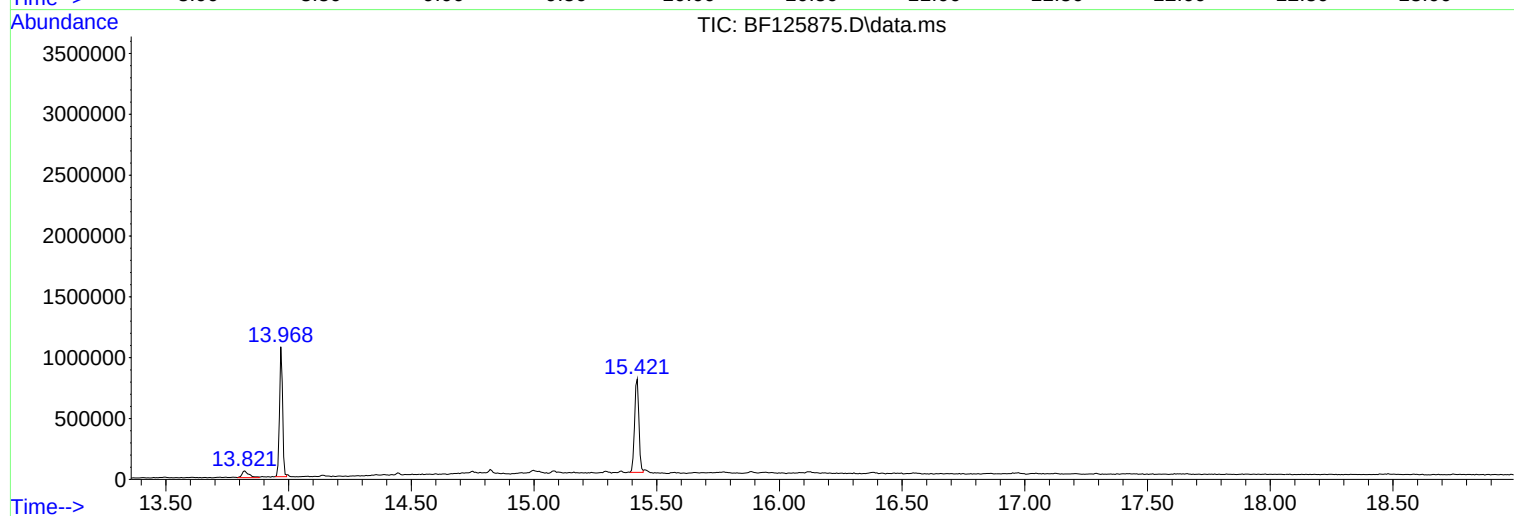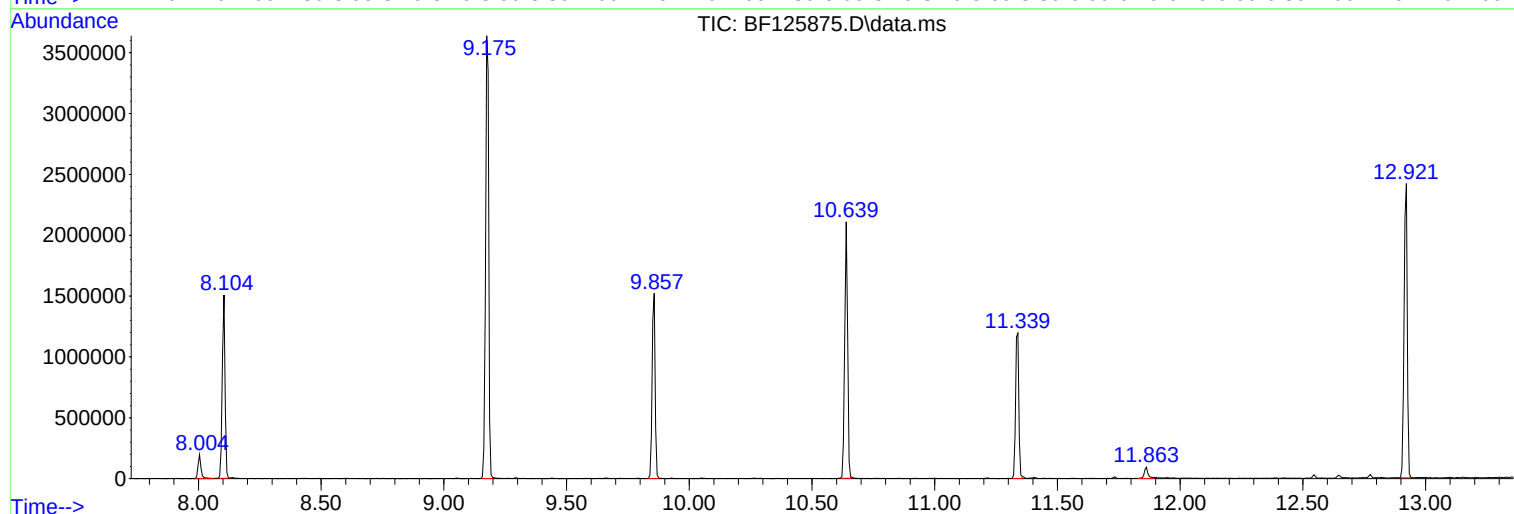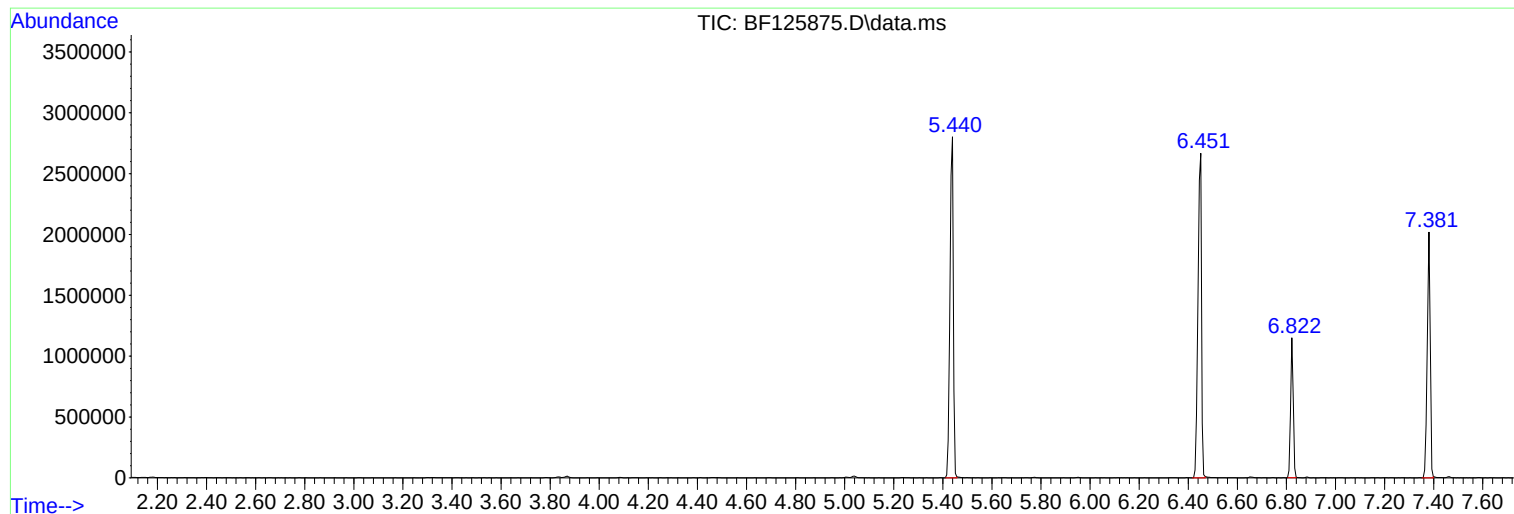

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125875.D
Acq On : 18 Oct 2021 14:06
Operator : JU/CG
Sample : M4260-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-DA-(1)









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.004	2.83 ng	168424	Naphthalene-d8	8.104

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethylene glycol monoisobutyl ether	118	C6H14O2	004439-24-1	64
3			Ethanol, 2-[2-(2-methylpropoxy)ethoxy]-	162	C8H18O3	018912-80-6	56
4			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	50
5			Methoxyacetic acid, 2-butyl ester	146	C7H14O3	070159-90-9	50

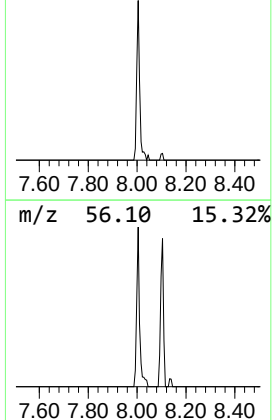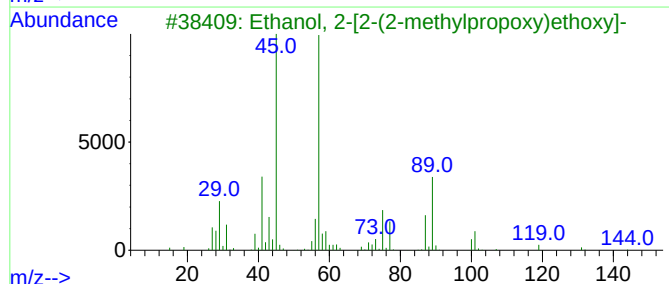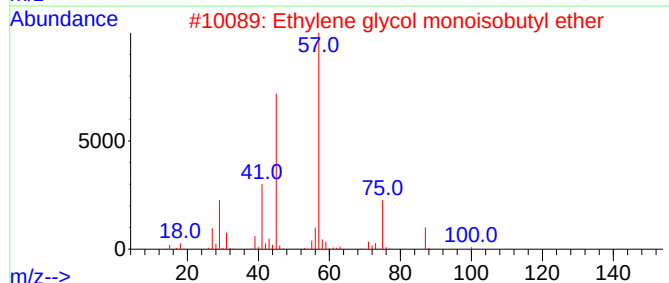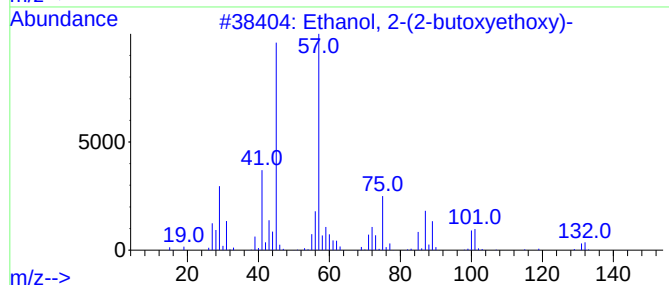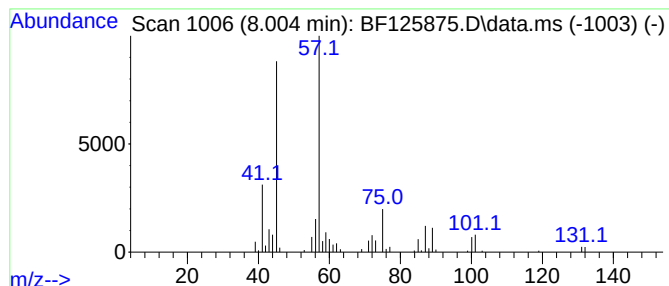

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125875.D
Acq On : 18 Oct 2021 14:06
Operator : JU/CG
Sample : M4260-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-DA-(1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Heneicosyl heptafluorobutyrate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.821	2.34 ng	108702	Chrysene-d12	13.968

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heneicosyl heptafluorobutyrate	508	C25H43F7O2	1000351-83-8	90
2			17-Pentatriacontene	491	C35H70	006971-40-0	90
3			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	83
4			Hexacosyl propyl ether	424	C29H60O	1000406-28-4	83
5			Octacosyl trifluoroacetate	506	C30H57F3O2	1000351-74-9	76

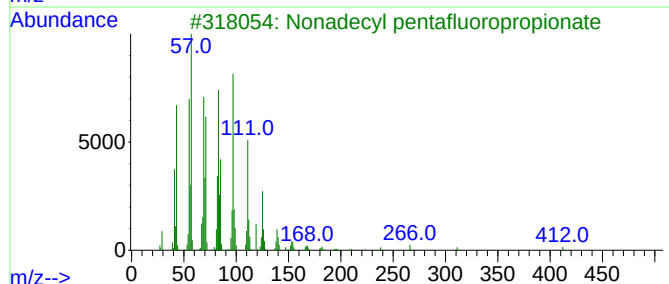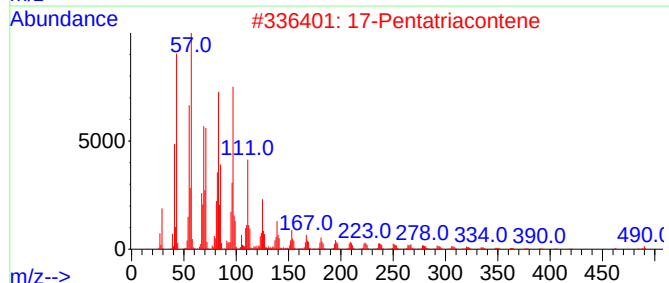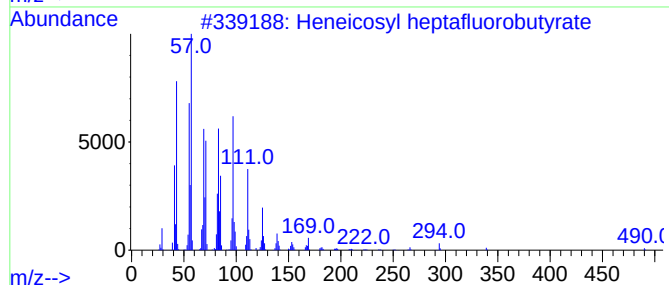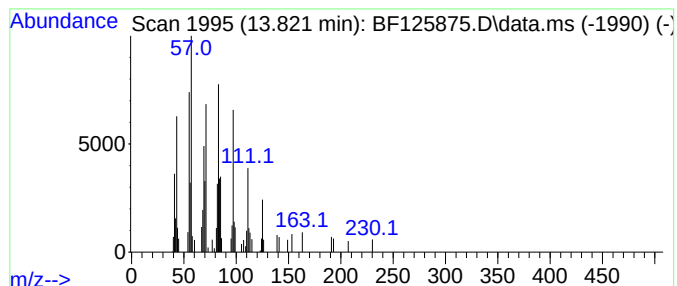

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125875.D
Acq On : 18 Oct 2021 14:06
Operator : JU/CG
Sample : M4260-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEST-DA-(1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	8.004	2.8	ng	168424	2	8.104	1189850	20.0
Heneicosyl hept...	13.821	2.3	ng	108702	5	13.968	927534	20.0