

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
 Data File : BF125881.D
 Acq On : 18 Oct 2021 17:16
 Operator : JU/CG
 Sample : M4243-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T3-COMP-(1-4)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.734	105	110	117	rVB	240906	331118	7.57%	1.293%
2	4.616	425	430	435	rBV	415850	418172	9.55%	1.633%
3	5.040	499	502	504	rBV	115161	135416	3.09%	0.529%
4	5.063	504	506	510	rVB	274926	245771	5.62%	0.960%
5	5.446	566	571	574	rBV	3473358	3252362	74.31%	12.701%
6	6.451	737	742	745	rBV	3043768	2938702	67.14%	11.476%
7	6.822	802	805	809	rBV	1028396	798741	18.25%	3.119%
8	7.381	895	900	903	rBV	2322085	2291819	52.36%	8.950%
9	8.104	1019	1023	1026	rBV	1325724	1082708	24.74%	4.228%
10	9.181	1201	1206	1209	rBV	4715135	4376786	100.00%	17.092%
11	9.851	1317	1320	1324	rBV	1322140	1173914	26.82%	4.584%
12	10.639	1450	1454	1457	rBV	2675884	2329572	53.23%	9.098%
13	11.333	1569	1572	1576	rBV	1121143	971381	22.19%	3.793%
14	12.663	1795	1798	1805	rVB	224231	201808	4.61%	0.788%
15	12.922	1838	1842	1845	rBV	3620596	3204077	73.21%	12.513%
16	13.969	2016	2020	2024	rBV	991153	824258	18.83%	3.219%
17	15.415	2261	2266	2270	rBV	646679	786236	17.96%	3.070%
18	15.880	2341	2345	2351	rBV3	38188	55757	1.27%	0.218%
19	16.380	2425	2430	2439	rVB	45114	70416	1.61%	0.275%
20	16.957	2524	2528	2537	rVB4	30797	60406	1.38%	0.236%
21	17.657	2641	2647	2657	rVB4	23799	57222	1.31%	0.223%




Sum of corrected areas: 25606642

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125881.D
Acq On : 18 Oct 2021 17:16
Operator : JU/CG
Sample : M4243-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T3-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

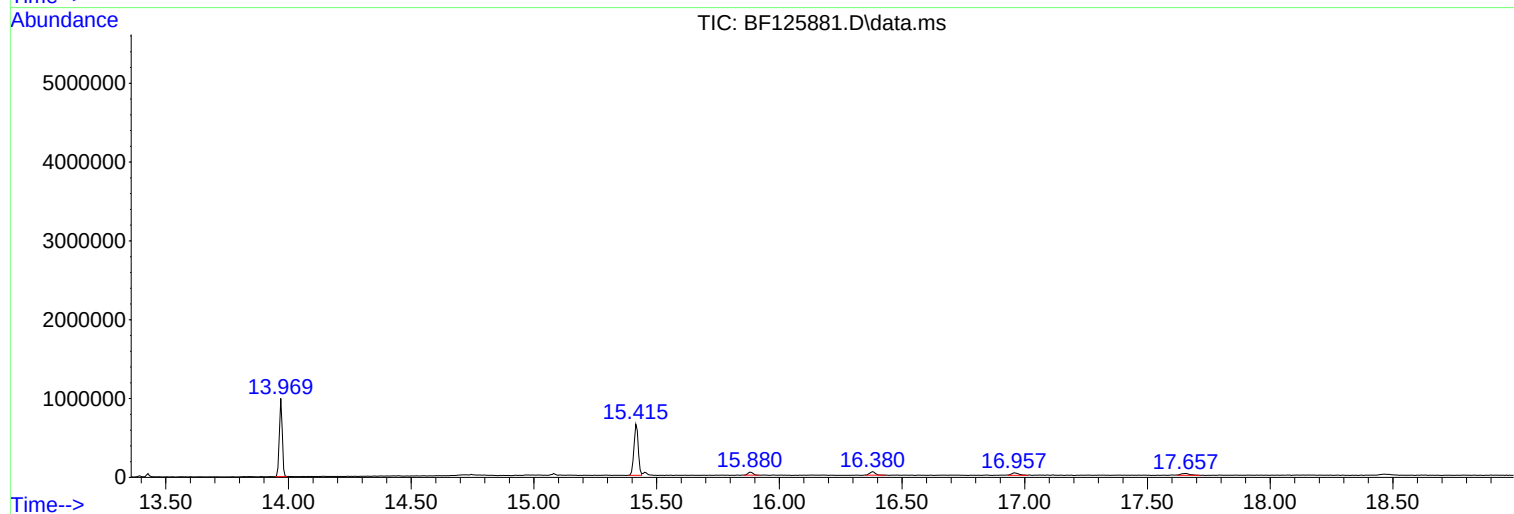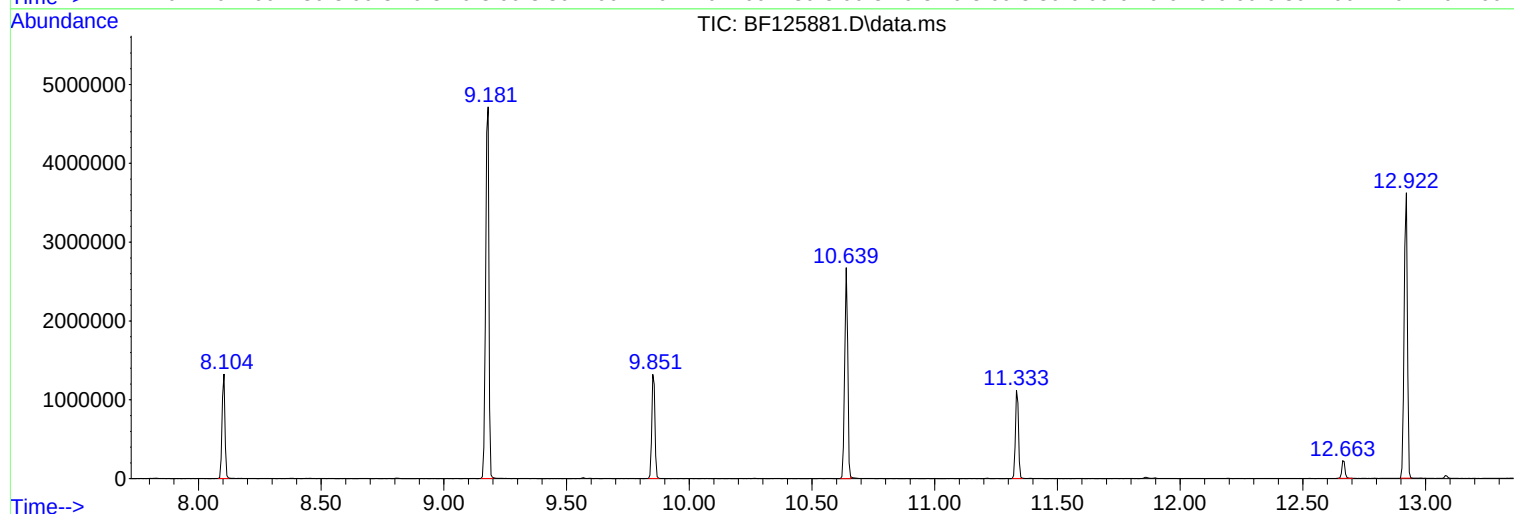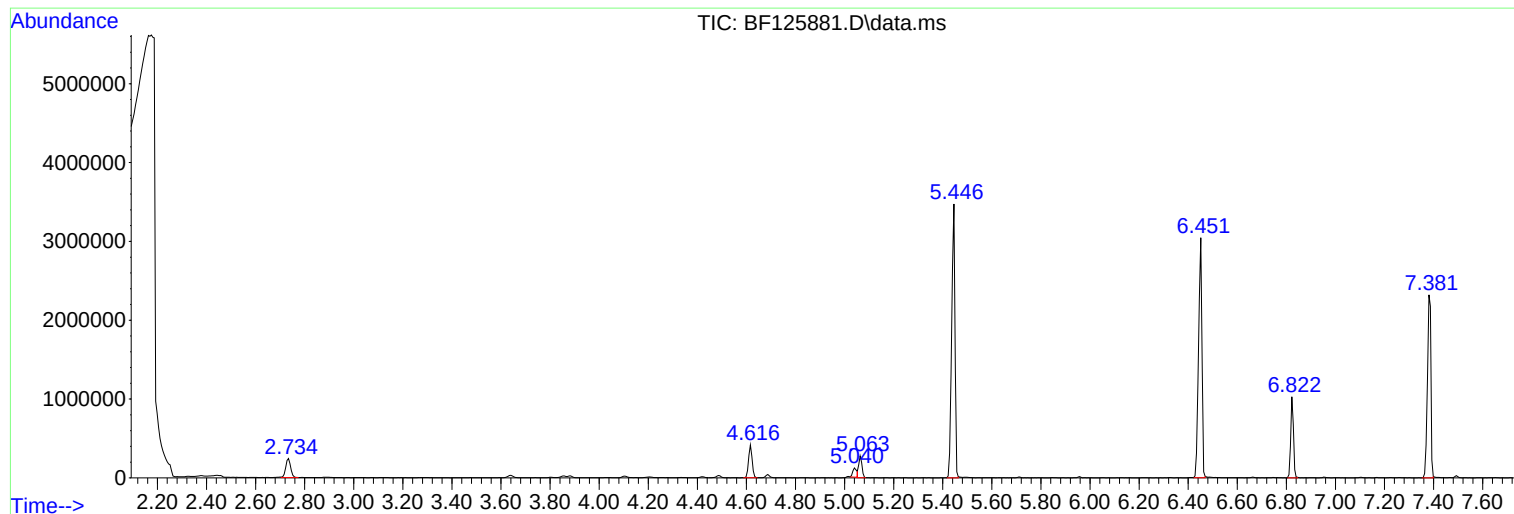

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125881.D
Acq On : 18 Oct 2021 17:16
Operator : JU/CG
Sample : M4243-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T3-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF101821\
Data File : BF125881.D
Acq On : 18 Oct 2021 17:16
Operator : JU/CG
Sample : M4243-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T3-COMP-(1-4)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------